

Data Path : Z:\HPCHEM1\BNA\_G\DATA\BG060615\  
 Data File : BG017516.D  
 Acq On : 7 Jun 2015 2:26  
 Operator : TP/IZ  
 Sample : G2457-25  
 Misc :  
 ALS Vial : 14 Sample Multiplier: 1

Instrument :  
 BNA\_G  
 ClientSampleId :  
 SP-5

Integration Parameters: rteint.p  
 Integrator: RTE  
 Smoothing : ON Filtering: 5  
 Sampling : 1 Min Area: 3 % of largest Peak  
 Start Thrs: 0.2 Max Peaks: 100  
 Stop Thrs : 0 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >  
 Peak separation: 5

Method : Z:\HPCHEM1\BNA\_G\METHODS\8270-BG060315.M  
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

Signal : TIC

| peak<br># | R.T.<br>min | first<br>scan | max<br>scan | last<br>scan | PK<br>TY | peak<br>height | corr.<br>area | corr.<br>% max. | % of<br>total |
|-----------|-------------|---------------|-------------|--------------|----------|----------------|---------------|-----------------|---------------|
| 1         | 2.777       | 10            | 15          | 20           | rVB      | 226100         | 321132        | 16.77%          | 3.753%        |
| 2         | 4.728       | 340           | 347         | 353          | rBV      | 62139          | 89213         | 4.66%           | 1.043%        |
| 3         | 5.215       | 425           | 430         | 442          | rVB      | 370161         | 554913        | 28.98%          | 6.485%        |
| 4         | 6.837       | 699           | 706         | 718          | rBV      | 359846         | 569641        | 29.75%          | 6.657%        |
| 5         | 7.166       | 755           | 762         | 773          | rBV      | 431809         | 659443        | 34.44%          | 7.707%        |
| 6         | 7.619       | 834           | 839         | 845          | rBV2     | 78571          | 117605        | 6.14%           | 1.374%        |
| 7         | 7.942       | 887           | 894         | 900          | rBV      | 308209         | 474497        | 24.78%          | 5.545%        |
| 8         | 8.788       | 1030          | 1038        | 1046         | rBV      | 254739         | 422782        | 22.08%          | 4.941%        |
| 9         | 10.415      | 1304          | 1315        | 1325         | rBV      | 90404          | 162585        | 8.49%           | 1.900%        |
| 10        | 12.906      | 1732          | 1739        | 1751         | rBV      | 694548         | 1004936       | 52.48%          | 11.744%       |
| 11        | 14.293      | 1966          | 1975        | 1982         | rBV      | 155456         | 237347        | 12.39%          | 2.774%        |
| 12        | 15.791      | 2222          | 2230        | 2245         | rBV      | 635656         | 947767        | 49.49%          | 11.076%       |
| 13        | 17.043      | 2437          | 2443        | 2454         | rVB      | 216367         | 321847        | 16.81%          | 3.761%        |
| 14        | 19.687      | 2887          | 2893        | 2900         | rBV      | 1593280        | 1914986       | 100.00%         | 22.380%       |
| 15        | 21.238      | 3151          | 3157        | 3165         | rBV      | 290539         | 383953        | 20.05%          | 4.487%        |
| 16        | 22.789      | 3414          | 3421        | 3425         | rBV8     | 8334           | 19938         | 1.04%           | 0.233%        |
| 17        | 23.476      | 3531          | 3538        | 3545         | rBV      | 184154         | 354195        | 18.50%          | 4.139%        |


Sum of corrected areas: 8556780

Data Path : Z:\HPCHEM1\BNA\_G\DATA\BG060615\  
Data File : BG017516.D  
Acq On : 7 Jun 2015 2:26  
Operator : TP/IZ  
Sample : G2457-25  
Misc :  
ALS Vial : 14 Sample Multiplier: 1

Instrument :  
BNA\_G  
ClientSampleId :  
SP-5

Quant Method : Z:\HPCHEM1\BNA\_G\METHODS\8270-BG060315.M  
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\DATABASE\NIST02.L  
TIC Integration Parameters: LSCINT.P

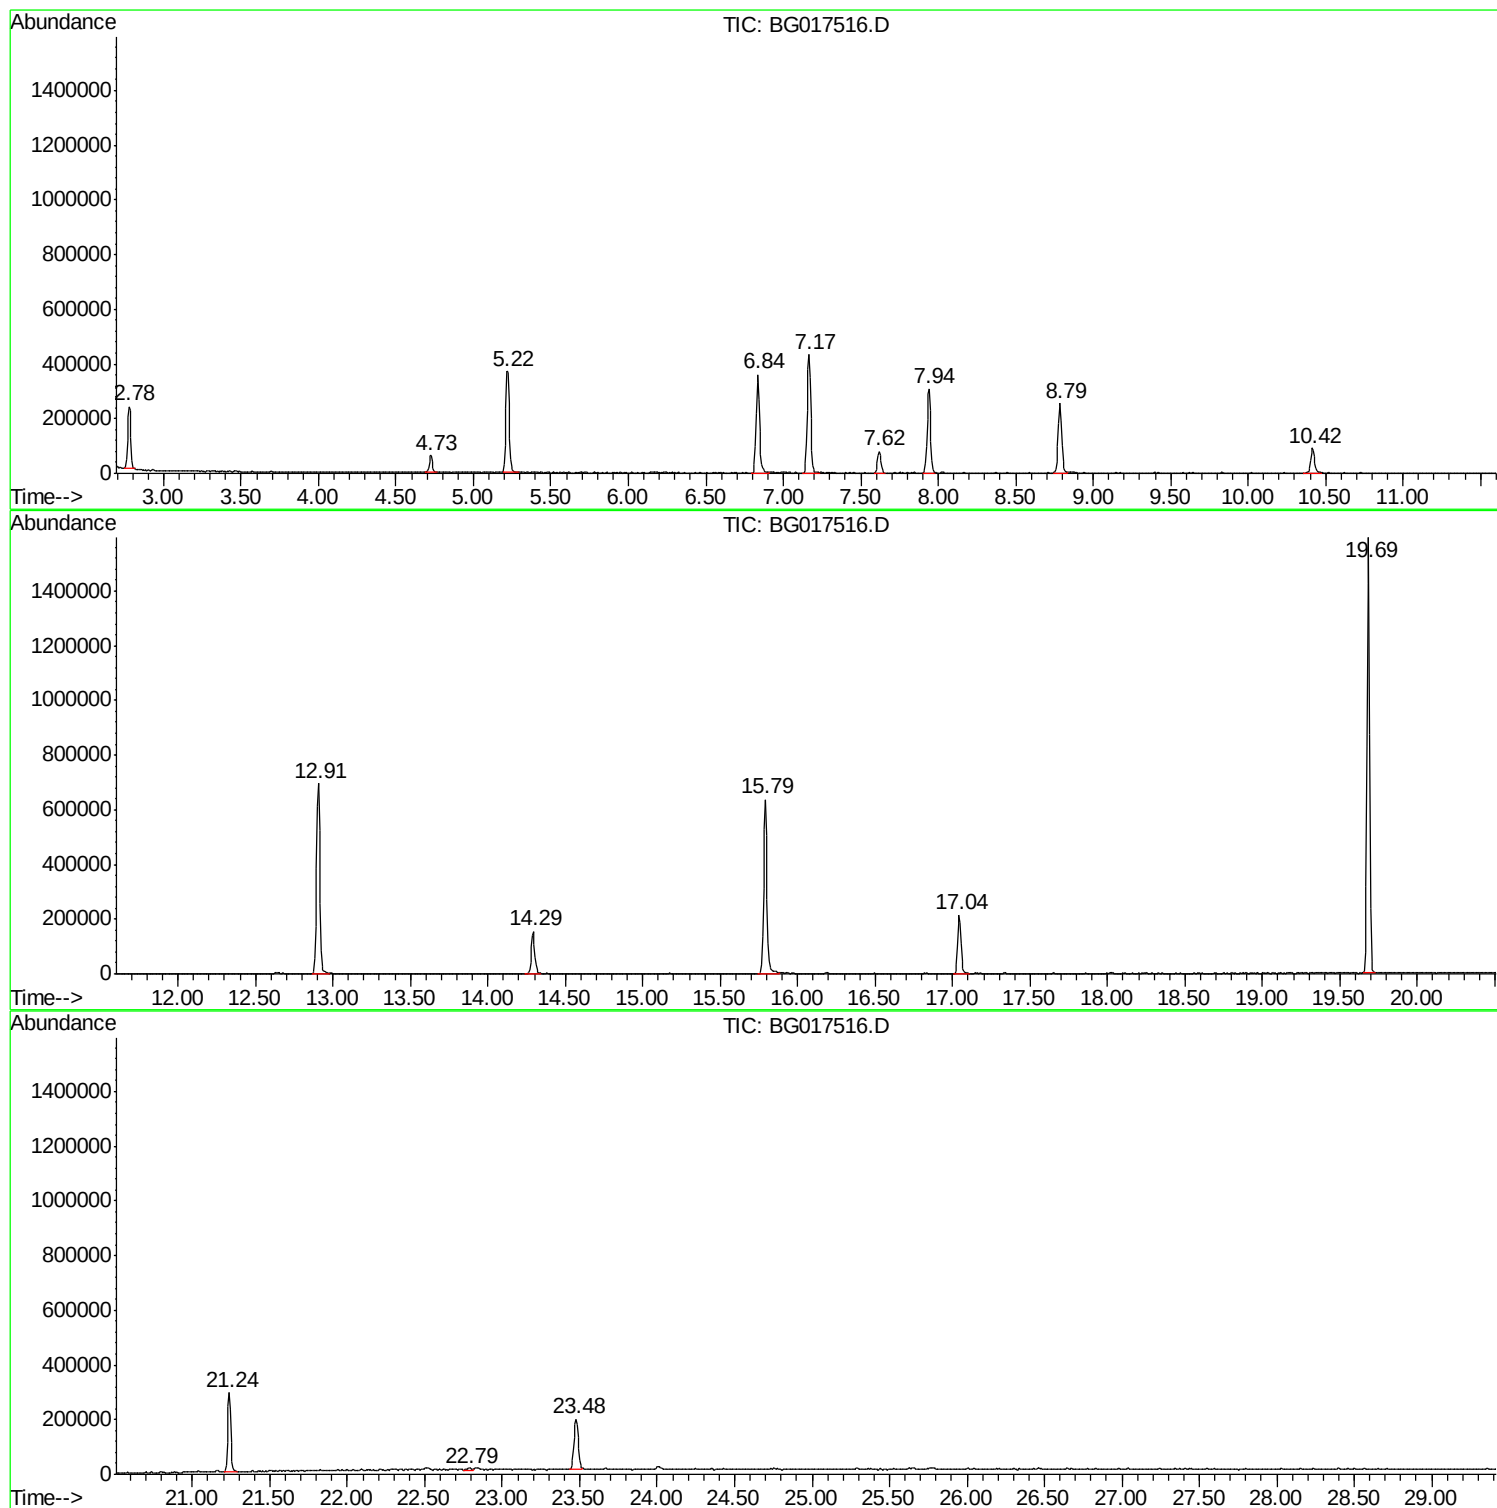

DbaaaPathh::ZZ\NRPBHHM1BBAAGGDBAA\BB0000655\  
 DbaaaFile::BB00I3566DD  
 Aeqq00n :: 77Jun2005 22206  
 Opeaaor ::TPPIZ  
 Samplee ::G0237225  
 Misc ::  
 ASSVaal ::14 SampleeMMultiplier:11

Instrument :  
 BNA\_G  
 ClientSampleId :  
 SP-5

QqaabMebbdd::ZZ\NRPBHHM1BBAAGGMEH00S8270BB000035MM  
 QqaabTitle ::ASBPBNASSANDBBSF00R55P000NTC6AIBRATION

TICCLibbaay ::CC\DATAABASSEN0\$5002LL  
 TICInteggaionPaaameess:LS6CNTTP

| TIC Top Hit name | RT | EstConc | Units | Response | ---Internal Standard--- |
|------------------|----|---------|-------|----------|-------------------------|
|                  |    |         |       | #        | RT Resp Conc            |

No Library Search Compounds Detected

\*\*\*\*\*