

Data Path : Z:\HPCHEM1\BNA_G\DATA\BG060616\
 Data File : BG022196.D
 Acq On : 7 Jun 2016 9:19
 Operator : UM/SJ
 Sample : H3399-08
 Misc :
 ALS Vial : 30 Sample Multiplier: 1

Instrument :
 BNA_G
 ClientSampleId :
 SB-12

Quant Time: Jun 07 15:17:57 2016
 Quant Method : Z:\HPCHEM1\BNA_G\METHODS\8270-BG060616.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Mon Jun 06 16:12:45 2016
 Response via : Initial Calibration


Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Dichlorobenzene-d4	8.12	152	25114	20.00	ng	0.00
21) Naphthalene-d8	10.94	136	118295	20.00	ng	0.00
38) Acenaphthene-d10	14.75	164	76514	20.00	ng	0.00
63) Phenanthrene-d10	17.49	188	176697	20.00	ng	0.00
75) Chrysene-d12	21.76	240	181161	20.00	ng	0.00
86) Perylene-d12	25.06	264	171507	20.00	ng	0.00
System Monitoring Compounds						
5) 2-Fluorophenol	5.66	112	244812	188.47	ng	0.00
7) Phenol-d6	7.28	99	349982	171.37	ng	0.00
23) Nitrobenzene-d5	9.29	82	176200	103.84	ng	0.00
41) 2,4,6-Tribromophenol	16.23	330	135818	157.09	ng	0.00
44) 2-Fluorobiphenyl	13.37	172	488320	97.26	ng	0.00
78) Terphenyl-d14	20.08	244	727073	95.28	ng	0.00
Target Compounds						
49) Dimethylphthalate	14.19	163	38413	6.05	ng	Qvalue 97


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\HPCHEM1\BNA_G\DATA\BG060616\
Data File : BG022196.D
Acq On : 7 Jun 2016 9:19
Operator : UM/SJ
Sample : H3399-08
Misc :
ALS Vial : 30 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
SB-12

Quant Time: Jun 07 15:17:57 2016
Quant Method : Z:\HPCHEM1\BNA_G\METHODS\8270-BG060616.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Mon Jun 06 16:12:45 2016
Response via : Initial Calibration

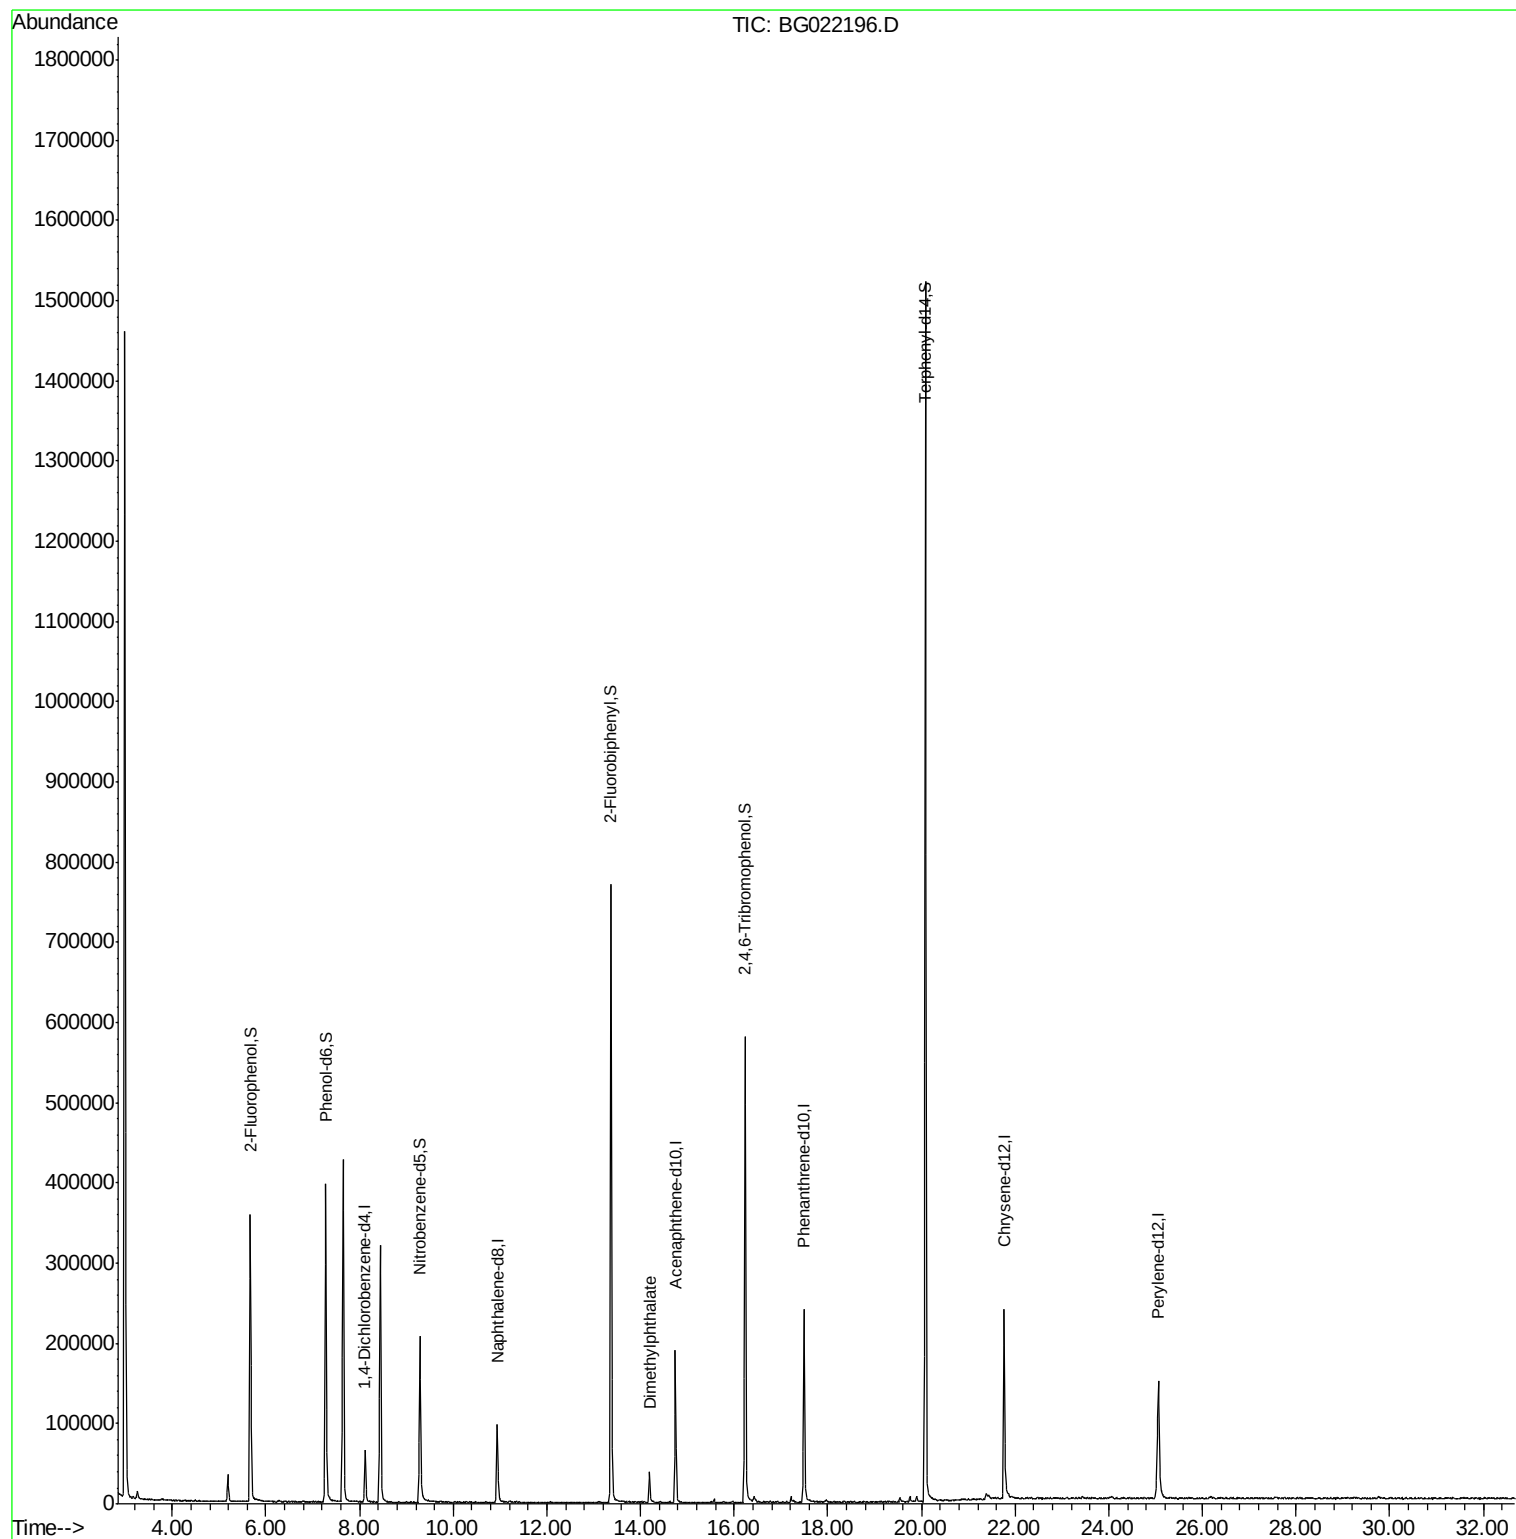

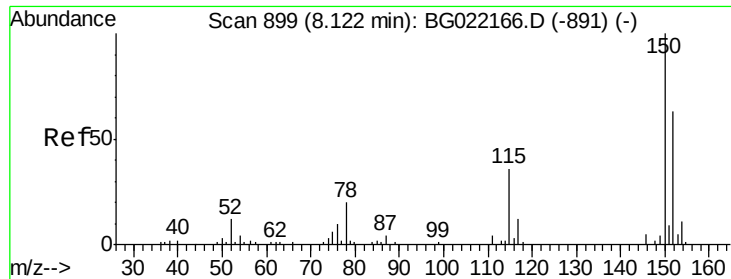

#1

1,4-Dichlorobenzene-d4

Concen: 20.00 ng

RT: 8.12 min Scan# 899

Delta R.T. -0.00 min

Lab File: BG022196.D

Acq: 7 Jun 2016 9:19

Instrument :

BNA_G

ClientSampleId :

SB-12





Tgt Ion:152 Resp: 25114

Ion Ratio Lower Upper

152 100

150 159.8 130.1 195.1

115 60.7 62.2 93.2#

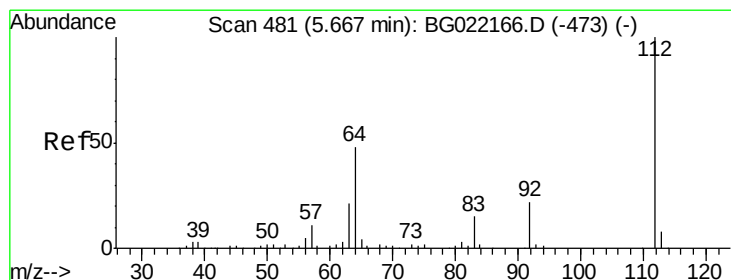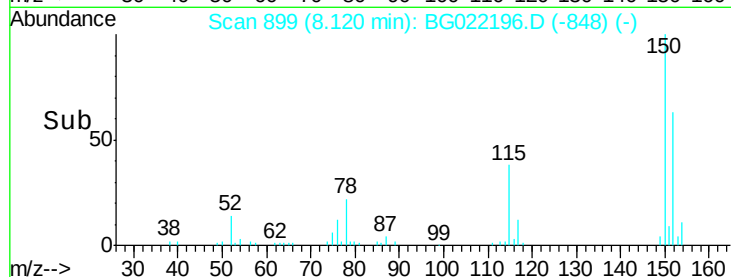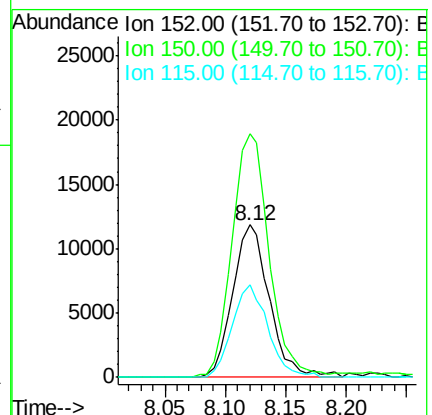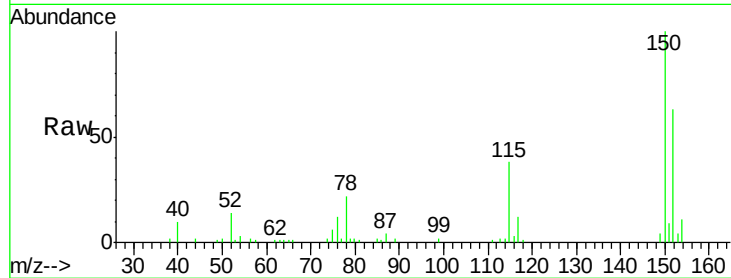

#5

2-Fluorophenol

Concen: 188.47 ng

RT: 5.66 min Scan# 481

Delta R.T. -0.00 min

Lab File: BG022196.D

Acq: 7 Jun 2016 9:19




Tgt Ion:112 Resp: 244812


Ion Ratio Lower Upper

112 100

64 46.8 51.1 76.7#

63 23.3 24.6 37.0#

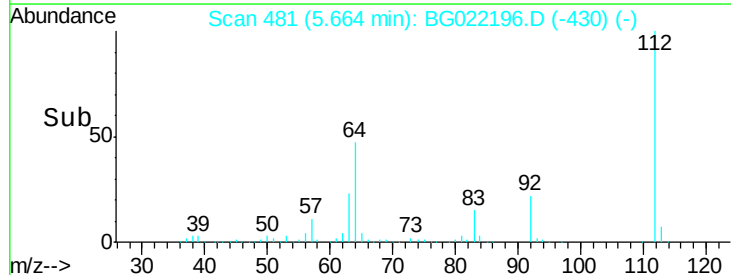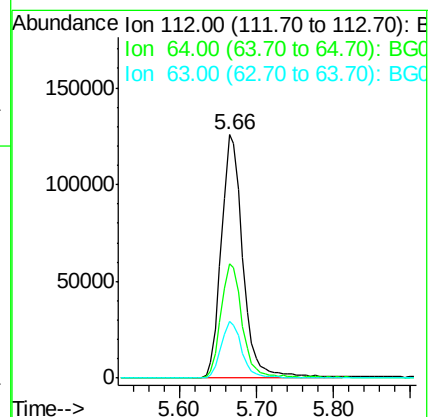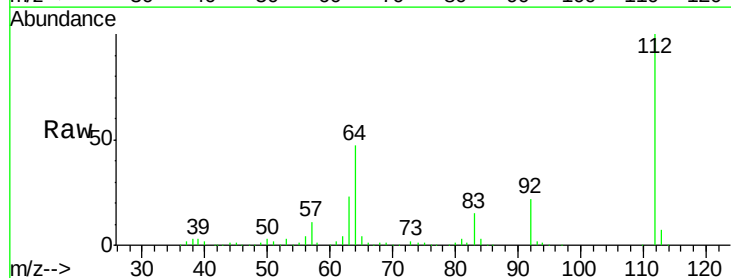

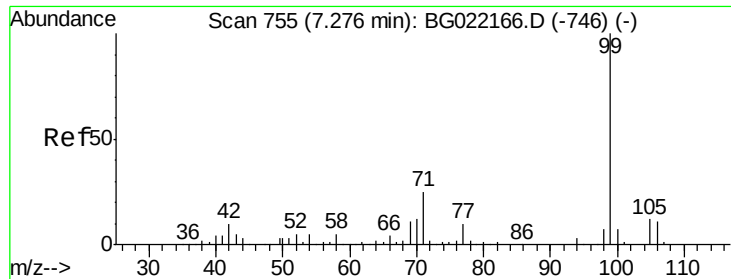

#7

Phenol-d6

Concen: 171.37 ng

RT: 7.28 min Scan# 756

Delta R.T. 0.00 min

Lab File: BG022196.D

Acq: 7 Jun 2016 9:19

Instrument :

BNA_G

ClientSampleId :

SB-12


Tgt Ion: 99 Resp: 349982

Ion Ratio Lower Upper




99 100

42 9.2 16.4 24.6#

71 24.9 25.0 37.4#

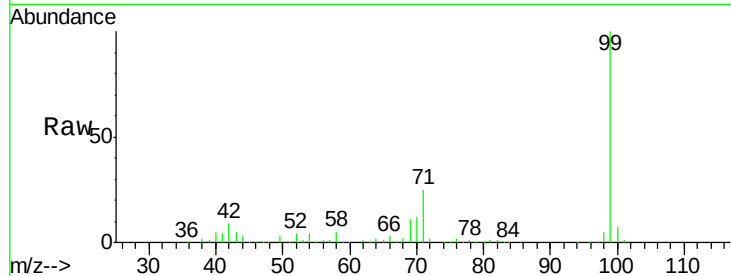

Abundance Ion 99.00 (98.70 to 99.70): BGC
Ion 42.00 (41.70 to 42.70): BGC
Ion 71.00 (70.70 to 71.70): BGC

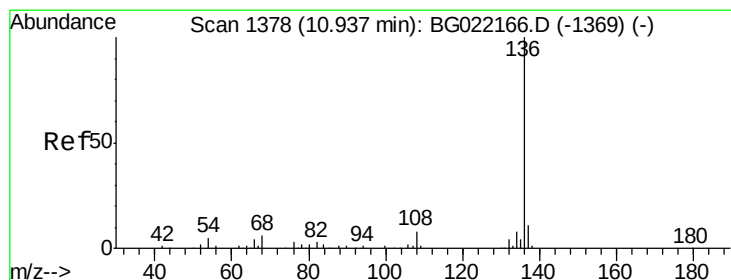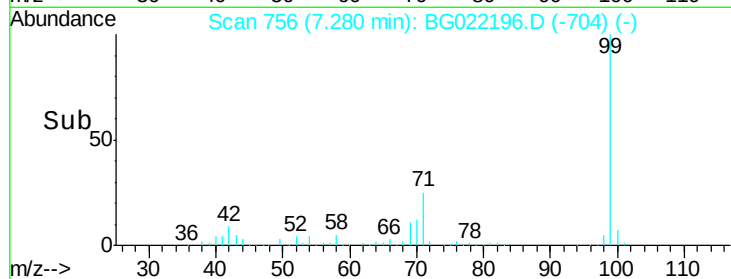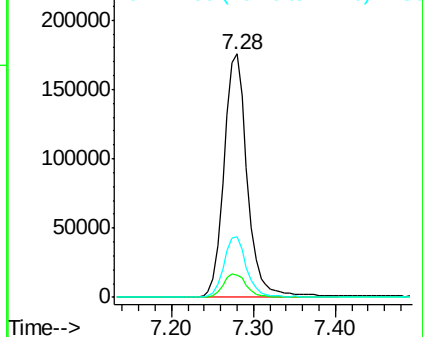

#21

Naphthalene-d8

Concen: 20.00 ng

RT: 10.94 min Scan# 1379

Delta R.T. 0.00 min

Lab File: BG022196.D

Acq: 7 Jun 2016 9:19

Tgt Ion: 136 Resp: 118295


Ion Ratio Lower Upper

136 100



137 11.1 9.0 13.4


54 5.6 9.6 14.4#

68 5.6 6.4 9.6#

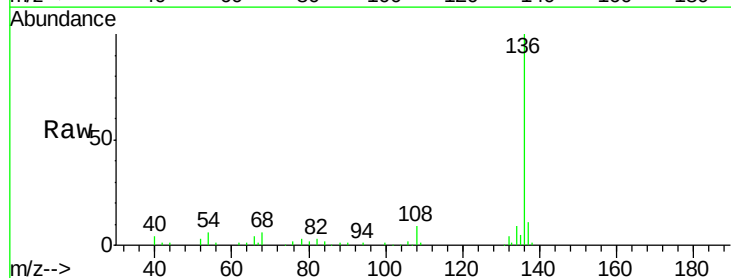

Abundance Ion 136.00 (135.70 to 136.70): BGC
Ion 137.00 (136.70 to 137.70): BGC
Ion 54.00 (53.70 to 54.70): BGC
Ion 68.00 (67.70 to 68.70): BGC

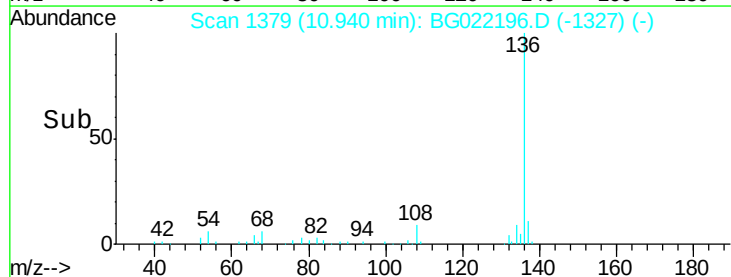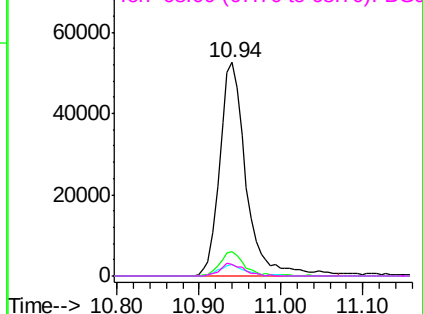


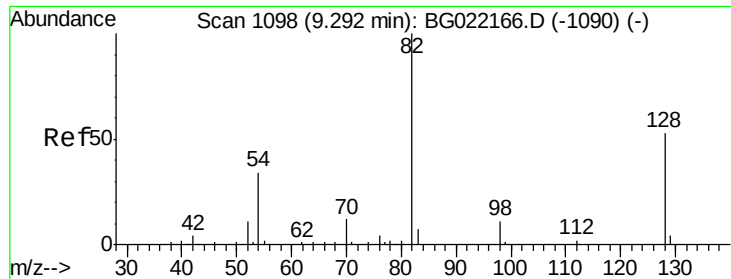




#23
 Nitrobenzene-d5
 Concen: 103.84 ng
 RT: 9.29 min Scan# 1098
 Delta R.T. -0.00 min
 Lab File: BG022196.D
 Acq: 7 Jun 2016 9:19

Instrument :
 BNA_G
 ClientSampleId :
 SB-12

Tgt Ion: 82 Resp: 176200
 Ion Ratio Lower Upper
 82 100
 128 50.1 33.4 50.0#
 54 32.9 46.1 69.1#

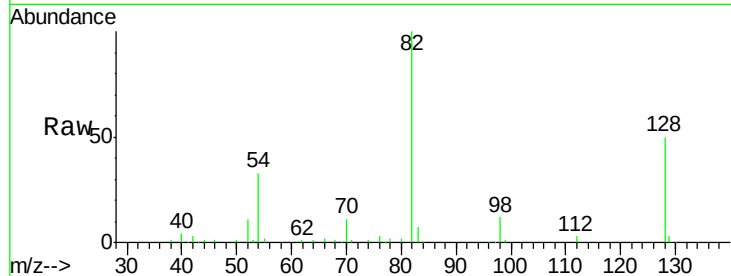


Abundance Ion 82.00 (81.70 to 82.70): BGC
 Ion 128.00 (127.70 to 128.70): BGC
 Ion 54.00 (53.70 to 54.70): BGC

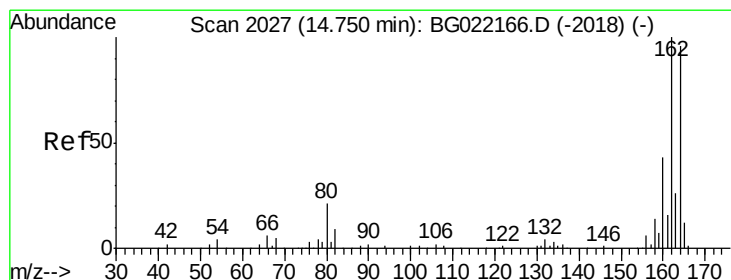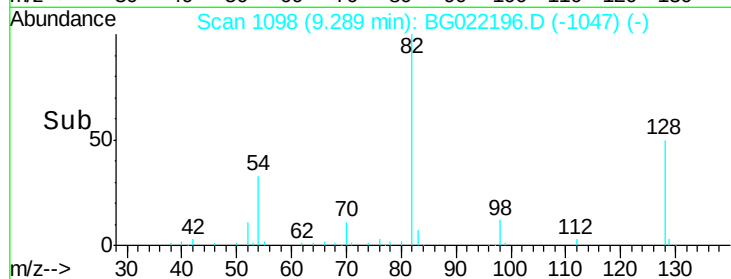
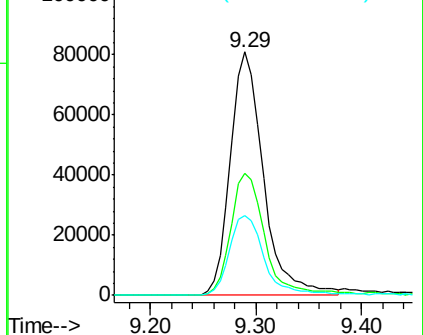



#38
 Acenaphthene-d10
 Concen: 20.00 ng
 RT: 14.75 min Scan# 2027
 Delta R.T. -0.00 min
 Lab File: BG022196.D
 Acq: 7 Jun 2016 9:19

Tgt Ion: 164 Resp: 76514
 Ion Ratio Lower Upper
 164 100
 162 99.8 78.0 117.0
 160 46.9 32.9 49.3

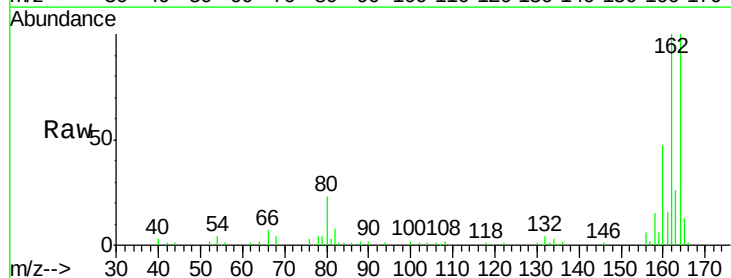

Abundance Ion 164.00 (163.70 to 164.70): BGC
 Ion 162.00 (161.70 to 162.70): BGC
 Ion 160.00 (159.70 to 160.70): BGC

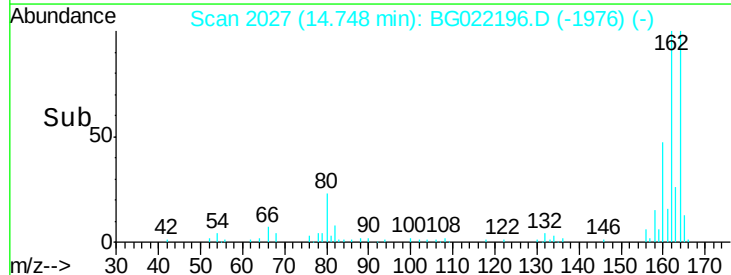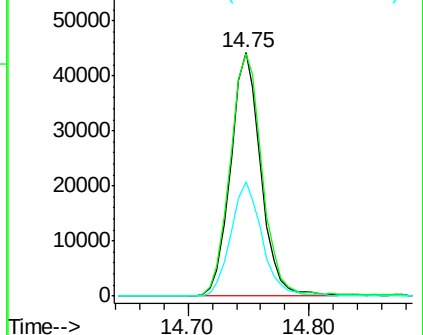


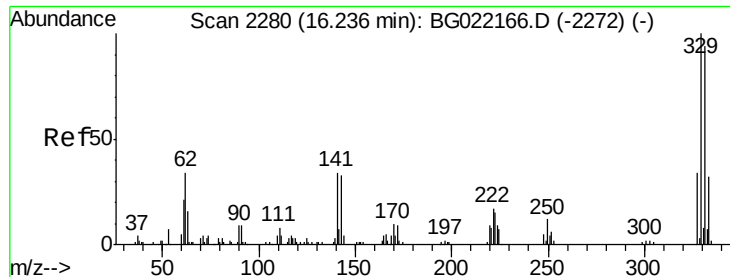




#41
 2,4,6-Tribromophenol
 Concen: 157.09 ng
 RT: 16.23 min Scan# 2280
 Delta R.T. -0.00 min
 Lab File: BG022196.D
 Acq: 7 Jun 2016 9:19

Instrument :
 BNA_G
 ClientSampleId :
 SB-12

Tgt Ion	Ratio	Lower	Upper
330	100		
332	95.9	78.0	117.0
141	38.5	33.8	50.8

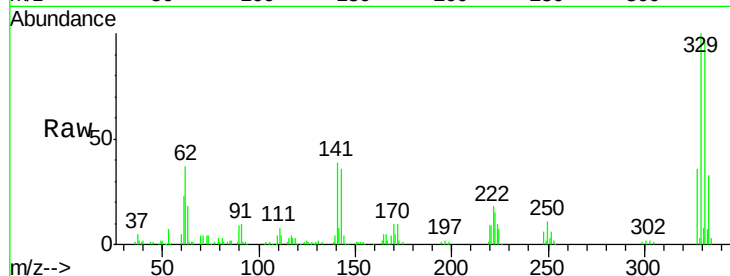


Abundance Ion 329.80 (329.50 to 330.50): E
 Ion 331.80 (331.50 to 332.50): E
 Ion 141.00 (140.70 to 141.70): E

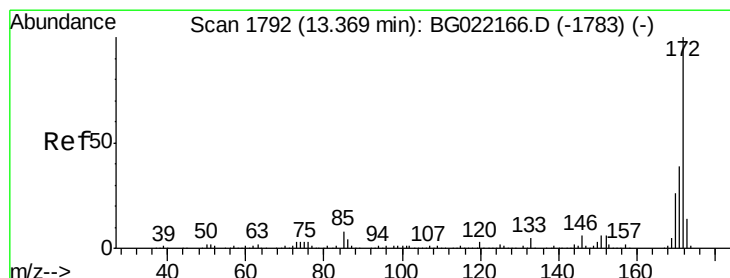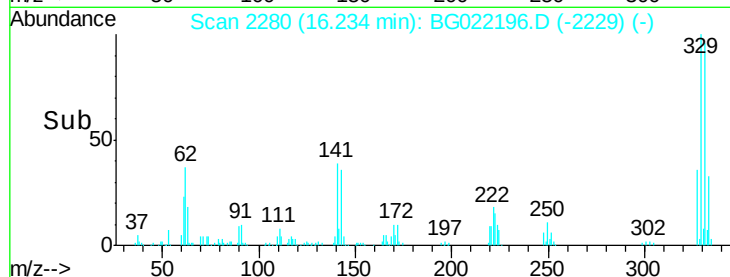
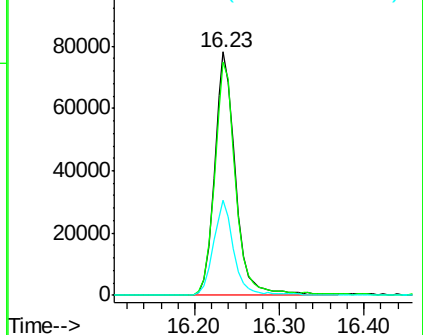



#44
 2-Fluorobiphenyl
 Concen: 97.26 ng
 RT: 13.37 min Scan# 1793
 Delta R.T. 0.00 min
 Lab File: BG022196.D
 Acq: 7 Jun 2016 9:19

Tgt Ion	Ratio	Lower	Upper
172	100		
171	39.1	27.8	41.6
170	25.7	19.6	29.4

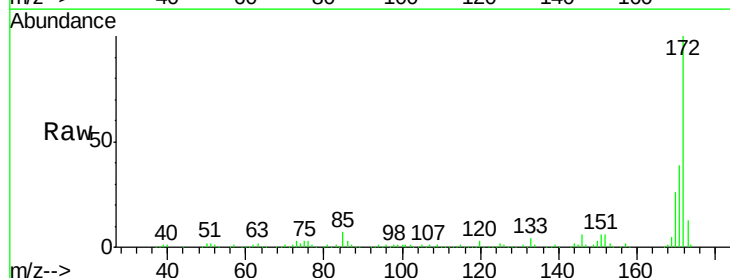

Abundance Ion 172.00 (171.70 to 172.70): E
 Ion 171.00 (170.70 to 171.70): E
 Ion 170.00 (169.70 to 170.70): E

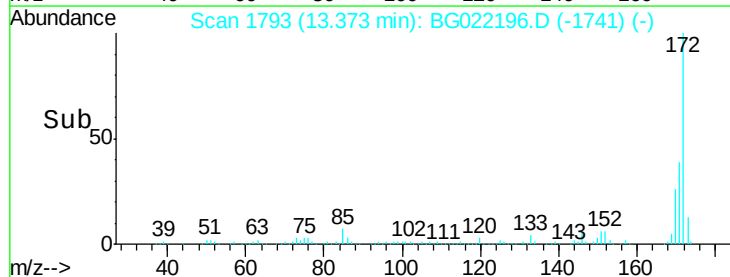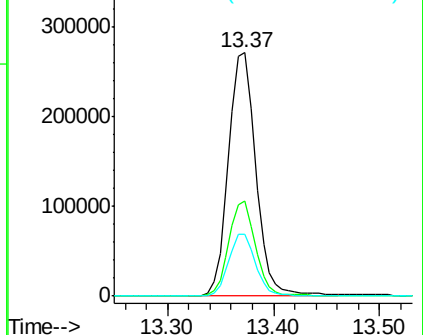

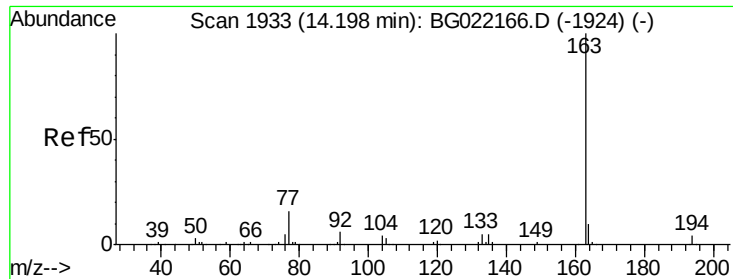

#49

Dimethylphthalate

Concen: 6.05 ng

RT: 14.19 min Scan# 1932

Delta R.T. -0.01 min

Lab File: BG022196.D

Acq: 7 Jun 2016 9:19

Instrument :

BNA_G

ClientSampled :

SB-12


Tgt Ion:163 Resp: 38413

Ion Ratio Lower Upper

163 100

194 3.7 3.0 4.6




164 8.5 8.1 12.1

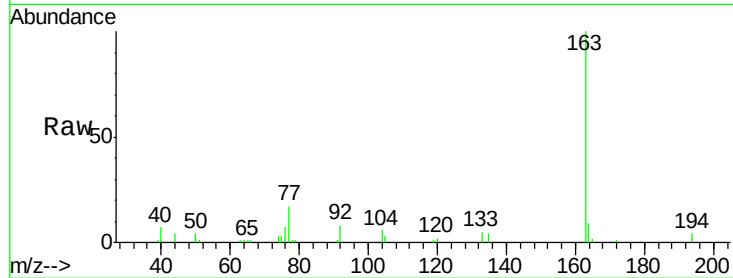

Abundance Ion 163.00 (162.70 to 163.70): E

Ion 194.00 (193.70 to 194.70): E

Ion 164.00 (163.70 to 164.70): E

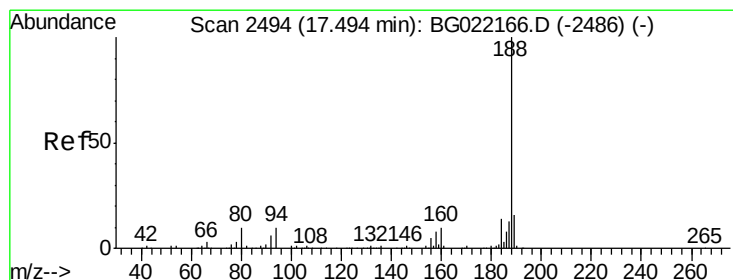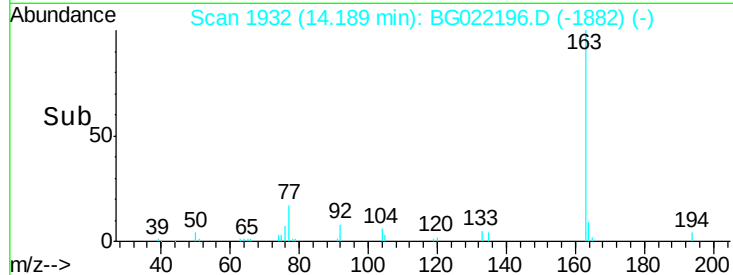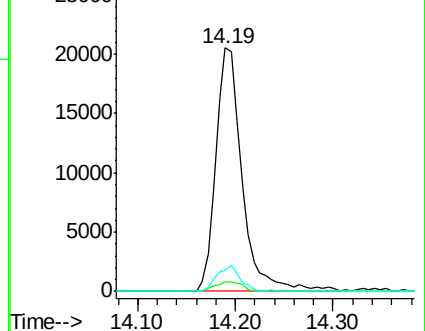

#63

Phenanthrene-d10

Concen: 20.00 ng

RT: 17.49 min Scan# 2494

Delta R.T. -0.00 min

Lab File: BG022196.D

Acq: 7 Jun 2016 9:19


Tgt Ion:188 Resp: 176697

Ion Ratio Lower Upper

188 100

94 9.0 7.5 11.3



80 10.6 8.6 13.0

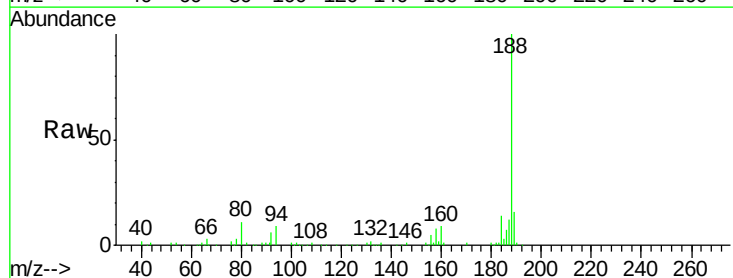


Abundance Ion 188.00 (187.70 to 188.70): E

Ion 94.00 (93.70 to 94.70): BGC

Ion 80.00 (79.70 to 80.70): BGC

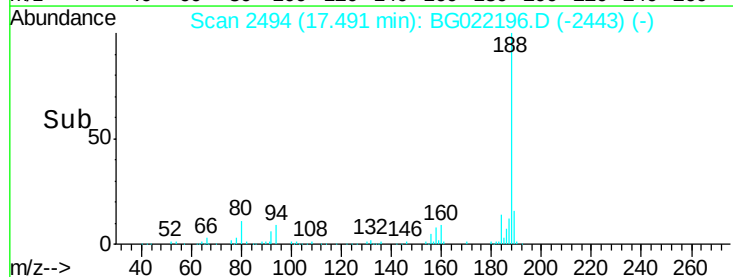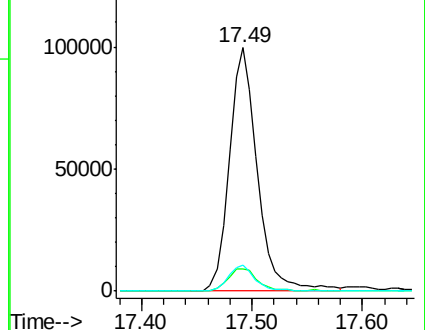

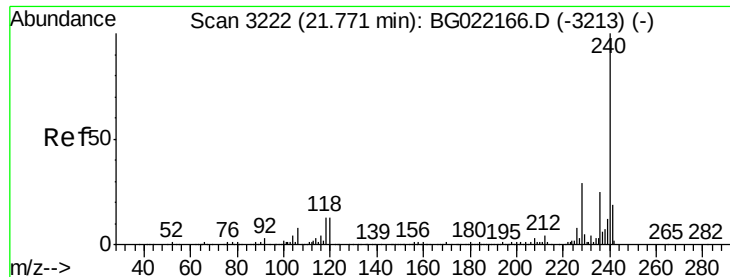

#75

Chrysene-d12

Concen: 20.00 ng

RT: 21.76 min Scan# 3221

Delta R.T. -0.01 min

Lab File: BG022196.D

Acq: 7 Jun 2016 9:19

Instrument :

BNA_G

ClientSampleId :

SB-12


Tgt Ion:240 Resp: 181161

Ion Ratio Lower Upper

240 100

120 13.9 8.4 12.6#




236 24.9 19.6 29.4

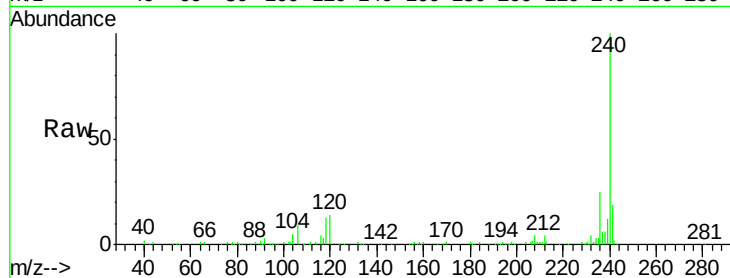

Abundance Ion 240.00 (239.70 to 240.70): E

Ion 120.00 (119.70 to 120.70): E

Ion 236.00 (235.70 to 236.70): E

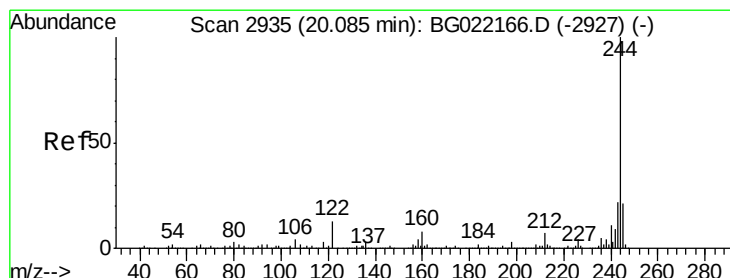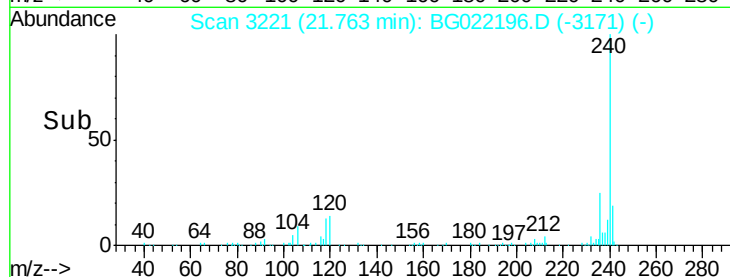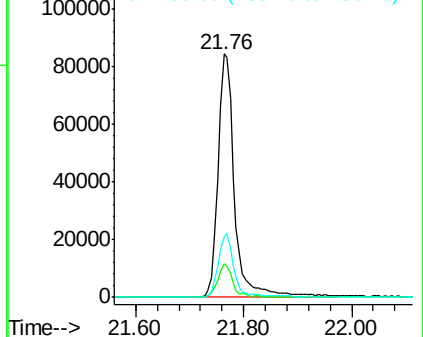

#78

Terphenyl-d14

Concen: 95.28 ng

RT: 20.08 min Scan# 2935

Delta R.T. -0.00 min

Lab File: BG022196.D

Acq: 7 Jun 2016 9:19


Tgt Ion:244 Resp: 727073

Ion Ratio Lower Upper

244 100

212 7.4 6.5 9.7



122 13.1 8.6 12.8#

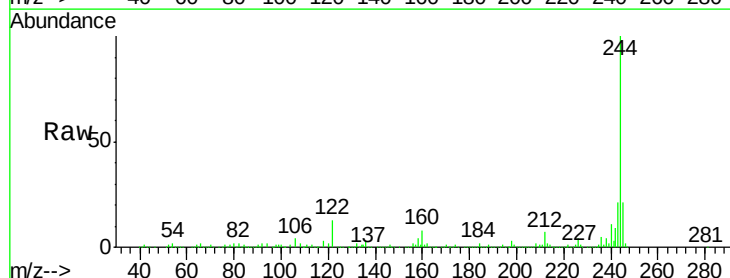


Abundance Ion 244.00 (243.70 to 244.70): E

Ion 212.00 (211.70 to 212.70): E

Ion 122.00 (121.70 to 122.70): E

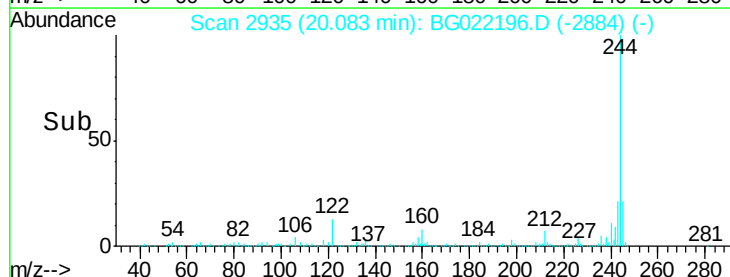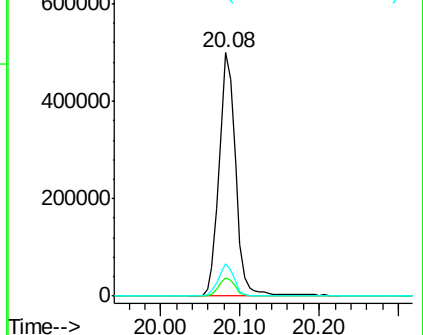

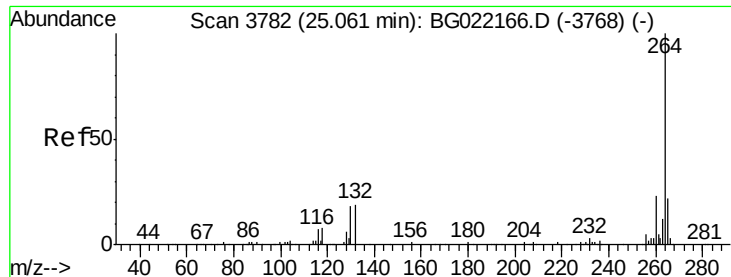

#86
Perylene-d12
Concen: 20.00 ng
RT: 25.06 min Scan# 3782
Delta R.T. -0.00 min
Lab File: BG022196.D
Acq: 7 Jun 2016 9:19

Instrument :
BNA_G
ClientSampleId :
SB-12

Tgt Ion	Ratio	Lower	Upper
264	100		
260	22.3	20.2	30.4
265	22.7	17.8	26.8

