
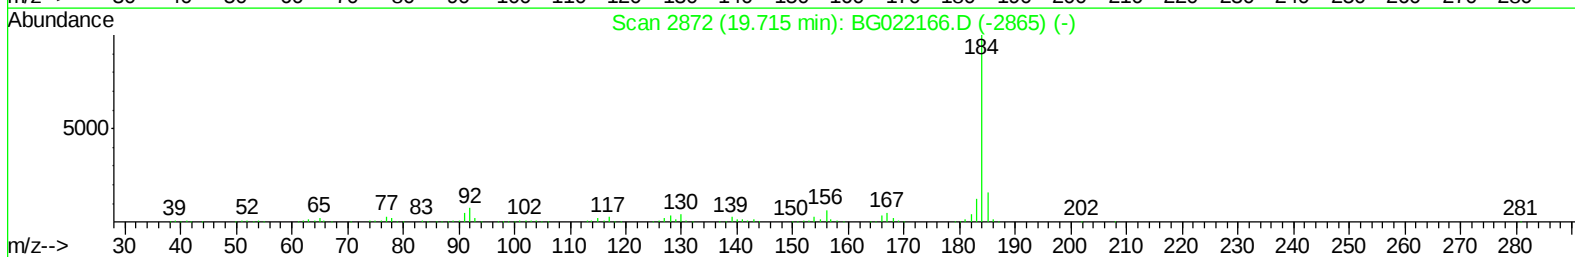
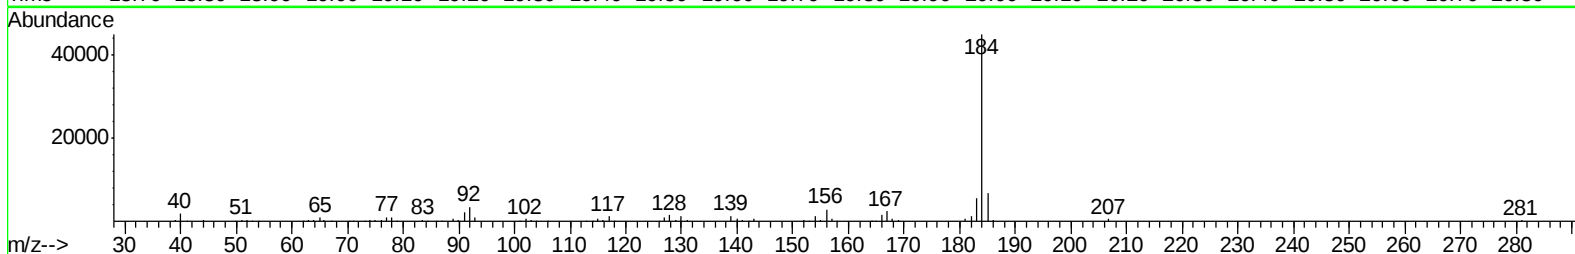


Data Path : Z:\HPCHEM1\BNA_G\DATA\BG060616\
Data File : BG022162.D
Acq On : 6 Jun 2016 10:06
Operator : UM/SJ
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Jun 07 07:38:35 2016
Quant Method : Z:\HPCHEM1\BNA_G\METHODS\8270-BG060616.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Mon Jun 06 16:12:45 2016
Response via : Initial Calibration

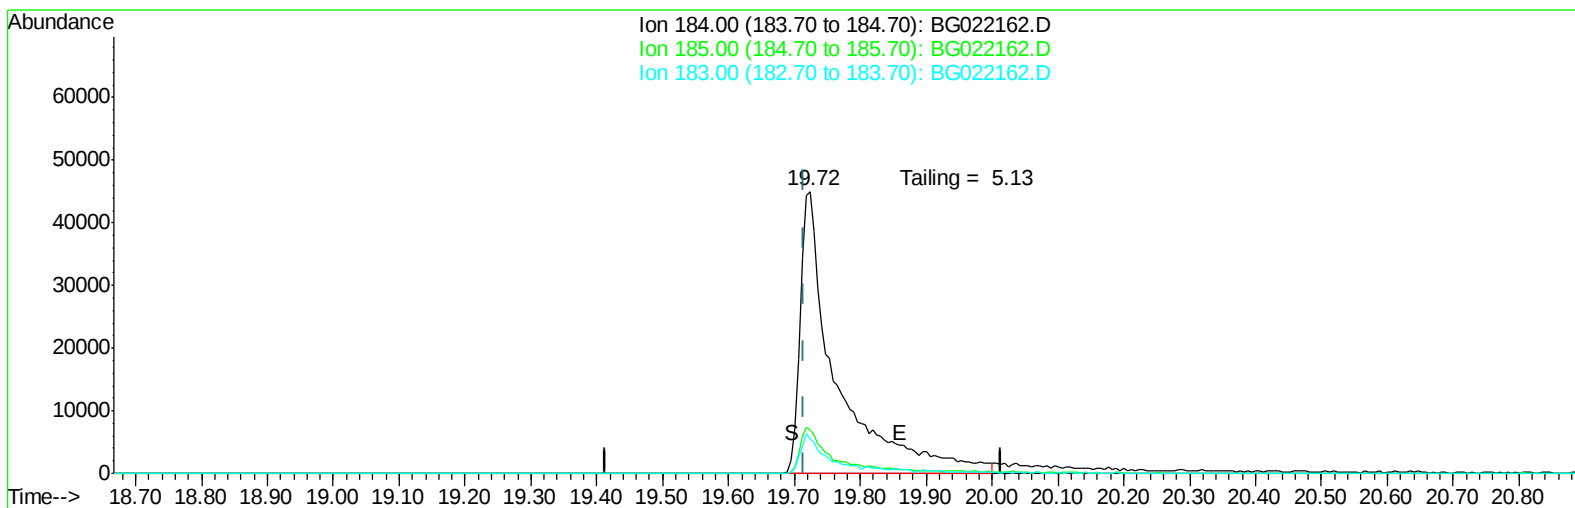

TIC: BG022162.D

(76) Benzidine




19.724min (+0.010) 0.00ng

response 156944

Ion	Exp%	Act%
184.00	100	100
185.00	14.40	15.62
183.00	12.80	12.34
0.00	0.00	0.00

Data Path : Z:\HPCHEM1\BNA_G\DATA\BG060616\
Data File : BG022162.D
Acq On : 6 Jun 2016 10:06
Operator : UM/SJ
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Jun 07 07:38:35 2016
Quant Method : Z:\HPCHEM1\BNA_G\METHODS\8270-BG060616.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Mon Jun 06 16:12:45 2016
Response via : Initial Calibration

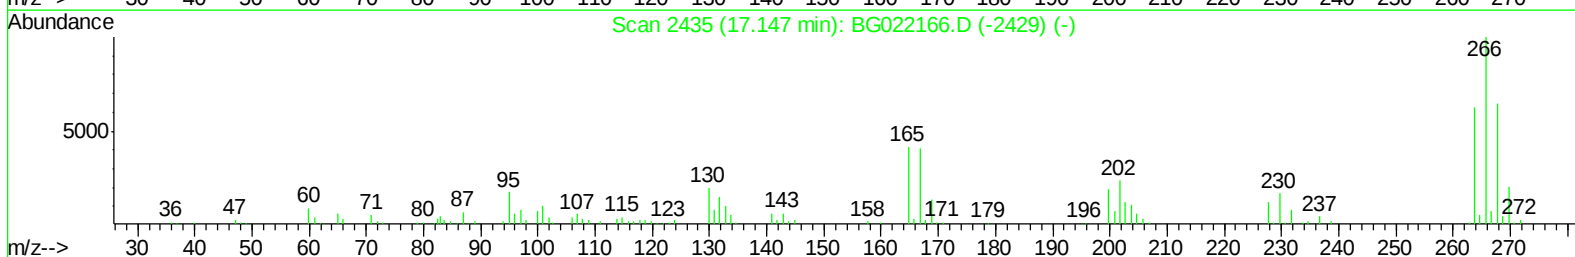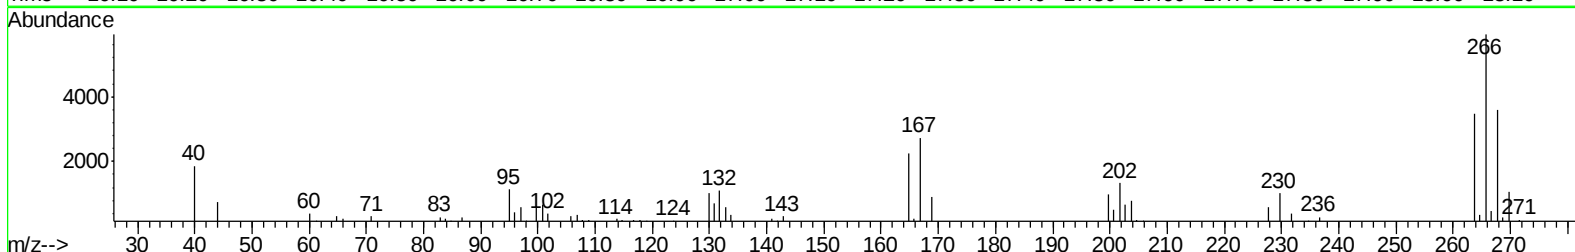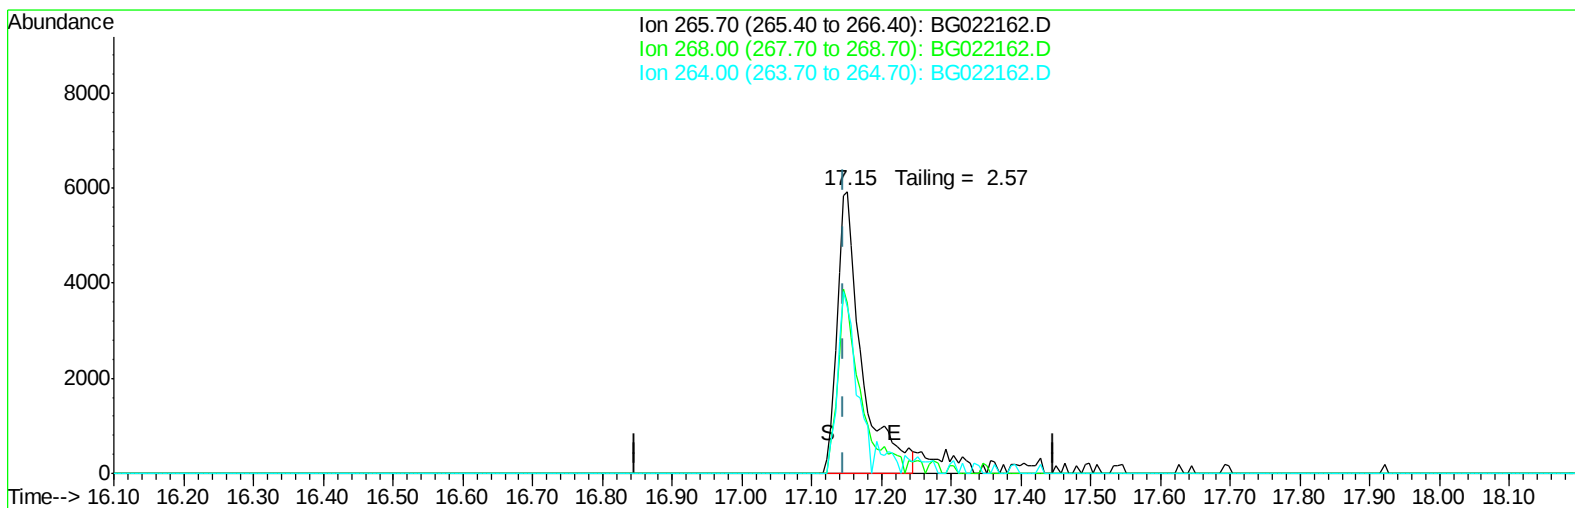

TIC: BG022162.D

(69) Pentachlorophenol (C)

17.151min (+0.004) 0.00ng

response 12496

Ion	Exp%	Act%
265.70	100	100
268.00	68.10	65.28
264.00	67.20	64.66
0.00	0.00	0.00