
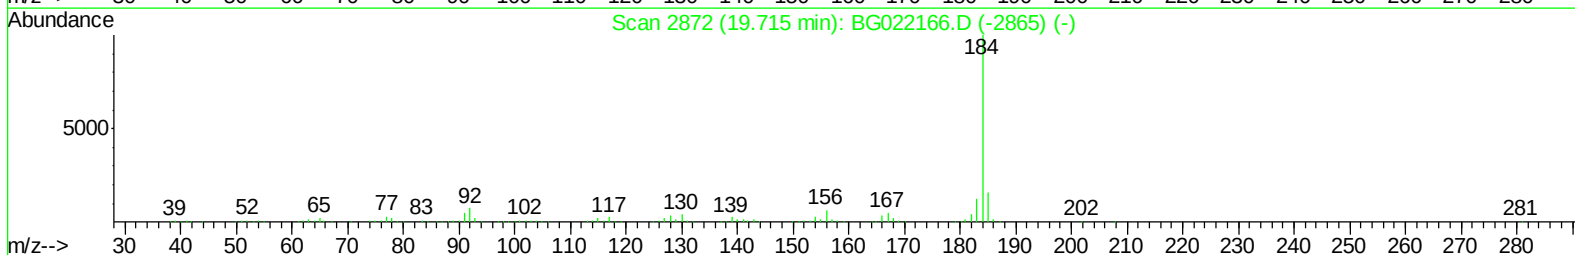
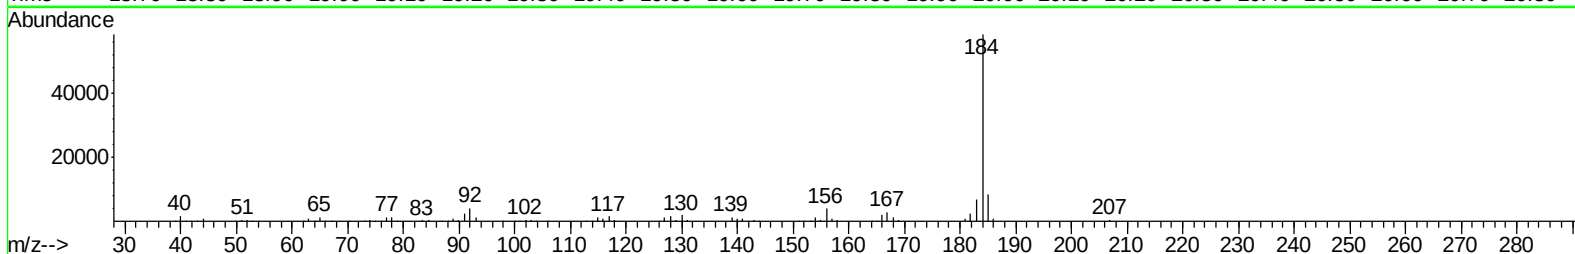


Data Path : Z:\HPCHEM1\BNA_G\DATA\BG060616\
Data File : BG022171.D
Acq On : 6 Jun 2016 16:22
Operator : UM/SJ
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Jun 07 07:39:20 2016
Quant Method : Z:\HPCHEM1\BNA_G\METHODS\8270-BG060616.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Mon Jun 06 16:12:45 2016
Response via : Initial Calibration

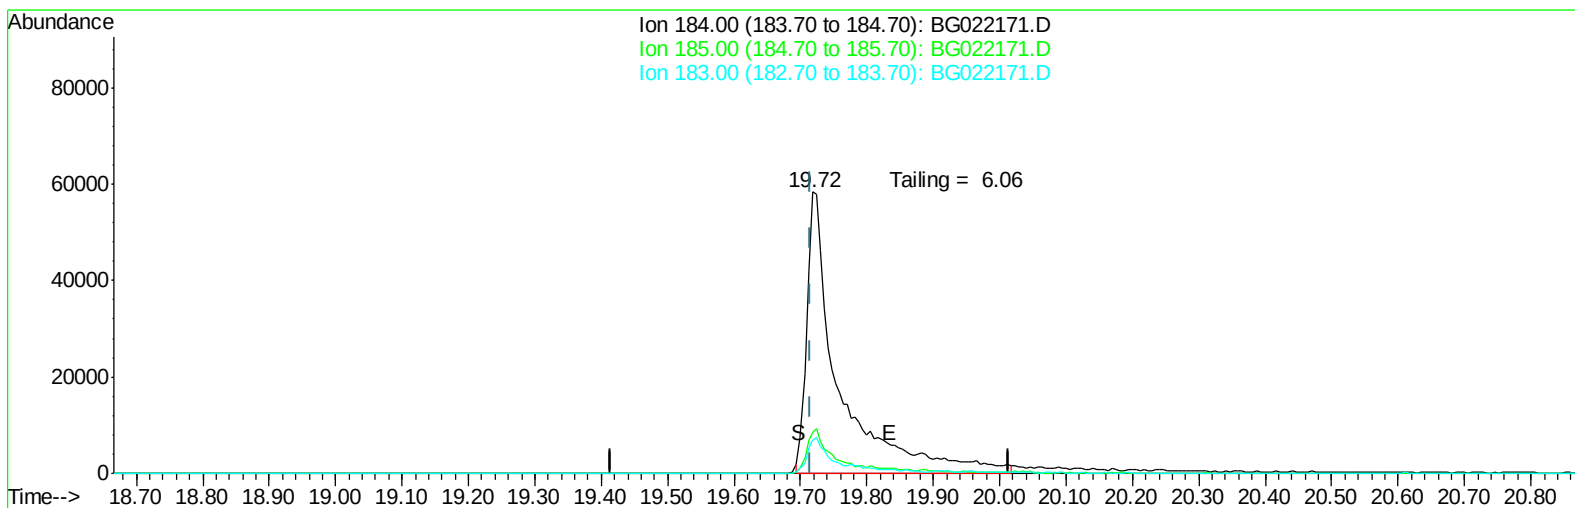

TIC: BG022171.D

(76) Benzidine




19.718min (+0.003) 0.00ng

response 177088

Ion	Exp%	Act%
184.00	100	100
185.00	14.40	14.76
183.00	12.80	12.02
0.00	0.00	0.00

Data Path : Z:\HPCHEM1\BNA_G\DATA\BG060616\
Data File : BG022171.D
Acq On : 6 Jun 2016 16:22
Operator : UM/SJ
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Jun 07 07:39:20 2016
Quant Method : Z:\HPCHEM1\BNA_G\METHODS\8270-BG060616.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Mon Jun 06 16:12:45 2016
Response via : Initial Calibration

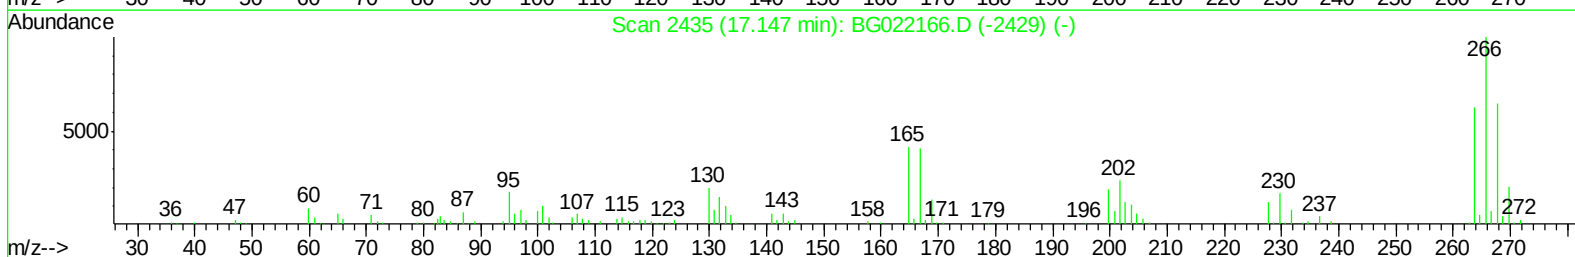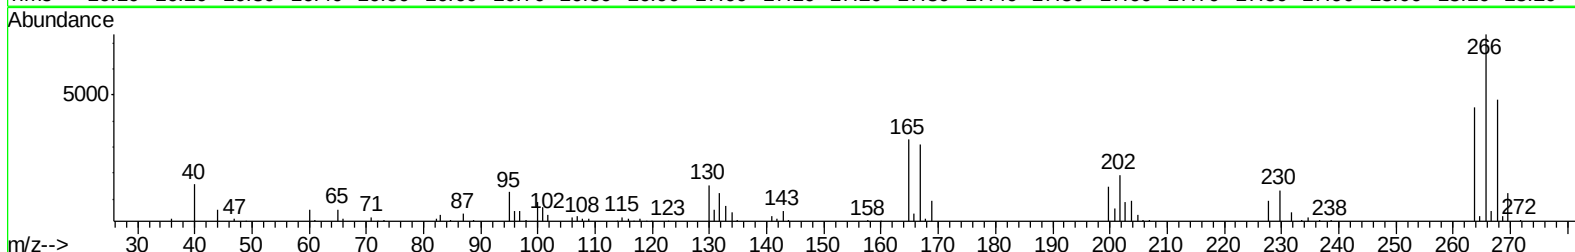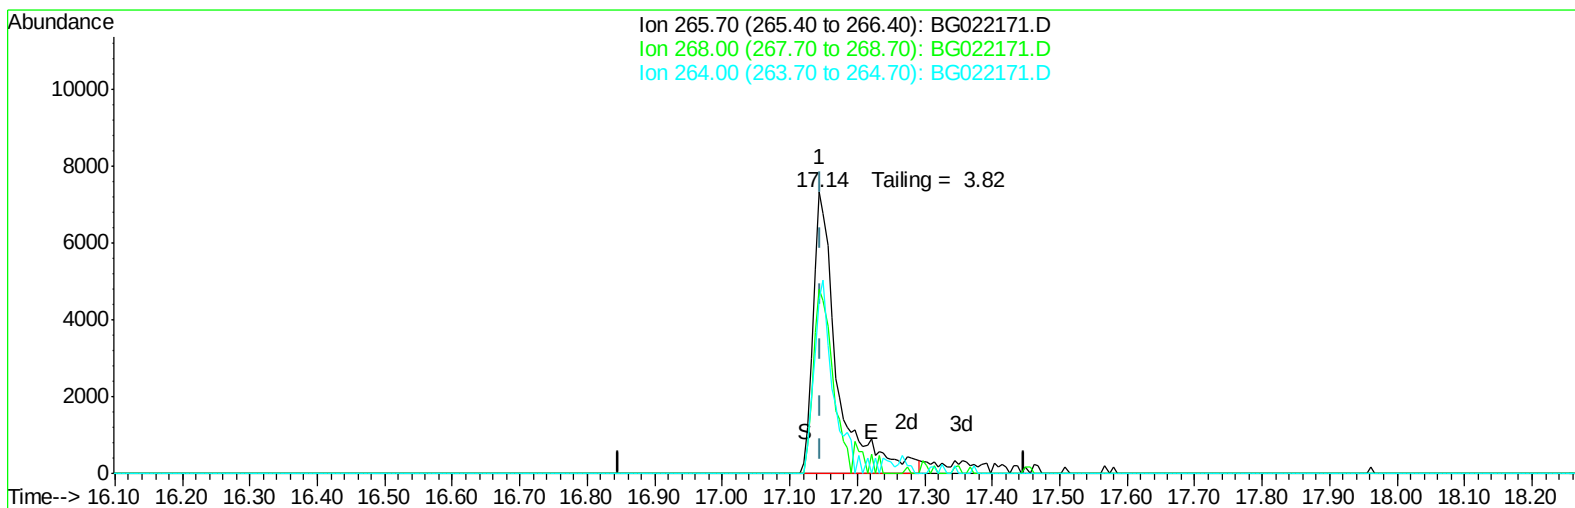

TIC: BG022171.D

(69) Pentachlorophenol (C)

17.144min (-0.003) 0.00ng

response 17467

Ion	Exp%	Act%
265.70	100	100
268.00	68.10	70.50
264.00	67.20	66.50
0.00	0.00	0.00