
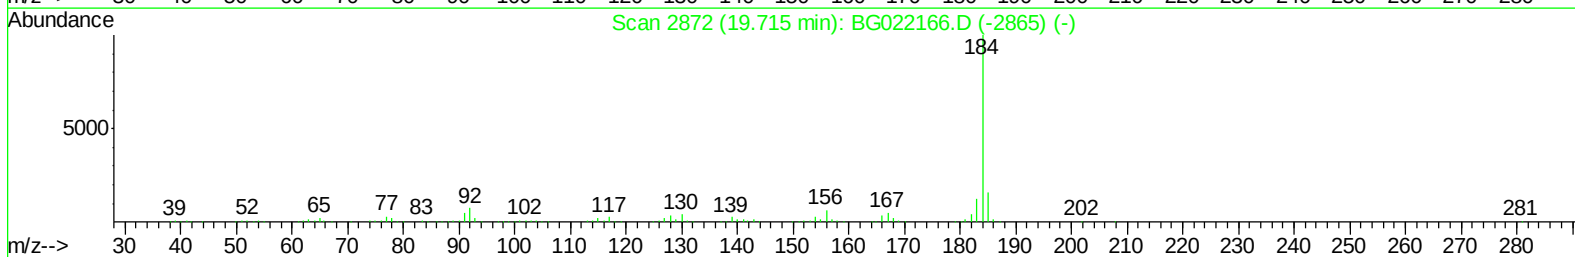
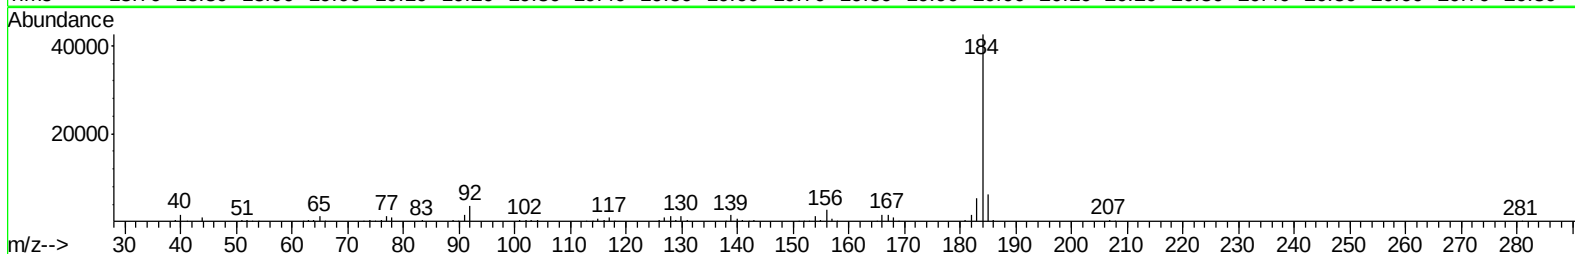


Data Path : Z:\HPCHEM1\BNA_G\DATA\BG060616\
Data File : BG022190.D
Acq On : 7 Jun 2016 5:14
Operator : UM/SJ
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Jun 07 07:40:04 2016
Quant Method : Z:\HPCHEM1\BNA_G\METHODS\8270-BG060616.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Mon Jun 06 16:12:45 2016
Response via : Initial Calibration

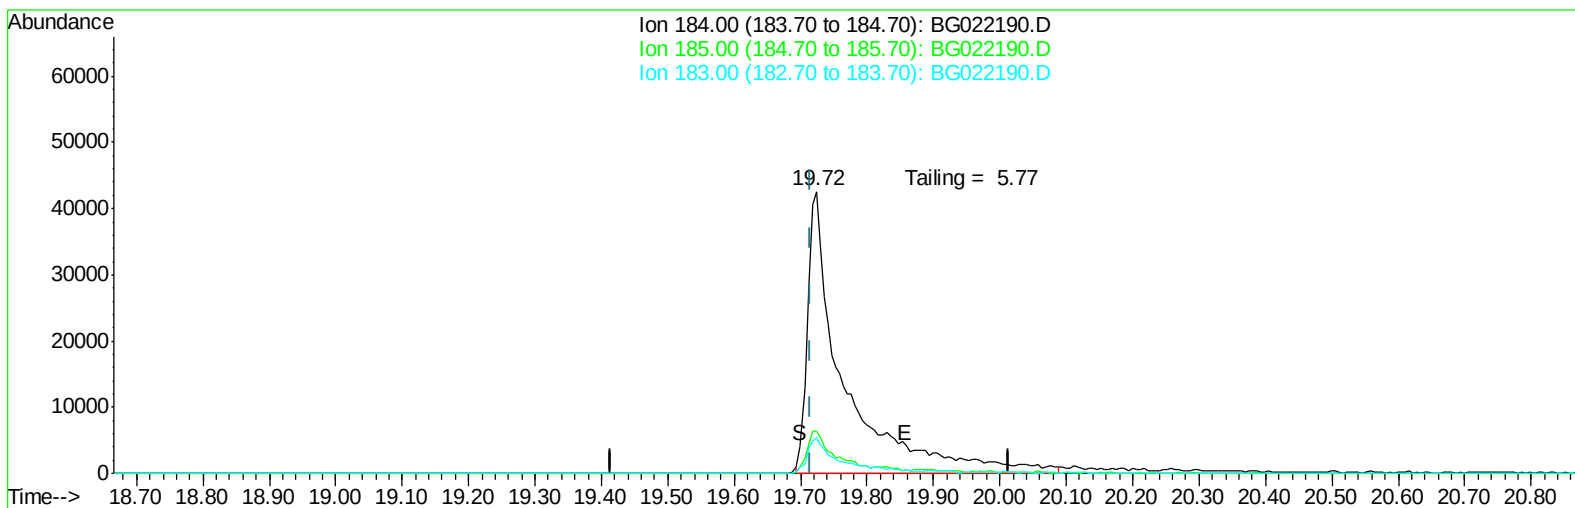

TIC: BG022190.D

(76) Benzidine




19.723min (+0.009) 86189.30ng

response 139740

Ion	Exp%	Act%
184.00	100	100
185.00	14.40	15.00
183.00	12.80	12.53
0.00	0.00	0.00

Data Path : Z:\HPCHEM1\BNA_G\DATA\BG060616\
Data File : BG022190.D
Acq On : 7 Jun 2016 5:14
Operator : UM/SJ
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Jun 07 07:40:04 2016
Quant Method : Z:\HPCHEM1\BNA_G\METHODS\8270-BG060616.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Mon Jun 06 16:12:45 2016
Response via : Initial Calibration

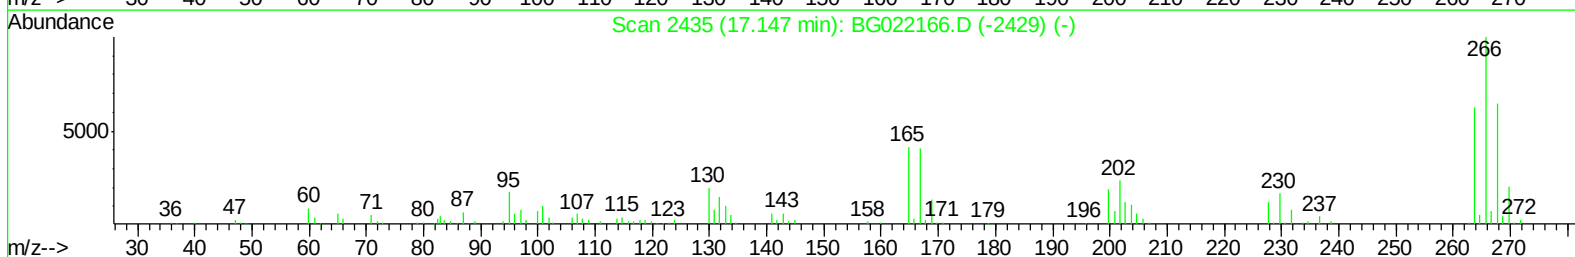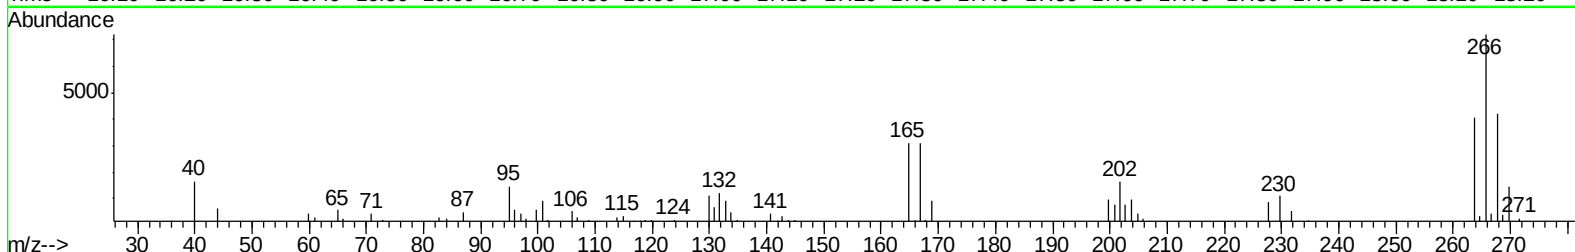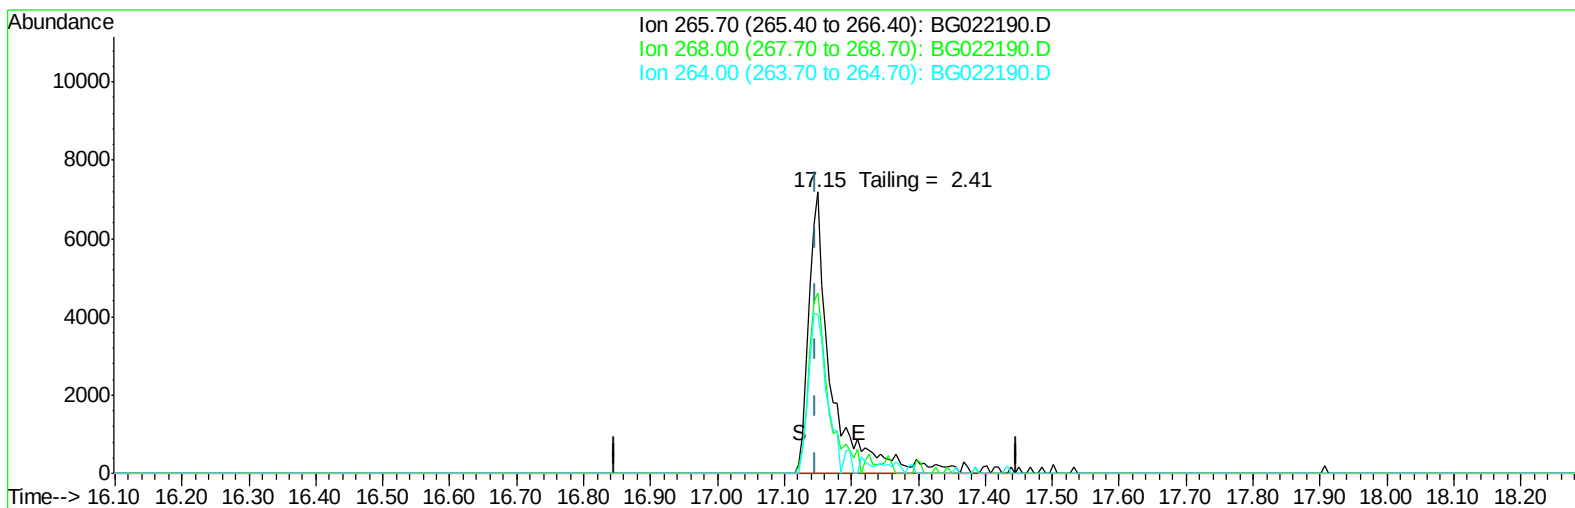

TIC: BG022190.D

(69) Pentachlorophenol (C)

17.150min (+0.003) 0.00ng

response 16508

Ion	Exp%	Act%
265.70	100	100
268.00	68.10	64.14
264.00	67.20	61.04
0.00	0.00	0.00