


Data Path : Z:\HPCHEM1\BNA_G\Data\BG060616\
 Data File : BG022162.D
 Acq On : 6 Jun 2016 10:06
 Operator : UM/SJ
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_G
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\HPCHEM1\BNA_G\METHODS\8270-BG060616.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Mon Jun 06 16:12:45 2016

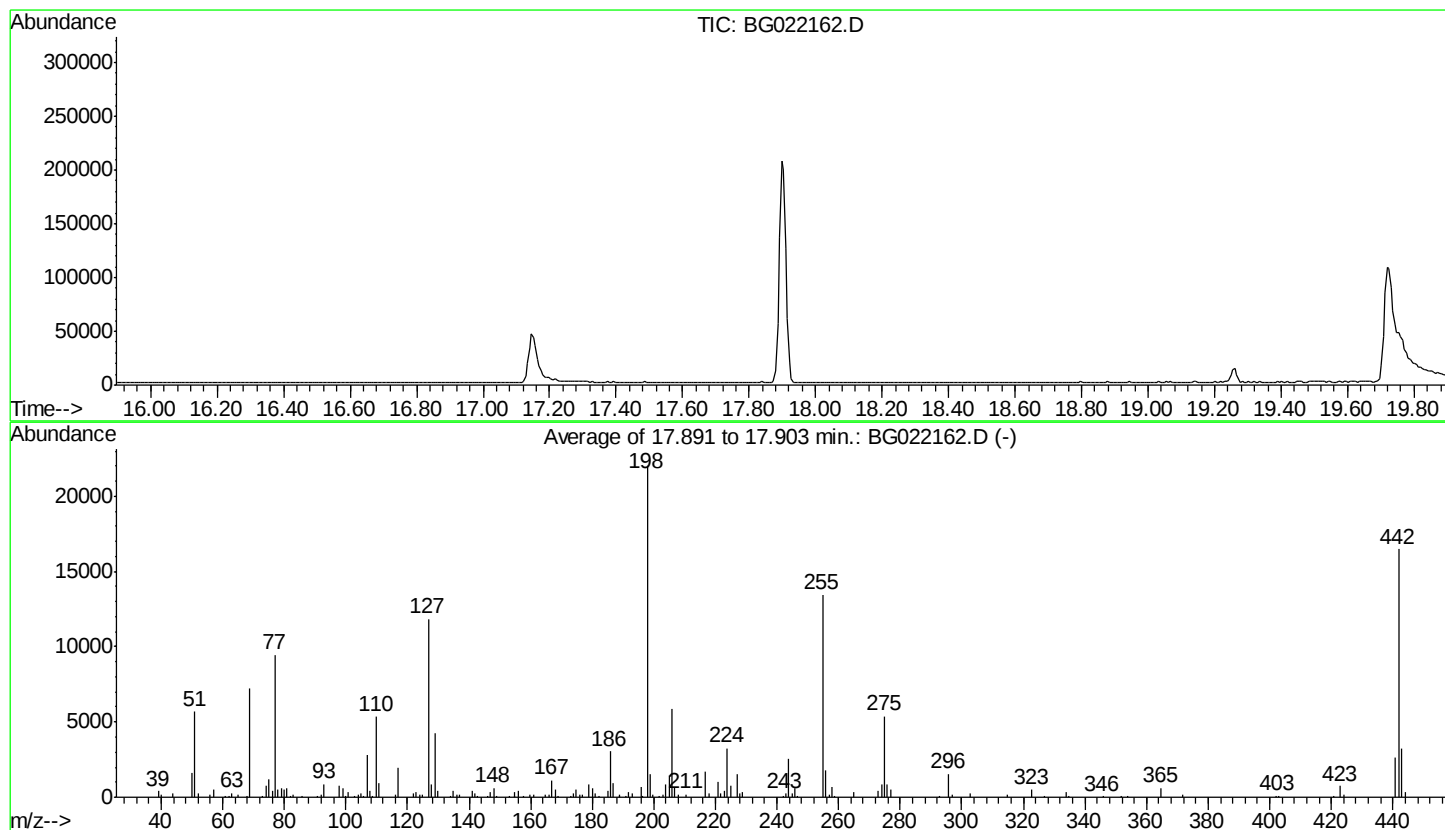

AutoFind: Scans 2562, 2563, 2564; Background Corrected with Scan 2556

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	25.8	5693	PASS
68	69	0.00	2	1.0	73	PASS
69	198	0.00	100	32.7	7202	PASS
70	69	0.00	2	0.0	0	PASS
127	198	10	80	53.8	11843	PASS
197	198	0.00	2	0.0	0	PASS
198	198	100	100	100.0	22032	PASS
199	198	5	9	6.9	1527	PASS
275	198	10	60	24.5	5402	PASS
365	198	1	100	2.9	629	PASS
441	442	0.01	24	15.8	2604	PASS
442	198	50	100	74.8	16472	PASS
443	442	15	24	19.8	3266	PASS