


Data Path : Z:\HPCHEM1\BNA_G\Data\BG060616\
 Data File : BG022190.D
 Acq On : 7 Jun 2016 5:14
 Operator : UM/SJ
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_G
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\HPCHEM1\BNA_G\METHODS\8270-BG060616.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Mon Jun 06 16:12:45 2016

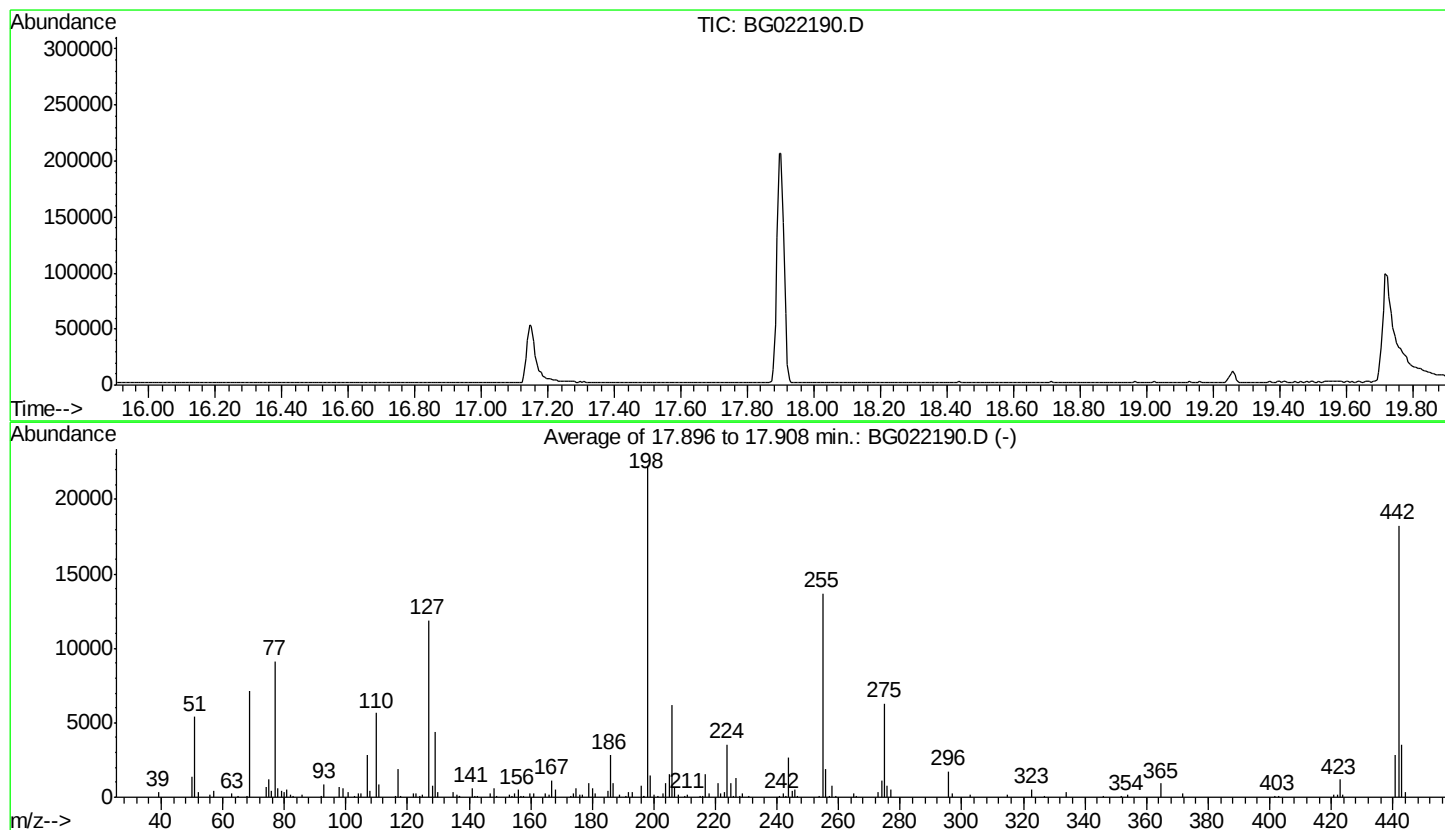

AutoFind: Scans 2563, 2564, 2565; Background Corrected with Scan 2556

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	24.2	5399	PASS
68	69	0.00	2	0.7	50	PASS
69	198	0.00	100	32.2	7172	PASS
70	69	0.00	2	0.0	0	PASS
127	198	10	80	53.3	11880	PASS
197	198	0.00	2	0.5	116	PASS
198	198	100	100	100.0	22269	PASS
199	198	5	9	6.7	1502	PASS
275	198	10	60	28.3	6307	PASS
365	198	1	100	4.2	931	PASS
441	442	0.01	24	15.6	2843	PASS
442	198	50	100	81.9	18232	PASS
443	442	15	24	19.4	3535	PASS