

Data Path : Z:\HPCHEM1\BNA G\DATA\BG060617\
 Data File : BG027260.D
 Acq On : 6 Jun 2017 22:08
 Operator : SJ/MA
 Sample : PB99501TB
 Misc :
 ALS Vial : 9 Sample Multiplier: 1

Instrument :
 BNA_G
 ClientSampleId :
 PB99501TB

Quant Time: Jun 07 05:18:21 2017
 Quant Method : Z:\HPCHEM1\BNA G\METHODS\8270-BG060517.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Mon Jun 05 16:00:35 2017
 Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Dichlorobenzene-d4	8.56	152	50763	20.00	ng	-0.01
21) Naphthalene-d8	11.38	136	229691	20.00	ng	-0.01
38) Acenaphthene-d10	15.14	164	152535	20.00	ng	-0.01
63) Phenanthrene-d10	17.89	188	374669	20.00	ng	-0.02
75) Chrysene-d12	22.28	240	417422	20.00	ng	-0.03
86) Perylene-d12	25.98	264	393424	20.00	ng	-0.04
System Monitoring Compounds						
5) 2-Fluorophenol	6.15	112	366304	110.11	ng	0.00
7) Phenol-d6	7.69	99	510468	104.54	ng	0.00
23) Nitrobenzene-d5	9.73	82	267907	73.35	ng	-0.01
41) 2,4,6-Tribromophenol	16.63	330	213548	106.32	ng	-0.01
44) 2-Fluorobiphenyl	13.77	172	711745	65.28	ng	-0.02
78) Terphenyl-d14	20.47	244	1133415	69.27	ng	-0.02


Target Compounds Qvalue


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\HPCHEM1\BNA G\DATA\BG060617\
Data File : BG027260.D
Acq On : 6 Jun 2017 22:08
Operator : SJ/MA
Sample : PB99501TB
Misc :
ALS Vial : 9 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
PB99501TB

Quant Time: Jun 07 05:18:21 2017
Quant Method : Z:\HPCHEM1\BNA G\METHODS\8270-BG060517.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Mon Jun 05 16:00:35 2017
Response via : Initial Calibration

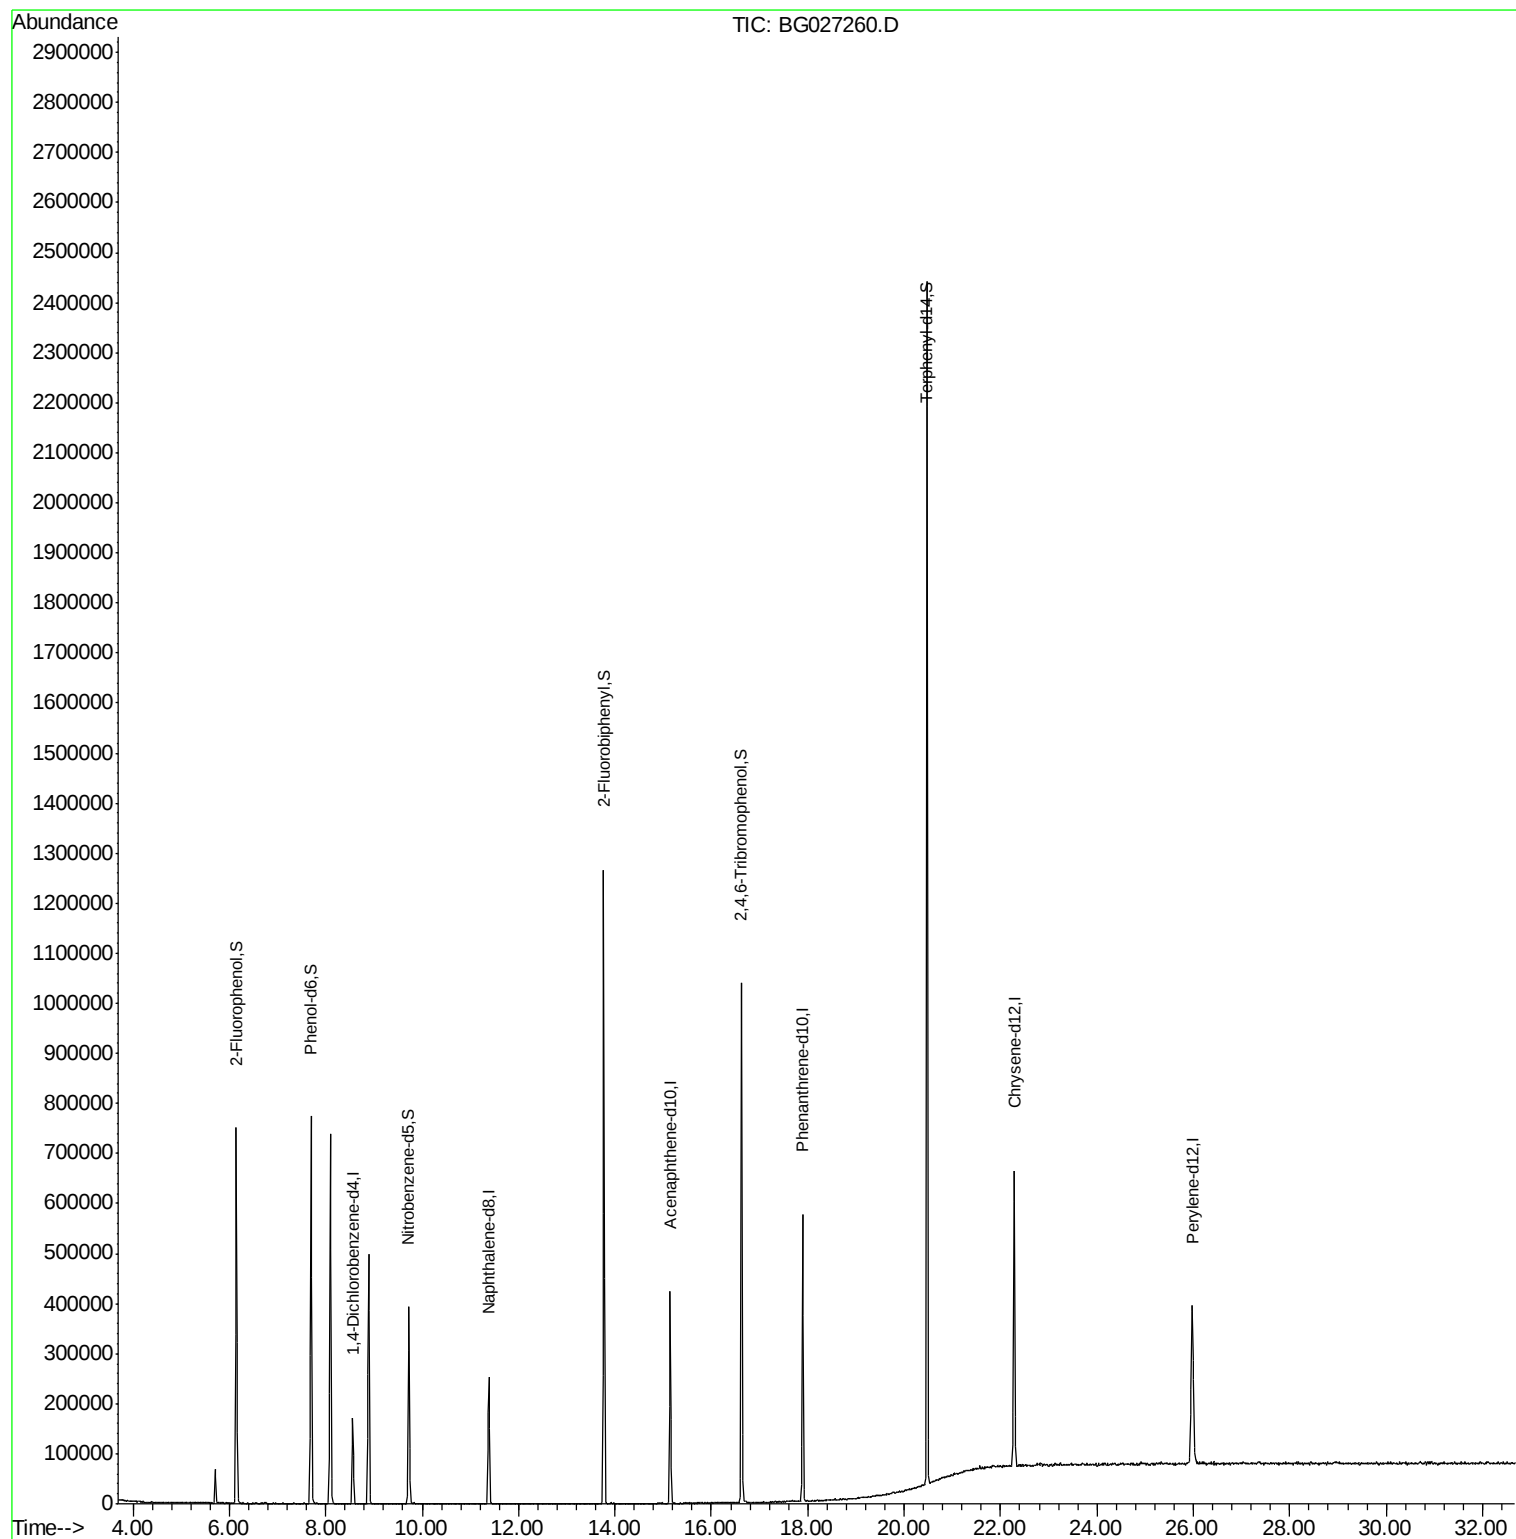

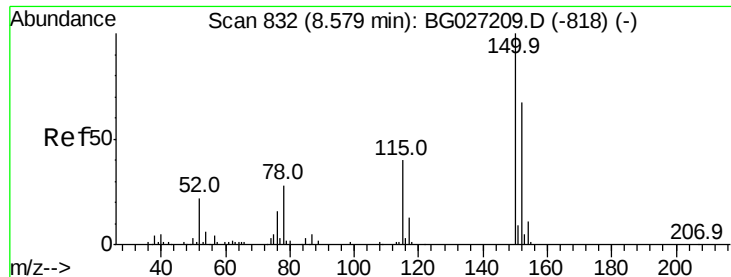


#1




1,4-Dichlorobenzene-d4
Concen: 20.00 ng
RT: 8.56 min Scan# 830
Delta R.T. -0.01 min
Lab File: BG027260.D
Acq: 6 Jun 2017 22:08

Instrument :
BNA_G
ClientSampleId :
PB99501TB

Tot Ion:152 Resp: 50763
Ion Ratio Lower Upper
152 100
150 157.3 114.0 171.0
115 64.1 48.1 72.1

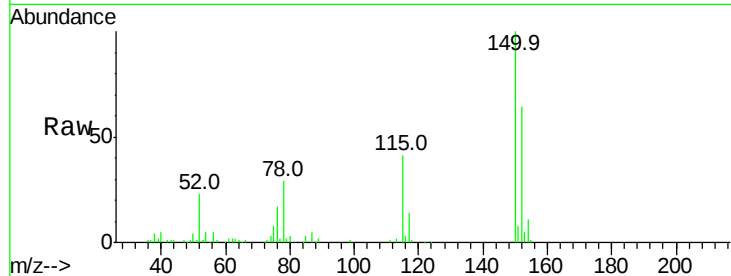


Abundance Ion 152.00 (151.70 to 152.70): E
Ion 150.00 (149.70 to 150.70): E
Ion 115.00 (114.70 to 115.70): E

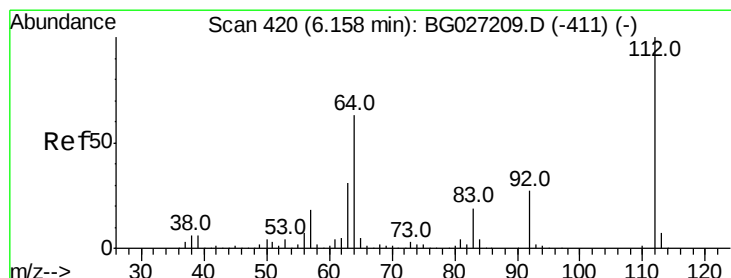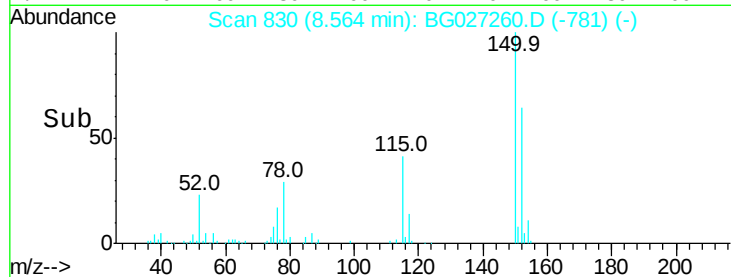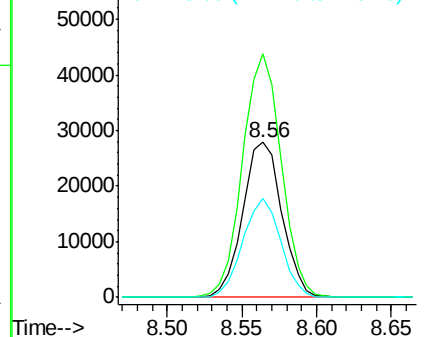



#5

2-Fluorophenol
Concen: 110.11 ng
RT: 6.15 min Scan# 419
Delta R.T. -0.01 min
Lab File: BG027260.D
Acq: 6 Jun 2017 22:08

Tgt Ion:112 Resp: 366304
Ion Ratio Lower Upper
112 100
64 64.6 61.8 92.6
63 32.6 37.2 55.8#

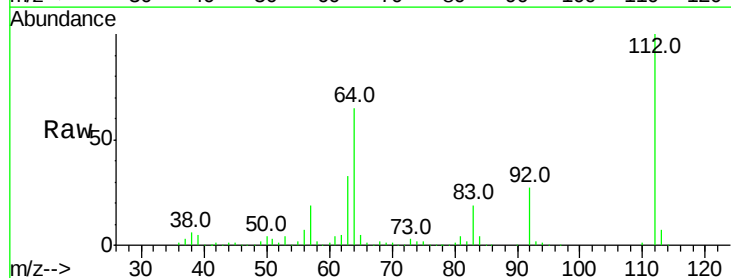

Abundance Ion 112.00 (111.70 to 112.70): E
Ion 64.00 (63.70 to 64.70): BGC
Ion 63.00 (62.70 to 63.70): BGC

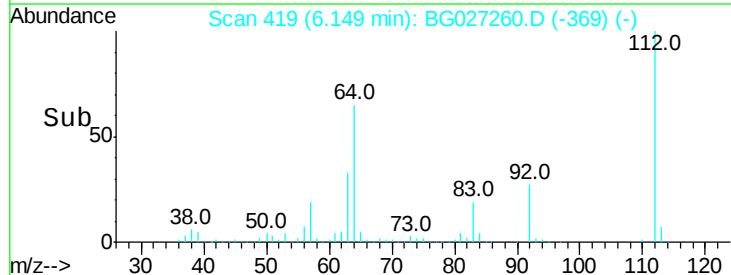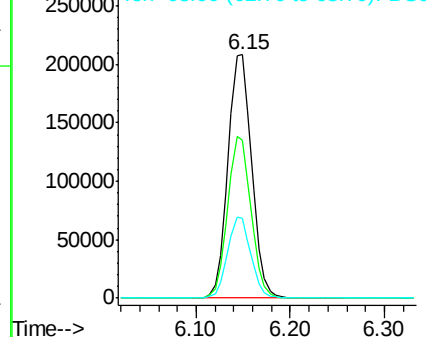



#7

Phenol-d6

Concen: 104.54 ng

RT: 7.69 min Scan# 682

Delta R.T. -0.01 min

Lab File: BG027260.D

Acq: 6 Jun 2017 22:08

Instrument :

BNA_G

ClientSampleId :

PB99501TB


Tot Ion: 99 Resp: 510468

Ion Ratio Lower Upper


99 100

42 16.9 20.5 30.7#



71 31.6 37.6 56.4#

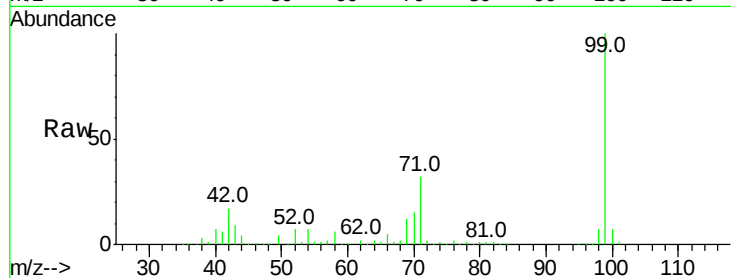

Abundance Ion 99.00 (98.70 to 99.70): BGC
Ion 42.00 (41.70 to 42.70): BGC
Ion 71.00 (70.70 to 71.70): BGC

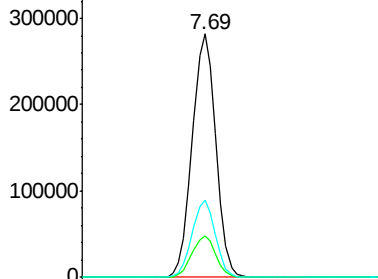

Time-->

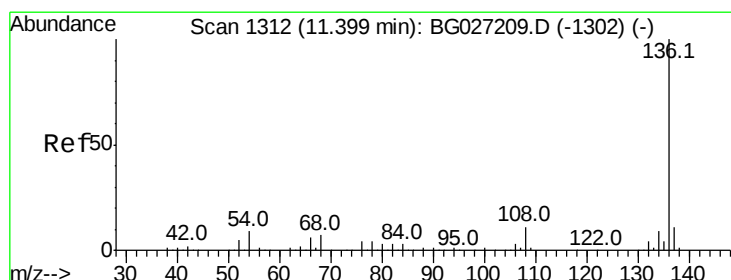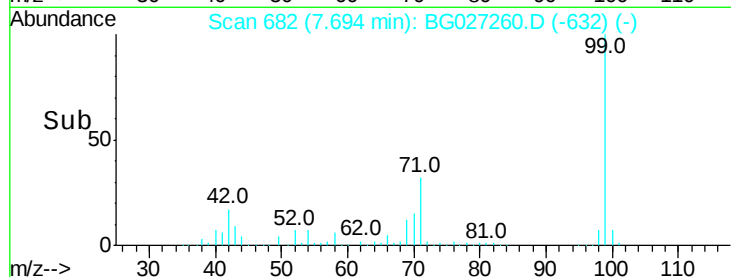

#21

Naphthalene-d8

Concen: 20.00 ng

RT: 11.38 min Scan# 1310

Delta R.T. -0.01 min

Lab File: BG027260.D

Acq: 6 Jun 2017 22:08

Tgt Ion: 136 Resp: 229691


Ion Ratio Lower Upper

136 100


137 11.0 8.9 13.3

54 10.1 9.3 13.9


68 7.4 5.1 7.7

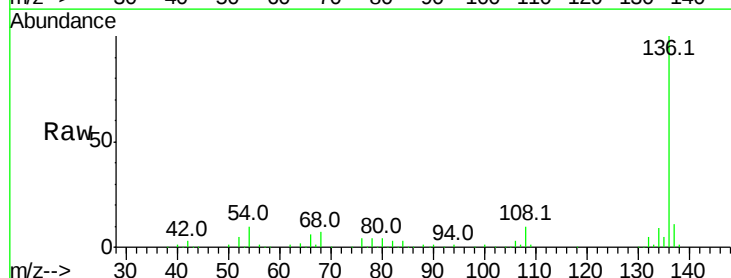


Abundance Ion 136.00 (135.70 to 136.70): BGC
Ion 137.00 (136.70 to 137.70): BGC
Ion 54.00 (53.70 to 54.70): BGC
Ion 68.00 (67.70 to 68.70): BGC

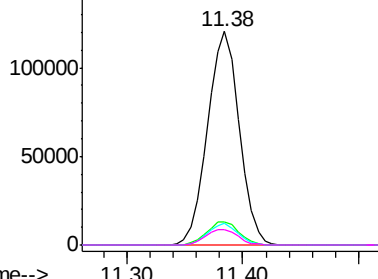

Time-->

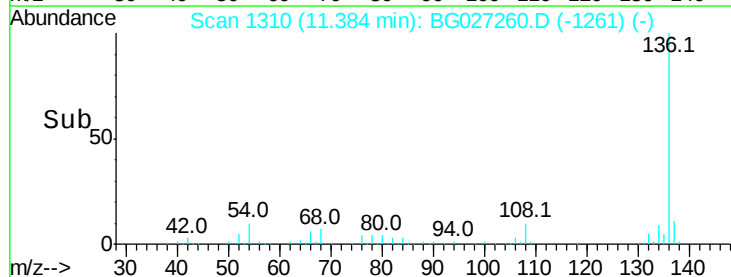


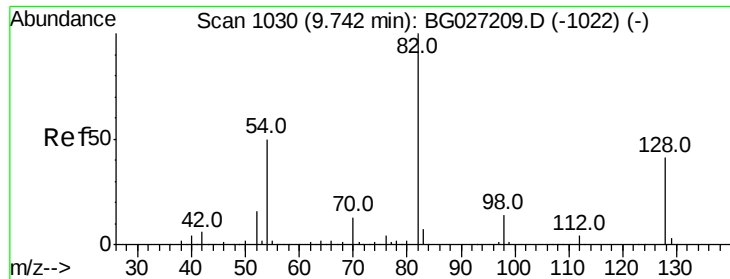




#23
Nitrobenzene-d5
Concen: 73.35 ng
RT: 9.73 min Scan# 1028
Delta R.T. -0.01 min
Lab File: BG027260.D
Acq: 6 Jun 2017 22:08

Instrument :
BNA_G
ClientSampleId :
PB99501TB

Tot Ion	82	Resp	267907
Ion Ratio	Lower	Upper	
82	100		
128	41.4	26.4	39.6#
54	49.8	49.4	74.2

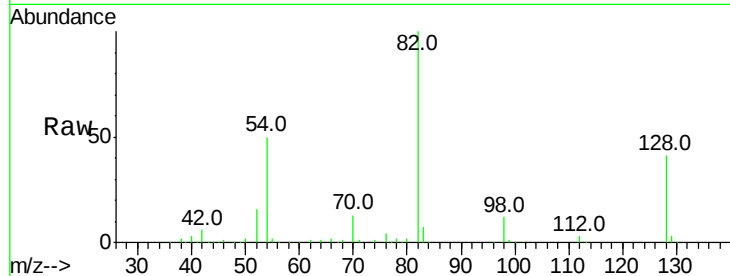


Abundance Ion 82.00 (81.70 to 82.70): BGC
Ion 128.00 (127.70 to 128.70): BGC
Ion 54.00 (53.70 to 54.70): BGC

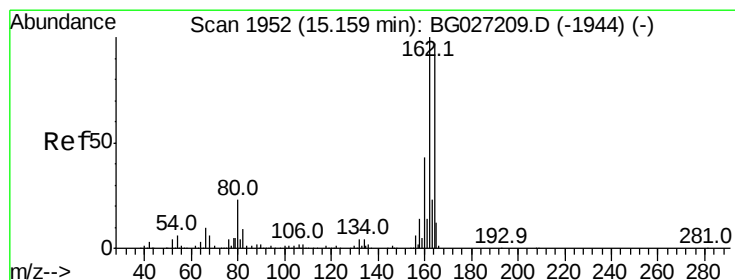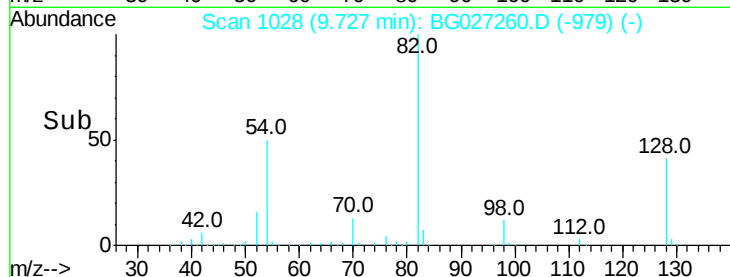
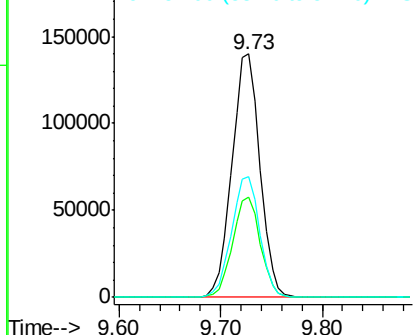


#38
Acenaphthene-d10
Concen: 20.00 ng
RT: 15.14 min Scan# 1950
Delta R.T. -0.01 min
Lab File: BG027260.D
Acq: 6 Jun 2017 22:08

Tgt Ion	164	Resp	152535
Ion Ratio	Lower	Upper	
164	100		
162	102.6	85.1	127.7
160	44.5	34.7	52.1

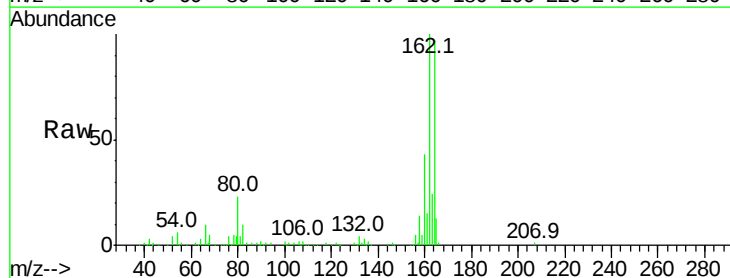

Abundance Ion 164.00 (163.70 to 164.70): BGC
Ion 162.00 (161.70 to 162.70): BGC
Ion 160.00 (159.70 to 160.70): BGC

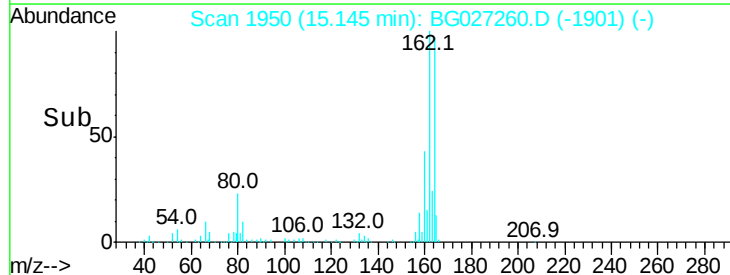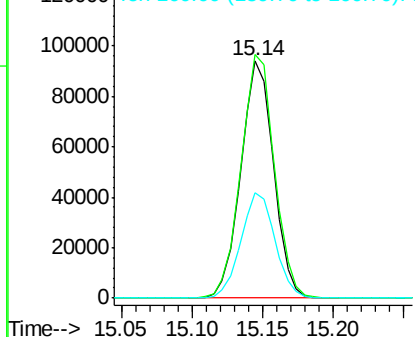







#41
 2,4,6-Tribromophenol
 Concen: 106.32 ng
 RT: 16.63 min Scan# 2203
 Delta R.T. -0.01 min
 Lab File: BG027260.D
 Acq: 6 Jun 2017 22:08

Instrument :
 BNA_G
 ClientSampleId :
 PB99501TB

Tot Ion	Ratio	Lower	Upper
330	100		
332	95.6	77.3	115.9
141	32.5	32.1	48.1

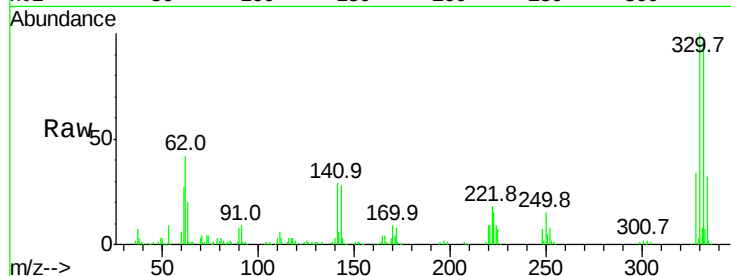


Abundance Ion 329.80 (329.50 to 330.50): E
 Ion 331.80 (331.50 to 332.50): E
 Ion 141.00 (140.70 to 141.70): E

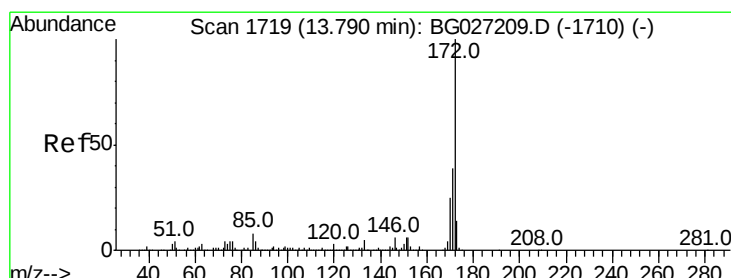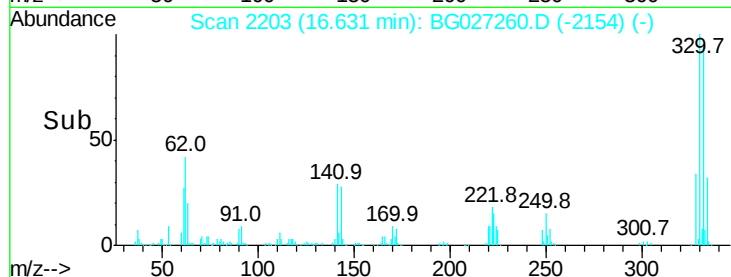
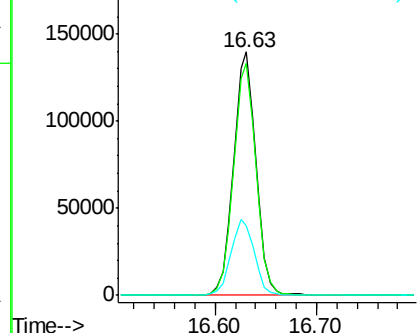



#44
 2-Fluorobiphenyl
 Concen: 65.28 ng
 RT: 13.77 min Scan# 1716
 Delta R.T. -0.02 min
 Lab File: BG027260.D
 Acq: 6 Jun 2017 22:08

Tgt Ion	Ratio	Lower	Upper
172	100		
171	36.9	32.2	48.2
170	24.2	21.8	32.6

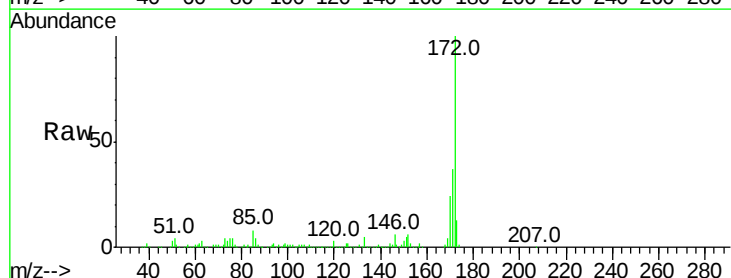

Abundance Ion 172.00 (171.70 to 172.70): E
 Ion 171.00 (170.70 to 171.70): E
 Ion 170.00 (169.70 to 170.70): E

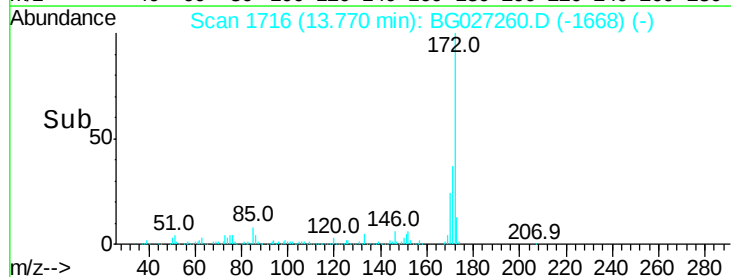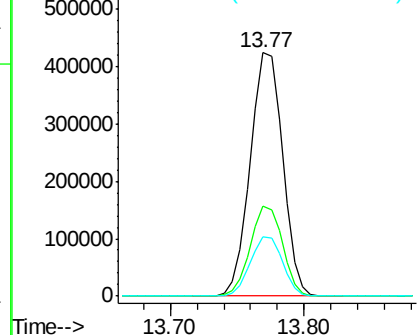


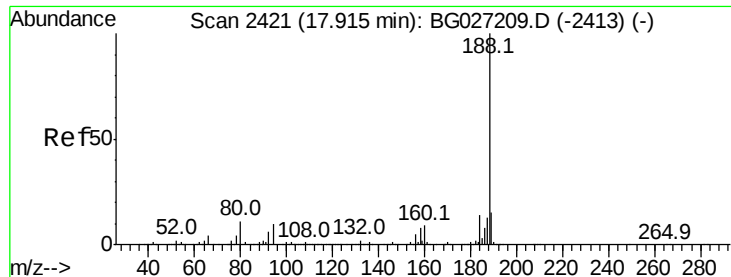




#63
Phenanthrene-d10
Concen: 20.00 ng
RT: 17.89 min Scan# 2418
Delta R.T. -0.02 min
Lab File: BG027260.D
Acq: 6 Jun 2017 22:08

Instrument :
BNA_G
ClientSampleId :
PB99501TB

Tot Ion:188 Resp: 374669
Ion Ratio Lower Upper
188 100
94 10.2 5.8 8.8#
80 12.0 7.5 11.3#

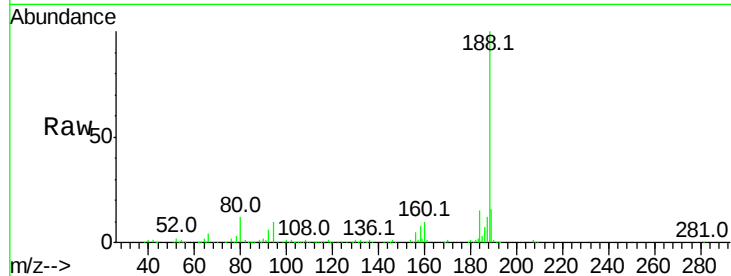


Abundance Ion 188.00 (187.70 to 188.70): E
Ion 94.00 (93.70 to 94.70): BGC
Ion 80.00 (79.70 to 80.70): BGC

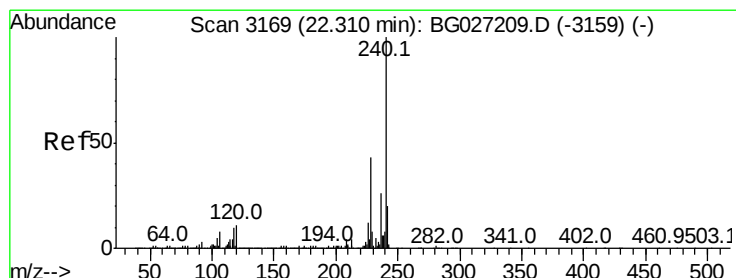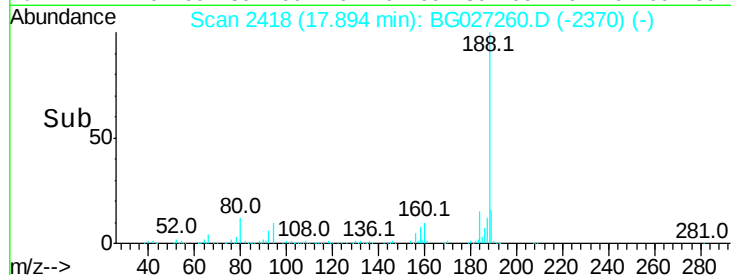
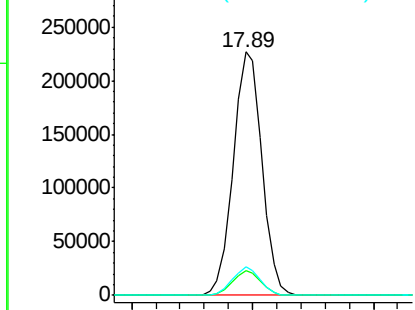



#75
Chrysene-d12
Concen: 20.00 ng
RT: 22.28 min Scan# 3165
Delta R.T. -0.03 min
Lab File: BG027260.D
Acq: 6 Jun 2017 22:08

Tgt Ion:240 Resp: 417422
Ion Ratio Lower Upper
240 100
120 10.3 5.7 8.5#
236 26.8 22.2 33.4

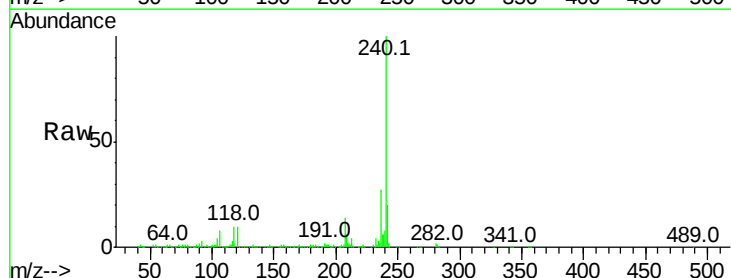

Abundance Ion 240.00 (239.70 to 240.70): E
Ion 120.00 (119.70 to 120.70): E
Ion 236.00 (235.70 to 236.70): E

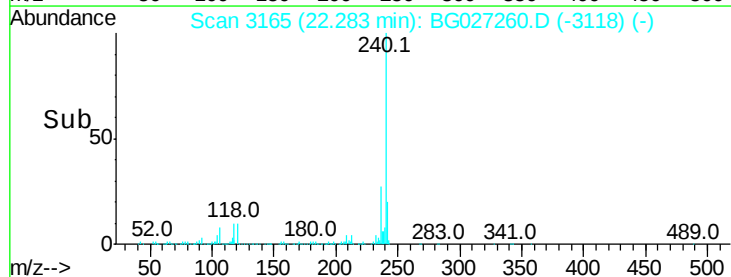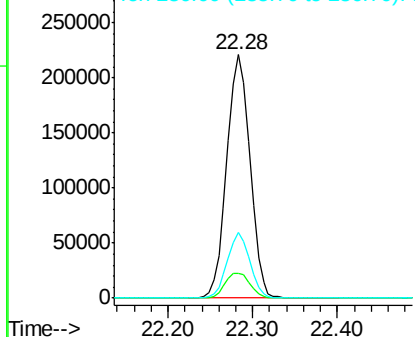

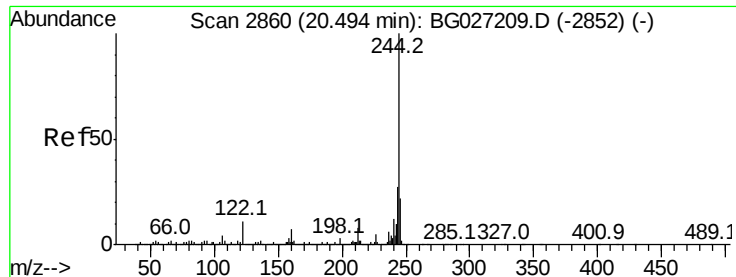

#78

Terphenyl-d14

Concen: 69.27 ng

RT: 20.47 min Scan# 2857

Delta R.T. -0.02 min

Lab File: BG027260.D

Acq: 6 Jun 2017 22:08

Instrument :


BNA_G

ClientSampleId :

PB99501TB

Tot Ion:244 Resp: 1133415




Ion	Ratio	Lower	Upper
244	100		
212	7.6	10.0	15.0#
122	10.8	8.6	12.8

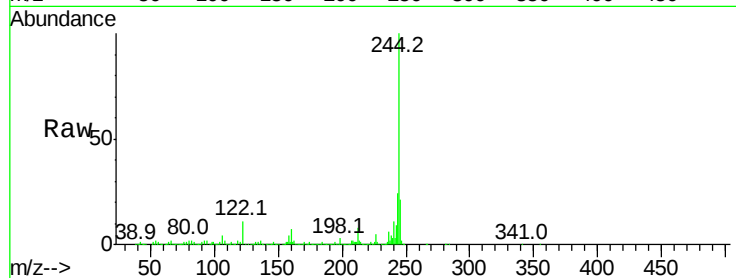

Abundance Ion 244.00 (243.70 to 244.70): E

Ion 212.00 (211.70 to 212.70): E

Ion 122.00 (121.70 to 122.70): E

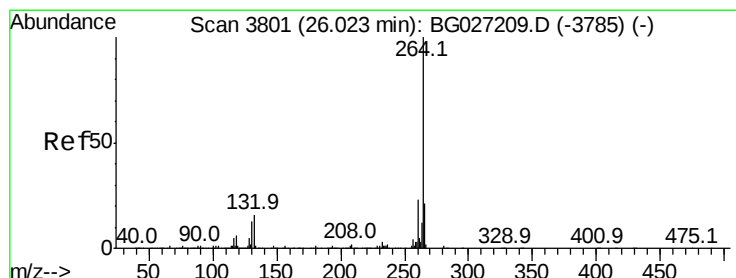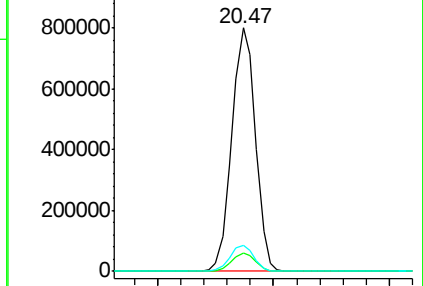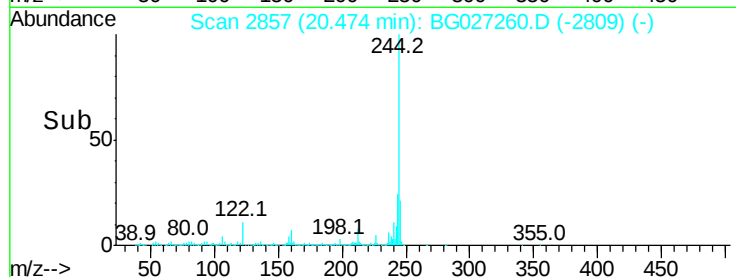

#86

Perylene-d12

Concen: 20.00 ng

RT: 25.98 min Scan# 3794


Delta R.T. -0.04 min

Lab File: BG027260.D

Acq: 6 Jun 2017 22:08

Tgt Ion:264 Resp: 393424

Ion	Ratio	Lower	Upper
264	100		
260	23.6	21.8	32.8
265	21.4	18.2	27.4

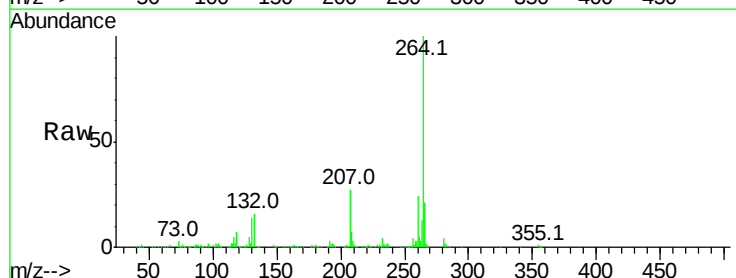

Abundance Ion 264.00 (263.70 to 264.70): E

Ion 260.00 (259.70 to 260.70): E

Ion 265.00 (264.70 to 265.70): E

