

Data Path : Z:\HPCHEM1\BNA G\DATA\BG060617\
 Data File : BG027263.D
 Acq On : 7 Jun 2017 00:05
 Operator : SJ/MA
 Sample : I3438-15
 Misc :
 ALS Vial : 12 Sample Multiplier: 1

Instrument :
 BNA_G
 ClientSampleId :

Quant Time: Jun 07 05:18:50 2017
 Quant Method : Z:\HPCHEM1\BNA G\METHODS\8270-BG060517.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Mon Jun 05 16:00:35 2017
 Response via : Initial Calibration


Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Dichlorobenzene-d4	8.56	152	47881	20.00	ng	-0.01
21) Naphthalene-d8	11.39	136	215650	20.00	ng	-0.01
38) Acenaphthene-d10	15.15	164	137926	20.00	ng	-0.01
63) Phenanthrene-d10	17.90	188	348999	20.00	ng	-0.02
75) Chrysene-d12	22.28	240	394150	20.00	ng	-0.03
86) Perylene-d12	25.97	264	362527	20.00	ng	-0.05
System Monitoring Compounds						
5) 2-Fluorophenol	6.14	112	470327	149.89	ng	-0.01
7) Phenol-d6	7.70	99	613336	133.16	ng	0.00
23) Nitrobenzene-d5	9.72	82	379490	110.67	ng	-0.02
41) 2,4,6-Tribromophenol	16.63	330	312549	172.09	ng	-0.02
44) 2-Fluorobiphenyl	13.77	172	957007	97.07	ng	-0.02
78) Terphenyl-d14	20.47	244	1608349	104.09	ng	-0.02
Target Compounds						
55) 4-Nitrophenol	15.54	139	252	6.24	ng	Qvalue # 1


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\HPCHEM1\BNA G\DATA\BG060617\
Data File : BG027263.D
Acq On : 7 Jun 2017 00:05
Operator : SJ/MA
Sample : I3438-15
Misc :
ALS Vial : 12 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :

Quant Time: Jun 07 05:18:50 2017
Quant Method : Z:\HPCHEM1\BNA G\METHODS\8270-BG060517.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Mon Jun 05 16:00:35 2017
Response via : Initial Calibration

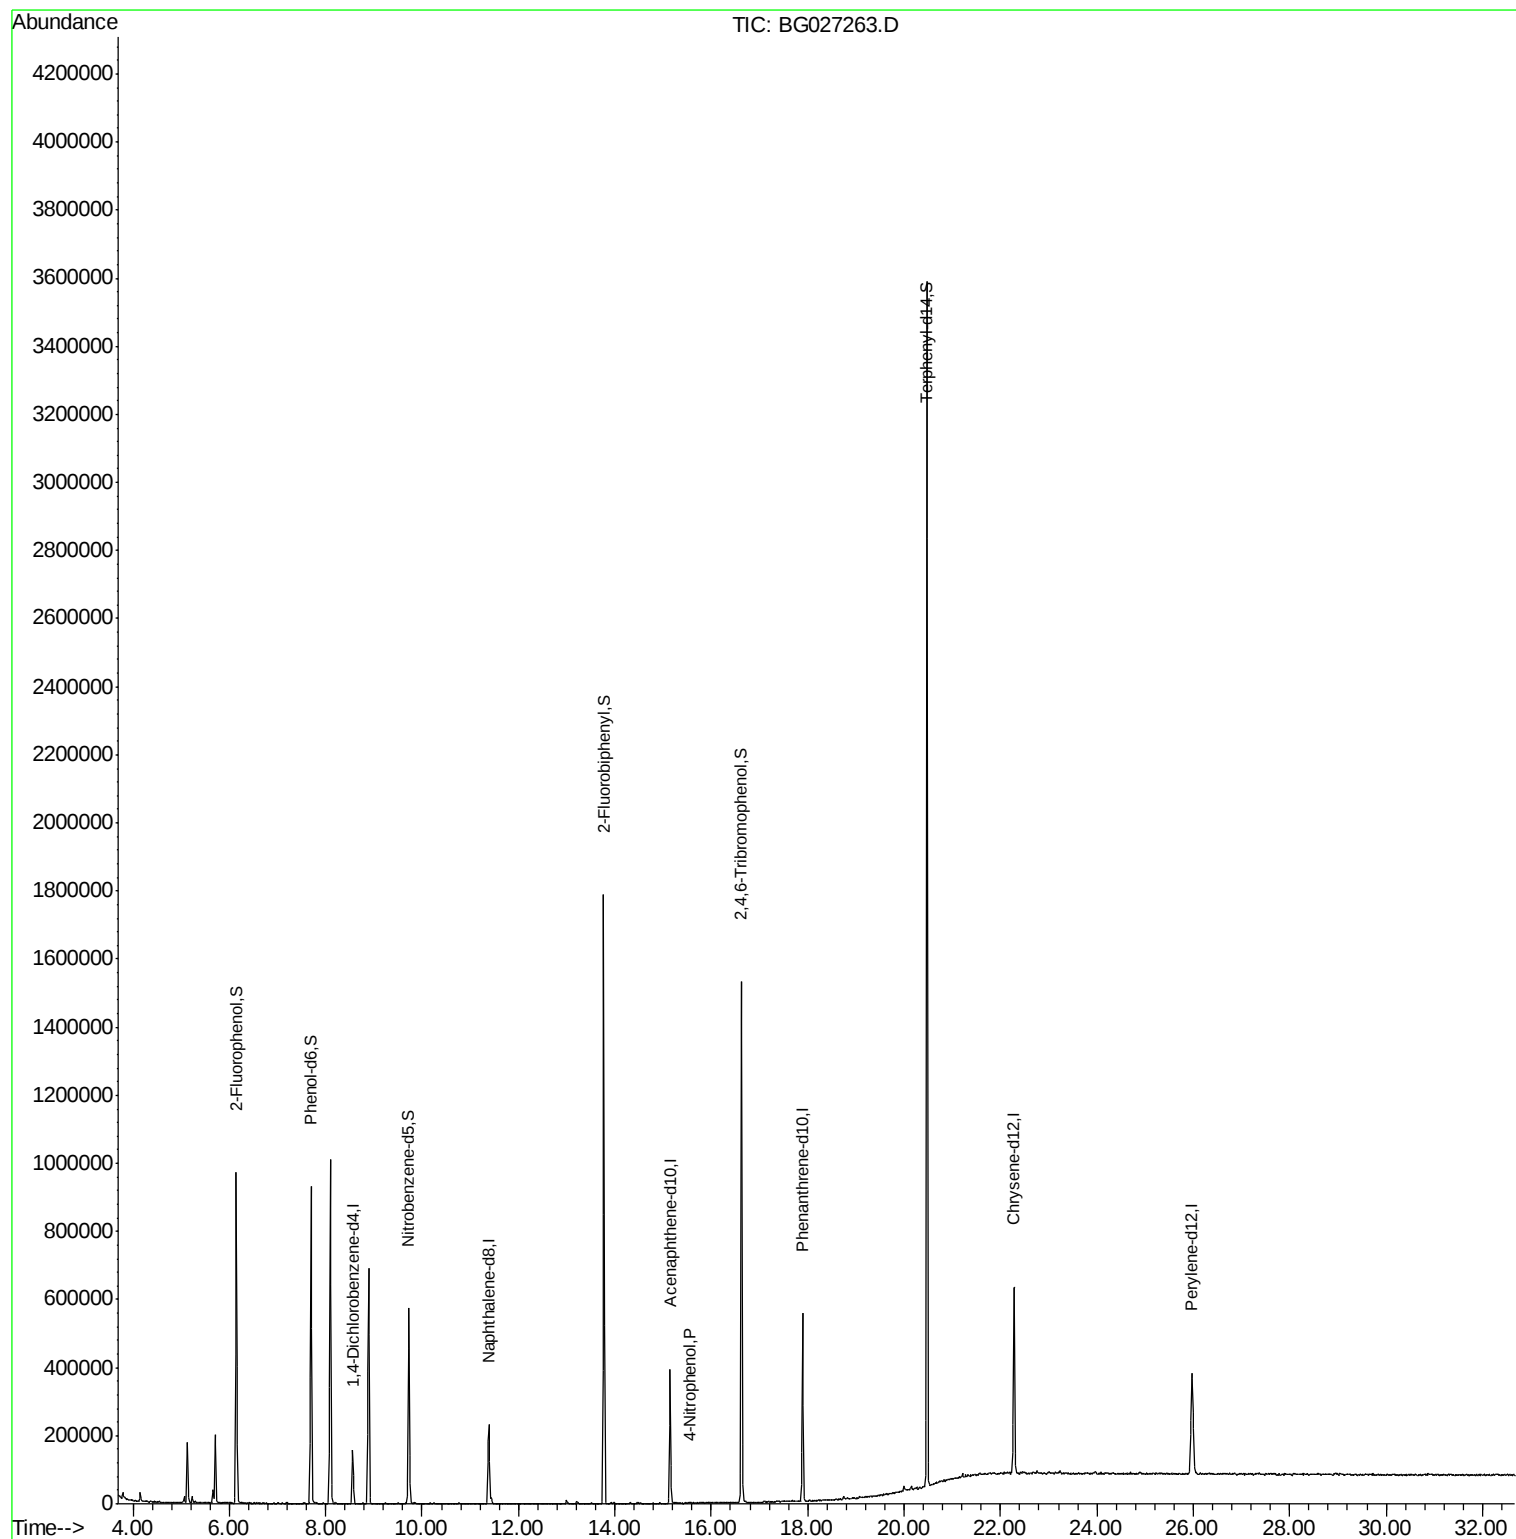

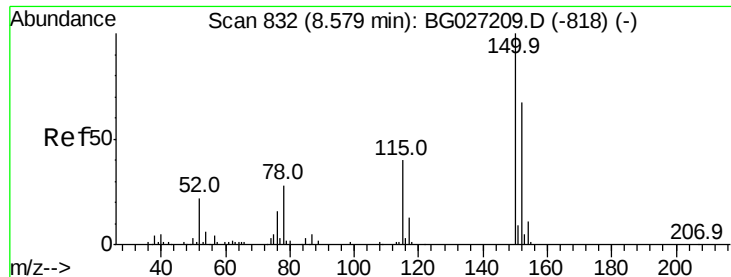

#1

1,4-Dichlorobenzene-d4

Concen: 20.00 ng

RT: 8.56 min Scan# 830

Delta R.T. -0.01 min

Lab File: BG027263.D

Acq: 7 Jun 2017 00:05

Instrument :

BNA_G

ClientSampleId :


Tot Ion:152 Resp: 47881

Ion Ratio Lower Upper

152 100

150 154.3 114.0 171.0




115 67.5 48.1 72.1

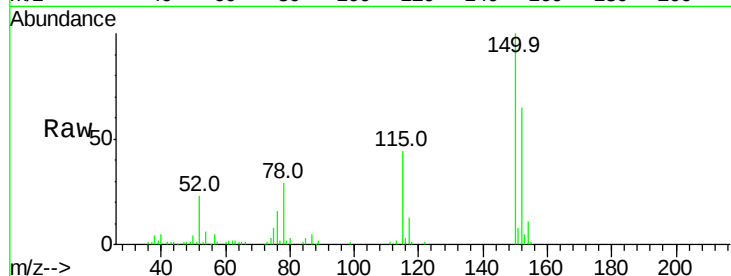

Abundance Ion 152.00 (151.70 to 152.70): E

Ion 150.00 (149.70 to 150.70): E

Ion 115.00 (114.70 to 115.70): E

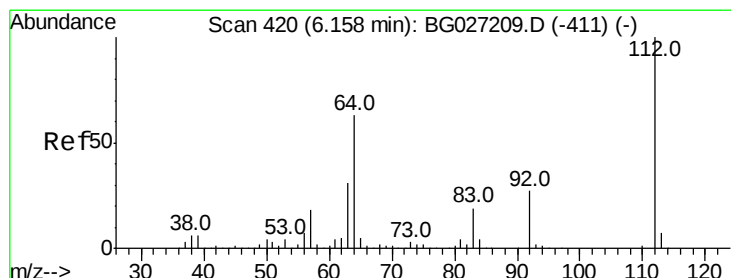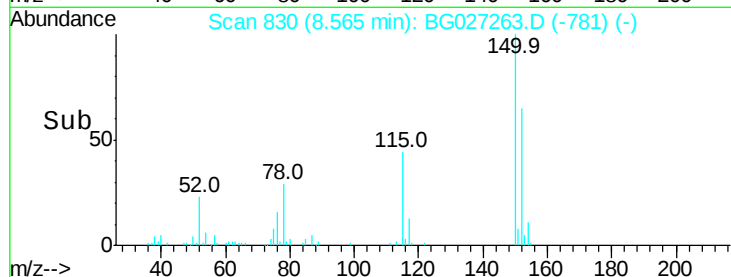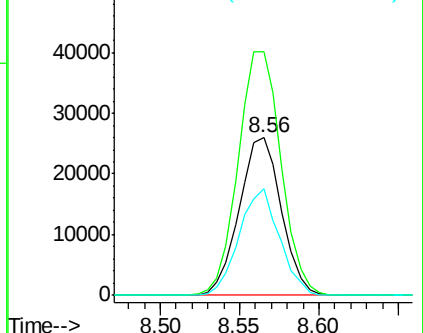

#5

2-Fluorophenol

Concen: 149.89 ng

RT: 6.14 min Scan# 418

Delta R.T. -0.01 min

Lab File: BG027263.D

Acq: 7 Jun 2017 00:05


Tgt Ion:112 Resp: 470327

Ion Ratio Lower Upper

112 100

64 64.8 61.8 92.6



63 32.9 37.2 55.8#

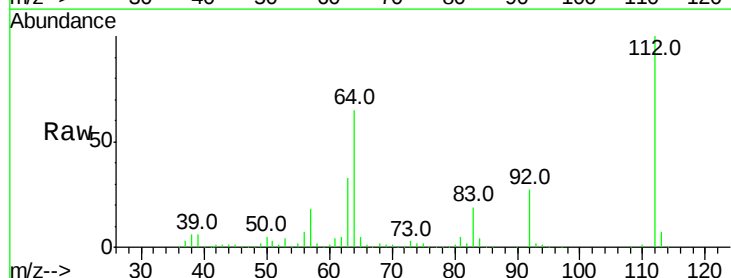


Abundance Ion 112.00 (111.70 to 112.70): E

Ion 64.00 (63.70 to 64.70): BGC

Ion 63.00 (62.70 to 63.70): BGC

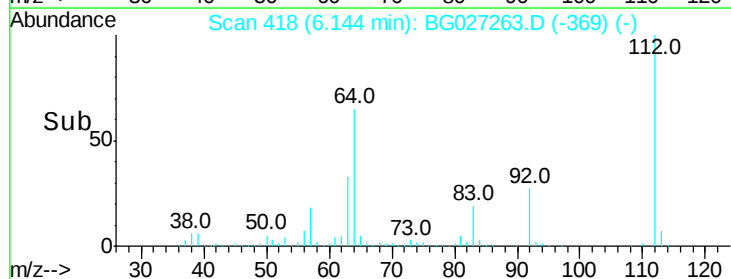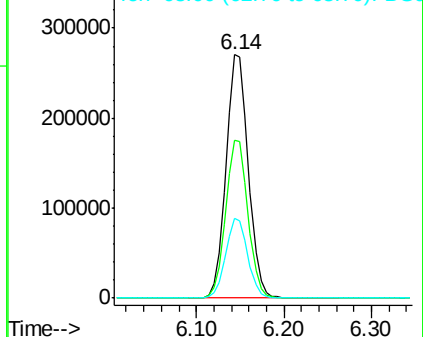

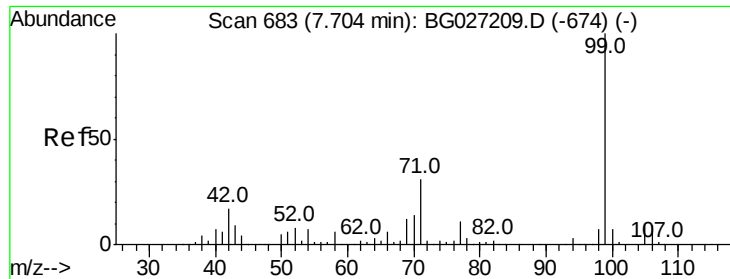

#7

Phenol-d6

Concen: 133.16 ng

RT: 7.70 min Scan# 682

Delta R.T. -0.01 min

Lab File: BG027263.D

Acq: 7 Jun 2017 00:05

Instrument :

BNA_G

ClientSampleId :


Tot Ion: 99 Resp: 613336

Ion Ratio Lower Upper




99 100

42 16.6 20.5 30.7#

71 32.4 37.6 56.4#

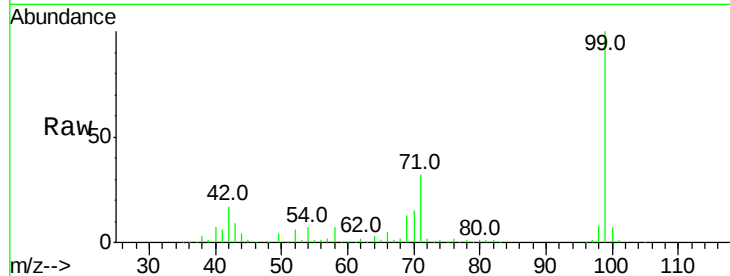

Abundance Ion 99.00 (98.70 to 99.70): BGC
Ion 42.00 (41.70 to 42.70): BGC
Ion 71.00 (70.70 to 71.70): BGC

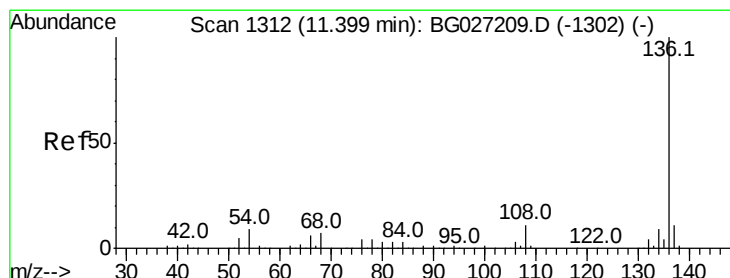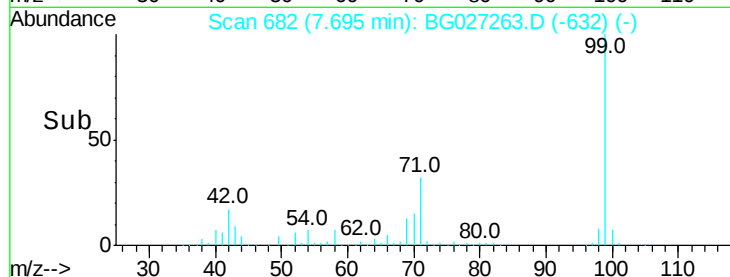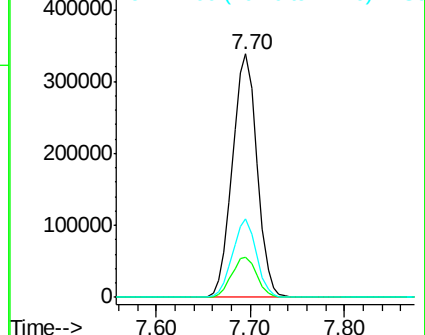

#21

Naphthalene-d8

Concen: 20.00 ng

RT: 11.39 min Scan# 1310

Delta R.T. -0.01 min

Lab File: BG027263.D

Acq: 7 Jun 2017 00:05

Tgt Ion: 136 Resp: 215650


Ion Ratio Lower Upper

136 100



137 10.2 8.9 13.3


54 9.3 9.3 13.9#

68 7.8 5.1 7.7#

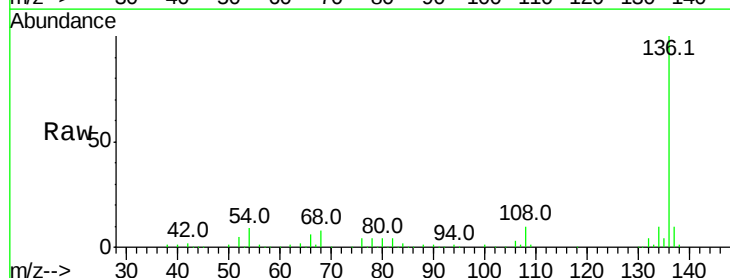

Abundance Ion 136.00 (135.70 to 136.70): BGC
Ion 137.00 (136.70 to 137.70): BGC
Ion 54.00 (53.70 to 54.70): BGC
Ion 68.00 (67.70 to 68.70): BGC



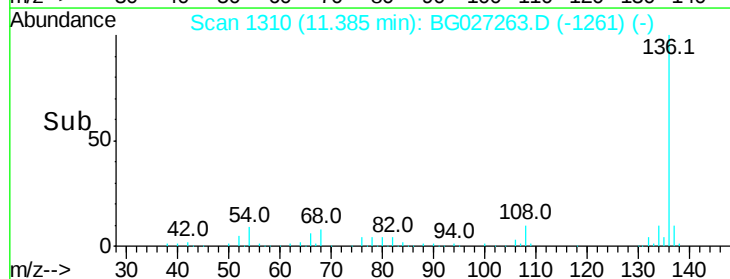
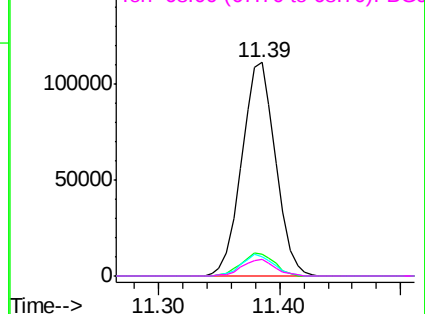


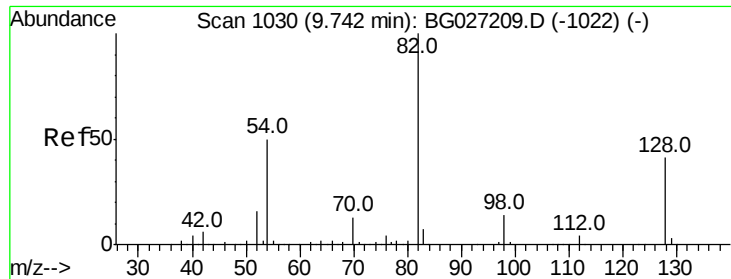

#23
 Nitrobenzene-d5
 Concen: 110.67 ng
 RT: 9.72 min Scan# 1027
 Delta R.T. -0.02 min
 Lab File: BG027263.D
 Acq: 7 Jun 2017 00:05




Instrument :
 BNA_G
 ClientSampleId :

Tot Ion	82	Resp	379490
Ion	Ratio	Lower	Upper
82	100		
128	40.2	26.4	39.6#
54	50.7	49.4	74.2

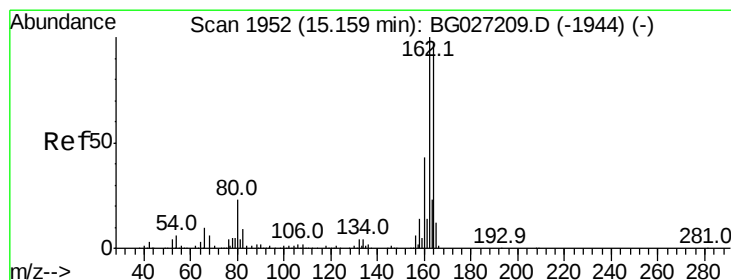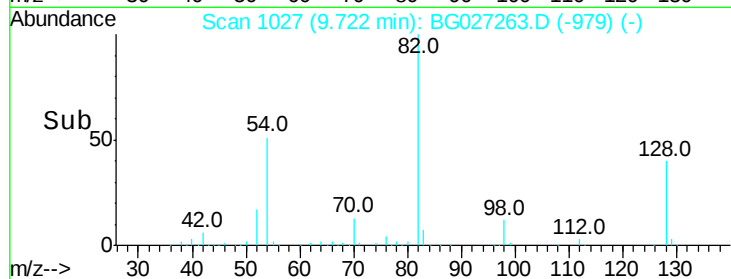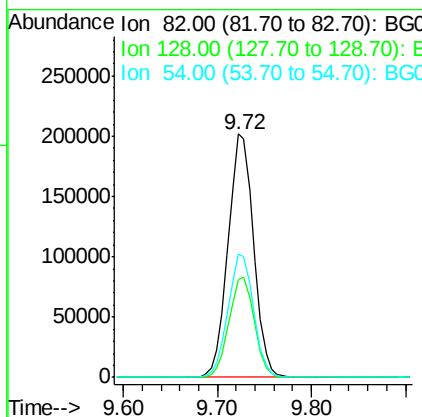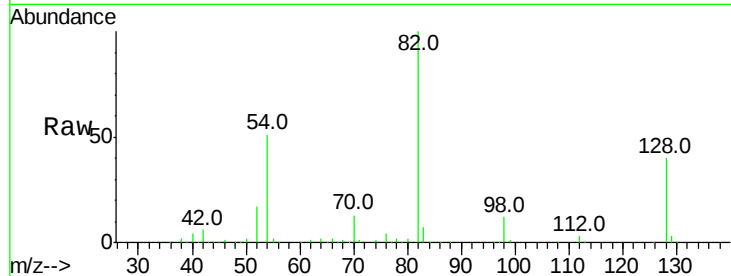

#38
 Acenaphthene-d10
 Concen: 20.00 ng
 RT: 15.15 min Scan# 1950
 Delta R.T. -0.01 min
 Lab File: BG027263.D
 Acq: 7 Jun 2017 00:05

Tgt Ion	164	Resp	137926
Ion	Ratio	Lower	Upper
164	100		
162	103.2	85.1	127.7
160	45.0	34.7	52.1

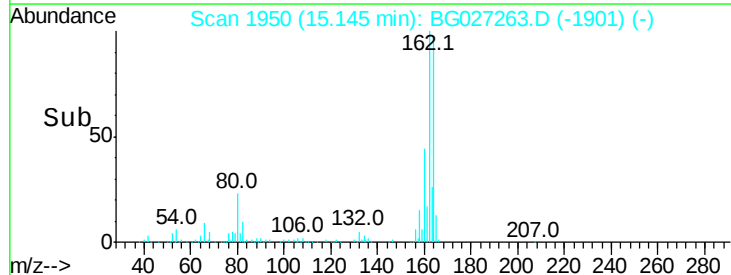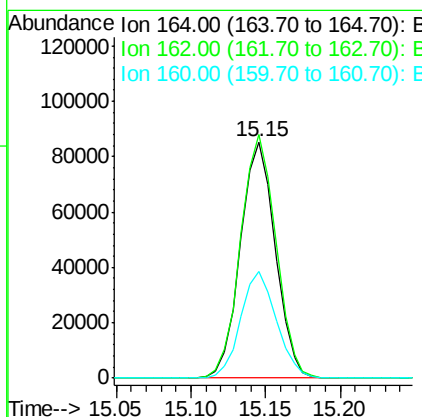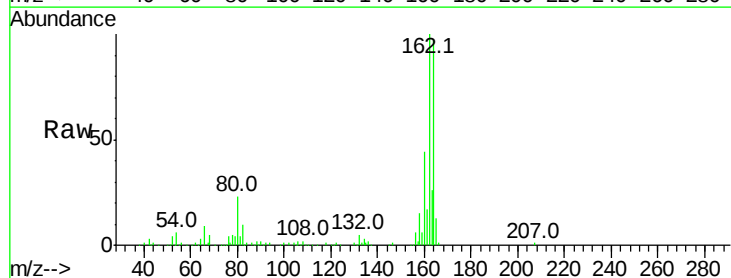







#41
 2,4,6-Tribromophenol
 Concen: 172.09 ng
 RT: 16.63 min Scan# 2202
 Delta R.T. -0.02 min
 Lab File: BG027263.D
 Acq: 7 Jun 2017 00:05

Instrument :
 BNA_G
 ClientSampled :

Tot Ion:330 Resp: 312549
 Ion Ratio Lower Upper
 330 100
 332 96.6 77.3 115.9
 141 32.5 32.1 48.1

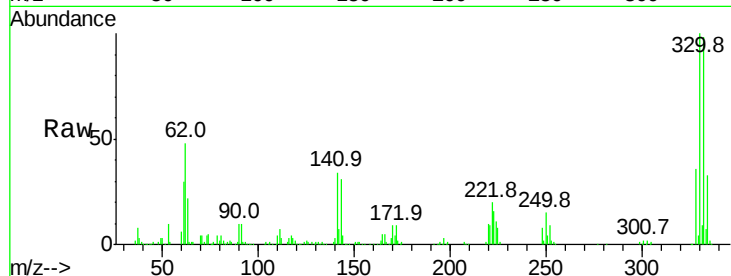


Abundance Ion 329.80 (329.50 to 330.50): E
 Ion 331.80 (331.50 to 332.50): E
 Ion 141.00 (140.70 to 141.70): E

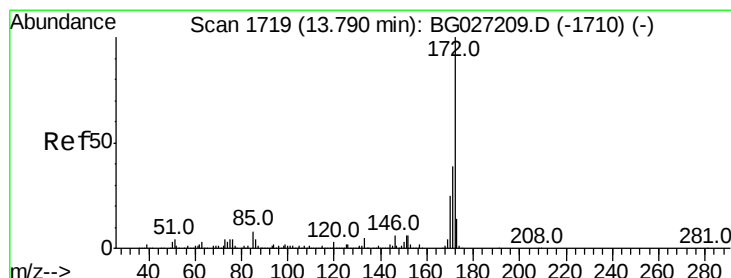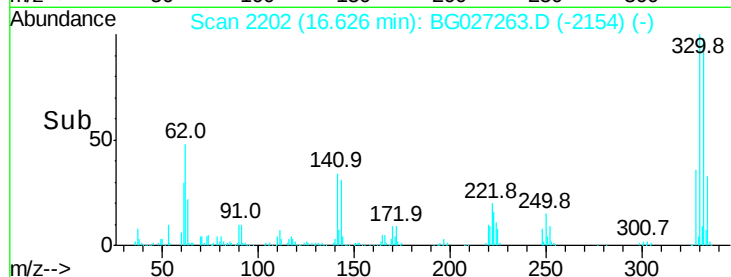
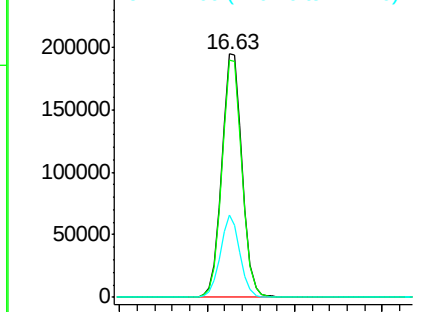



#44
 2-Fluorobiphenyl
 Concen: 97.07 ng
 RT: 13.77 min Scan# 1716
 Delta R.T. -0.02 min
 Lab File: BG027263.D
 Acq: 7 Jun 2017 00:05

Tgt Ion:172 Resp: 957007
 Ion Ratio Lower Upper
 172 100
 171 36.6 32.2 48.2
 170 24.8 21.8 32.6

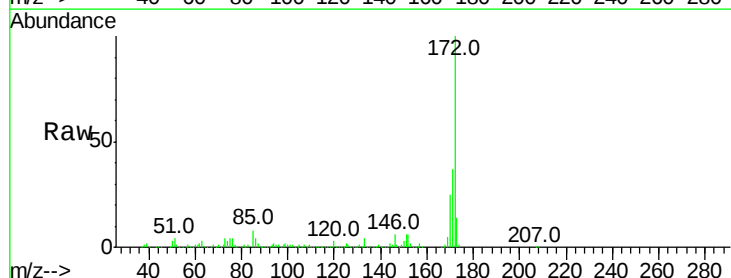

Abundance Ion 172.00 (171.70 to 172.70): E
 Ion 171.00 (170.70 to 171.70): E
 Ion 170.00 (169.70 to 170.70): E

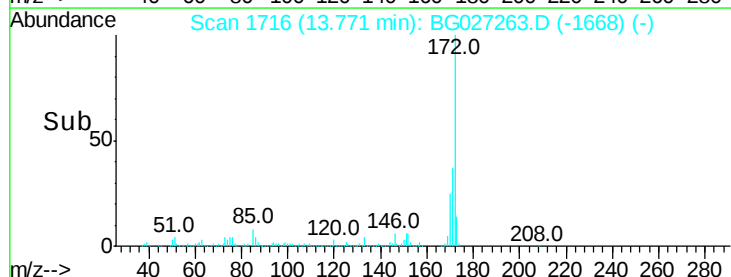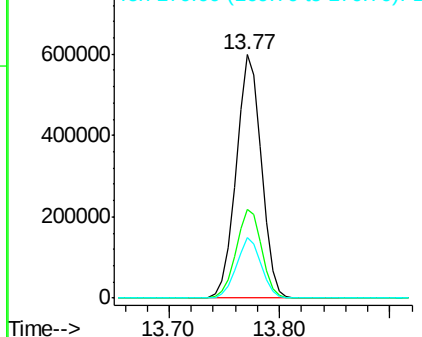

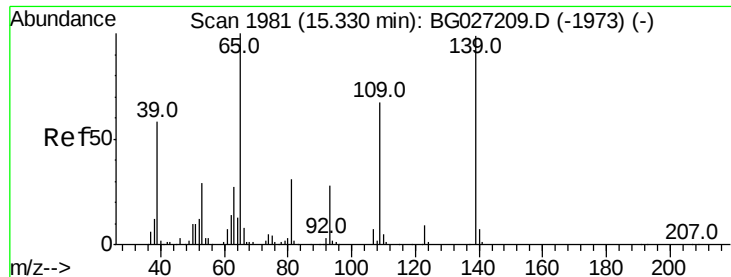

#55

4-Nitrophenol

Concen: 6.24 ng

RT: 15.54 min Scan# 2017

Delta R.T. 0.21 min

Lab File: BG027263.D

Acq: 7 Jun 2017 00:05

Instrument :

BNA_G

ClientSampleId :


Tot Ion:139 Resp: 252

Ion Ratio Lower Upper

139 100

109 0.0 101.2 141.2#




65 0.0 135.3 175.3#

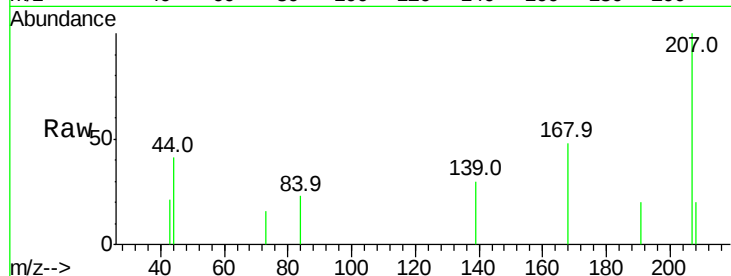

Abundance Ion 139.00 (138.70 to 139.70): E

Ion 109.00 (108.70 to 109.70): E

Ion 65.00 (64.70 to 65.70): BGC

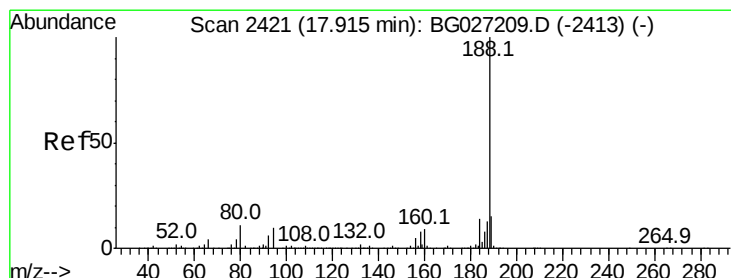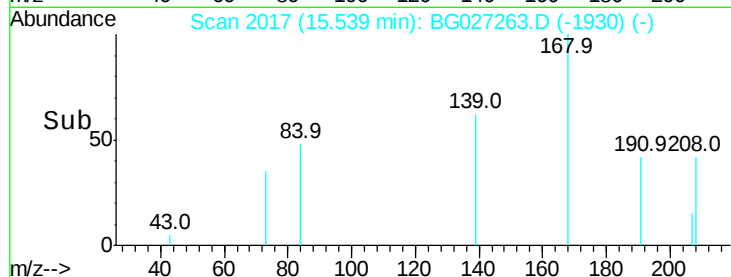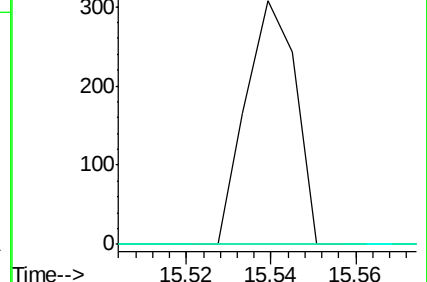

#63

Phenanthrene-d10

Concen: 20.00 ng

RT: 17.90 min Scan# 2418

Delta R.T. -0.02 min

Lab File: BG027263.D

Acq: 7 Jun 2017 00:05


Tgt Ion:188 Resp: 348999

Ion Ratio Lower Upper

188 100

94 10.0 5.8 8.8#



80 11.4 7.5 11.3#

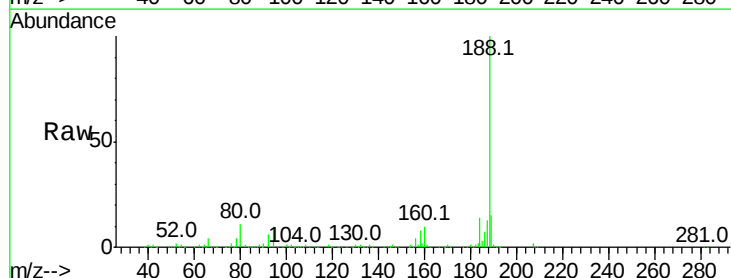


Abundance Ion 188.00 (187.70 to 188.70): E

Ion 94.00 (93.70 to 94.70): BGC

Ion 80.00 (79.70 to 80.70): BGC

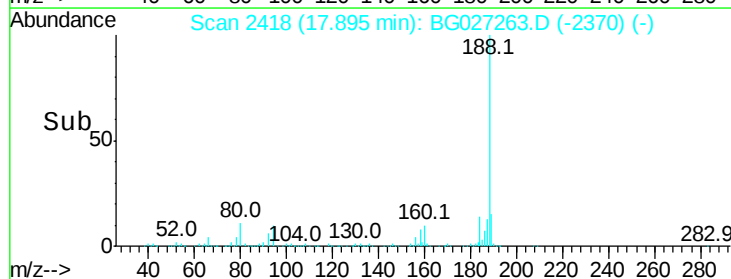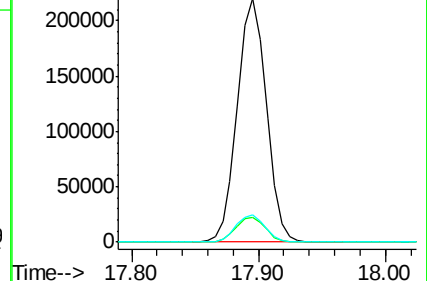

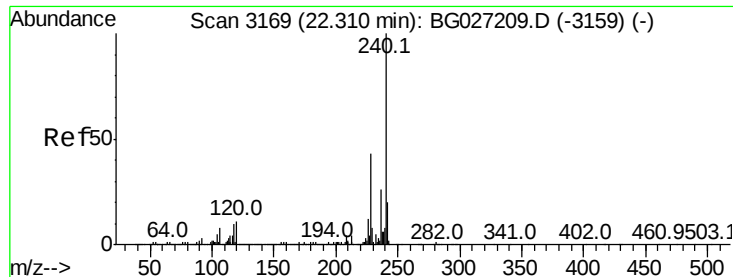

#75

Chrysene-d12

Concen: 20.00 ng

RT: 22.28 min Scan# 3164

Delta R.T. -0.03 min

Lab File: BG027263.D

Acq: 7 Jun 2017 00:05

Instrument :

BNA_G

ClientSampleId :


Tot Ion:240 Resp: 394150

Ion Ratio Lower Upper

240 100

120 11.3 5.7 8.5#




236 25.9 22.2 33.4

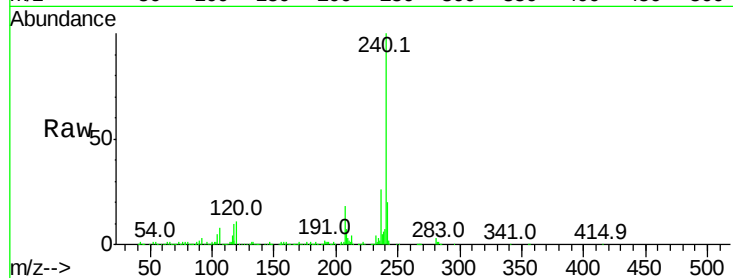

Abundance Ion 240.00 (239.70 to 240.70): E

Ion 120.00 (119.70 to 120.70): E

Ion 236.00 (235.70 to 236.70): E

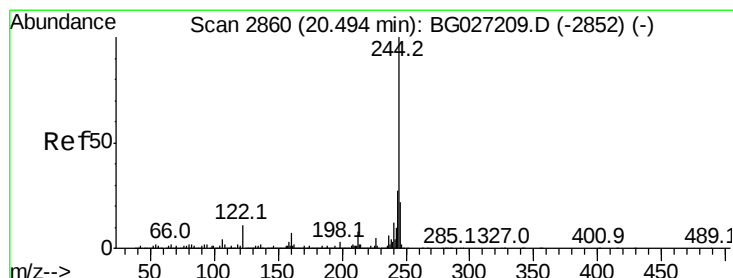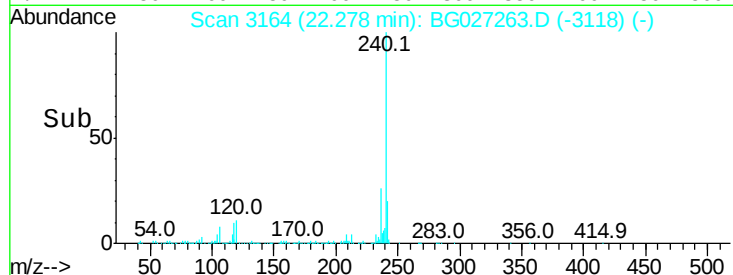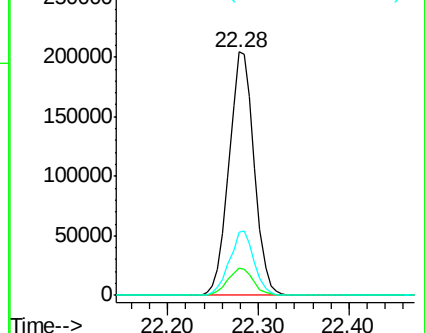

#78

Terphenyl-d14

Concen: 104.09 ng

RT: 20.47 min Scan# 2857

Delta R.T. -0.02 min

Lab File: BG027263.D

Acq: 7 Jun 2017 00:05


Tgt Ion:244 Resp: 1608349

Ion Ratio Lower Upper

244 100

212 8.0 10.0 15.0#



122 11.4 8.6 12.8

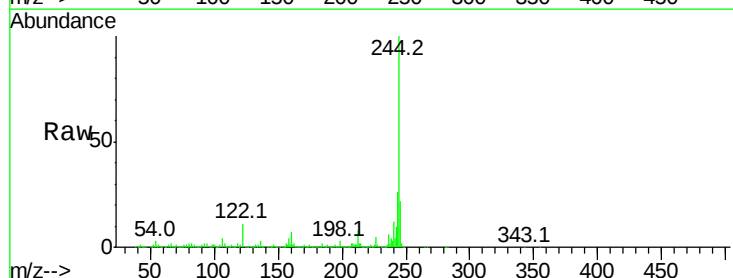


Abundance Ion 244.00 (243.70 to 244.70): E

Ion 212.00 (211.70 to 212.70): E

Ion 122.00 (121.70 to 122.70): E

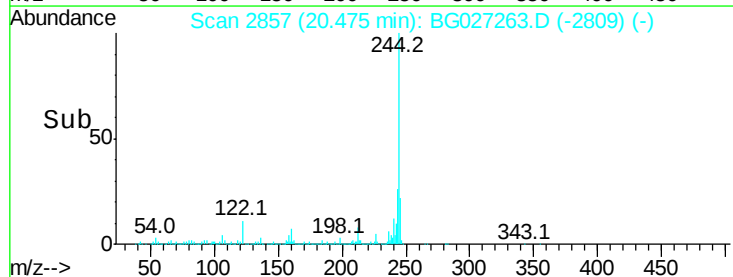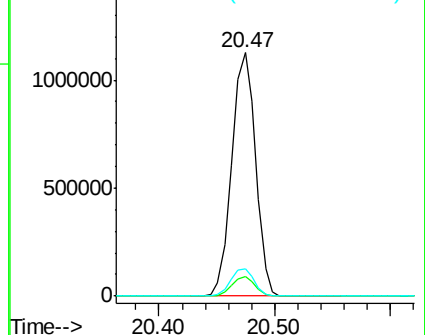


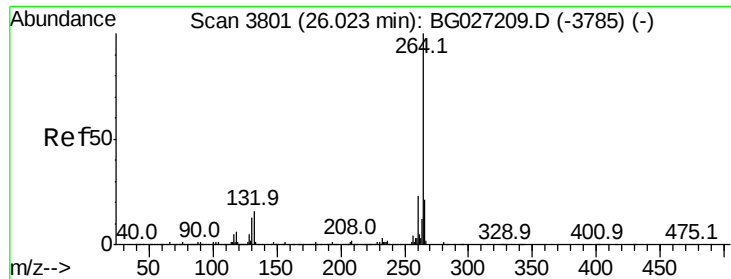

#86
Pervlene-d12
Concen: 20.00 ng
RT: 25.97 min Scan# 3793
Delta R.T. -0.05 min
Lab File: BG027263.D
Acq: 7 Jun 2017 00:05

Instrument :
BNA_G
ClientSampleId :

Tot Ion	Ratio	Lower	Upper
264	100		
260	24.4	21.8	32.8
265	22.7	18.2	27.4

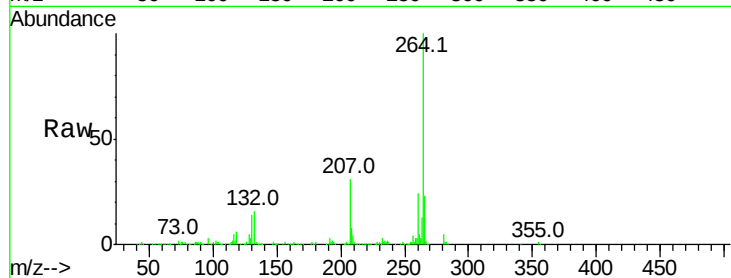

Abundance Ion 264.00 (263.70 to 264.70): E
Ion 260.00 (259.70 to 260.70): E
Ion 265.00 (264.70 to 265.70): E

