

Data Path : Z:\HPCHEM1\BNA G\DATA\BG060617\
 Data File : BG027270.D
 Acq On : 7 Jun 2017 4:39
 Operator : SJ/MA
 Sample : I3466-04
 Misc :
 ALS Vial : 19 Sample Multiplier: 1

Instrument :
 BNA_G
 ClientSampleId :
 SU-RO-4672-060217

Quant Time: Jun 07 05:21:44 2017
 Quant Method : Z:\HPCHEM1\BNA G\METHODS\8270-BG060517.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Mon Jun 05 16:00:35 2017
 Response via : Initial Calibration


Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Dichlorobenzene-d4	8.56	152	49925	20.00	ng	-0.02
21) Naphthalene-d8	11.38	136	230692	20.00	ng	-0.02
38) Acenaphthene-d10	15.14	164	152014	20.00	ng	-0.02
63) Phenanthrene-d10	17.89	188	368797	20.00	ng	-0.02
75) Chrysene-d12	22.28	240	420121	20.00	ng	-0.03
86) Perylene-d12	25.97	264	392531	20.00	ng	-0.05
System Monitoring Compounds						
5) 2-Fluorophenol	6.15	112	466048	142.45	ng	0.00
7) Phenol-d6	7.69	99	612217	127.48	ng	0.00
23) Nitrobenzene-d5	9.73	82	389623	106.22	ng	-0.01
41) 2,4,6-Tribromophenol	16.63	330	312991	156.36	ng	-0.02
44) 2-Fluorobiphenyl	13.77	172	943479	86.83	ng	-0.02
78) Terphenyl-d14	20.47	244	1578461	95.85	ng	-0.02
Target Compounds						
55) 4-Nitrophenol	15.54	139	777	6.44	ng	Qvalue # 1


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\HPCHEM1\BNA G\DATA\BG060617\
Data File : BG027270.D
Acq On : 7 Jun 2017 4:39
Operator : SJ/MA
Sample : I3466-04
Misc :
ALS Vial : 19 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
SU-RO-4672-060217

Quant Time: Jun 07 05:21:44 2017
Quant Method : Z:\HPCHEM1\BNA G\METHODS\8270-BG060517.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Mon Jun 05 16:00:35 2017
Response via : Initial Calibration

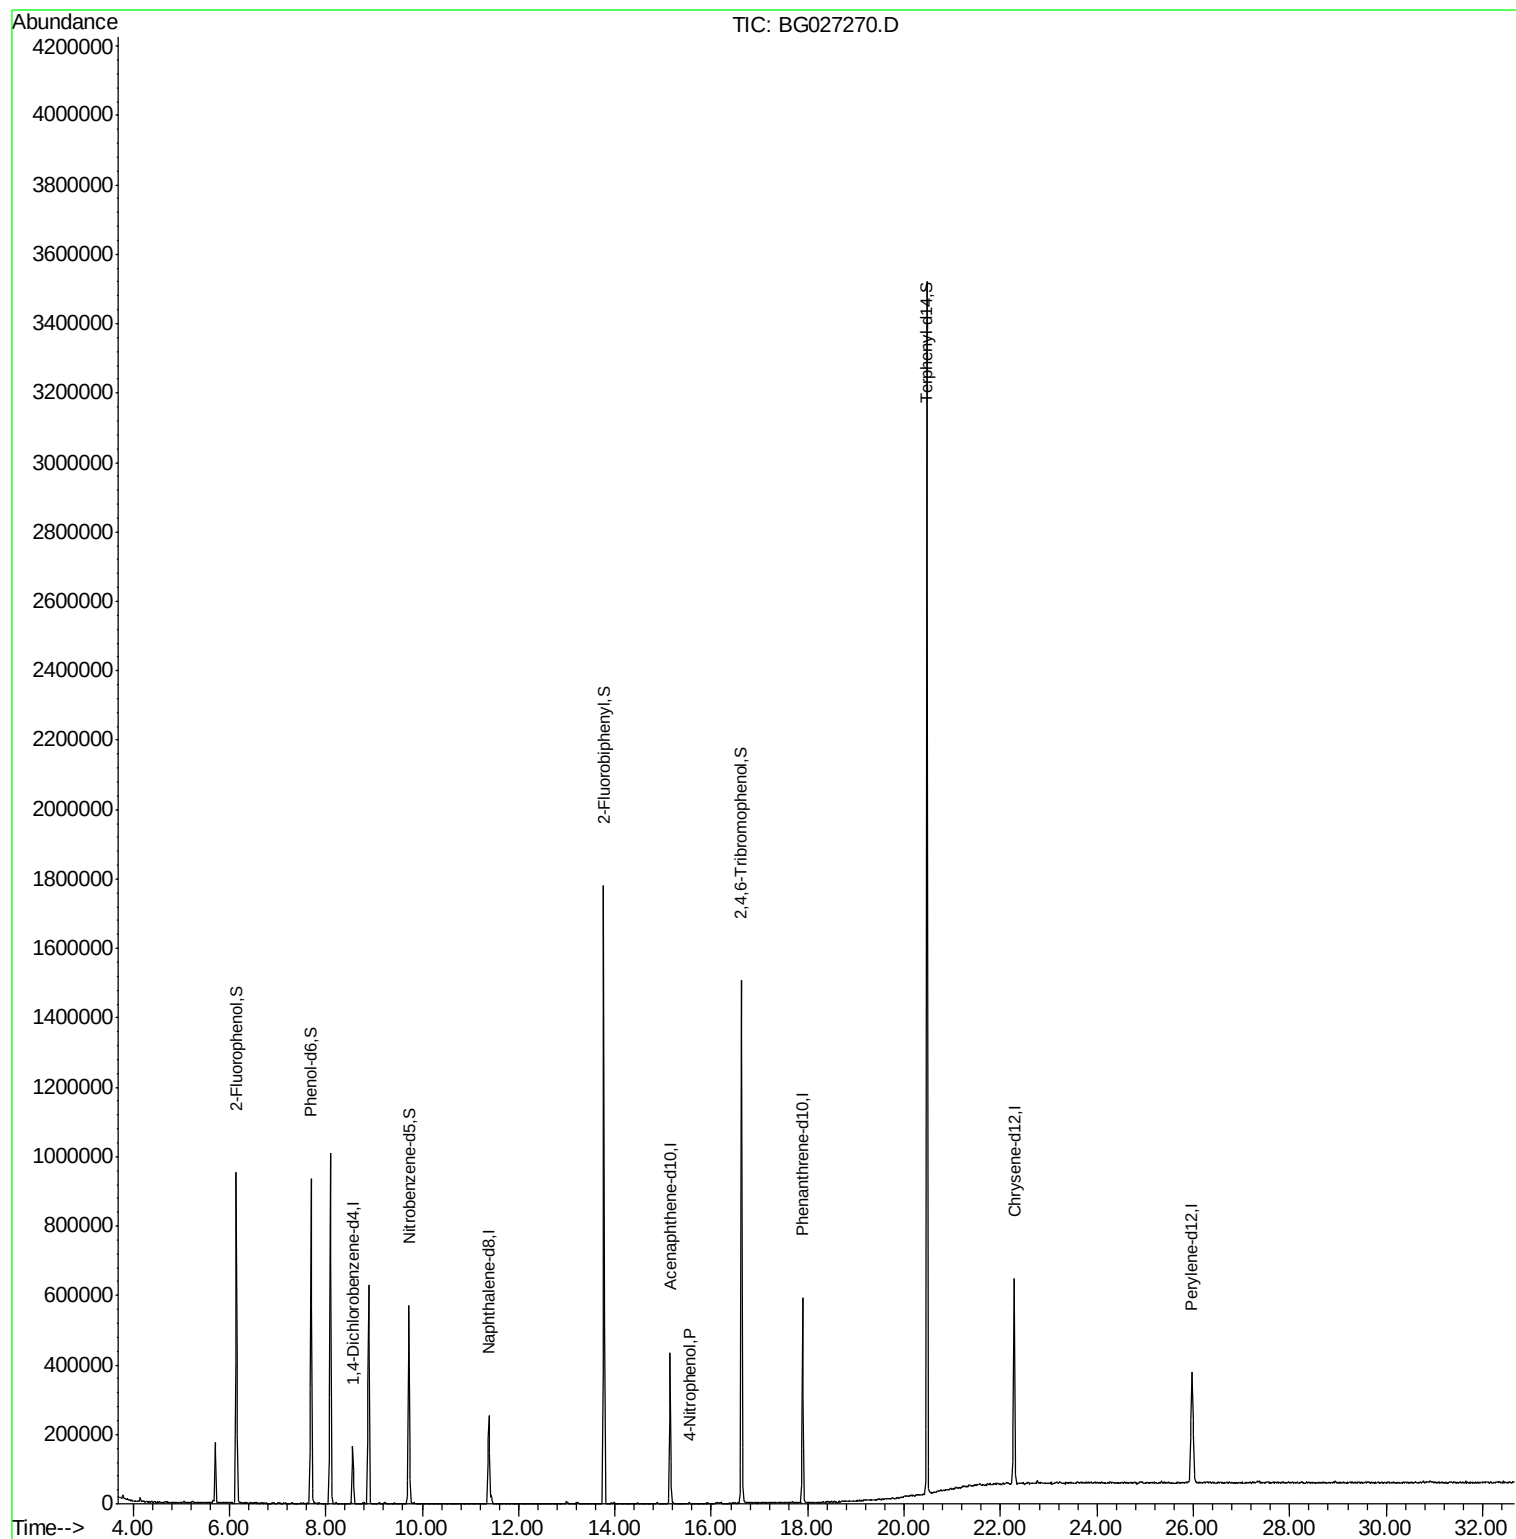

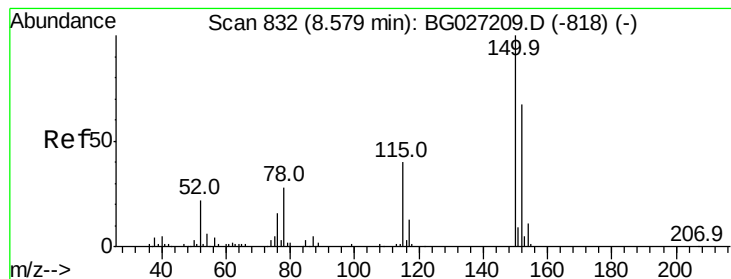

#1

1,4-Dichlorobenzene-d4

Concen: 20.00 ng

RT: 8.56 min Scan# 830

Delta R.T. -0.02 min

Lab File: BG027270.D

Acq: 7 Jun 2017 4:39

Instrument :

BNA_G

ClientSampleId :

SU-RO-4672-060217


Tot Ion:152 Resp: 49925

Ion Ratio Lower Upper

152 100

150 159.4 114.0 171.0




115 68.6 48.1 72.1

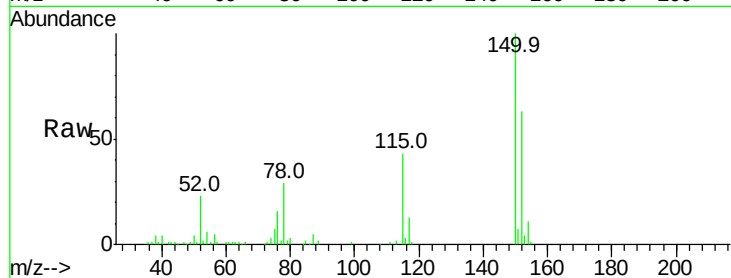

Abundance Ion 152.00 (151.70 to 152.70): E

Ion 150.00 (149.70 to 150.70): E

Ion 115.00 (114.70 to 115.70): E

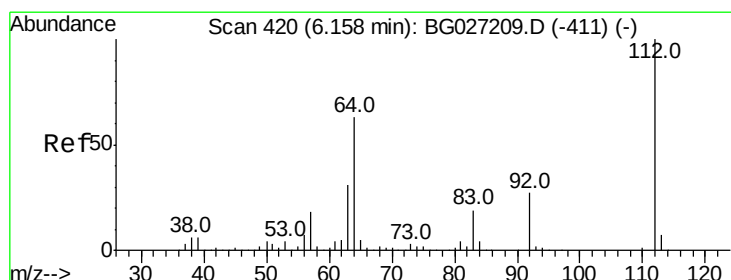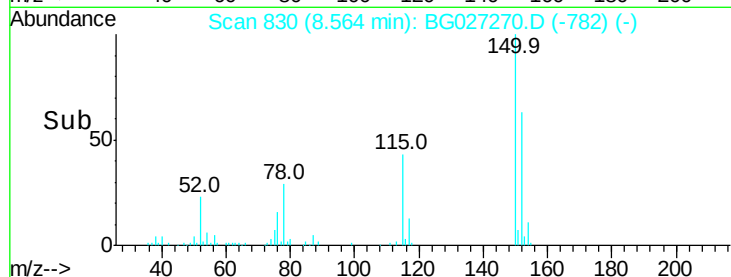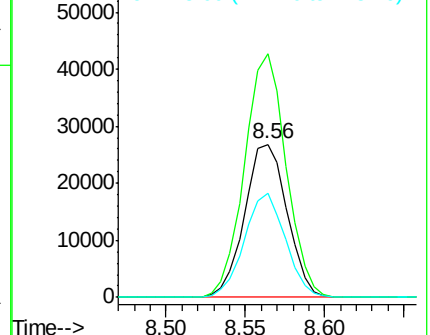

#5

2-Fluorophenol

Concen: 142.45 ng

RT: 6.15 min Scan# 419

Delta R.T. -0.01 min

Lab File: BG027270.D

Acq: 7 Jun 2017 4:39


Tgt Ion:112 Resp: 466048

Ion Ratio Lower Upper

112 100

64 65.3 61.8 92.6



63 31.5 37.2 55.8#

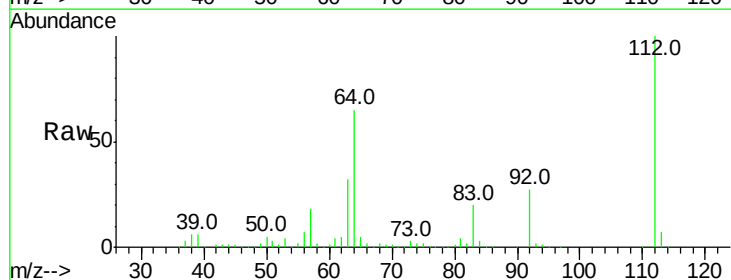


Abundance Ion 112.00 (111.70 to 112.70): E

Ion 64.00 (63.70 to 64.70): BGC

Ion 63.00 (62.70 to 63.70): BGC

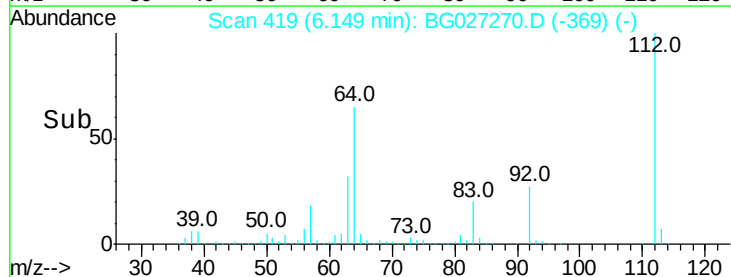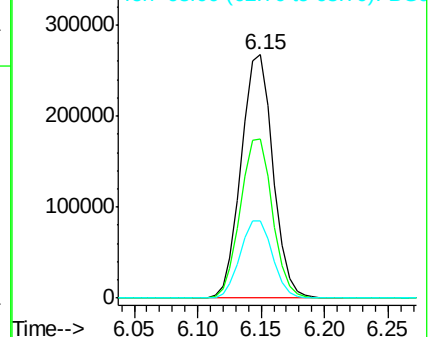

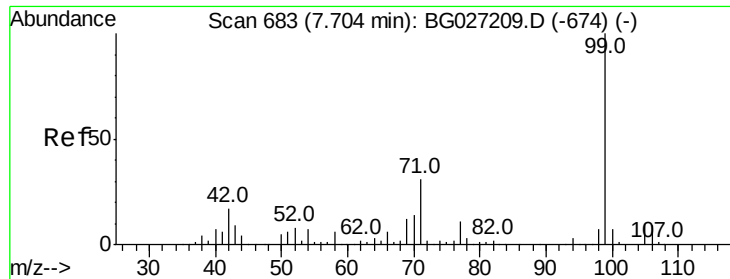

#7

Phenol-d6

Concen: 127.48 ng

RT: 7.69 min Scan# 682

Delta R.T. -0.01 min

Lab File: BG027270.D

Acq: 7 Jun 2017 4:39

Instrument :

BNA_G

ClientSampleId :

SU-RO-4672-060217


Tot Ion: 99 Resp: 612217

Ion Ratio Lower Upper




99 100

42 16.9 20.5 30.7#

71 31.4 37.6 56.4#

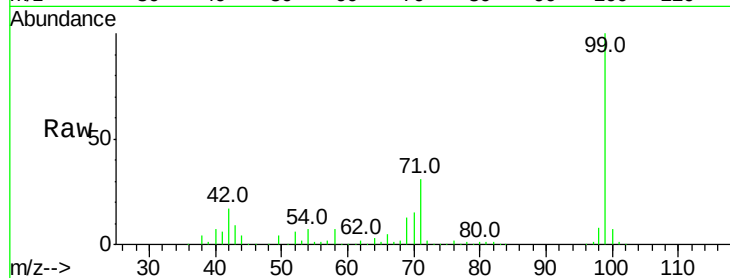

Abundance Ion 99.00 (98.70 to 99.70): BGC
Ion 42.00 (41.70 to 42.70): BGC
Ion 71.00 (70.70 to 71.70): BGC

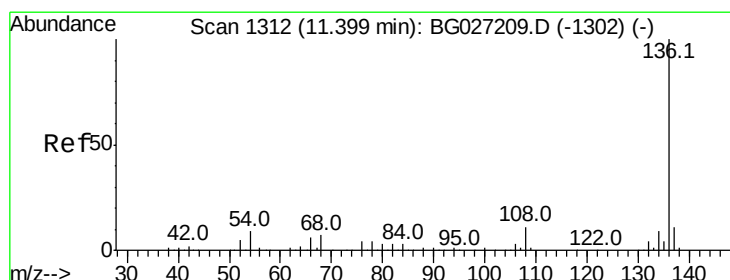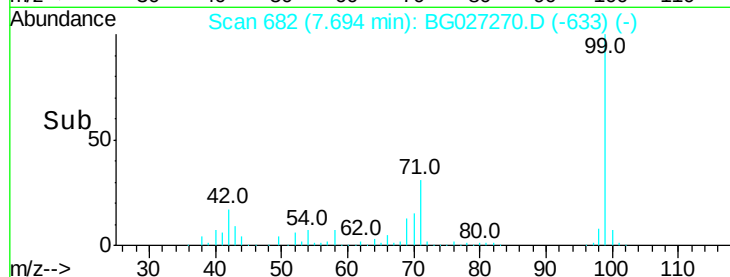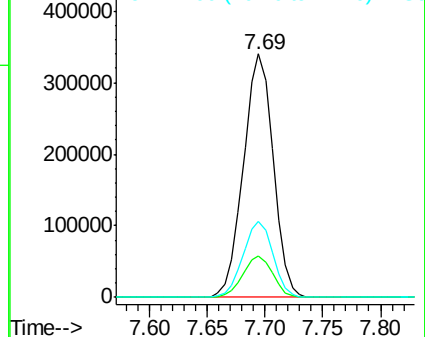

#21

Naphthalene-d8

Concen: 20.00 ng

RT: 11.38 min Scan# 1310

Delta R.T. -0.02 min

Lab File: BG027270.D

Acq: 7 Jun 2017 4:39

Tgt Ion: 136 Resp: 230692


Ion Ratio Lower Upper

136 100



137 11.1 8.9 13.3


54 9.2 9.3 13.9#

68 7.3 5.1 7.7

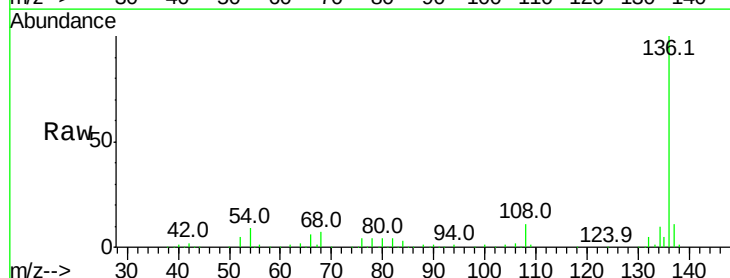

Abundance Ion 136.00 (135.70 to 136.70): BGC
Ion 137.00 (136.70 to 137.70): BGC
Ion 54.00 (53.70 to 54.70): BGC
Ion 68.00 (67.70 to 68.70): BGC



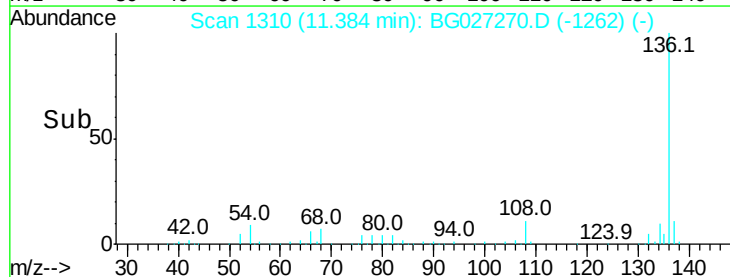
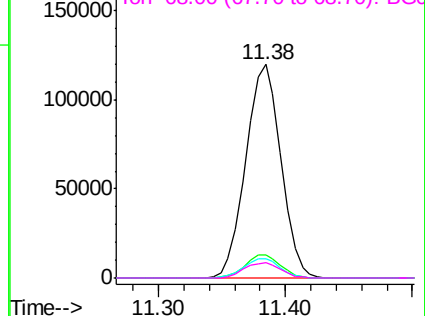


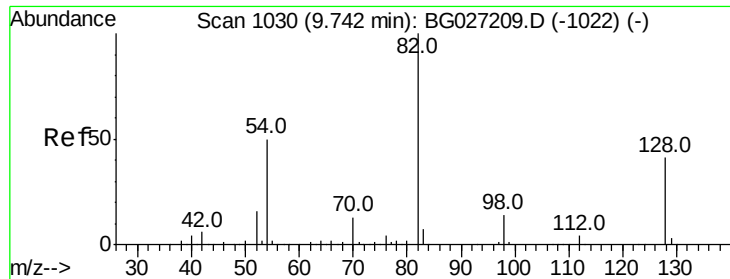

#23
 Nitrobenzene-d5
 Concen: 106.22 ng
 RT: 9.73 min Scan# 1028
 Delta R.T. -0.01 min
 Lab File: BG027270.D
 Acq: 7 Jun 2017 4:39




Instrument :
 BNA_G
 ClientSampleId :
 SU-RO-4672-060217


Tot Ion	82	Resp	389623
Ion	Ratio	Lower	Upper
82	100		
128	41.8	26.4	39.6#
54	51.0	49.4	74.2

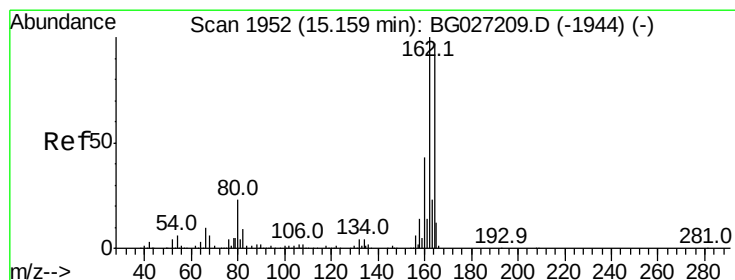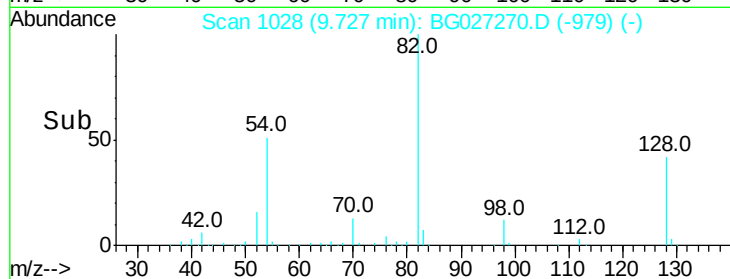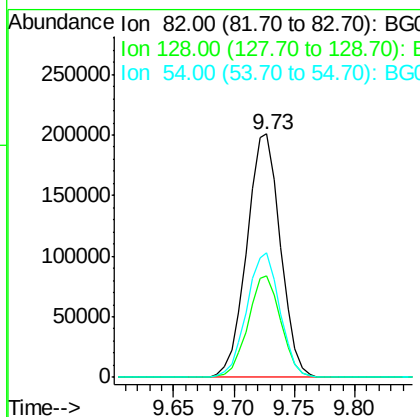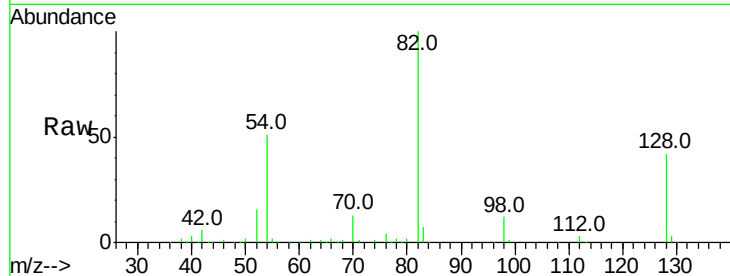

#38
 Acenaphthene-d10
 Concen: 20.00 ng
 RT: 15.14 min Scan# 1950
 Delta R.T. -0.02 min
 Lab File: BG027270.D
 Acq: 7 Jun 2017 4:39

Tgt Ion	164	Resp	152014
Ion	Ratio	Lower	Upper
164	100		
162	106.1	85.1	127.7
160	44.7	34.7	52.1


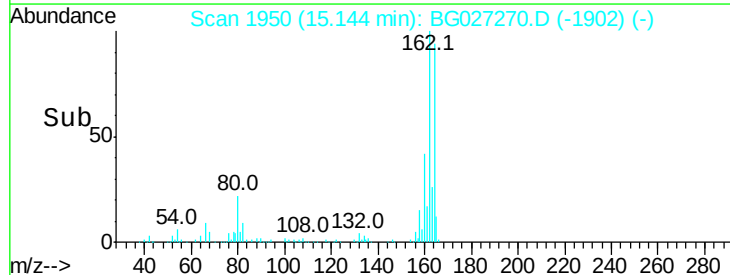
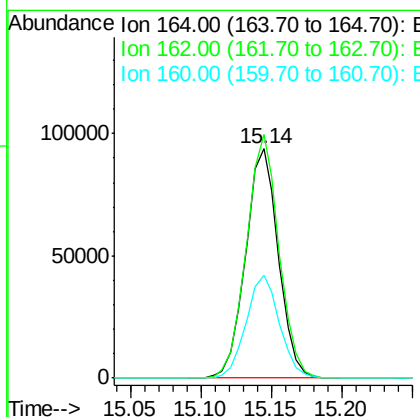
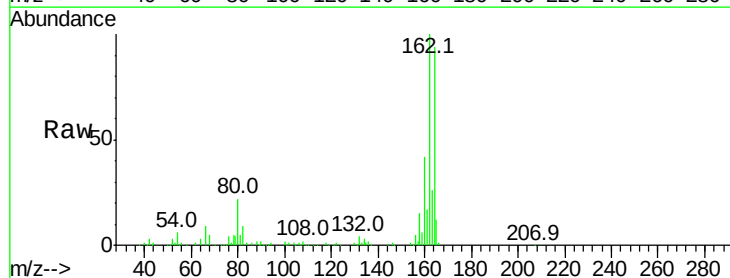


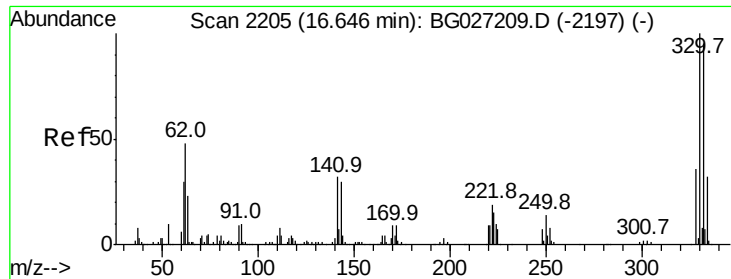

#41
 2,4,6-Tribromophenol
 Concen: 156.36 ng
 RT: 16.63 min Scan# 2202
 Delta R.T. -0.02 min
 Lab File: BG027270.D
 Acq: 7 Jun 2017 4:39




Instrument :
 BNA_G
 ClientSampleId :
 SU-RO-4672-060217


Tot Ion	Ratio	Lower	Upper
330	100		
332	95.9	77.3	115.9
141	32.7	32.1	48.1

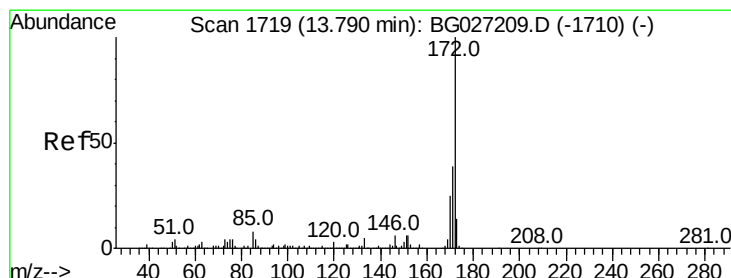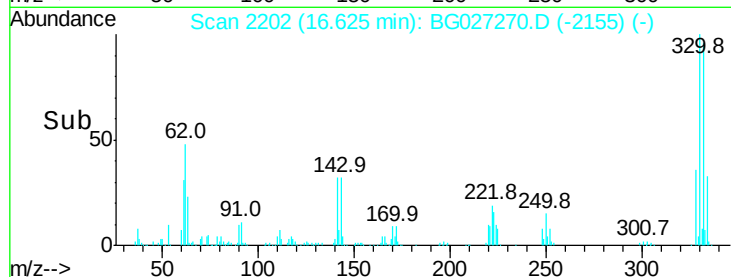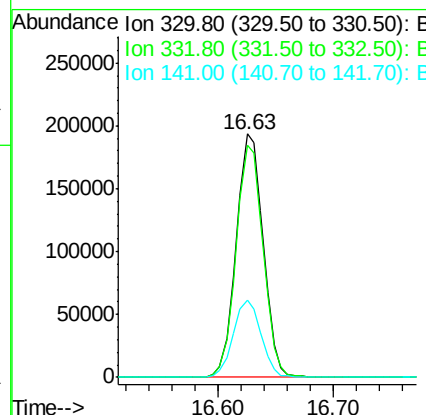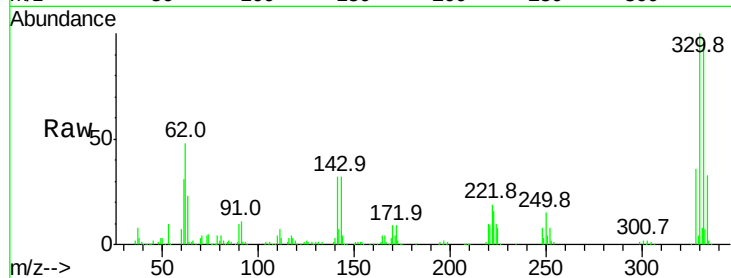

#44
 2-Fluorobiphenyl
 Concen: 86.83 ng
 RT: 13.77 min Scan# 1716
 Delta R.T. -0.02 min
 Lab File: BG027270.D
 Acq: 7 Jun 2017 4:39

Tgt Ion	Ratio	Lower	Upper
172	100		
171	37.9	32.2	48.2
170	25.0	21.8	32.6

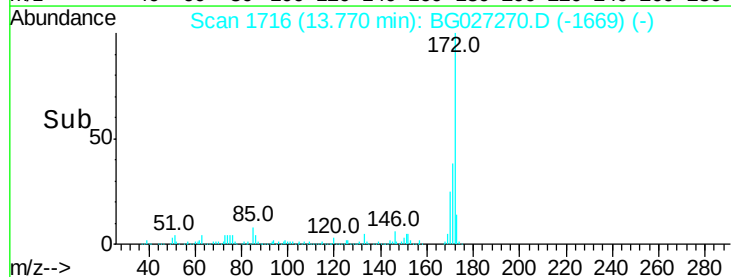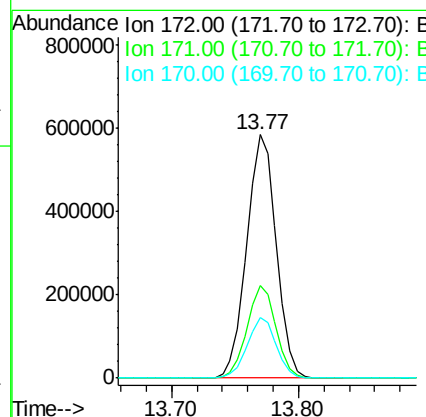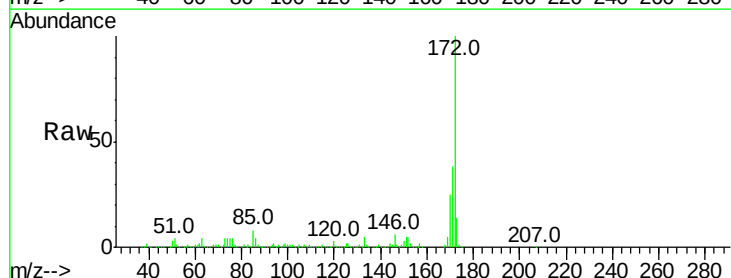


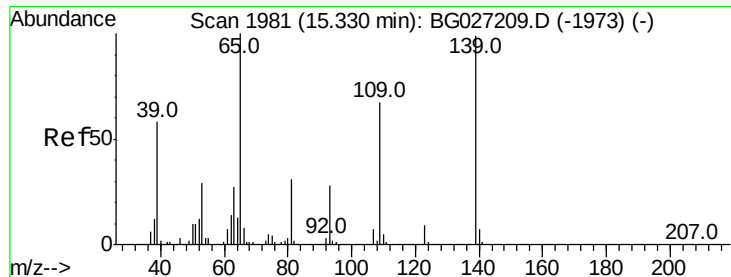




#55
4-Nitrophenol
Concen: 6.44 ng
RT: 15.54 min Scan# 2018
Delta R.T. 0.21 min
Lab File: BG027270.D
Acq: 7 Jun 2017 4:39

Instrument :
BNA_G
ClientSampleId :
SU-RO-4672-060217

Tot Ion:139 Resp: 777
Ion Ratio Lower Upper
139 100
109 0.0 101.2 141.2#
65 0.0 135.3 175.3#

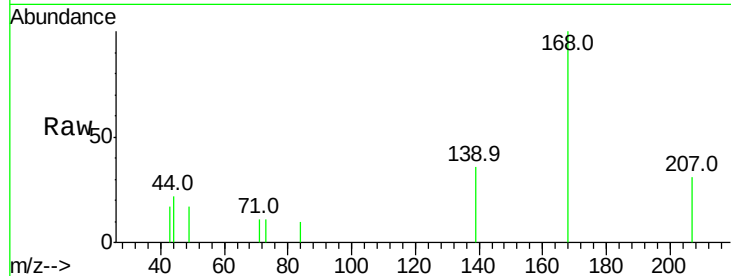


Abundance Ion 139.00 (138.70 to 139.70): E
Ion 109.00 (108.70 to 109.70): E
Ion 65.00 (64.70 to 65.70): BGC

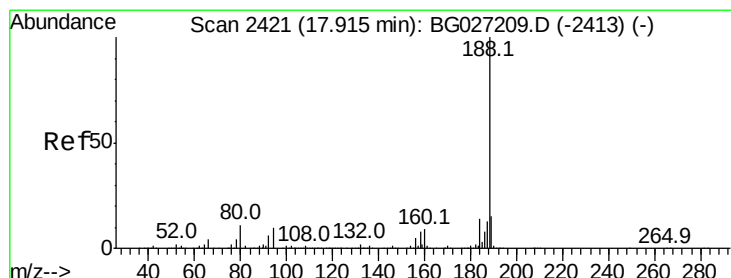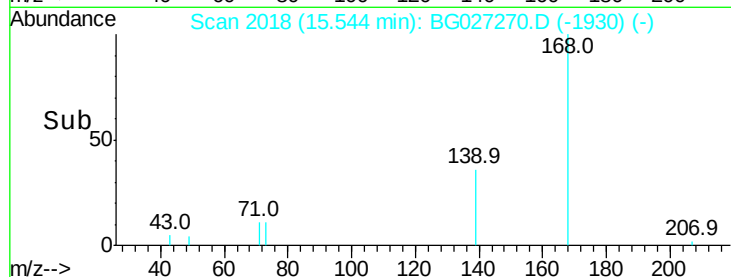
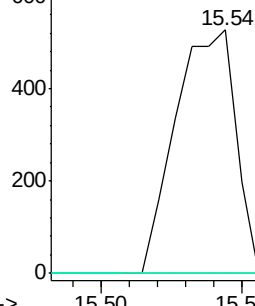



#63
Phenanthrene-d10
Concen: 20.00 ng
RT: 17.89 min Scan# 2418
Delta R.T. -0.02 min
Lab File: BG027270.D
Acq: 7 Jun 2017 4:39

Tgt Ion:188 Resp: 368797
Ion Ratio Lower Upper
188 100
94 10.5 5.8 8.8#
80 12.9 7.5 11.3#

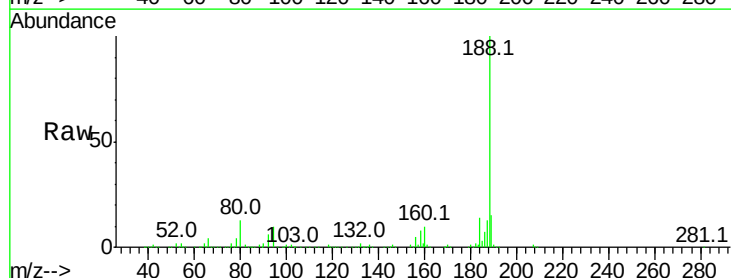

Abundance Ion 188.00 (187.70 to 188.70): E
Ion 94.00 (93.70 to 94.70): BGC
Ion 80.00 (79.70 to 80.70): BGC

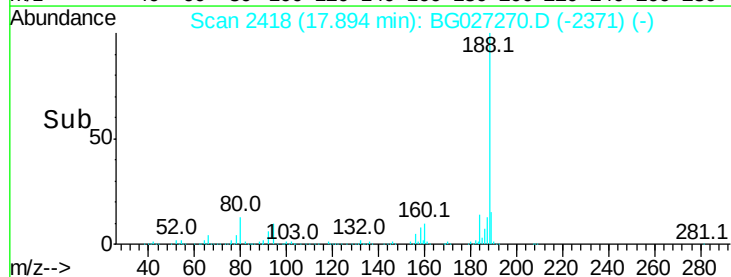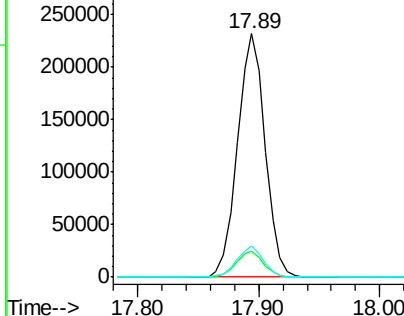

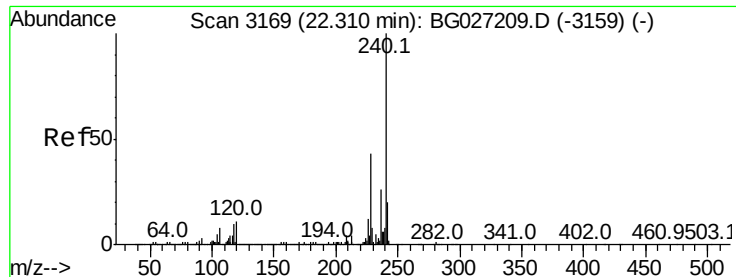

#75

Chrysene-d12

Concen: 20.00 ng

RT: 22.28 min Scan# 3165

Delta R.T. -0.03 min

Lab File: BG027270.D

Acq: 7 Jun 2017 4:39

Instrument :

BNA_G

ClientSampleId :

SU-RO-4672-060217


Tot Ion:240 Resp: 420121

Ion Ratio Lower Upper

240 100

120 10.6 5.7 8.5#




236 25.1 22.2 33.4

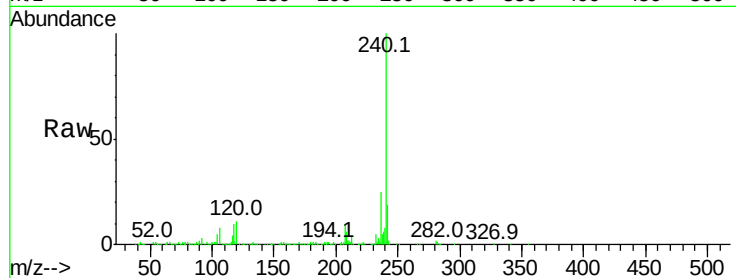

Abundance Ion 240.00 (239.70 to 240.70): E

Ion 120.00 (119.70 to 120.70): E

Ion 236.00 (235.70 to 236.70): E

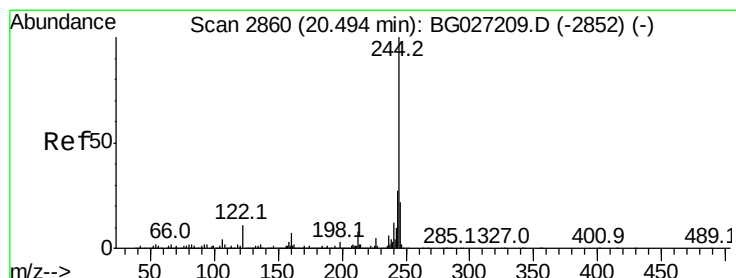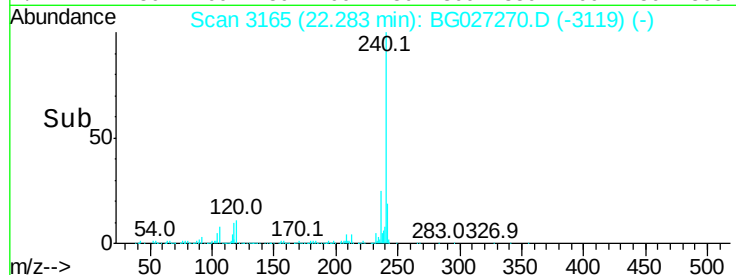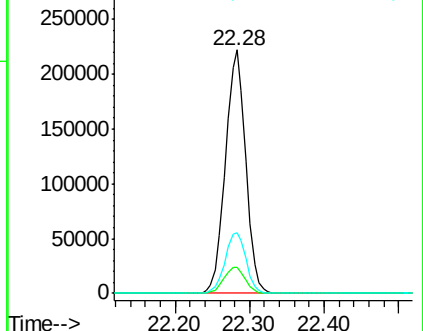

#78

Terphenyl-d14

Concen: 95.85 ng

RT: 20.47 min Scan# 2857

Delta R.T. -0.02 min

Lab File: BG027270.D

Acq: 7 Jun 2017 4:39


Tgt Ion:244 Resp: 1578461

Ion Ratio Lower Upper

244 100

212 7.9 10.0 15.0#



122 11.2 8.6 12.8

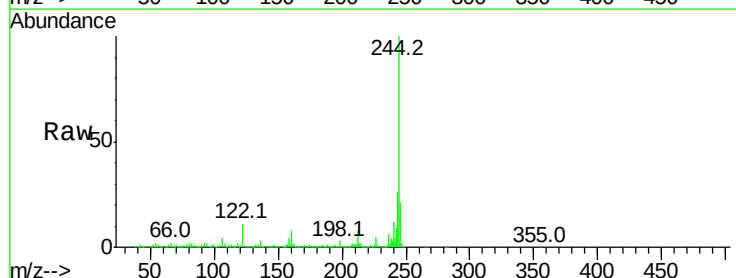


Abundance Ion 244.00 (243.70 to 244.70): E

Ion 212.00 (211.70 to 212.70): E

Ion 122.00 (121.70 to 122.70): E

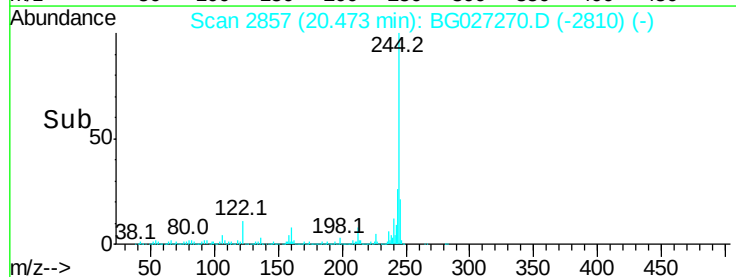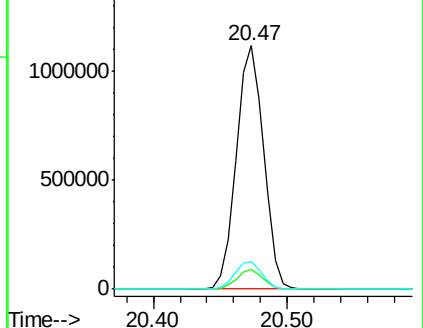

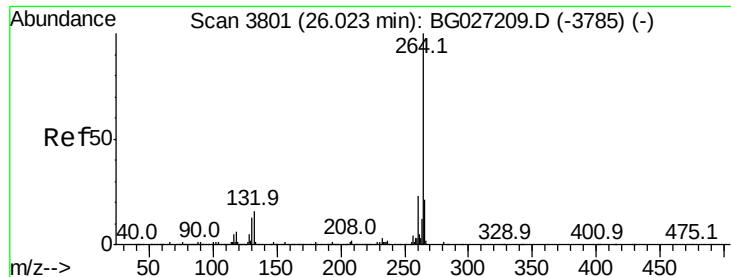

#86
Pervlene-d12
Concen: 20.00 ng
RT: 25.97 min Scan# 3793
Delta R.T. -0.05 min
Lab File: BG027270.D
Acq: 7 Jun 2017 4:39

Instrument :
BNA_G
ClientSampleId :
SU-RO-4672-060217

Tot Ion	Ratio	Lower	Upper
264	100		
260	23.5	21.8	32.8
265	21.6	18.2	27.4

