
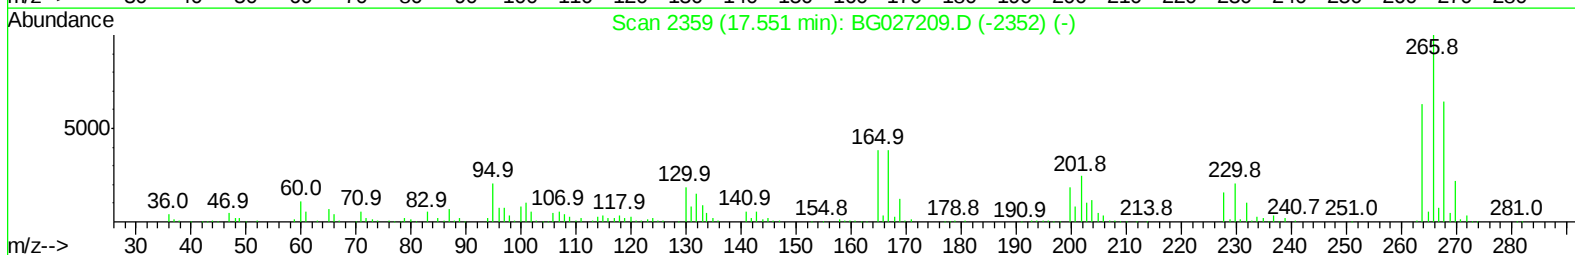
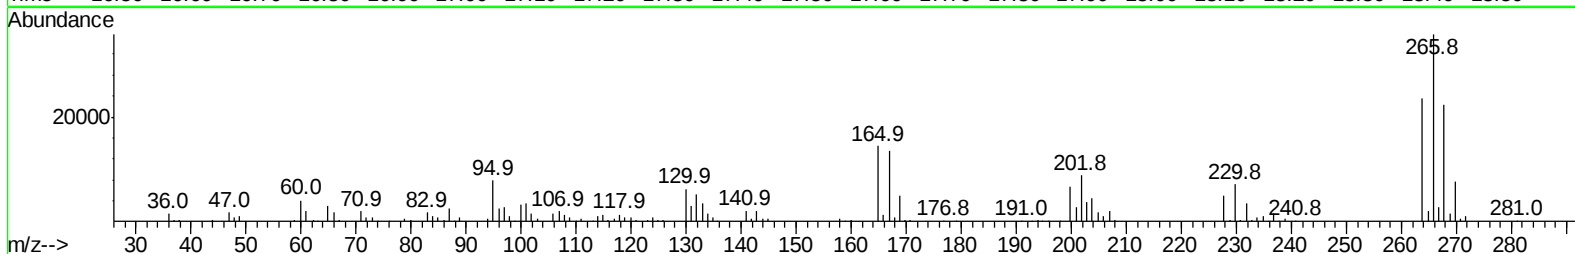


Data Path : Z:\HPCHEM1\BNA G\Data\BG060617\
Data File : BG027271.D
Acq On : 7 Jun 2017 6:04
Operator : SJ/MA
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Jun 07 08:27:54 2017
Quant Method : Z:\HPCHEM1\BNA G\METHODS\8270-BG060517.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Mon Jun 05 16:00:35 2017
Response via : Initial Calibration

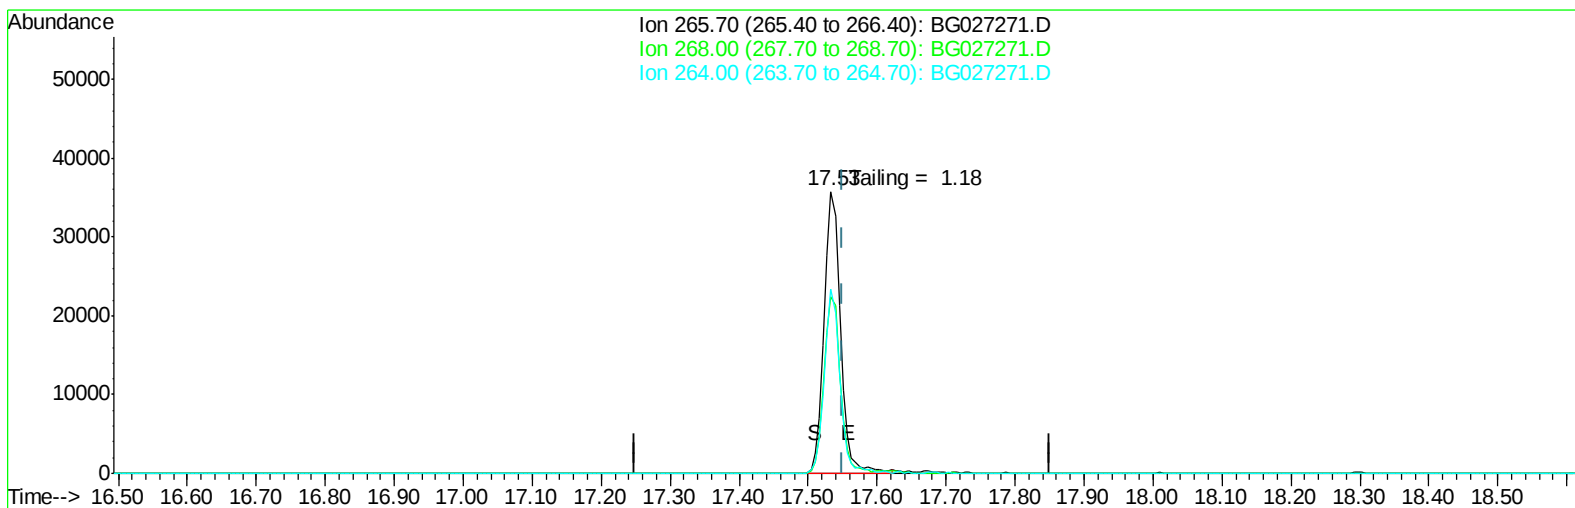

TIC: BG027271.D

(69) Pentachlorophenol (C)



17.533min (-0.017) 0.00ng

response 58935

Ion	Exp%	Act%
265.70	100	100
268.00	60.70	62.65
264.00	62.60	65.63
0.00	0.00	0.00

Data Path : Z:\HPCHEM1\BNA G\Data\BG060617\
Data File : BG027271.D
Acq On : 7 Jun 2017 6:04
Operator : SJ/MA
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Jun 07 08:27:54 2017
Quant Method : Z:\HPCHEM1\BNA G\METHODS\8270-BG060517.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Mon Jun 05 16:00:35 2017
Response via : Initial Calibration

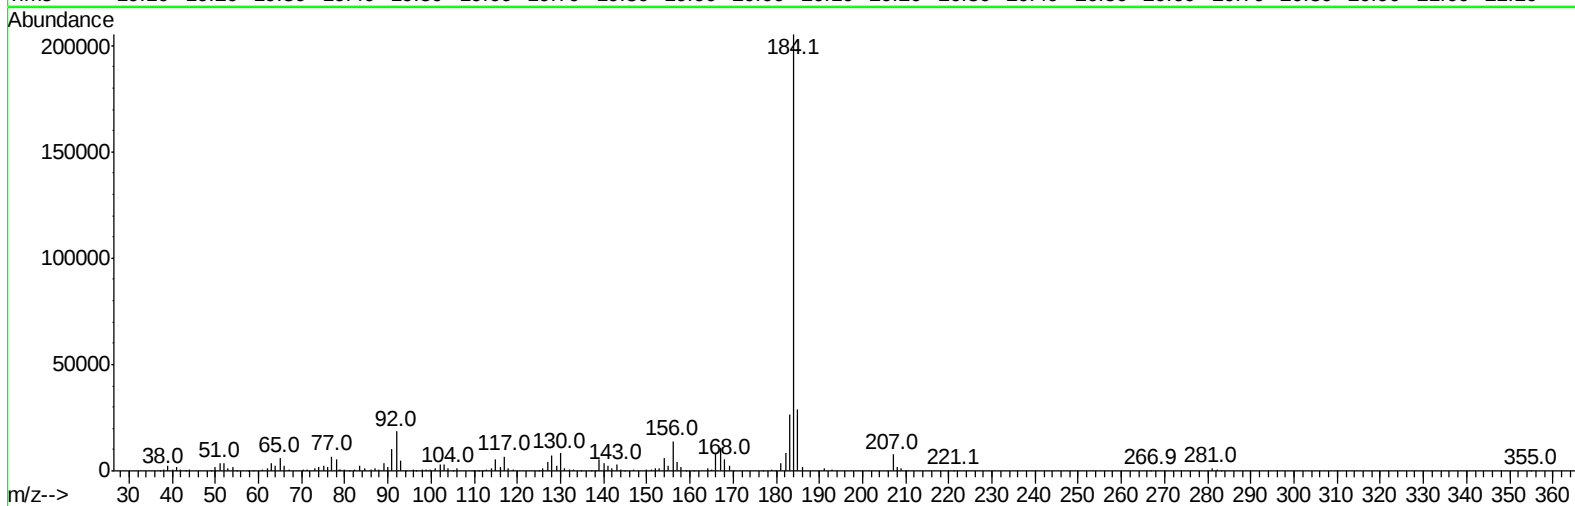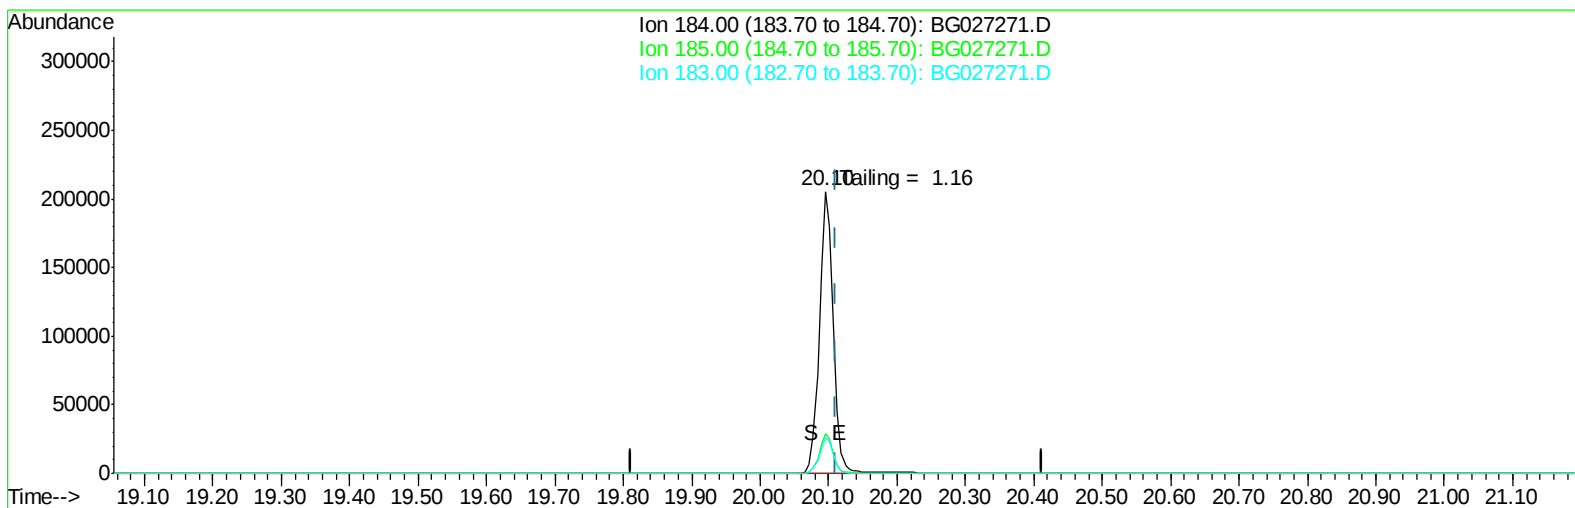

TIC: BG027271.D

(76) Benzidine

20.095min (-0.017) 0.00ng

response 294150

Ion	Exp%	Act%
184.00	100	100
185.00	16.30	14.09
183.00	13.80	12.82
0.00	0.00	0.00