

Data Path : Z:\HPCHEM1\BNA_G\DATA\BG060617\
 Data File : BG027263.D
 Acq On : 7 Jun 2017 00:05
 Operator : SJ/MA
 Sample : I3438-15
 Misc :
 ALS Vial : 12 Sample Multiplier: 1

Instrument :
 BNA_G
 ClientSampleId :
 TP-8-9

Quant Time: Jun 07 06:52:13 2017
 Quant Method : Z:\HPCHEM1\BNA_G\METHODS\8270-BG060517.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Mon Jun 05 16:00:35 2017
 Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Dichlorobenzene-d4	8.56	152	47881	20.00	ng	-0.01
21) Naphthalene-d8	11.39	136	215650	20.00	ng	-0.01
38) Acenaphthene-d10	15.15	164	137926	20.00	ng	-0.01
63) Phenanthrene-d10	17.90	188	348999	20.00	ng	-0.02
75) Chrysene-d12	22.28	240	394150	20.00	ng	-0.03
86) Perylene-d12	25.97	264	362527	20.00	ng	-0.05
System Monitoring Compounds						
5) 2-Fluorophenol	6.14	112	470327	149.89	ng	-0.01
7) Phenol-d6	7.70	99	613336	133.16	ng	0.00
23) Nitrobenzene-d5	9.72	82	379490	110.67	ng	-0.02
41) 2,4,6-Tribromophenol	16.63	330	312549	172.09	ng	-0.02
44) 2-Fluorobiphenyl	13.77	172	957007	97.07	ng	-0.02
78) Terphenyl-d14	20.47	244	1608349	104.09	ng	-0.02


Target Compounds	Qvalue
------------------	--------


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\HPCHEM1\BNA_G\DATA\BG060617\
Data File : BG027263.D
Acq On : 7 Jun 2017 00:05
Operator : SJ/MA
Sample : I3438-15
Misc :
ALS Vial : 12 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
TP-8-9

Quant Time: Jun 07 06:52:13 2017
Quant Method : Z:\HPCHEM1\BNA_G\METHODS\8270-BG060517.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Mon Jun 05 16:00:35 2017
Response via : Initial Calibration

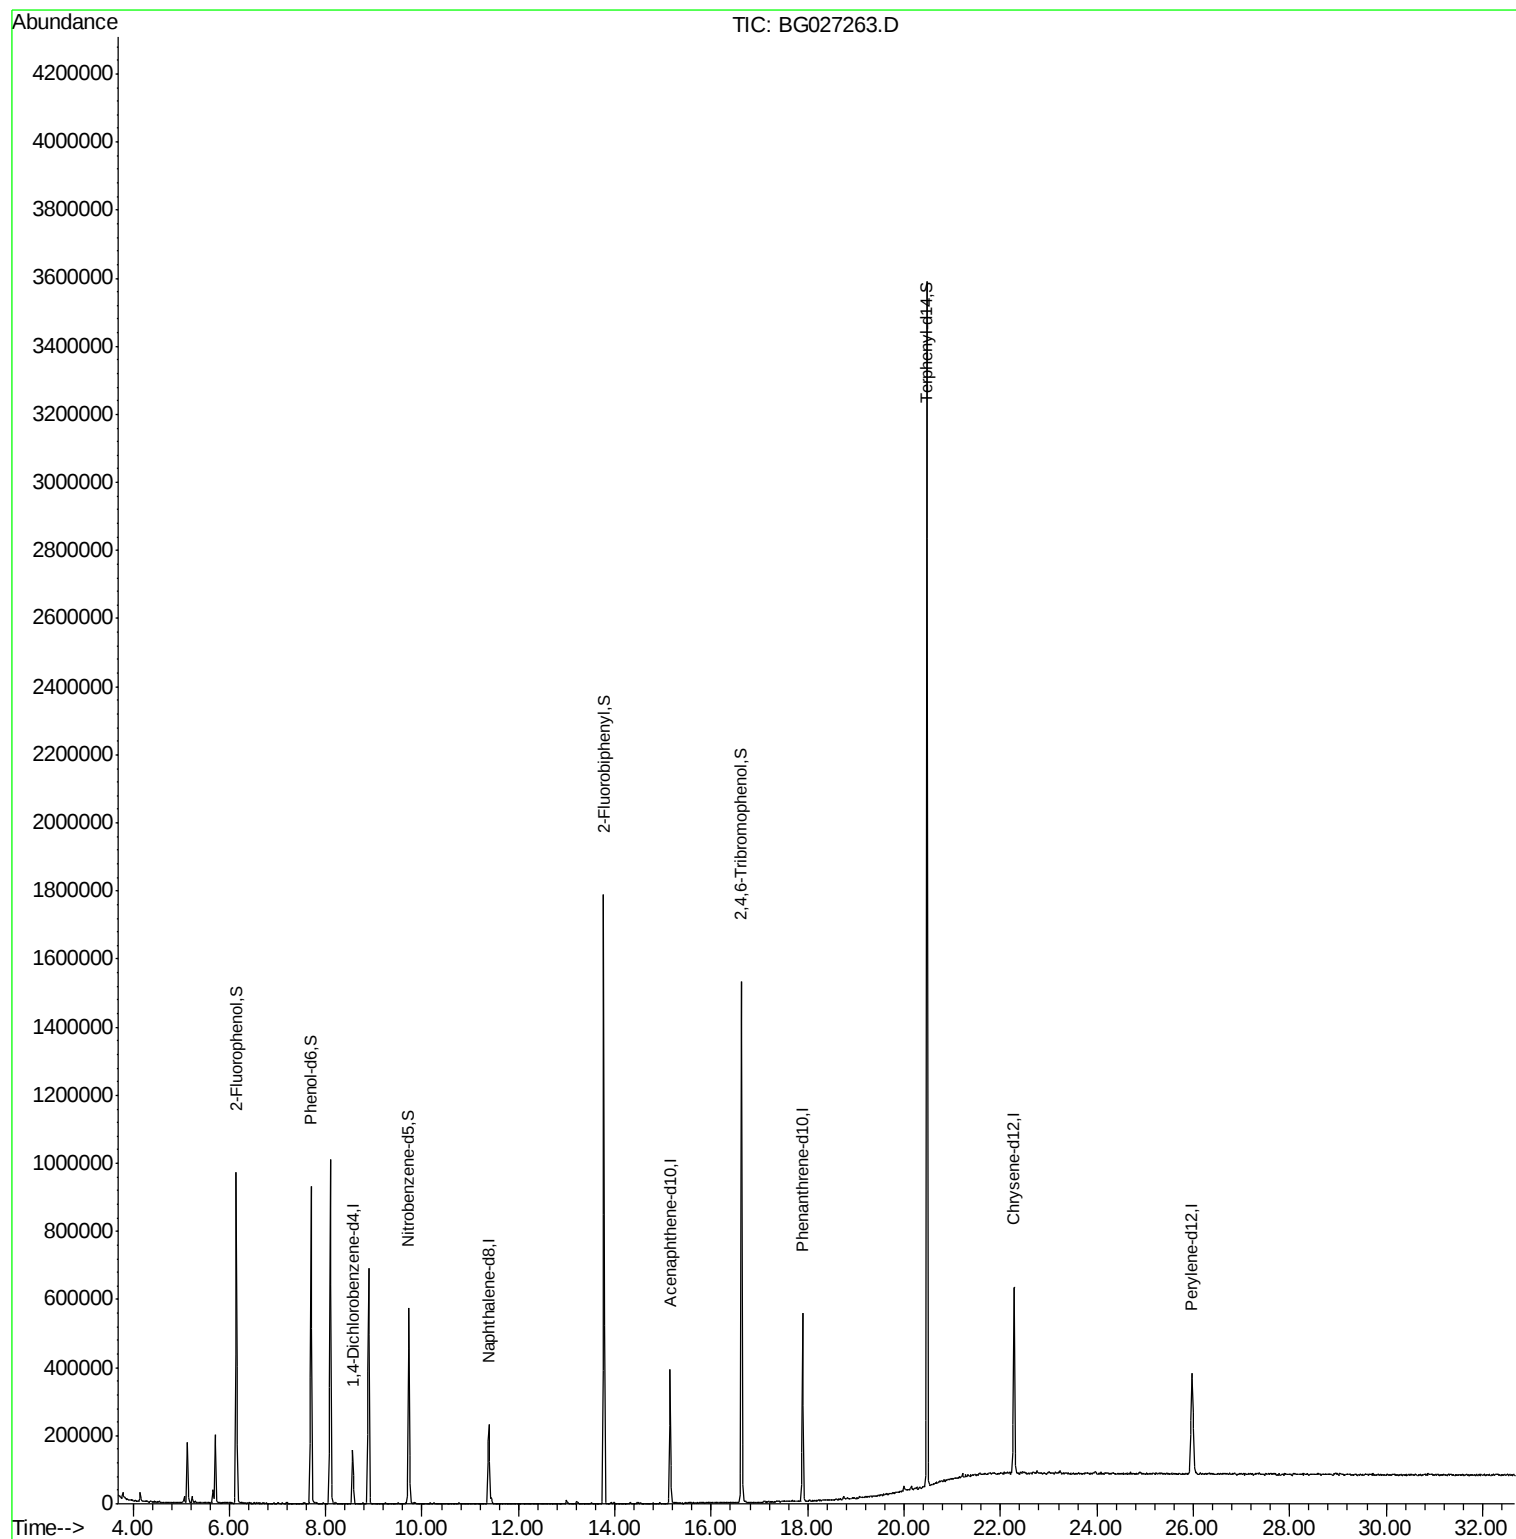




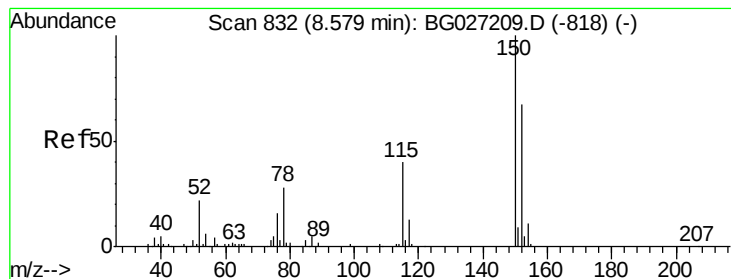


#1

1,4-Dichlorobenzene-d4
Concen: 20.000 ng
RT: 8.56 min Scan# 830
Delta R.T. -0.01 min
Lab File: BG027263.D
Acq: 7 Jun 2017 00:05

Instrument :
BNA_G
ClientSampleId :
TP-8-9




Tgt Ion:152 Resp: 47881
Ion Ratio Lower Upper
152 100
150 154.3 114.0 171.0
115 67.5 48.1 72.1

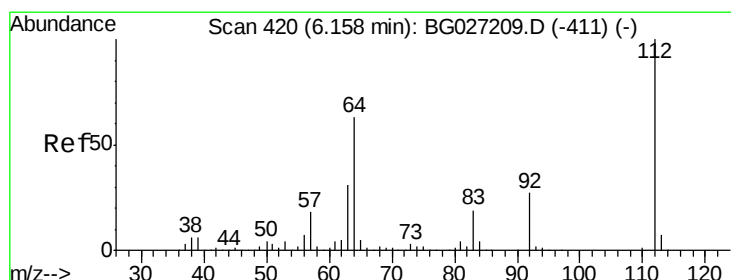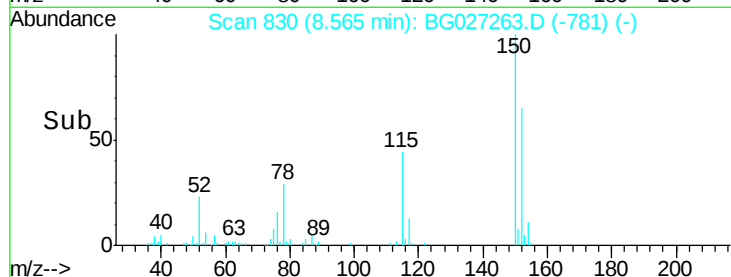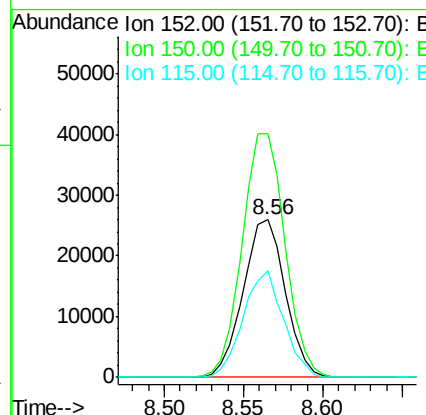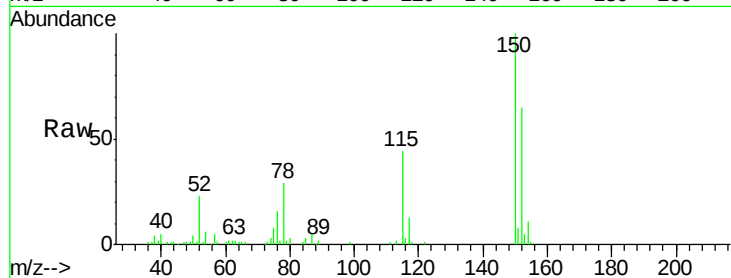


#5

2-Fluorophenol
Concen: 149.893 ng
RT: 6.14 min Scan# 418
Delta R.T. -0.01 min
Lab File: BG027263.D
Acq: 7 Jun 2017 00:05

Tgt Ion:112 Resp: 470327
Ion Ratio Lower Upper
112 100
64 64.8 61.8 92.6
63 32.9 37.2 55.8#

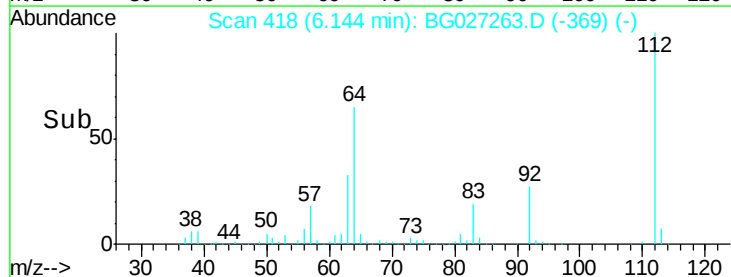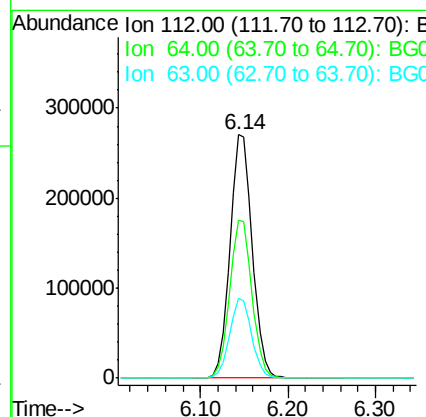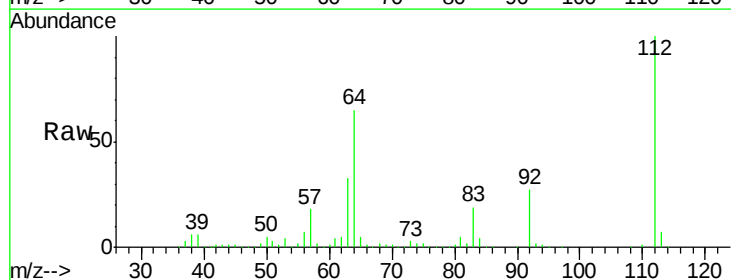

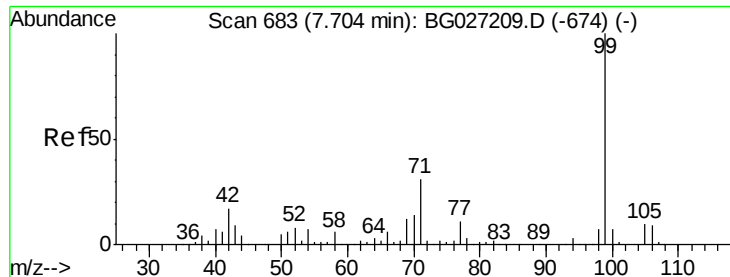

#7

Phenol-d6

Concen: 133.164 ng

RT: 7.70 min Scan# 682

Delta R.T. -0.01 min

Lab File: BG027263.D

Acq: 7 Jun 2017 00:05

Instrument :

BNA_G

ClientSampleId :

TP-8-9


Tgt Ion: 99 Resp: 613336

Ion Ratio Lower Upper




99 100

42 16.6 20.5 30.7#

71 32.4 37.6 56.4#

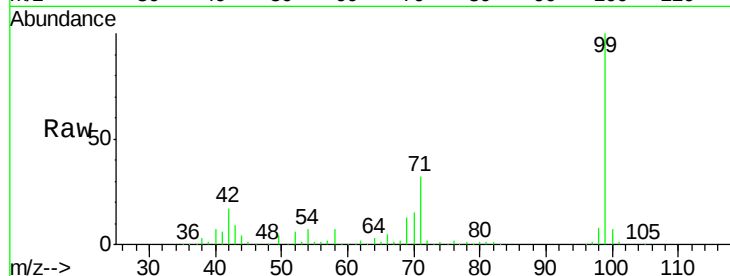

Abundance Ion 99.00 (98.70 to 99.70): BGC
Ion 42.00 (41.70 to 42.70): BGC
Ion 71.00 (70.70 to 71.70): BGC

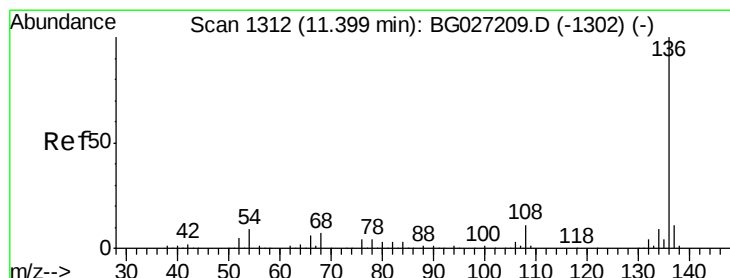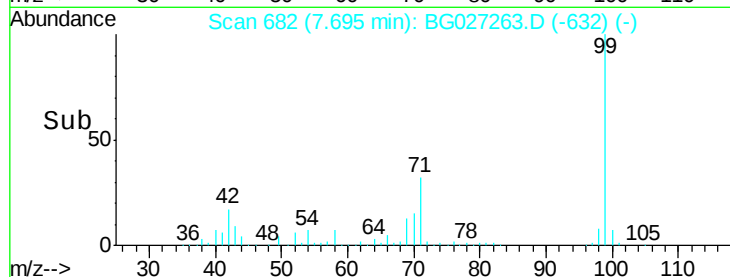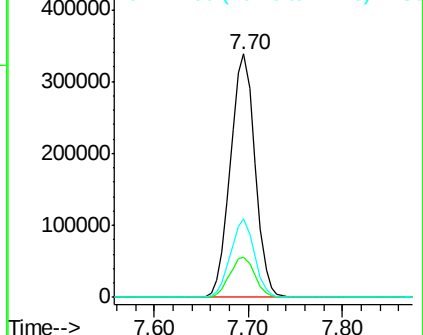

#21

Naphthalene-d8

Concen: 20.000 ng

RT: 11.39 min Scan# 1310

Delta R.T. -0.01 min

Lab File: BG027263.D

Acq: 7 Jun 2017 00:05

Tgt Ion: 136 Resp: 215650


Ion Ratio Lower Upper

136 100



137 10.2 8.9 13.3


54 9.3 9.3 13.9#

68 7.8 5.1 7.7#

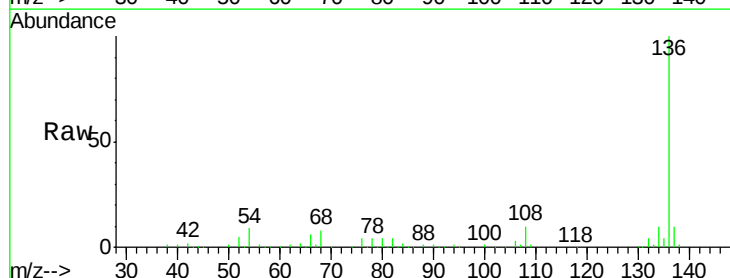

Abundance Ion 136.00 (135.70 to 136.70): BGC
Ion 137.00 (136.70 to 137.70): BGC
Ion 54.00 (53.70 to 54.70): BGC
Ion 68.00 (67.70 to 68.70): BGC



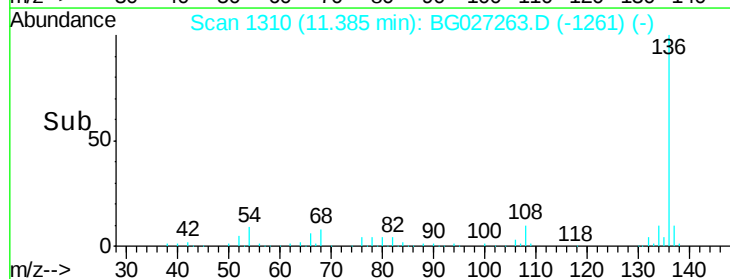
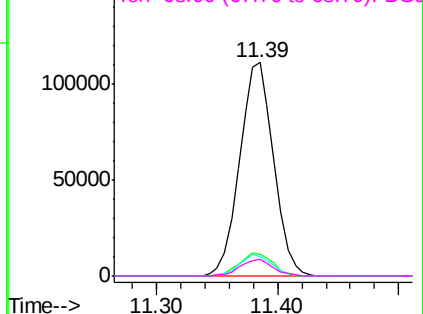


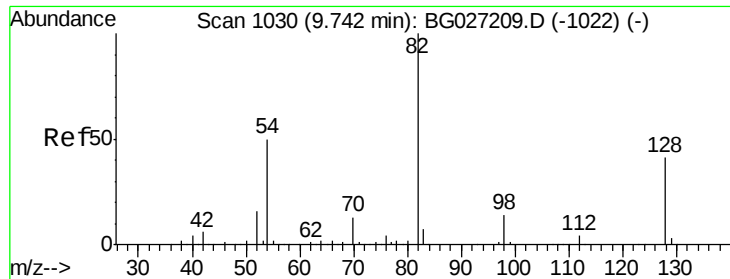

#23
 Nitrobenzene-d5
 Concen: 110.670 ng
 RT: 9.72 min Scan# 1027
 Delta R.T. -0.02 min
 Lab File: BG027263.D
 Acq: 7 Jun 2017 00:05




Instrument :
 BNA_G
 ClientSampleId :
 TP-8-9

Tgt Ion: 82 Resp: 379490
 Ion Ratio Lower Upper
 82 100
 128 40.2 26.4 39.6#
 54 50.7 49.4 74.2

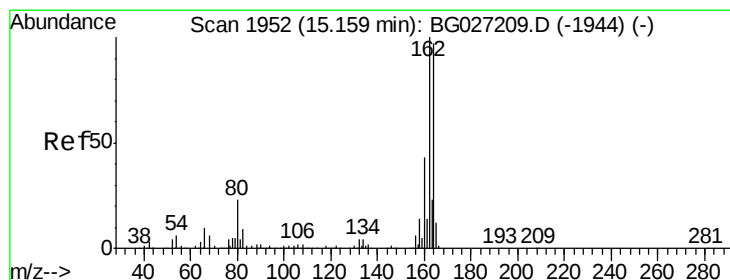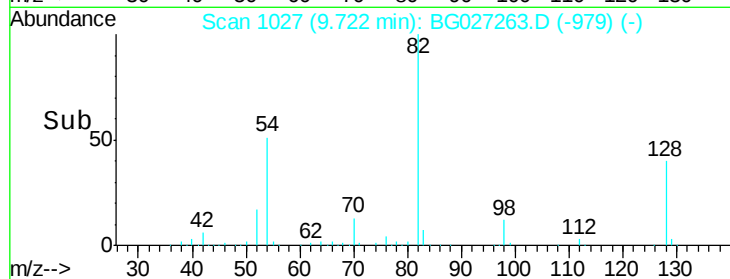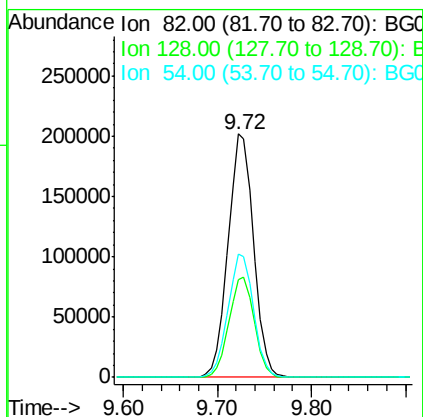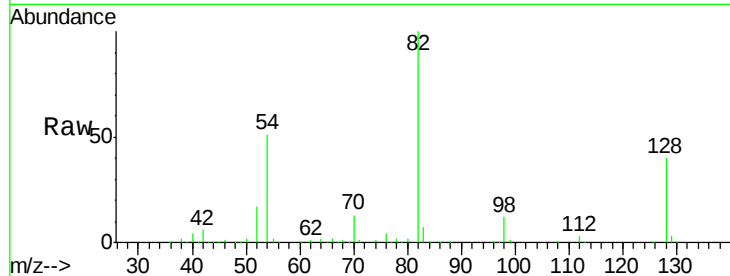

#38
 Acenaphthene-d10
 Concen: 20.000 ng
 RT: 15.15 min Scan# 1950
 Delta R.T. -0.01 min
 Lab File: BG027263.D
 Acq: 7 Jun 2017 00:05

Tgt Ion: 164 Resp: 137926
 Ion Ratio Lower Upper
 164 100
 162 103.2 85.1 127.7
 160 45.0 34.7 52.1

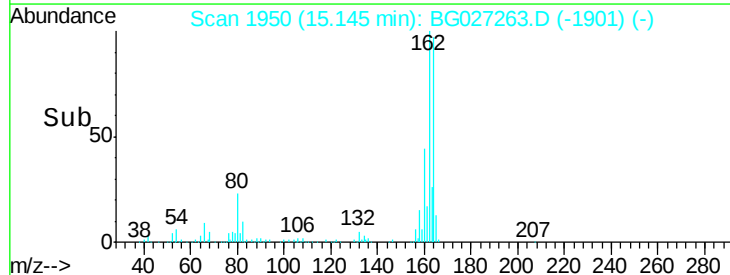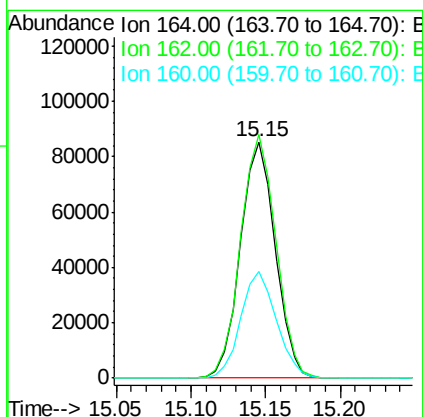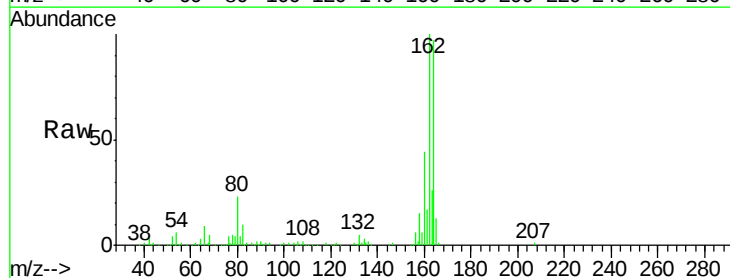







#41
 2,4,6-Tribromophenol
 Concen: 172.085 ng
 RT: 16.63 min Scan# 2202
 Delta R.T. -0.02 min
 Lab File: BG027263.D
 Acq: 7 Jun 2017 00:05

Instrument :
 BNA_G
 ClientSampleId :
 TP-8-9

Tgt Ion:330 Resp: 312549
 Ion Ratio Lower Upper
 330 100
 332 96.6 77.3 115.9
 141 32.5 32.1 48.1

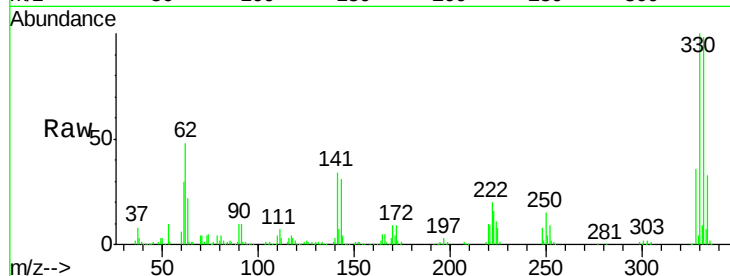


Abundance Ion 329.80 (329.50 to 330.50): E
 Ion 331.80 (331.50 to 332.50): E
 Ion 141.00 (140.70 to 141.70): E

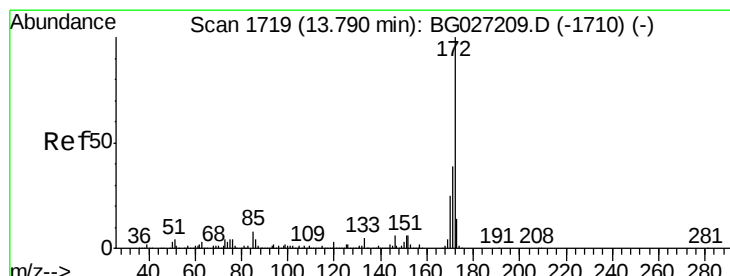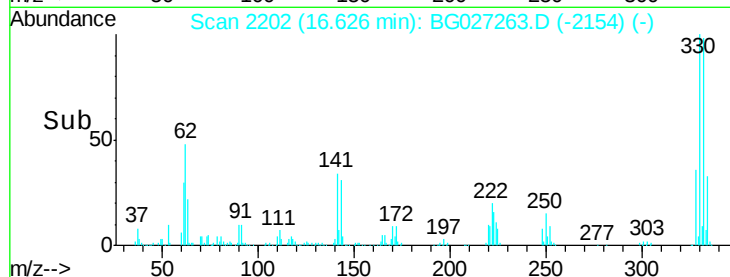
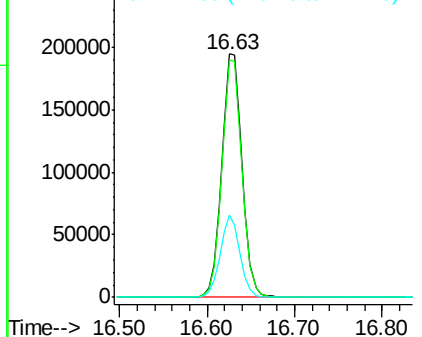


#44
 2-Fluorobiphenyl
 Concen: 97.069 ng
 RT: 13.77 min Scan# 1716
 Delta R.T. -0.02 min
 Lab File: BG027263.D
 Acq: 7 Jun 2017 00:05

Tgt Ion:172 Resp: 957007
 Ion Ratio Lower Upper
 172 100
 171 36.6 32.2 48.2
 170 24.8 21.8 32.6

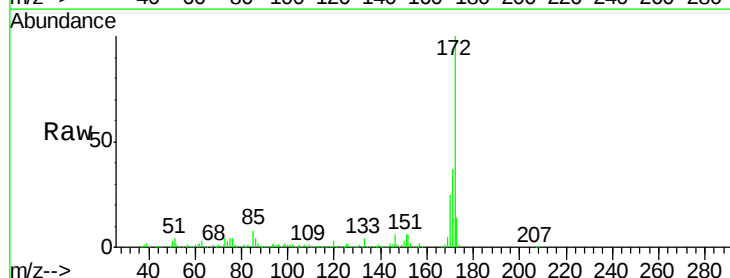

Abundance Ion 172.00 (171.70 to 172.70): E
 Ion 171.00 (170.70 to 171.70): E
 Ion 170.00 (169.70 to 170.70): E



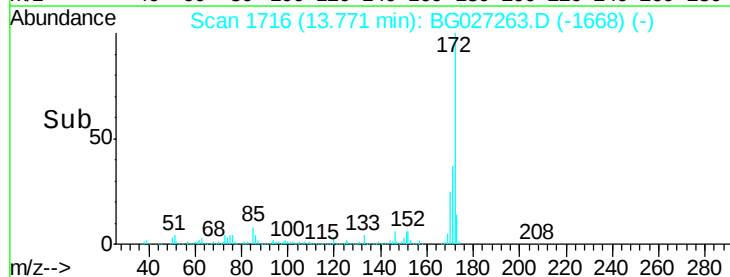
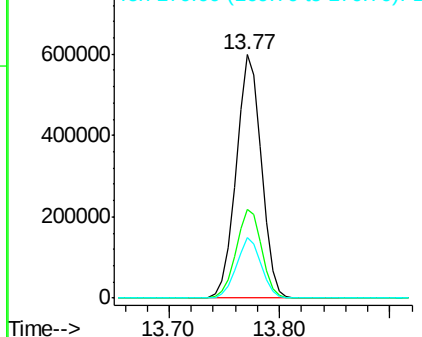




#63
Phenanthrene-d10
Concen: 20.000 ng
RT: 17.90 min Scan# 2418
Delta R.T. -0.02 min
Lab File: BG027263.D
Acq: 7 Jun 2017 00:05




Instrument :
BNA_G
ClientSampleId :
TP-8-9

Tgt Ion:188 Resp: 348999
Ion Ratio Lower Upper
188 100
94 10.0 5.8 8.8#
80 11.4 7.5 11.3#

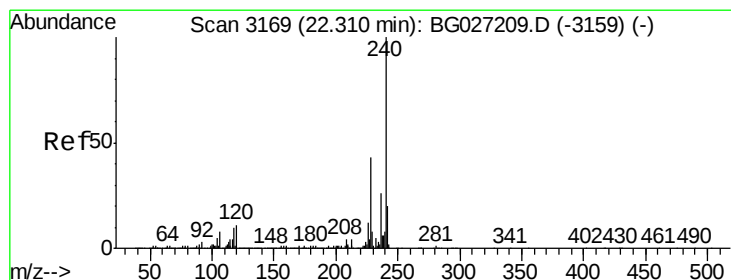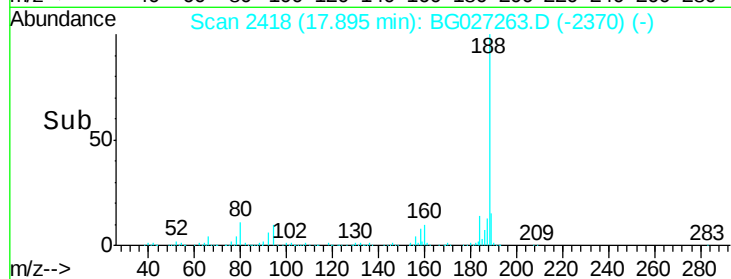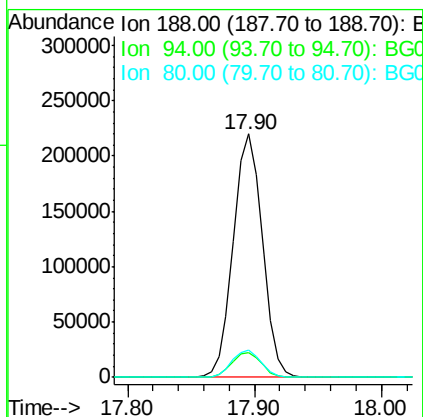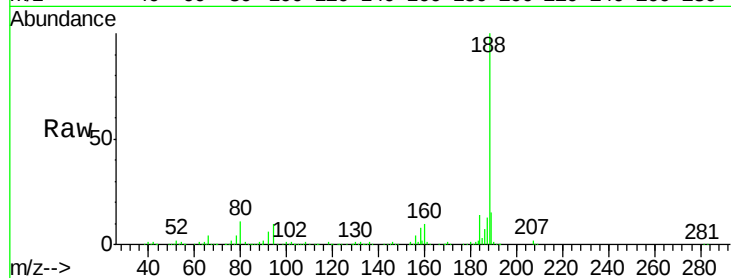

#75
Chrysene-d12
Concen: 20.000 ng
RT: 22.28 min Scan# 3164
Delta R.T. -0.03 min
Lab File: BG027263.D
Acq: 7 Jun 2017 00:05

Tgt Ion:240 Resp: 394150
Ion Ratio Lower Upper
240 100
120 11.3 5.7 8.5#
236 25.9 22.2 33.4

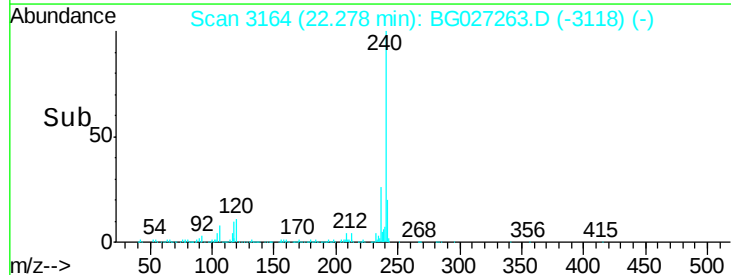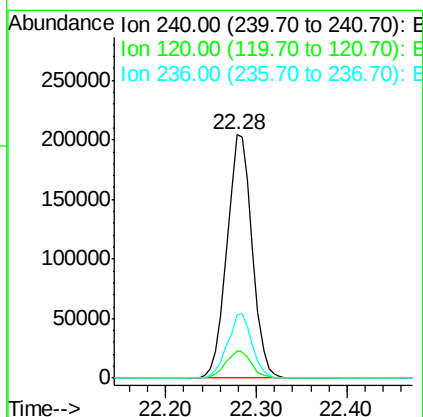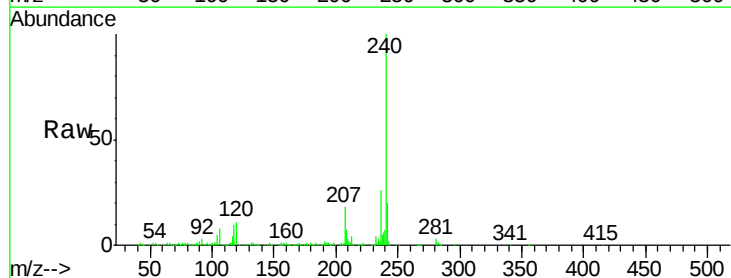



#78

Terphenyl-d14

Concen: 104.095 ng

RT: 20.47 min Scan# 2857

Delta R.T. -0.02 min

Lab File: BG027263.D

Acq: 7 Jun 2017 00:05

Instrument :

BNA_G

ClientSampleId :

TP-8-9


Tgt Ion:244 Resp: 1608349

Ion Ratio Lower Upper

244 100

212 8.0 10.0 15.0#




122 11.4 8.6 12.8

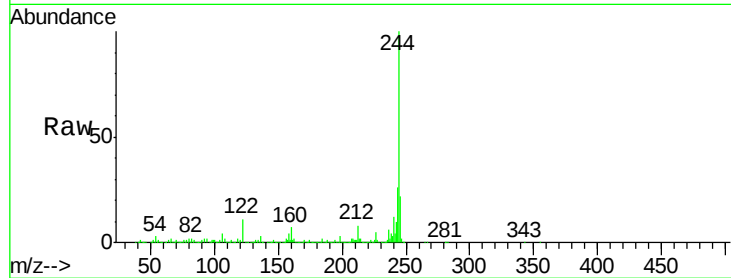

Abundance Ion 244.00 (243.70 to 244.70): E

Ion 212.00 (211.70 to 212.70): E

Ion 122.00 (121.70 to 122.70): E

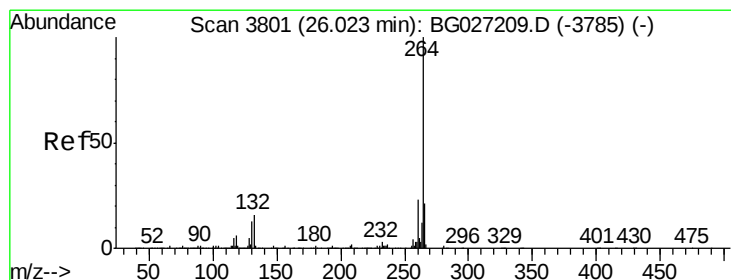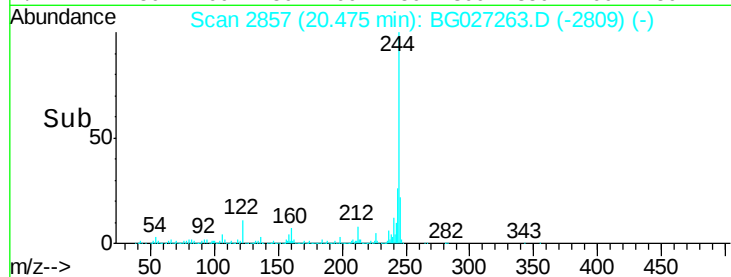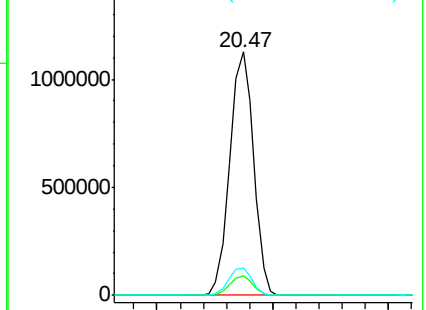

#86

Perylene-d12

Concen: 20.000 ng

RT: 25.97 min Scan# 3793

Delta R.T. -0.05 min

Lab File: BG027263.D

Acq: 7 Jun 2017 00:05


Tgt Ion:264 Resp: 362527

Ion Ratio Lower Upper

264 100

260 24.4 21.8 32.8

265 22.7 18.2 27.4

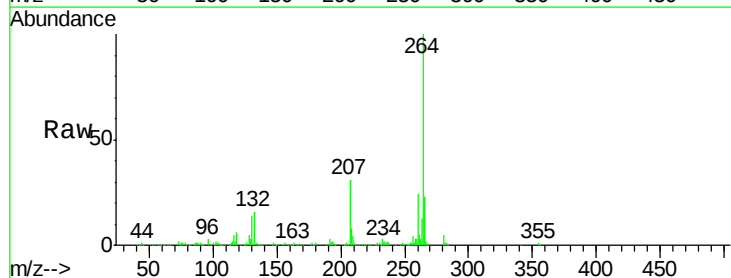

Abundance Ion 264.00 (263.70 to 264.70): E

Ion 260.00 (259.70 to 260.70): E

Ion 265.00 (264.70 to 265.70): E

