

Data Path : Z:\HPCHEM1\BNA_G\DATA\BG060617\
 Data File : BG027264.D
 Acq On : 7 Jun 2017 00:44
 Operator : SJ/MA
 Sample : I3466-02
 Misc :
 ALS Vial : 13 Sample Multiplier: 1

Instrument :
 BNA_G
 ClientSampleId :
 SU-RO-230-060217

Quant Time: Jun 07 06:55:41 2017
 Quant Method : Z:\HPCHEM1\BNA_G\METHODS\8270-BG060517.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Mon Jun 05 16:00:35 2017
 Response via : Initial Calibration


Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Dichlorobenzene-d4	8.56	152	52563	20.00	ng	-0.01
21) Naphthalene-d8	11.39	136	235570	20.00	ng	-0.01
38) Acenaphthene-d10	15.15	164	152643	20.00	ng	-0.01
63) Phenanthrene-d10	17.90	188	383023	20.00	ng	-0.02
75) Chrysene-d12	22.28	240	433236	20.00	ng	-0.03
86) Perylene-d12	25.98	264	404801	20.00	ng	-0.04
System Monitoring Compounds						
5) 2-Fluorophenol	6.15	112	480791	139.58	ng	0.00
7) Phenol-d6	7.70	99	613531	121.34	ng	0.00
23) Nitrobenzene-d5	9.73	82	395904	105.69	ng	-0.01
41) 2,4,6-Tribromophenol	16.63	330	336378	167.35	ng	-0.01
44) 2-Fluorobiphenyl	13.77	172	984348	90.22	ng	-0.02
78) Terphenyl-d14	20.47	244	1686576	99.31	ng	-0.02
Target Compounds						
31) Naphthalene	11.43	128	73266	5.691	ng	Qvalue 98


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\HPCHEM1\BNA_G\DATA\BG060617\
Data File : BG027264.D
Acq On : 7 Jun 2017 00:44
Operator : SJ/MA
Sample : I3466-02
Misc :
ALS Vial : 13 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
SU-RO-230-060217

Quant Time: Jun 07 06:55:41 2017
Quant Method : Z:\HPCHEM1\BNA_G\METHODS\8270-BG060517.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Mon Jun 05 16:00:35 2017
Response via : Initial Calibration

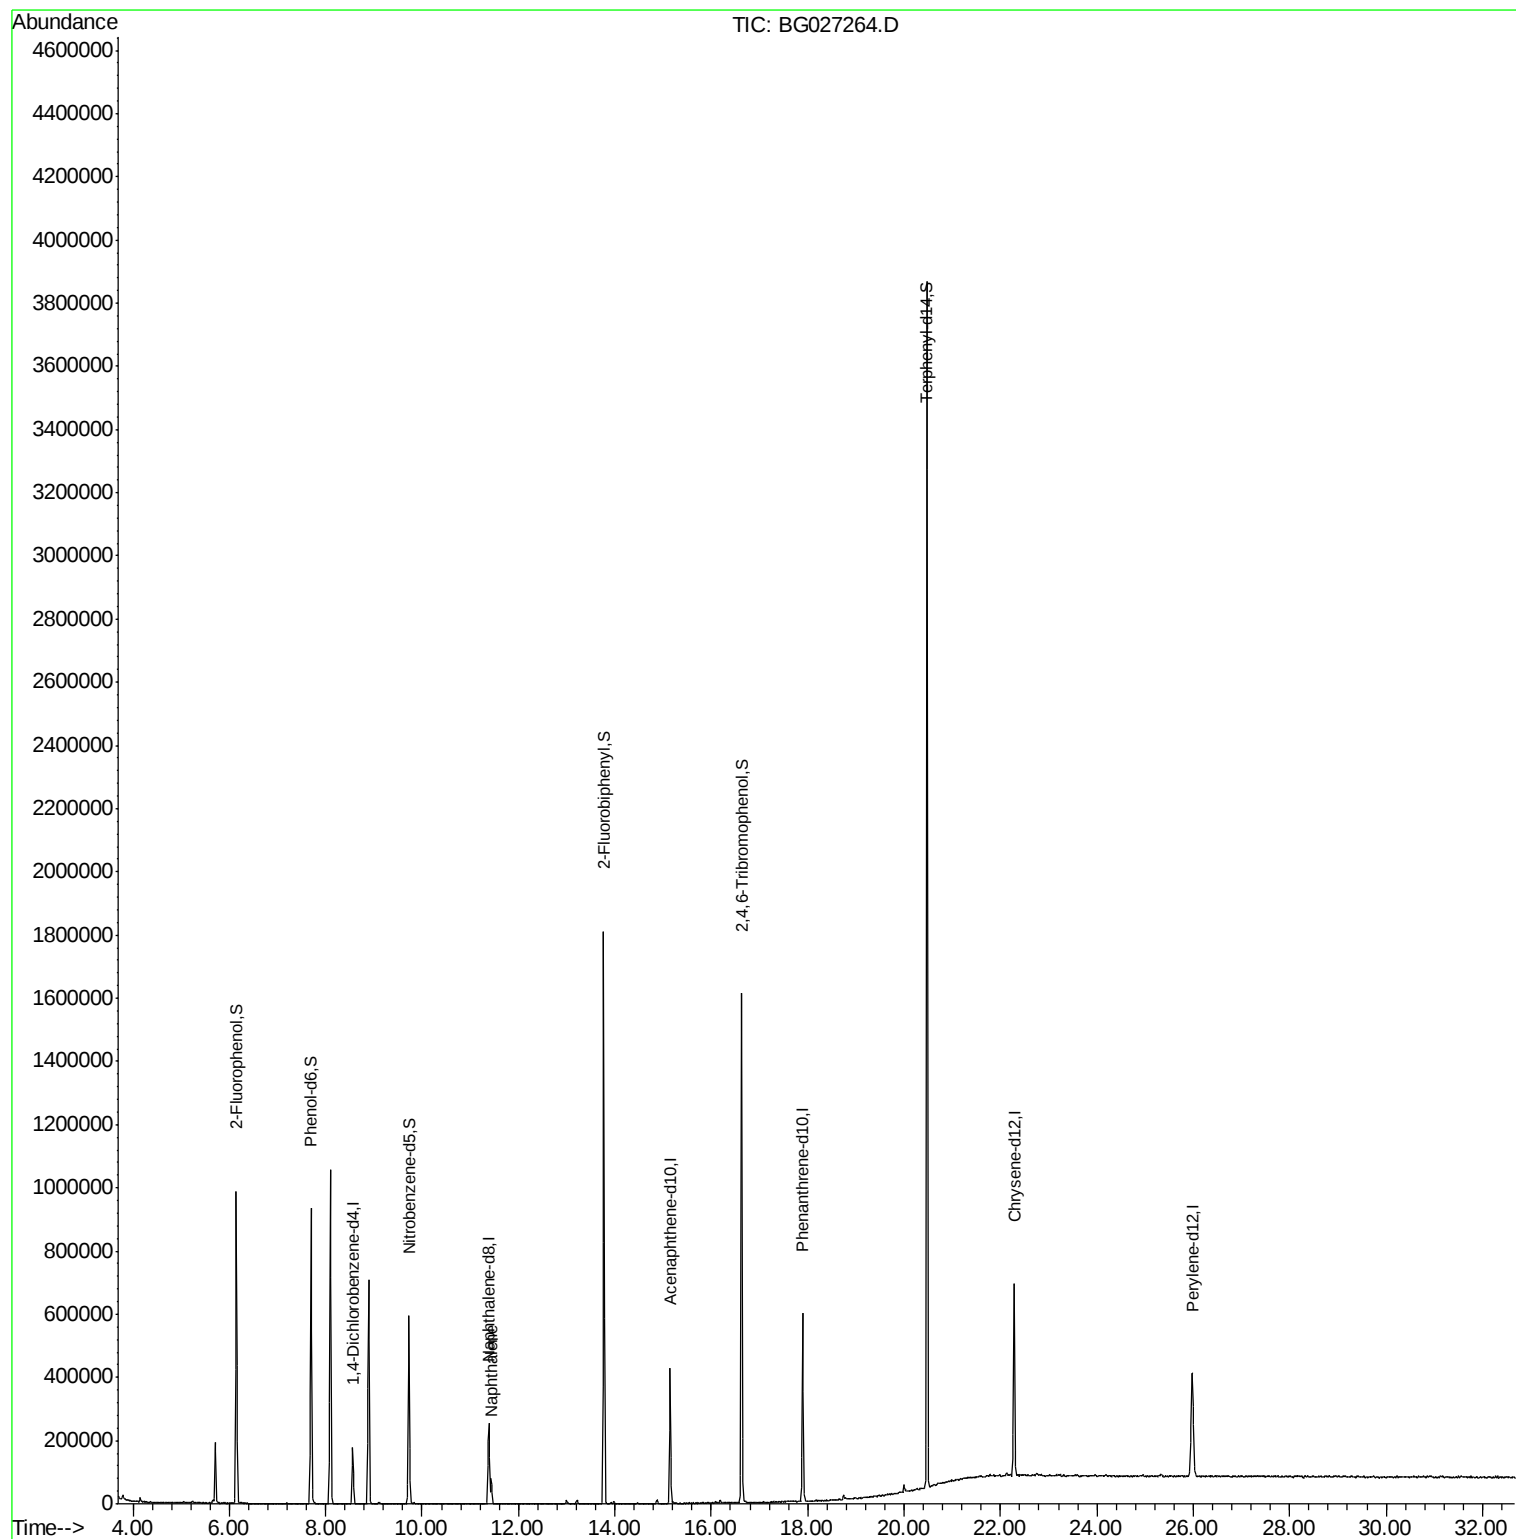

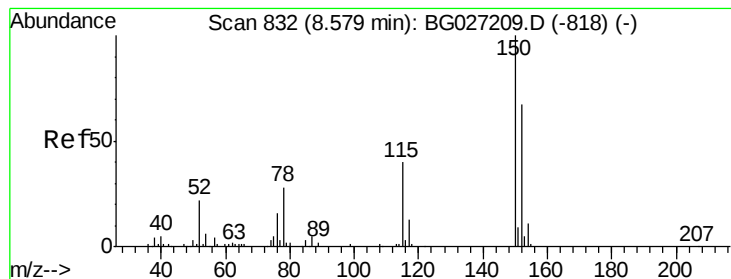


#1




1,4-Dichlorobenzene-d4
Concen: 20.000 ng
RT: 8.56 min Scan# 830
Delta R.T. -0.01 min
Lab File: BG027264.D
Acq: 7 Jun 2017 00:44

Instrument :
BNA_G
ClientSampleId :
SU-RO-230-060217

Tgt Ion:152 Resp: 52563
Ion Ratio Lower Upper
152 100
150 162.0 114.0 171.0
115 62.0 48.1 72.1

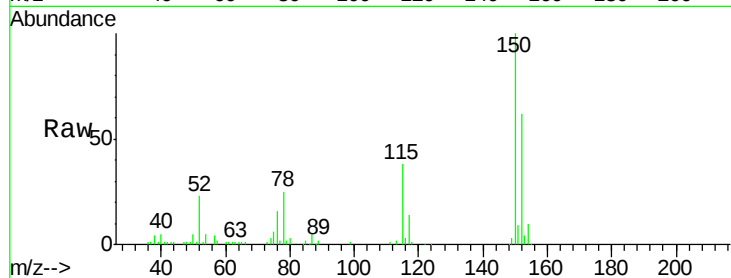


Abundance Ion 152.00 (151.70 to 152.70): E
Ion 150.00 (149.70 to 150.70): E
Ion 115.00 (114.70 to 115.70): E

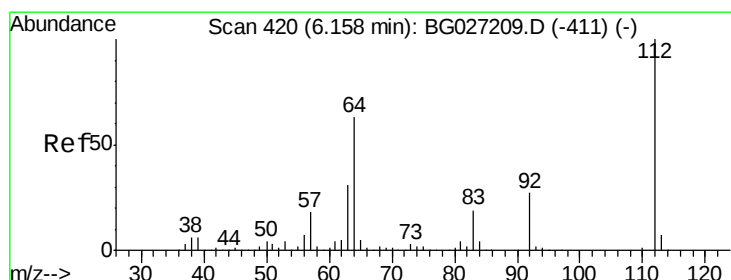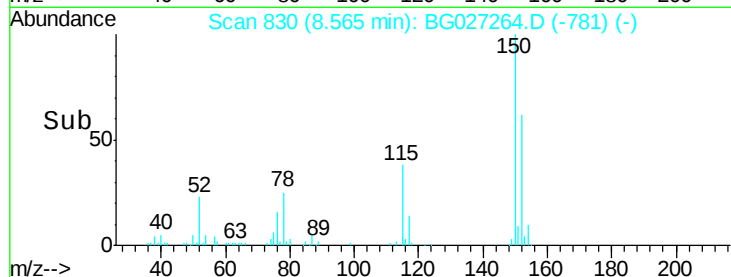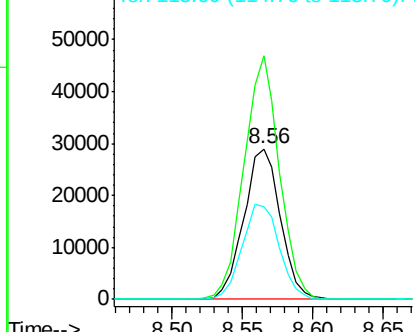



#5


2-Fluorophenol
Concen: 139.579 ng
RT: 6.15 min Scan# 419
Delta R.T. -0.01 min
Lab File: BG027264.D
Acq: 7 Jun 2017 00:44

Tgt Ion:112 Resp: 480791
Ion Ratio Lower Upper
112 100
64 63.6 61.8 92.6
63 33.0 37.2 55.8#

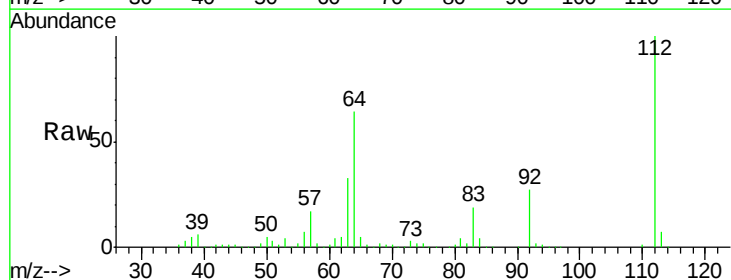

Abundance Ion 112.00 (111.70 to 112.70): E
Ion 64.00 (63.70 to 64.70): BGC
Ion 63.00 (62.70 to 63.70): BGC

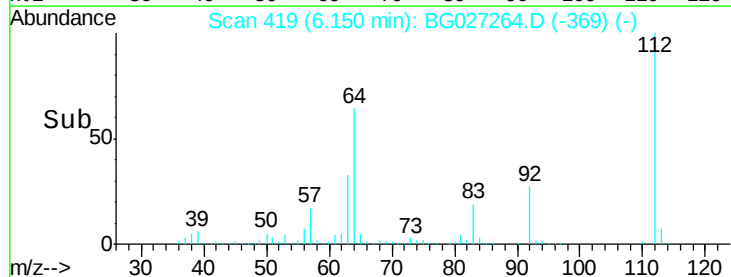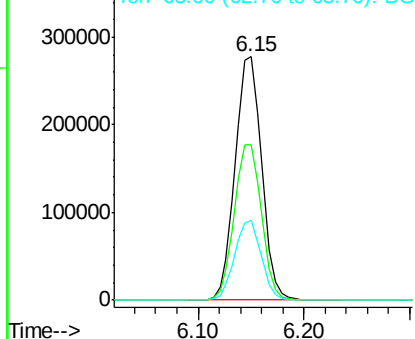

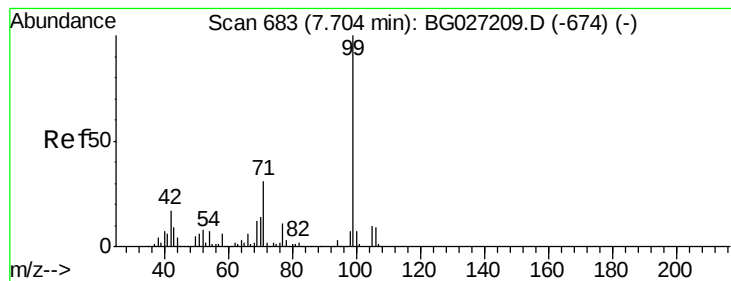

#7

Phenol-d6

Concen: 121.341 ng

RT: 7.70 min Scan# 682

Delta R.T. -0.01 min

Lab File: BG027264.D

Acq: 7 Jun 2017 00:44

Instrument :

BNA_G

ClientSampleId :

SU-RO-230-060217


Tgt Ion: 99 Resp: 613531

Ion Ratio Lower Upper




99 100

42 16.9 20.5 30.7#

71 31.0 37.6 56.4#

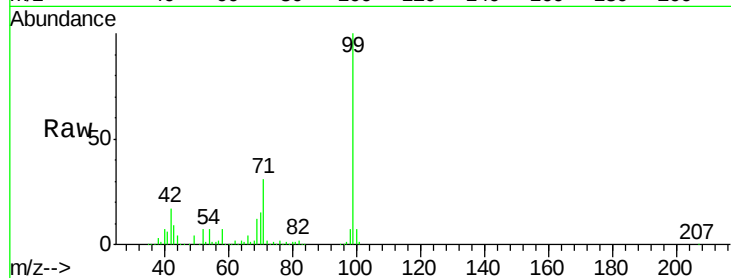

Abundance Ion 99.00 (98.70 to 99.70): BGC
Ion 42.00 (41.70 to 42.70): BGC
Ion 71.00 (70.70 to 71.70): BGC

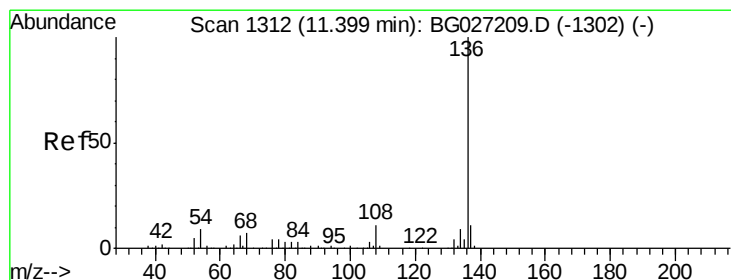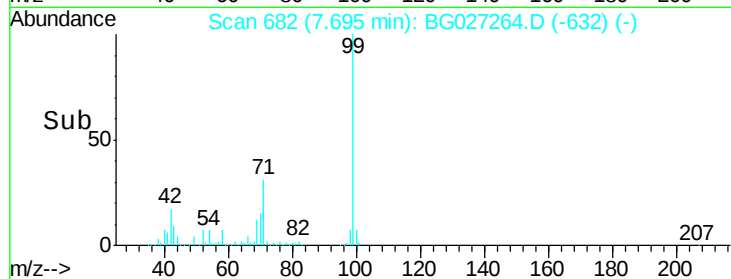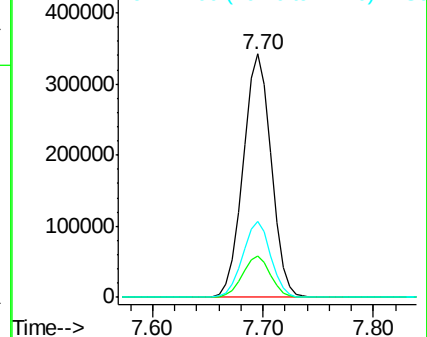

#21

Naphthalene-d8

Concen: 20.000 ng

RT: 11.39 min Scan# 1310

Delta R.T. -0.01 min

Lab File: BG027264.D

Acq: 7 Jun 2017 00:44

Tgt Ion: 136 Resp: 235570


Ion Ratio Lower Upper

136 100



137 10.9 8.9 13.3


54 9.7 9.3 13.9

68 7.5 5.1 7.7

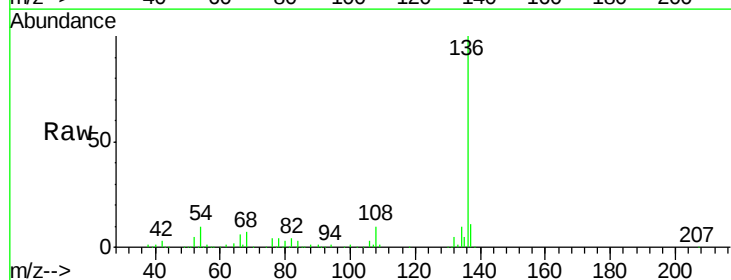

Abundance Ion 136.00 (135.70 to 136.70): BGC
Ion 137.00 (136.70 to 137.70): BGC
Ion 54.00 (53.70 to 54.70): BGC
Ion 68.00 (67.70 to 68.70): BGC

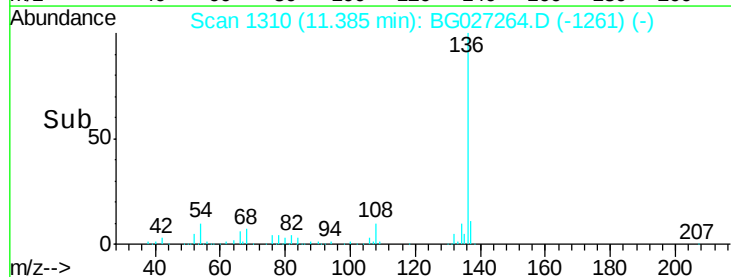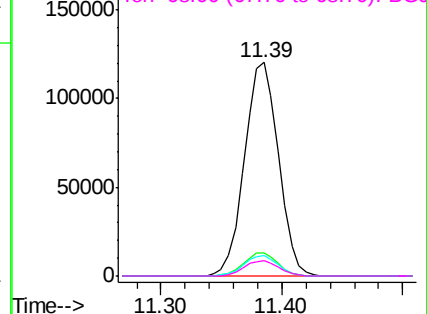







#23
Nitrobenzene-d5
Concen: 105.694 ng
RT: 9.73 min Scan# 1028
Delta R.T. -0.01 min
Lab File: BG027264.D
Acq: 7 Jun 2017 00:44

Instrument :
BNA_G
ClientSampleId :
SU-RO-230-060217

Tgt Ion: 82 Resp: 395904
Ion Ratio Lower Upper
82 100
128 42.3 26.4 39.6#
54 49.8 49.4 74.2

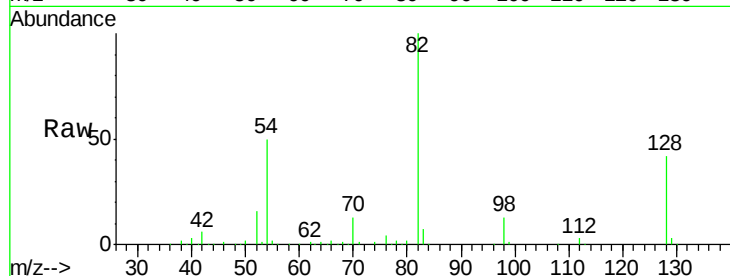


Abundance Ion 82.00 (81.70 to 82.70): BGC
Ion 128.00 (127.70 to 128.70): BGC
Ion 54.00 (53.70 to 54.70): BGC


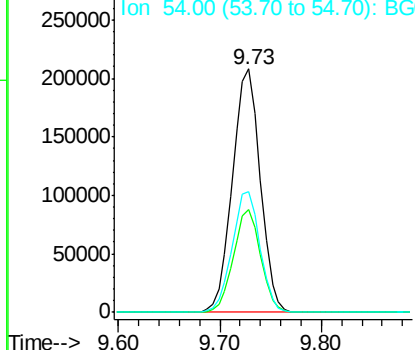



#31
Naphthalene
Concen: 5.691 ng
RT: 11.43 min Scan# 1318
Delta R.T. -0.02 min
Lab File: BG027264.D
Acq: 7 Jun 2017 00:44

Tgt Ion: 128 Resp: 73266
Ion Ratio Lower Upper
128 100
129 11.8 9.3 13.9
127 13.1 11.4 17.0



Abundance Ion 128.00 (127.70 to 128.70): BGC
Ion 129.00 (128.70 to 129.70): BGC
Ion 127.00 (126.70 to 127.70): BGC

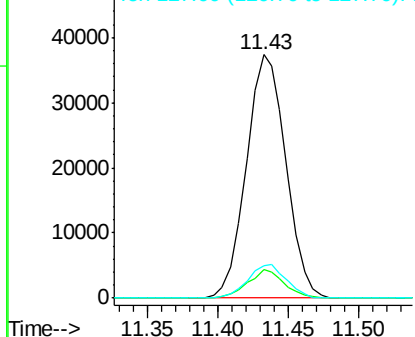



#38

Acenaphthene-d10

Concen: 20.000 ng

RT: 15.15 min Scan# 1950

Delta R.T. -0.01 min

Lab File: BG027264.D

Acq: 7 Jun 2017 00:44

Instrument :

BNA_G

ClientSampleId :

SU-RO-230-060217


Tgt Ion:164 Resp: 152643

Ion Ratio Lower Upper

164 100

162 102.7 85.1 127.7




160 43.4 34.7 52.1



Abundance Ion 164.00 (163.70 to 164.70): E

Ion 162.00 (161.70 to 162.70): E

Ion 160.00 (159.70 to 160.70): E

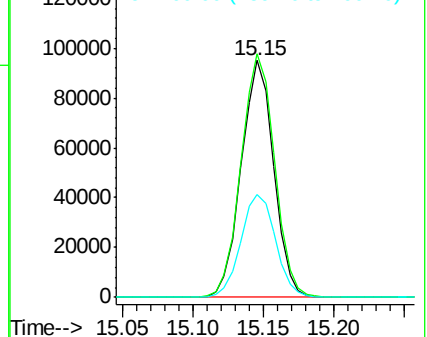

#41

2,4,6-Tribromophenol

Concen: 167.349 ng

RT: 16.63 min Scan# 2203

Delta R.T. -0.01 min

Lab File: BG027264.D

Acq: 7 Jun 2017 00:44


Tgt Ion:330 Resp: 336378

Ion Ratio Lower Upper

330 100

332 96.2 77.3 115.9



141 32.7 32.1 48.1




Abundance Ion 329.80 (329.50 to 330.50): E

Ion 331.80 (331.50 to 332.50): E

Ion 141.00 (140.70 to 141.70): E

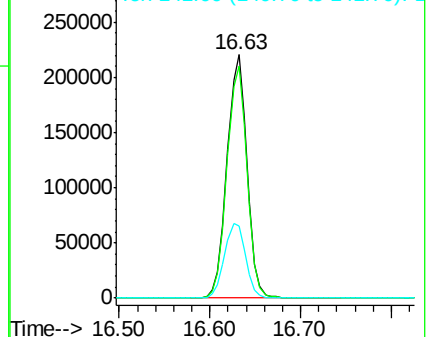



#44

2-Fluorobiphenyl

Concen: 90.216 ng

RT: 13.77 min Scan# 1716

Delta R.T. -0.02 min

Lab File: BG027264.D

Acq: 7 Jun 2017 00:44

Instrument :

BNA_G

ClientSampleId :

SU-RO-230-060217


Tgt Ion:172 Resp: 984348

Ion Ratio Lower Upper

172 100

171 37.7 32.2 48.2




170 25.2 21.8 32.6



Abundance Ion 172.00 (171.70 to 172.70): E

Ion 171.00 (170.70 to 171.70): E

Ion 170.00 (169.70 to 170.70): E

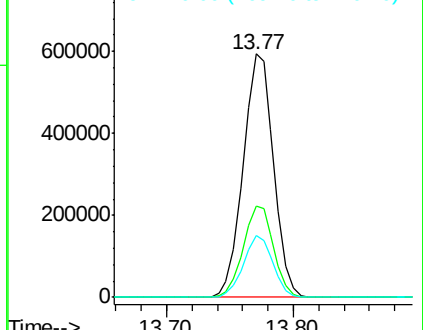

#63

Phenanthrene-d10

Concen: 20.000 ng

RT: 17.90 min Scan# 2418

Delta R.T. -0.02 min

Lab File: BG027264.D

Acq: 7 Jun 2017 00:44


Tgt Ion:188 Resp: 383023

Ion Ratio Lower Upper

188 100

94 10.4 5.8 8.8#



80 12.0 7.5 11.3#




Abundance Ion 188.00 (187.70 to 188.70): E

Ion 94.00 (93.70 to 94.70): BG0

Ion 80.00 (79.70 to 80.70): BG0




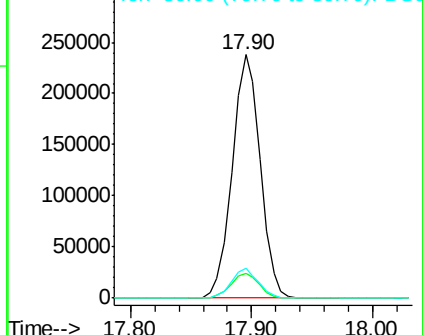


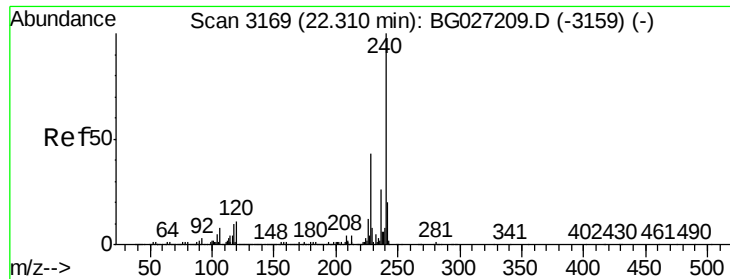

#75
 Chrysene-d12
 Concen: 20.000 ng
 RT: 22.28 min Scan# 3165
 Delta R.T. -0.03 min
 Lab File: BG027264.D
 Acq: 7 Jun 2017 00:44




Instrument :
 BNA_G
 ClientSampleId :
 SU-RO-230-060217


Tgt Ion:240 Resp: 433236
 Ion Ratio Lower Upper
 240 100
 120 10.5 5.7 8.5#
 236 26.0 22.2 33.4

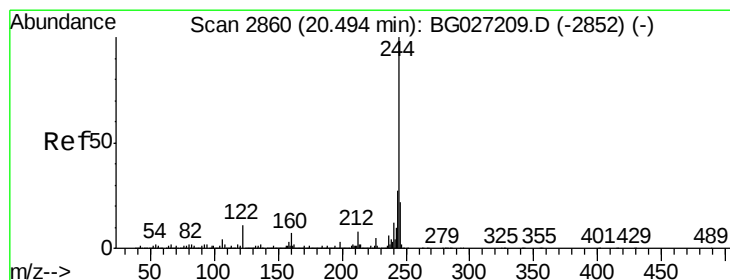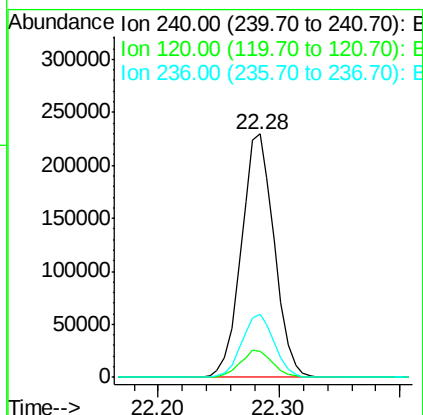

#78
 Terphenyl-d14
 Concen: 99.310 ng
 RT: 20.47 min Scan# 2857
 Delta R.T. -0.02 min
 Lab File: BG027264.D
 Acq: 7 Jun 2017 00:44

Tgt Ion:244 Resp: 1686576
 Ion Ratio Lower Upper
 244 100
 212 8.2 10.0 15.0#
 122 11.7 8.6 12.8

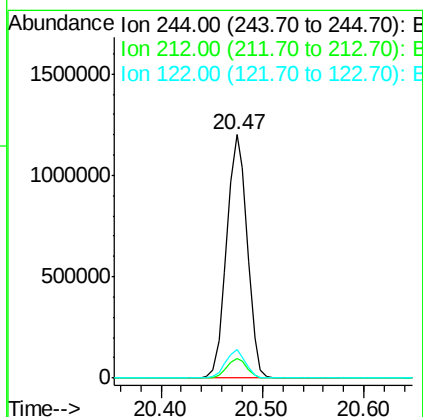


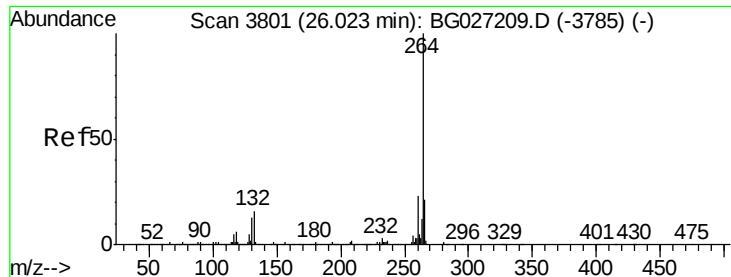

#86
Perylene-d12
Concen: 20.000 ng
RT: 25.98 min Scan# 3794
Delta R.T. -0.04 min
Lab File: BG027264.D
Acq: 7 Jun 2017 00:44

Instrument :
BNA_G
ClientSampleId :
SU-RO-230-060217

Tgt Ion	Ratio	Lower	Upper
264	100		
260	23.9	21.8	32.8
265	21.0	18.2	27.4

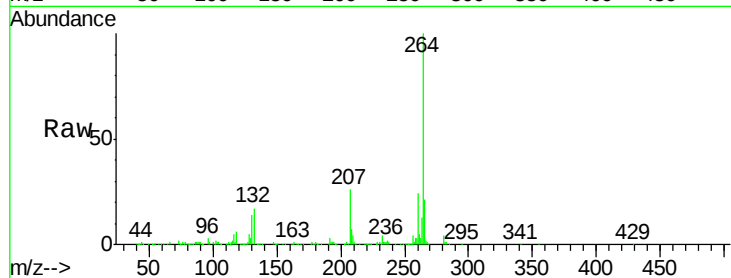

Abundance

Ion 264.00 (263.70 to 264.70): E

Ion 260.00 (259.70 to 260.70): E

Ion 265.00 (264.70 to 265.70): E

