


Data Path : Z:\HPCHEM1\BNA_G\Data\BG060617\
 Data File : BG027238.D
 Acq On : 6 Jun 2017 7:41
 Operator : SJ/MA
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_G
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\HPCHEM1\BNA_G\METHODS\8270-BG060517.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Mon Jun 05 16:00:35 2017

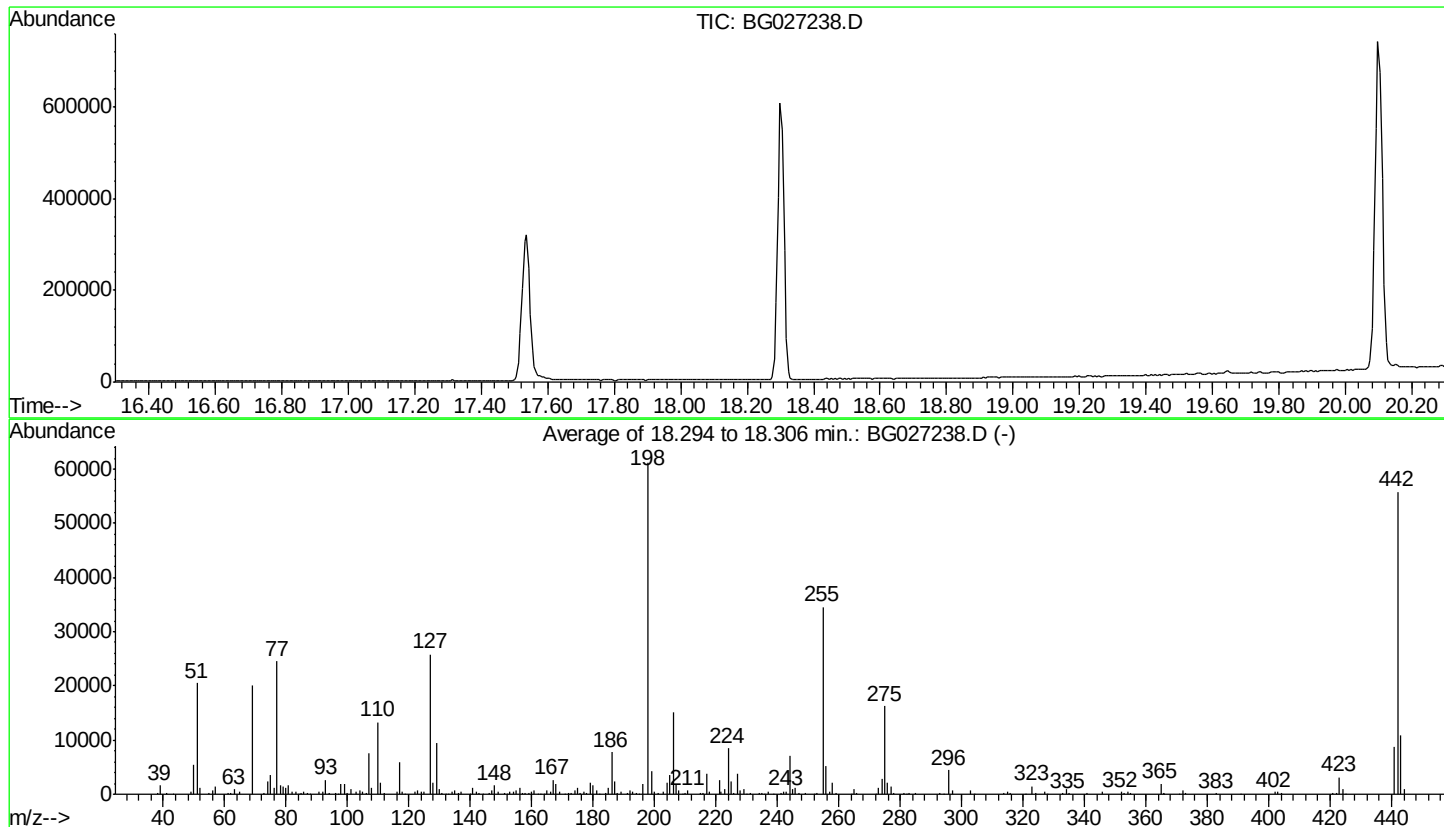

AutoFind: Scans 2486, 2487, 2488; Background Corrected with Scan 2480

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	33.5	20474	PASS
68	69	0.00	2	0.0	0	PASS
69	198	0.00	100	32.7	20013	PASS
70	69	0.00	2	0.0	0	PASS
127	198	10	80	42.2	25818	PASS
197	198	0.00	2	0.0	0	PASS
198	198	100	100	100.0	61184	PASS
199	198	5	9	6.9	4235	PASS
275	198	10	60	26.5	16211	PASS
365	198	1	100	3.3	2013	PASS
441	442	0.01	24	15.8	8798	PASS
442	198	50	100	91.3	55856	PASS
443	442	15	24	19.6	10928	PASS