


Data Path : Z:\HPCHEM1\BNA_G\Data\BG060617\
 Data File : BG027252.D
 Acq On : 6 Jun 2017 16:53
 Operator : SJ/MA
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_G
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\HPCHEM1\BNA_G\METHODS\8270-BG060517.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Mon Jun 05 16:00:35 2017

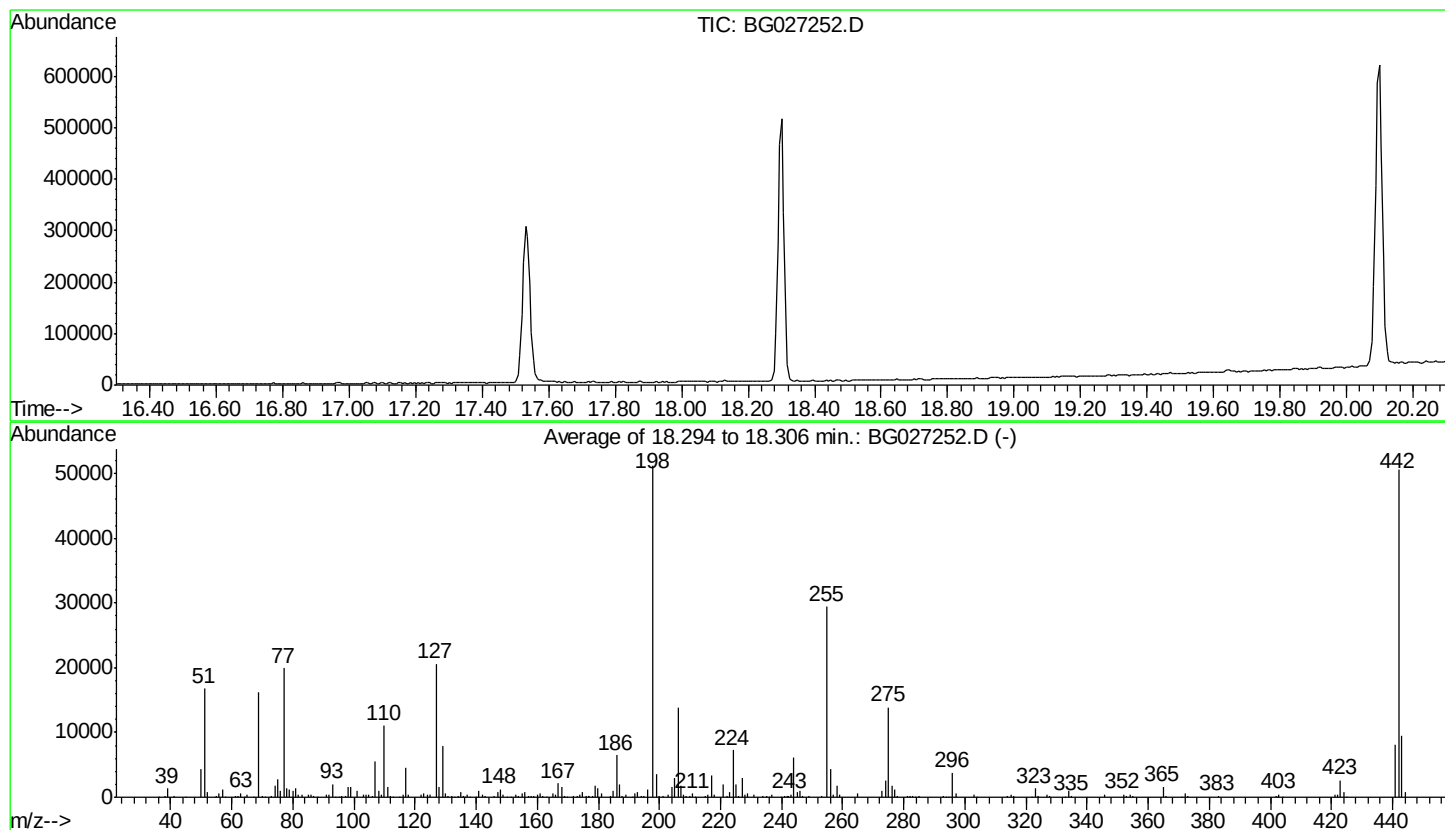

AutoFind: Scans 2486, 2487, 2488; Background Corrected with Scan 2479

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	32.8	16786	PASS
68	69	0.00	2	0.0	0	PASS
69	198	0.00	100	31.6	16212	PASS
70	69	0.00	2	1.0	157	PASS
127	198	10	80	40.3	20628	PASS
197	198	0.00	2	0.0	0	PASS
198	198	100	100	100.0	51224	PASS
199	198	5	9	6.9	3550	PASS
275	198	10	60	27.1	13859	PASS
365	198	1	100	3.2	1663	PASS
441	442	0.01	24	16.1	8130	PASS
442	198	50	100	98.7	50562	PASS
443	442	15	24	18.8	9481	PASS