


Data Path : Z:\HPCHEM1\BNA_G\Data\BG060617\
 Data File : BG027271.D
 Acq On : 7 Jun 2017 6:04
 Operator : SJ/MA
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_G
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\HPCHEM1\BNA_G\METHODS\8270-BG060517.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Mon Jun 05 16:00:35 2017

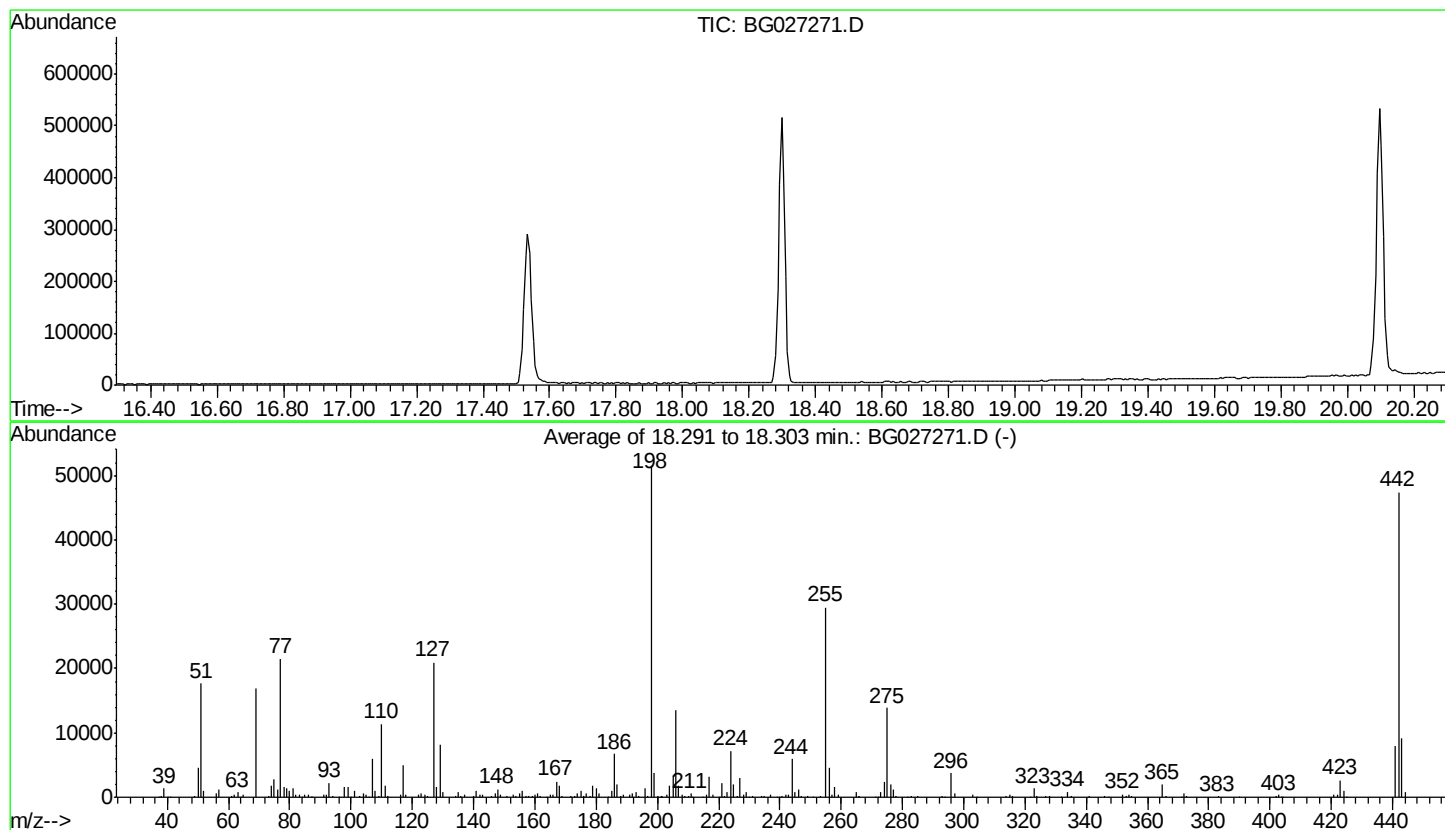

AutoFind: Scans 2485, 2486, 2487; Background Corrected with Scan 2478

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	34.2	17617	PASS
68	69	0.00	2	0.0	0	PASS
69	198	0.00	100	32.8	16912	PASS
70	69	0.00	2	0.0	0	PASS
127	198	10	80	40.6	20896	PASS
197	198	0.00	2	0.3	162	PASS
198	198	100	100	100.0	51512	PASS
199	198	5	9	7.2	3712	PASS
275	198	10	60	26.9	13861	PASS
365	198	1	100	3.8	1967	PASS
441	442	0.01	24	17.0	8031	PASS
442	198	50	100	91.9	47360	PASS
443	442	15	24	19.3	9125	PASS