
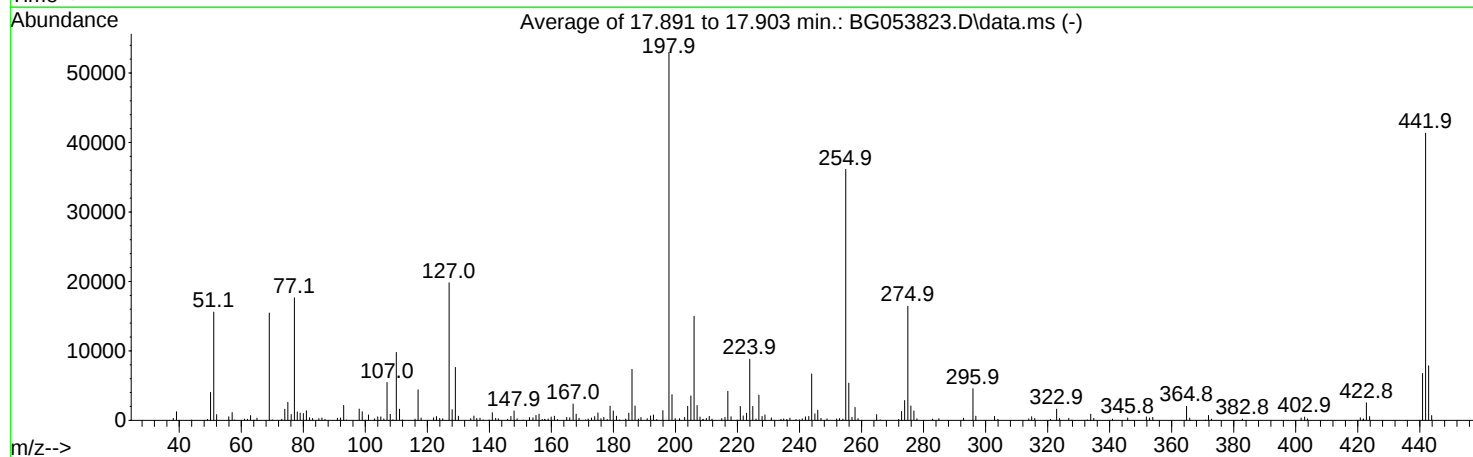


Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG060622\
 Data File : BG053823.D
 Acq On : 6 Jun 2022 10:23
 Operator : CG/JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_G
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\8270-BG060222.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Thu Jun 02 23:22:27 2022

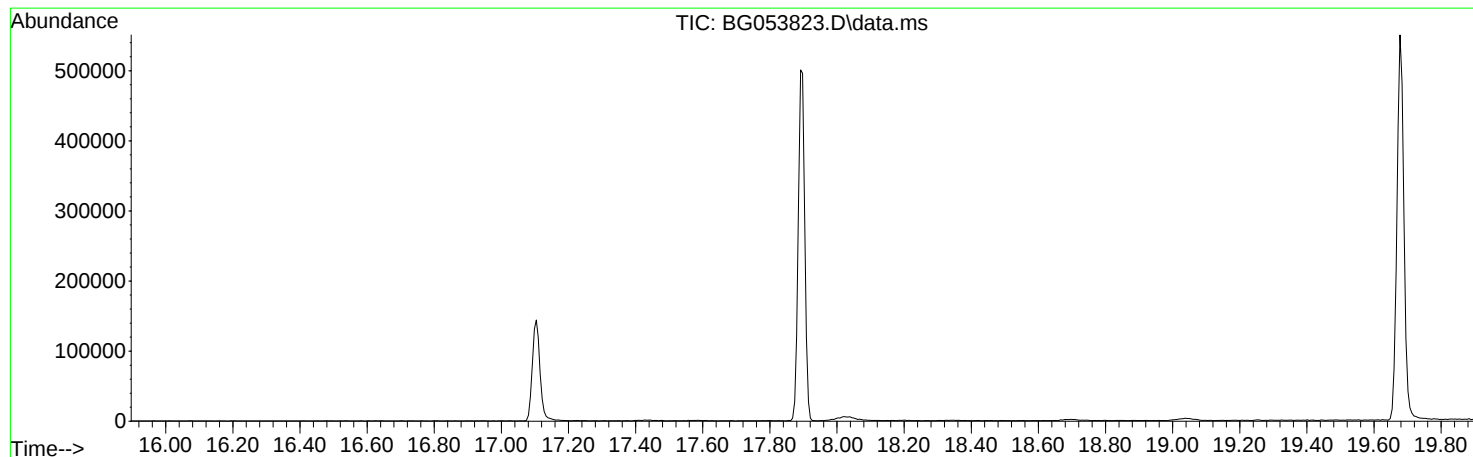




AutoFind: Scans 2468, 2469, 2470; Background Corrected with Scan 2461

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	29.4	15588	PASS
68	69	0.00	2	0.0	0	PASS
69	198	0.00	100	29.2	15446	PASS
70	69	0.00	2	0.5	71	PASS
127	198	10	80	37.4	19809	PASS
197	198	0.00	2	0.0	0	PASS
198	198	100	100	100.0	52957	PASS
199	198	5	9	7.0	3712	PASS
275	198	10	60	31.0	16434	PASS
365	198	1	100	3.8	2029	PASS
441	198	0.01	100	12.8	6760	PASS
442	442	50	100	100.0	41352	PASS
443	442	15	24	19.0	7852	PASS

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG060622\
Data File : BG053823.D
Acq On : 6 Jun 2022 10:23
Operator : CG/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
DFTPP

Quant Time: Jun 07 06:16:23 2022
Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\8270-BG060222.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Thu Jun 02 23:22:27 2022
Response via : Initial Calibration

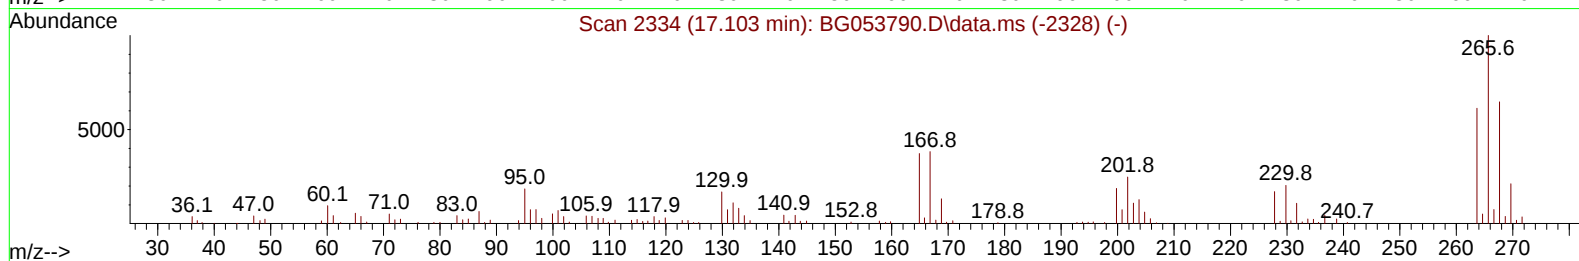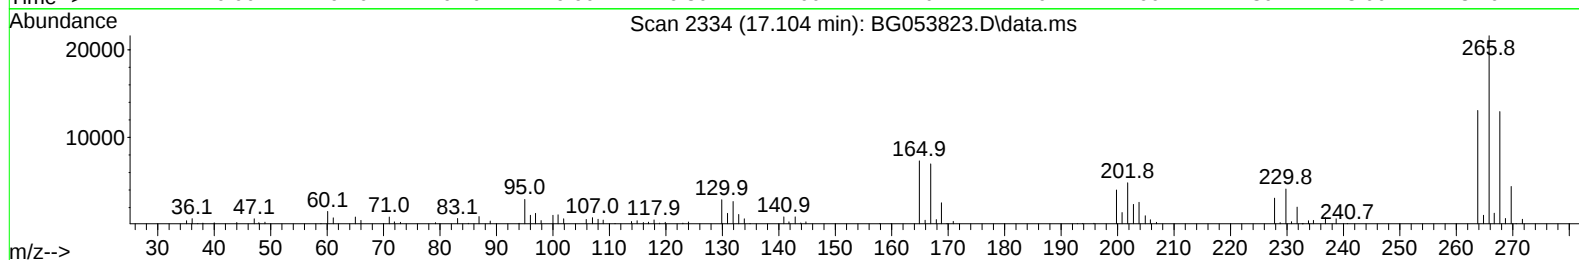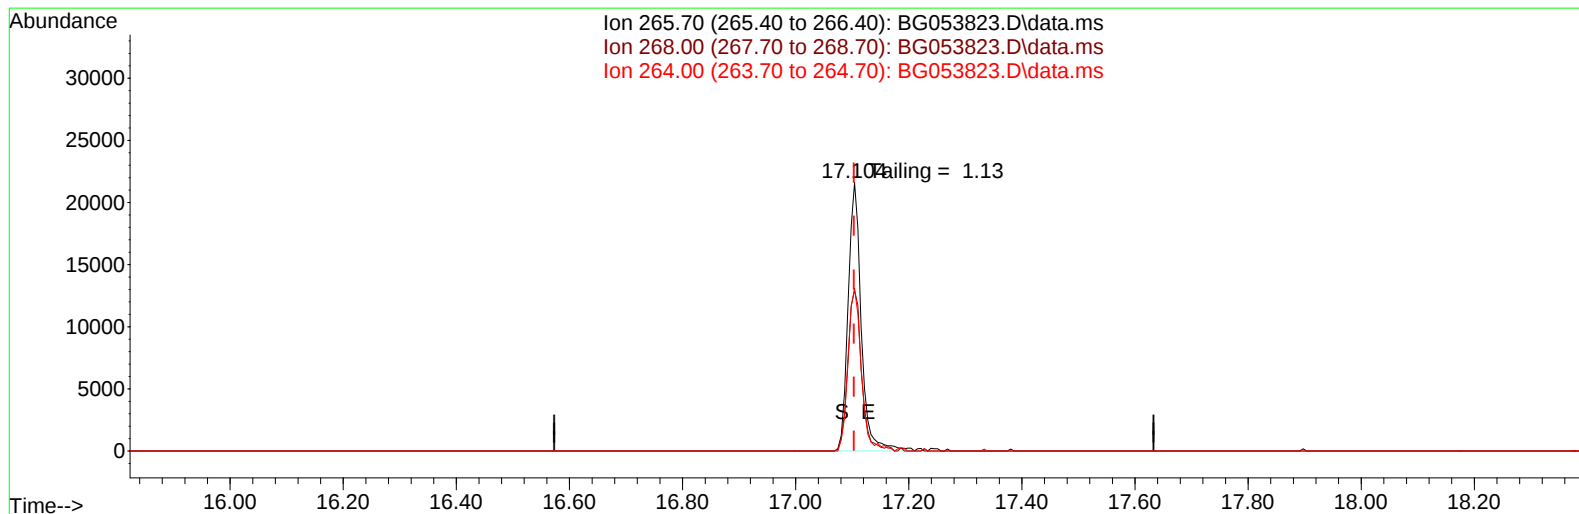

TIC: BG053823.D\data.ms

(70) Pentachlorophenol (C)

17.104min (+ 0.001) 14461.07 ng




response 34954

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	70.20	63.45
264.00	66.20	60.56
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG060622\
Data File : BG053823.D
Acq On : 6 Jun 2022 10:23
Operator : CG/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
DFTPP

Quant Time: Jun 07 06:16:23 2022
Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\8270-BG060222.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Thu Jun 02 23:22:27 2022
Response via : Initial Calibration

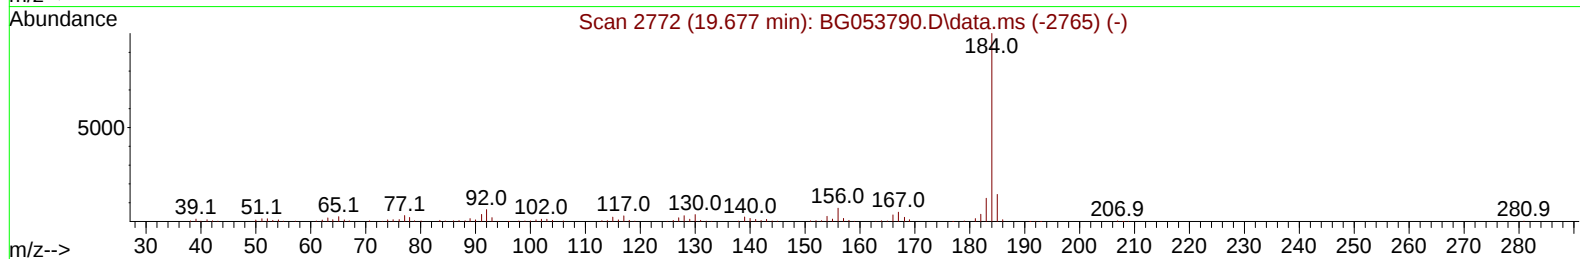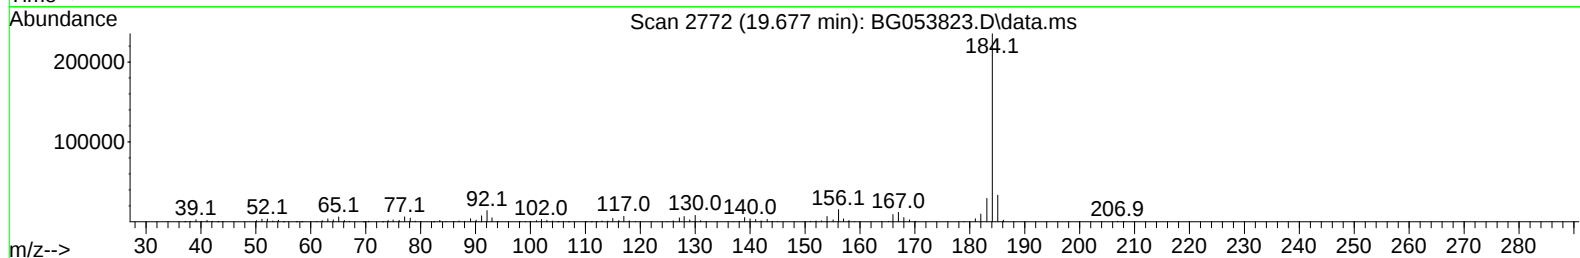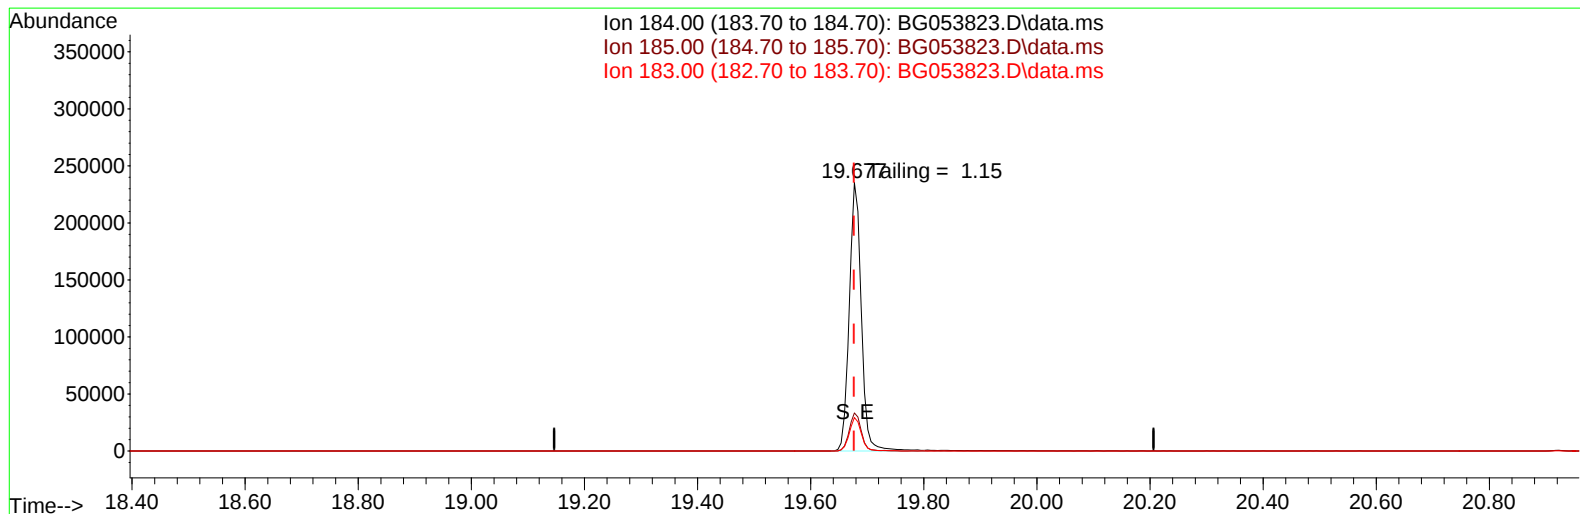

TIC: BG053823.D\data.ms

(77) Benzidine

19.677min (+ 0.001) 0.00 ng

response 347802

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	14.70	14.19
183.00	11.10	12.49
0.00	0.00	0.00

DDT Breakdown

Date	Instrument Name	DFTPP Data File
6/6/2022	BNA_G	<u>BG053823.D</u>
Compound Name	Response	Retention Time
DDT	118878	20.923
DDD	955	20.477
DDE	128	19.971
SUM(DDD+DDE)	SUM(DDT+DDD+DDE)	% Breakdown Of DDT
1083	119961	0.90

Instrument :
BNA_G
ClientSampleId :
DFTPP