

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG060624\
Data File : BG061519.D
Acq On : 6 Jun 2024 21:09
Operator : MA/JU
Sample : P2739-02
Misc :
ALS Vial : 7 Sample Multiplier: 1




Instrument :
BNA_G
ClientSampleId :
E0005

Manual IntegrationsAPPROVED

Reviewed By :Jagrut Upadhyay 06/07/2024
Supervised By :mohammad ahmed 06/08/2024

Supervised By :mohammad
ahmed
06/08/2024

Quant Time: Jun 06 22:44:51 2024
Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\SFAM-EPA-BG052124.MA.M
Quant Title : SVOA CALIBRATION
QLast Update : Thu Jun 06 12:15:45 2024
Response via : Initial Calibration

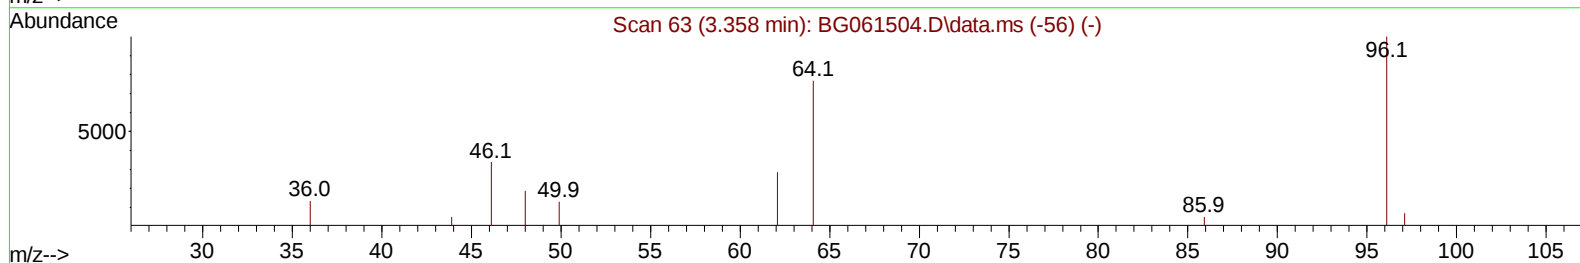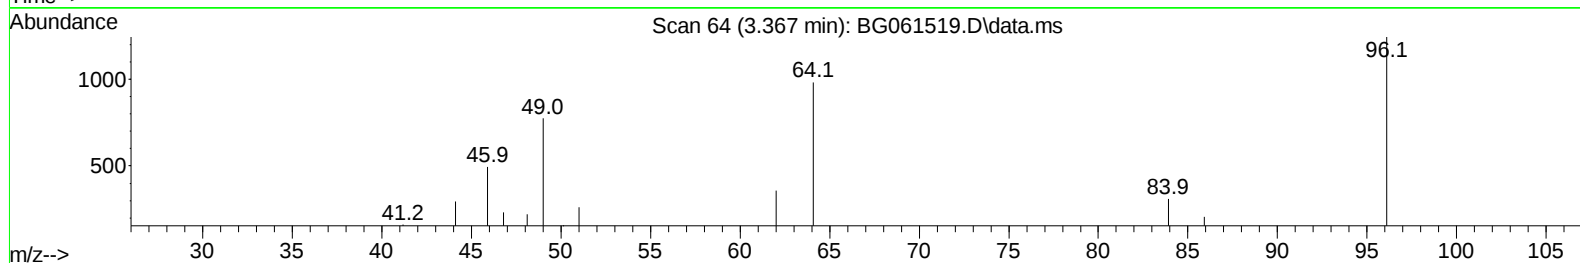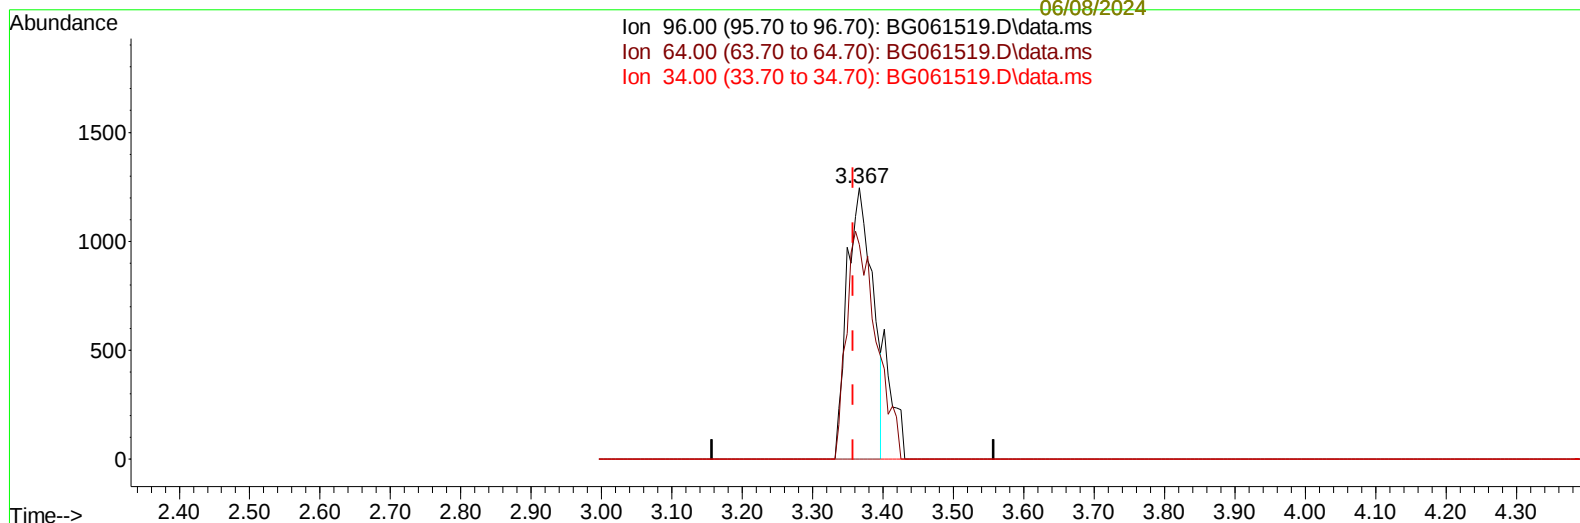

TIC: BG061519.D\data.ms

(3) 1,4-Dioxane-d8 (S)

3.367min (+ 0.009) 5.86 ng/uL

response 3123

Ion	Exp%	Act%
96.00	100.00	100.00
64.00	91.80	79.04
34.00	0.00	0.00
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG060624\
Data File : BG061519.D
Acq On : 6 Jun 2024 21:09
Operator : MA/JU
Sample : P2739-02
Misc :
ALS Vial : 7 Sample Multiplier: 1




Instrument :
BNA_G
ClientSampleId :
E0005

Manual IntegrationsAPPROVED

Reviewed By :Jagrut Upadhyay 06/07/2024
Supervised By :mohammad ahmed 06/08/2024

Supervised By :mohammad
ahmed
06/08/2024

Quant Time: Jun 06 22:44:51 2024
Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\SFAM-EPA-BG052124.MA.M
Quant Title : SVOA CALIBRATION
QLast Update : Thu Jun 06 12:15:45 2024
Response via : Initial Calibration

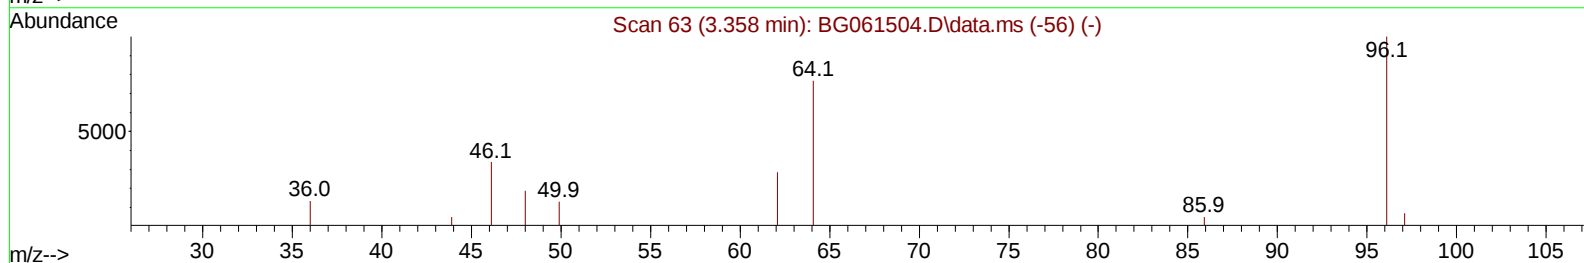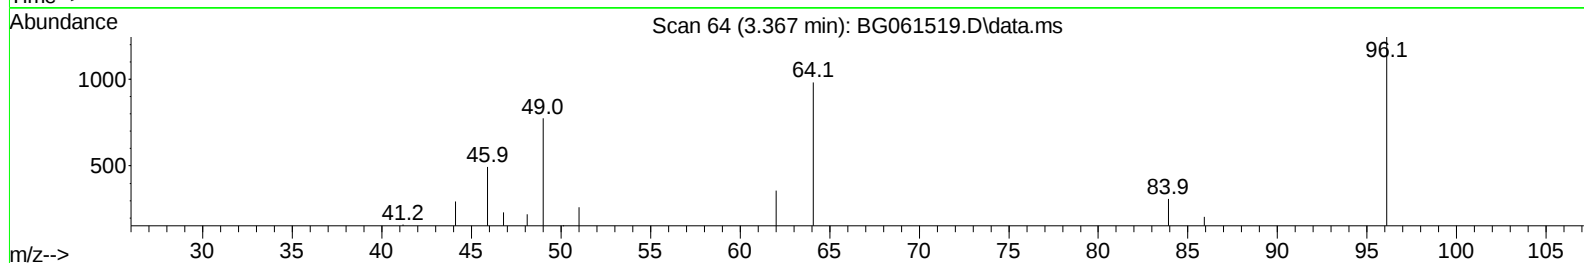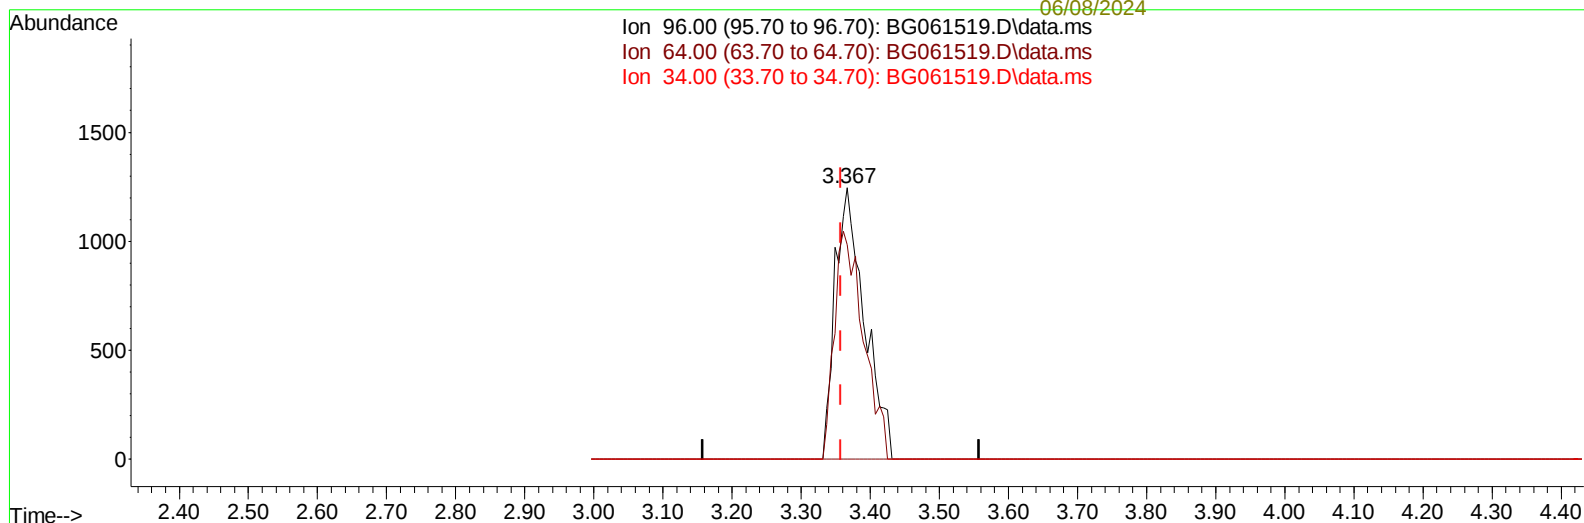

TIC: BG061519.D\data.ms

(3) 1,4-Dioxane-d8 (S)

3.367min (+ 0.009) 6.97 ng/uL m

response 3715

Ion	Exp%	Act%
96.00	100.00	100.00
64.00	91.80	79.04
34.00	0.00	0.00
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG060624\
 Data File : BG061519.D
 Acq On : 6 Jun 2024 21:09
 Operator : MA/JU
 Sample : P2739-02
 Misc :
 ALS Vial : 7 Sample Multiplier: 1




Instrument :
 BNA_G
 ClientSampleId :
 E0005

Manual IntegrationsAPPROVED

Quant Time: Jun 06 22:44:51 2024
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\SFAM-EPA-BG052124.MA.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Thu Jun 06 12:15:45 2024
 Response via : Initial Calibration

Reviewed By :Jagrut Upadhyay 06/07/2024
 Supervised By :mohammad ahmed 06/08/2024

Supervised By :mohammad
 ahmed
 06/08/2024

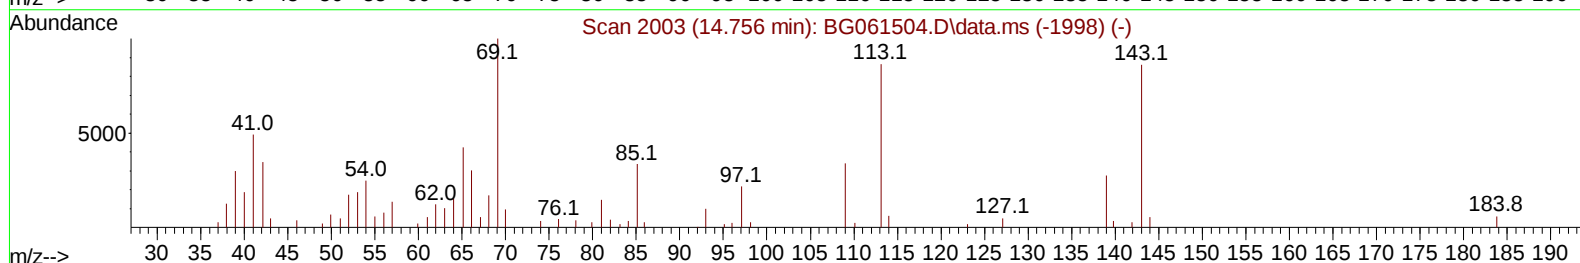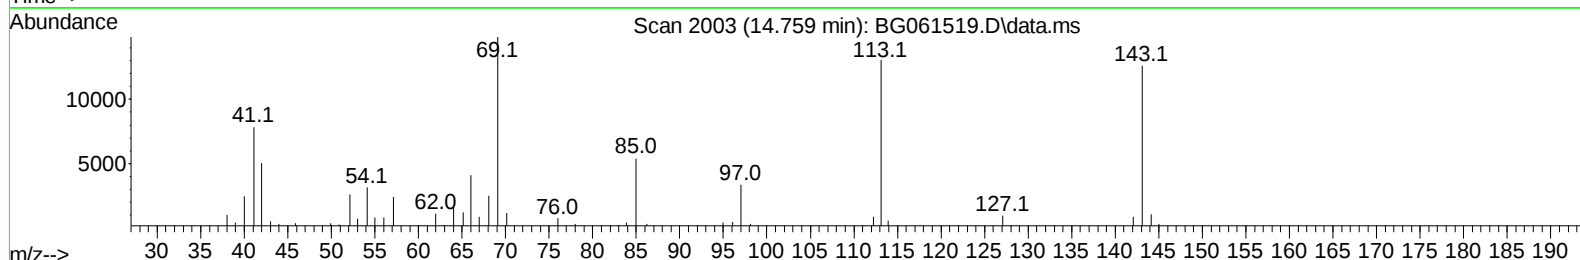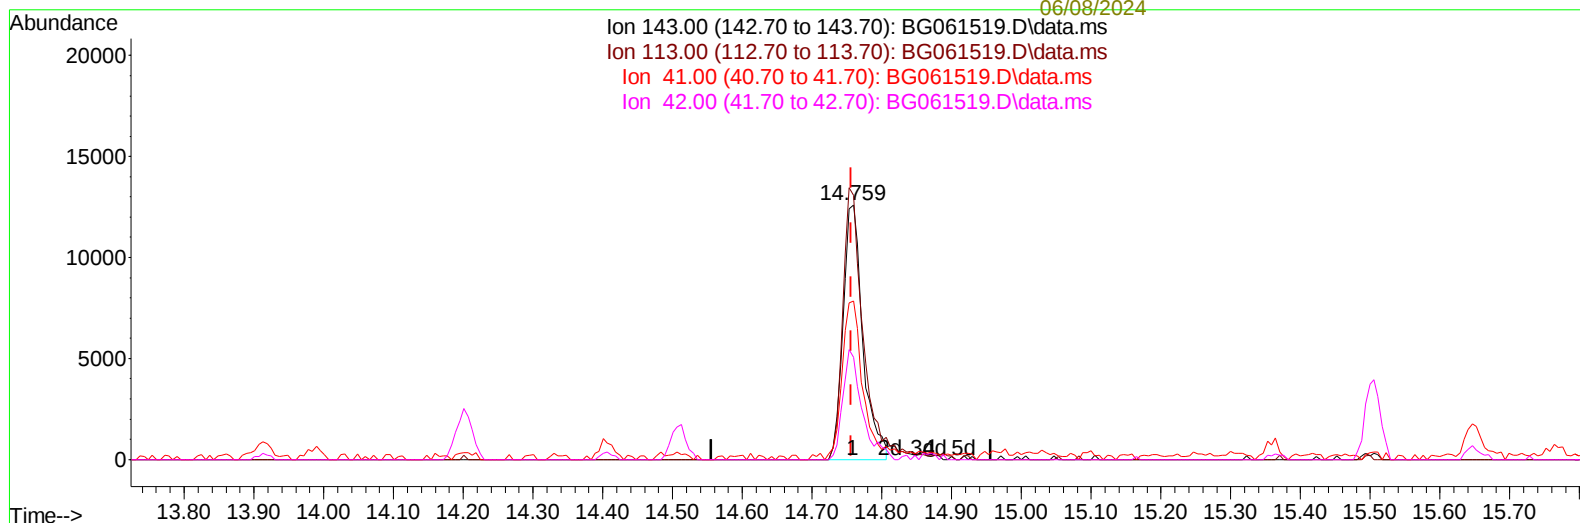

TIC: BG061519.D\data.ms

(54) 4-Nitrophenol-d4 (S)

14.759min (+ 0.003) 34.44 ng/u1

response 24794

Ion	Exp%	Act%
143.00	100.00	100.00
113.00	122.20	103.54
41.00	77.10	62.14
42.00	49.50	40.06

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG060624\
 Data File : BG061519.D
 Acq On : 6 Jun 2024 21:09
 Operator : MA/JU
 Sample : P2739-02
 Misc :
 ALS Vial : 7 Sample Multiplier: 1




Instrument :
 BNA_G
 ClientSampleId :
 E0005

Manual IntegrationsAPPROVED

Reviewed By :Jagrut Upadhyay 06/07/2024
 Supervised By :mohammad ahmed 06/08/2024

Quant Time: Jun 06 22:44:51 2024
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\SFAM-EPA-BG052124.MA.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Thu Jun 06 12:15:45 2024
 Response via : Initial Calibration

Supervised By :mohammad
 ahmed
 06/08/2024

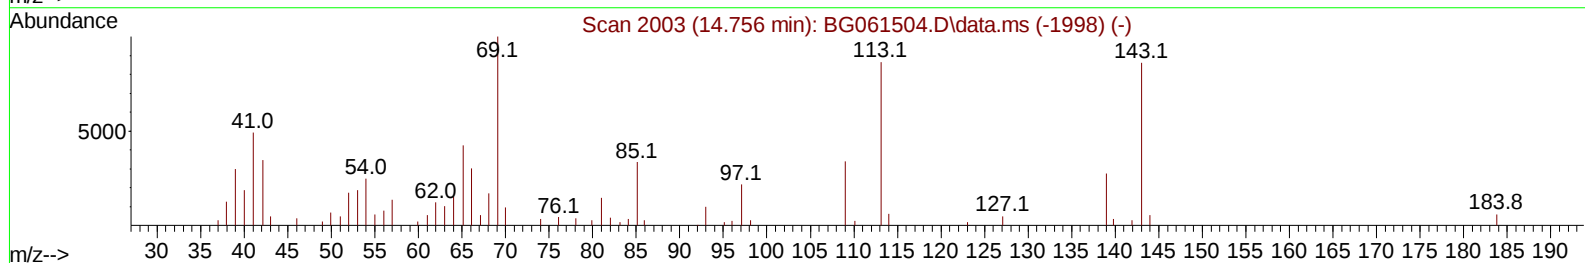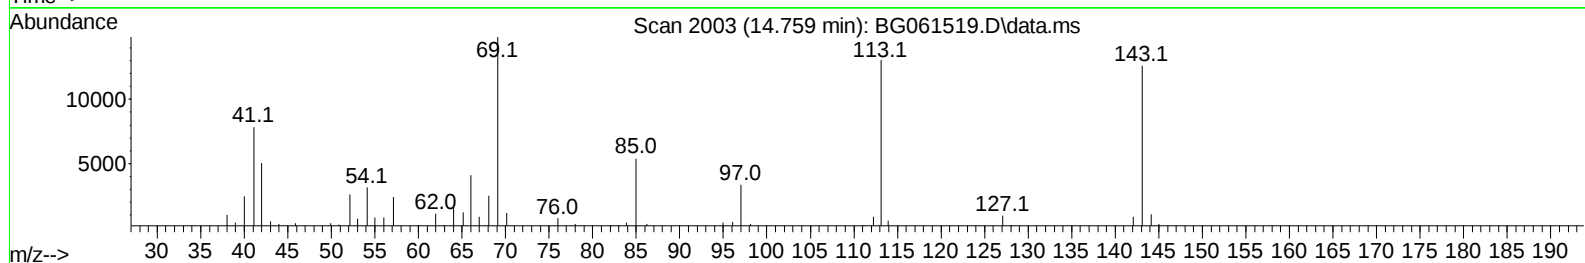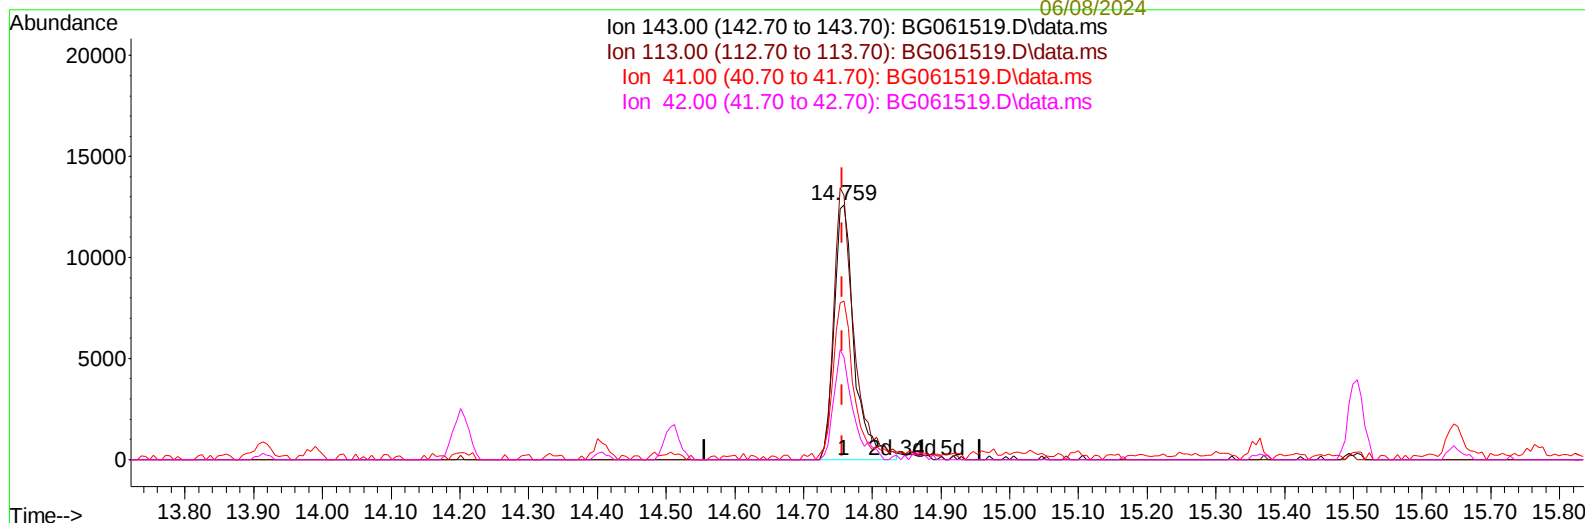

TIC: BG061519.D\data.ms

(54) 4-Nitrophenol-d4 (S)

14.759min (+ 0.003) 35.63 ng/ul m

response 25656

Ion	Exp%	Act%
143.00	100.00	100.00
113.00	122.20	103.54
41.00	77.10	62.14
42.00	49.50	40.06

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG060624\
Data File : BG061519.D
Acq On : 6 Jun 2024 21:09
Operator : MA/JU
Sample : P2739-02
Misc :
ALS Vial : 7 Sample Multiplier: 1




Instrument :
BNA_G
ClientSampleId :
E0005

Manual IntegrationsAPPROVED

Reviewed By :Jagrut Upadhyay 06/07/2024
Supervised By :mohammad ahmed 06/08/2024

Quant Time: Jun 06 22:44:51 2024
Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\SFAM-EPA-BG052124.MA.M
Quant Title : SVOA CALIBRATION
QLast Update : Thu Jun 06 12:15:45 2024
Response via : Initial Calibration

Supervised By :mohammad
ahmed
06/08/2024

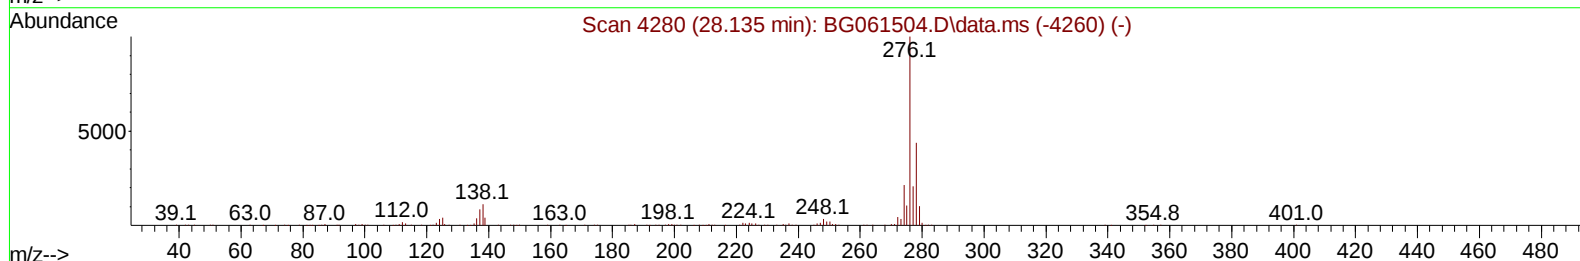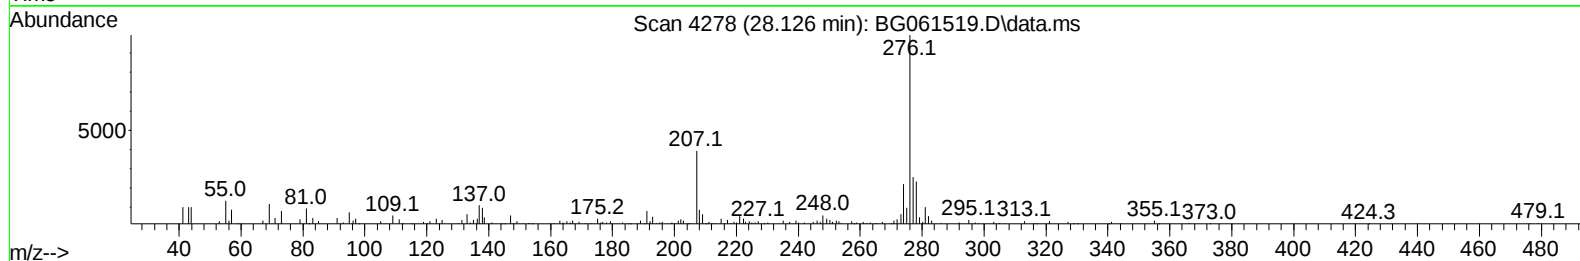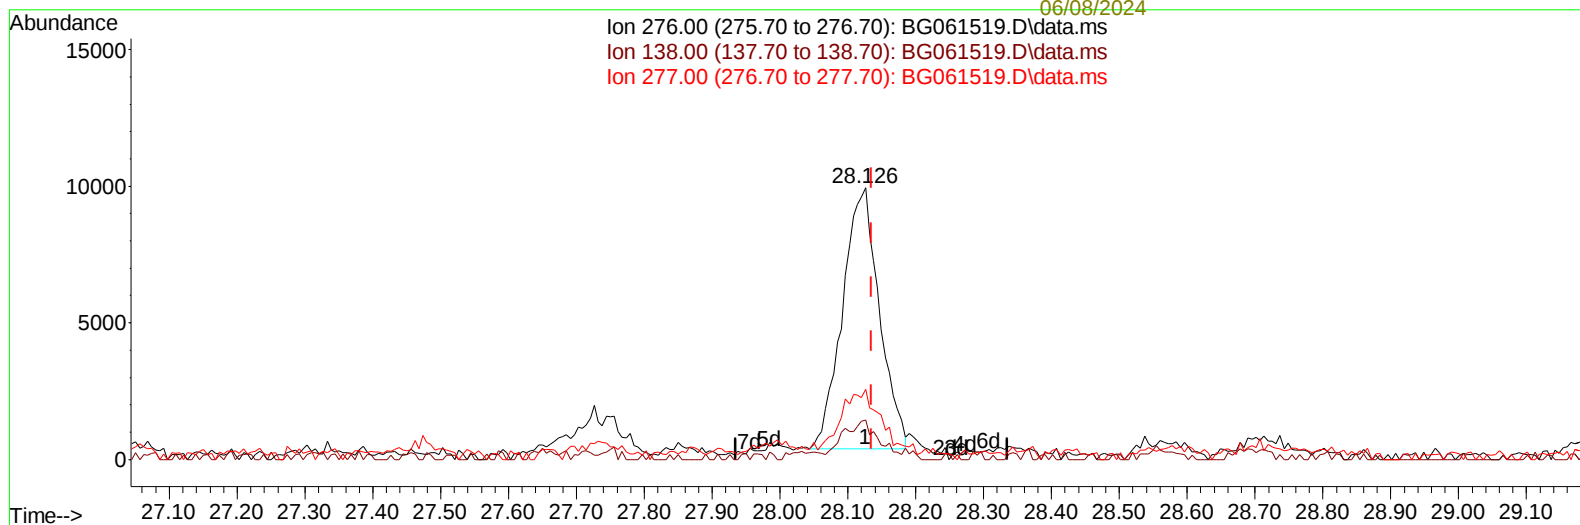

TIC: BG061519.D\data.ms

(94) Indeno(1,2,3-cd)pyrene

28.126min (-0.009) 2.52 ng/u1

response 35983

Ion	Exp%	Act%
276.00	100.00	100.00
138.00	10.80	14.47#
277.00	24.60	25.75
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG060624\
 Data File : BG061519.D
 Acq On : 6 Jun 2024 21:09
 Operator : MA/JU
 Sample : P2739-02
 Misc :
 ALS Vial : 7 Sample Multiplier: 1




Instrument :
 BNA_G
 ClientSampleId :
 E0005

Manual IntegrationsAPPROVED

Reviewed By :Jagrut Upadhyay 06/07/2024
 Supervised By :mohammad ahmed 06/08/2024

Quant Time: Jun 06 22:44:51 2024
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\SFAM-EPA-BG052124.MA.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Thu Jun 06 12:15:45 2024
 Response via : Initial Calibration

Supervised By :mohammad
 ahmed
 06/08/2024

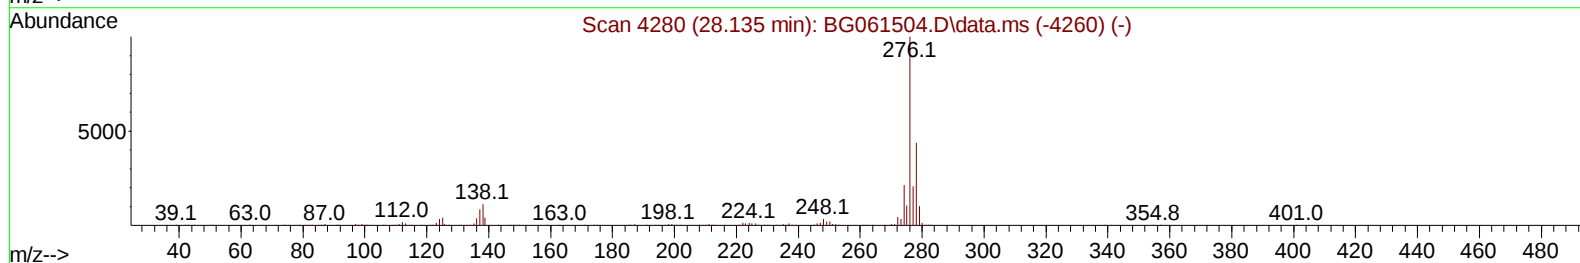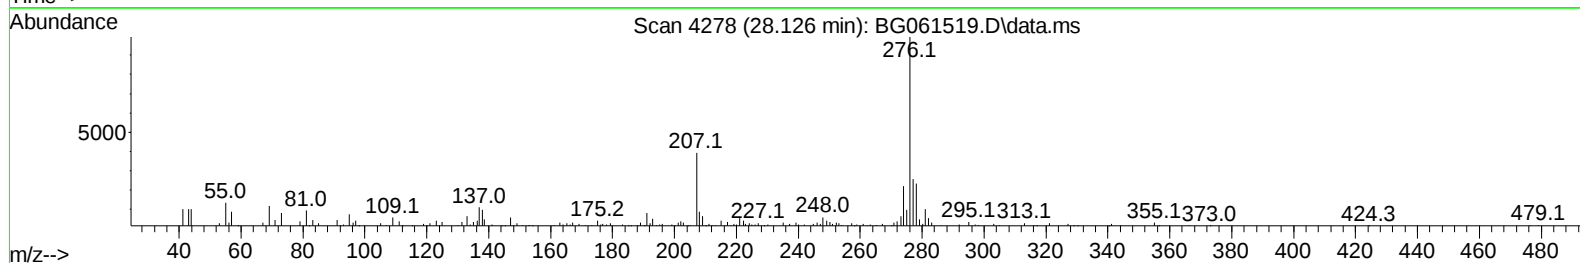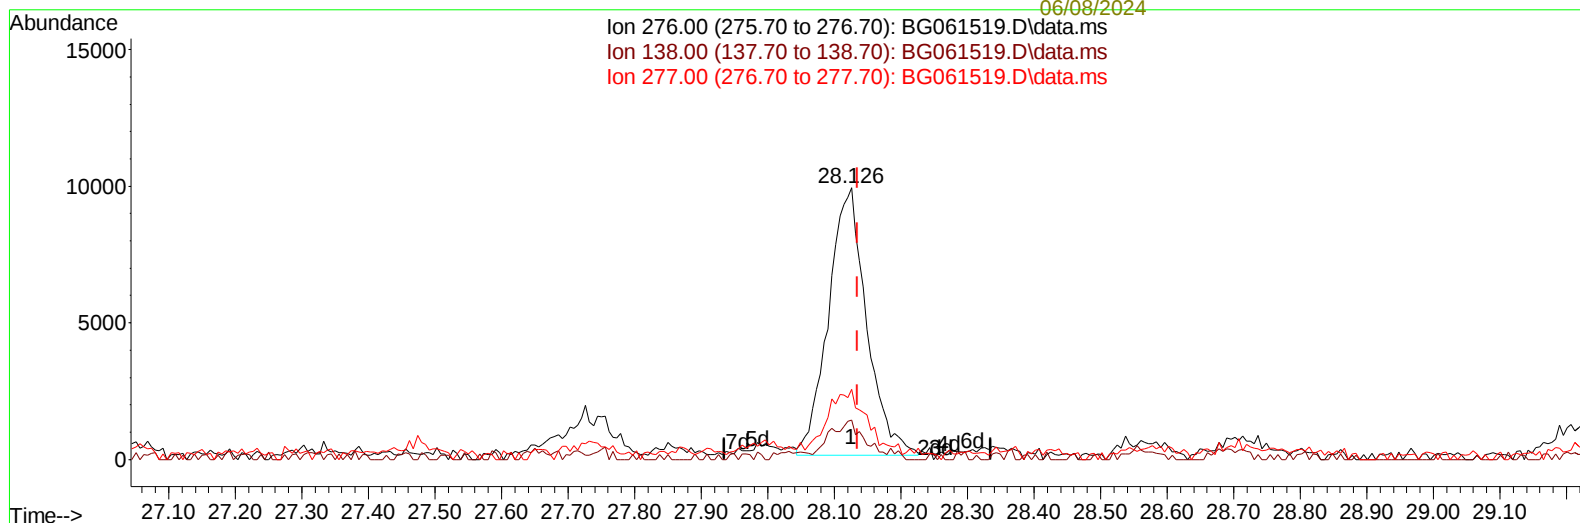

TIC: BG061519.D\data.ms

(94) Indeno(1,2,3-cd)pyrene

28.126min (-0.009) 2.74 ng/ul m

response 39086

Ion	Exp%	Act%
276.00	100.00	100.00
138.00	10.80	9.75
277.00	24.60	25.75
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG060624\
 Data File : BG061519.D
 Acq On : 6 Jun 2024 21:09
 Operator : MA/JU
 Sample : P2739-02
 Misc :
 ALS Vial : 7 Sample Multiplier: 1

Instrument :
 BNA_G
 ClientSampleId :
 E0005


Manual IntegrationsAPPROVED

Quant Time: Jun 06 23:04:11 2024
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\SFAM-EPA-BG052124.MA.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Thu Jun 06 12:15:45 2024
 Response via : Initial Calibration


Reviewed By :Jagrut Upadhyay 06/07/2024
 Supervised By :mohammad ahmed 06/08/2024

Supervised By :mohammad
 ahmed
 06/08/2024


Ion 278.00 (277.70 to 278.70): BG061519.D\data.ms
 Ion 139.00 (138.70 to 139.70): BG061519.D\data.ms
 Ion 279.00 (278.70 to 279.70): BG061519.D\data.ms

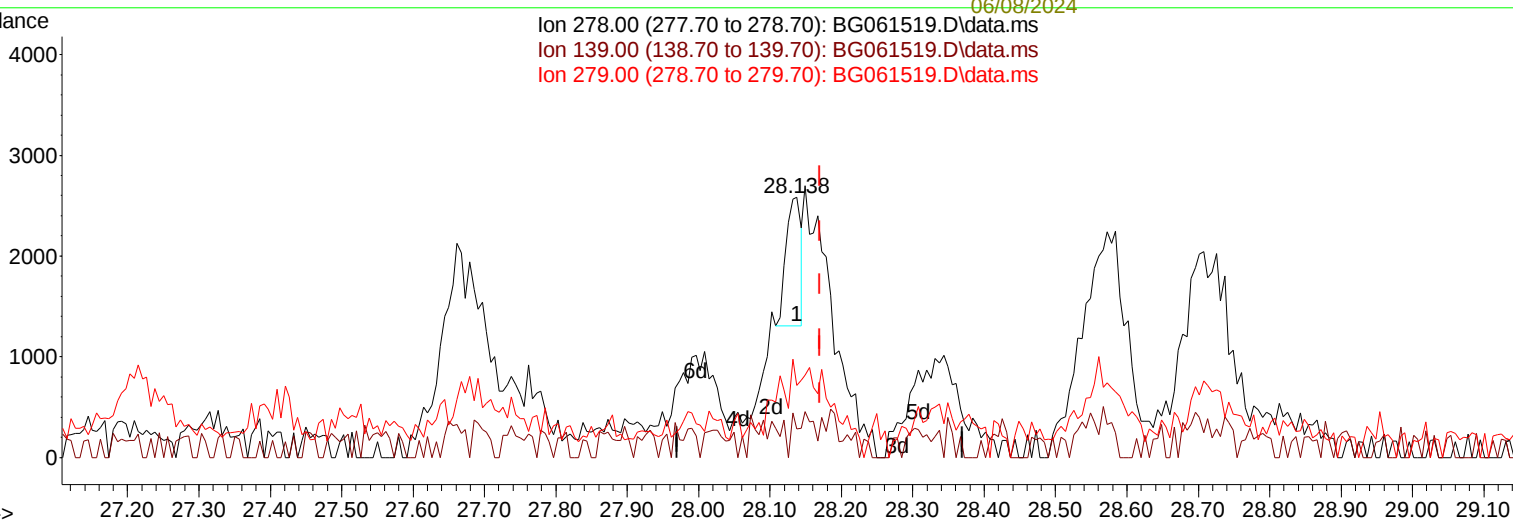

Scan 4280 (28.137 min): BG061519.D\data.ms

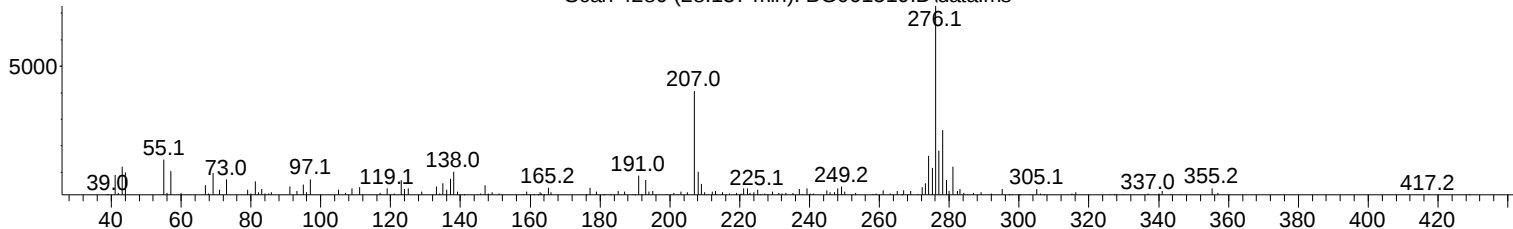

Scan 4286 (28.170 min): BG061504.D\data.ms (-4265) (-)

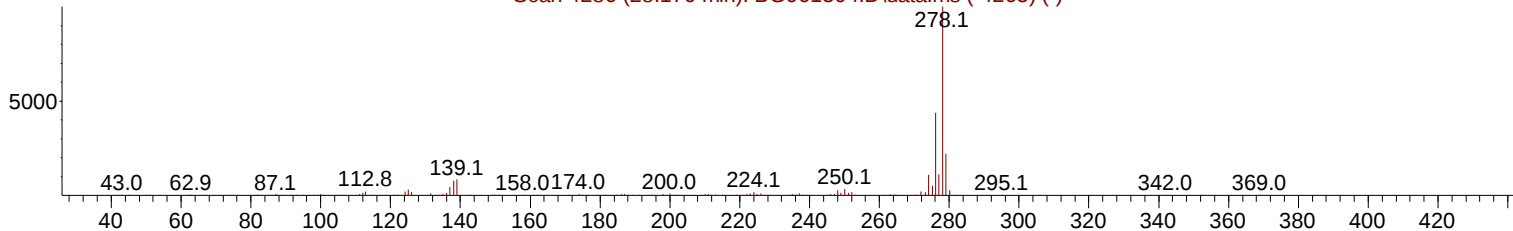

TIC: BG061519.D\data.ms

(95) Dibenzo(a,h)anthracene

28.137min (-0.033) 0.16 ng/u1

response 1836

Ion	Exp%	Act%
278.00	100.00	100.00
139.00	8.00	10.84#
279.00	24.90	27.76
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG060624\
 Data File : BG061519.D
 Acq On : 6 Jun 2024 21:09
 Operator : MA/JU
 Sample : P2739-02
 Misc :
 ALS Vial : 7 Sample Multiplier: 1

Instrument :
 BNA_G
 ClientSampleId :
 E0005

Manual IntegrationsAPPROVED

Reviewed By :Jagrut Upadhyay 06/07/2024
 Supervised By :mohammad ahmed 06/08/2024

Supervised By :mohammad
 ahmed
 06/08/2024

Quant Time: Jun 06 23:05:05 2024
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\SFAM-EPA-BG052124.MA.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Thu Jun 06 12:15:45 2024
 Response via : Initial Calibration

Compound	R.T.	Q	Ion	Response	Conc	Units	Dev(Min)

Internal Standards							
1) 1,4-Dichlorobenzene-d4	7.879	152		29820	20.000	ng/ul	0.00
20) Naphthalene-d8	10.670	136		106962	20.000	ng/ul	0.00
38) Acenaphthene-d10	14.506	164		75090	20.000	ng/ul	0.00
64) Phenanthrene-d10	17.262	188		168548	20.000	ng/ul	0.00
79) Chrysene-d12	21.516	240		186330	20.000	ng/ul	0.00
88) Perylene-d12	24.612	264		208463	20.000	ng/ul	0.00
System Monitoring Compounds							
3) 1,4-Dioxane-d8	3.367	96		3715m	6.972	ng/uL	0.00
4) Pyridine-d5	3.772	84		17116	9.029	ng/ul	0.00
7) Phenol-d5	7.068	99		83828	34.232	ng/ul	0.00
9) Bis-(2-Chloroethyl)eth...	7.209	67		52778	34.289	ng/ul	0.00
11) 2-Chlorophenol-d4	7.421	132		71043	39.200	ng/ul	0.00
15) 4-Methylphenol-d8	8.596	113		62097	29.739	ng/ul	0.00
21) Nitrobenzene-d5	9.036	128		34820	42.281	ng/ul	0.00
24) 2-Nitrophenol-d4	9.759	143		41278	42.828	ng/ul	0.00
28) 2,4-Dichlorophenol-d3	10.305	165		78938	42.011	ng/ul	0.00
31) 4-Chloroaniline-d4	10.805	131		77379	31.478	ng/ul	0.00
46) Dimethylphthalate-d6	13.919	166		247179	42.443	ng/ul	0.00
49) Acenaphthylene-d8	14.201	160		265321	43.821	ng/ul	0.00
54) 4-Nitrophenol-d4	14.759	143		25656m	35.633	ng/ul	0.00
60) Fluorene-d10	15.505	176		218741	43.504	ng/ul	0.00
65) 4,6-Dinitro-2-methylph...	15.646	200		29457	28.896	ng/ul	0.00
73) Anthracene-d10	17.362	188		354396	47.693	ng/ul	0.00
81) Pyrene-d10	19.653	212		383642	40.100	ng/ul	0.00
92) Benzo(a)pyrene-d12	24.401	264		333954	33.322	ng/ul	0.00
Target Compounds							
						Qvalue	
72) Phenanthrene	17.303	178		32800	4.009	ng/ul	98
74) Anthracene	17.397	178		8637	1.021	ng/ul	96
80) Fluoranthene	19.318	202		112989	9.845	ng/ul	99
82) Pyrene	19.683	202		86890	7.294	ng/ul	99
85) Benzo(a)anthracene	21.498	228		65202	5.071	ng/ul	99
87) Chrysene	21.563	228		65403	5.525	ng/ul	95
90) Benzo(b)fluoranthene	23.631	252		103474	8.337	ng/ul	97
91) Benzo(k)fluoranthene	23.690	252		30370	2.410	ng/ul#	95
93) Benzo(a)pyrene	24.459	252		40197	3.411	ng/ul#	87
94) Indeno(1,2,3-cd)pyrene	28.126	276		39086m	2.742	ng/ul	
95) Dibenzo(a,h)anthracene	28.149	278		14382m	1.224	ng/ul	

(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG060624\
Data File : BG061519.D
Acq On : 6 Jun 2024 21:09
Operator : MA/JU
Sample : P2739-02
Misc :
ALS Vial : 7 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
E0005

Manual IntegrationsAPPROVED

Reviewed By :Jagrut Upadhyay 06/07/2024
Supervised By :mohammad ahmed 06/08/2024

Supervised By :mohammad
ahmed
06/08/2024

Quant Time: Jun 06 23:05:05 2024
Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\SFAM-EPA-BG052124.MA.M
Quant Title : SVOA CALIBRATION
QLast Update : Thu Jun 06 12:15:45 2024
Response via : Initial Calibration

