

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG060624\
 Data File : BG061515.D
 Acq On : 6 Jun 2024 18:23
 Operator : MA/JU
 Sample : PB161173BL
 Misc :
 ALS Vial : 3 Sample Multiplier: 1

Instrument :
 BNA_G
 ClientSampleId :
 SBLK173

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Sampling : 1

Start Thrs: 0.2

Stop Thrs : 0

Filtering: 5

Min Area: 0.1 % of largest Peak

Max Peaks: 100

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\SFAM-EPA-BG052124.MA.M
 Title : SVOA CALIBRATION

Signal : TIC: BG061515.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	3.096	13	18	19	rBV3	8994	13118	1.41%	0.137%
2	3.361	56	63	64	rBV4	4615	6513	0.70%	0.068%
3	3.772	126	133	155	rVB	64222	193716	20.87%	2.029%
4	4.083	183	186	189	rBV3	831	1136	0.12%	0.012%
5	7.068	688	694	703	rBV	138914	254115	27.38%	2.662%
6	7.209	710	718	728	rBB	94577	160030	17.24%	1.677%
7	7.421	746	754	763	rBB	136897	243692	26.26%	2.553%
8	7.879	825	832	839	rBV	143961	249505	26.88%	2.614%
9	8.602	948	955	964	rVB	164448	290731	31.33%	3.046%
10	9.036	1021	1029	1037	rBB	137863	246432	26.55%	2.582%
11	9.753	1145	1151	1159	rBB	124895	220522	23.76%	2.310%
12	10.306	1239	1245	1258	rBB	166167	302390	32.58%	3.168%
13	10.670	1298	1307	1314	rBV	186343	318037	34.27%	3.332%
14	10.811	1323	1331	1342	rBB	161030	288119	31.04%	3.018%
15	12.262	1573	1578	1584	rBV2	2320	3770	0.41%	0.039%
16	13.913	1853	1859	1867	rVB	290711	415610	44.78%	4.354%
17	14.201	1900	1908	1918	rBV	308313	489263	52.72%	5.126%
18	14.512	1954	1961	1968	rBV	282370	433458	46.70%	4.541%
19	14.759	1997	2003	2013	rBV2	69901	141047	15.20%	1.478%
20	15.505	2123	2130	2137	rVB	407966	593839	63.99%	6.221%
21	15.652	2149	2155	2166	rBV	99933	158583	17.09%	1.661%
22	15.740	2168	2170	2175	rVB2	1575	1854	0.20%	0.019%
23	17.262	2422	2429	2436	rBV	364757	528062	56.90%	5.532%
24	17.362	2439	2446	2452	rVV	464451	667197	71.89%	6.990%
25	18.948	2712	2716	2719	rVV2	758	1109	0.12%	0.012%
26	19.213	2758	2761	2767	rVB2	7098	10112	1.09%	0.106%
27	19.289	2770	2774	2780	rVV2	5548	8712	0.94%	0.091%
28	19.330	2780	2781	2786	rVV3	1138	1181	0.13%	0.012%
29	19.366	2786	2787	2790	rVB	1255	1209	0.13%	0.013%
30	19.577	2819	2823	2826	rBV2	2103	2581	0.28%	0.027%
31	19.653	2830	2836	2842	rBV	594307	817556	88.09%	8.565%
32	19.695	2842	2843	2847	rVB3	1654	1266	0.14%	0.013%
33	19.812	2861	2863	2866	rVB2	1753	1814	0.20%	0.019%
34	19.894	2873	2877	2878	rBV4	1722	1379	0.15%	0.014%
35	19.947	2883	2886	2888	rBV3	981	1206	0.13%	0.013%
36	19.988	2891	2893	2894	rVB2	1751	962	0.10%	0.010%

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG060624\
 Data File : BG061515.D
 Acq On : 6 Jun 2024 18:23
 Operator : MA/JU
 Sample : PB161173BL
 Misc :
 ALS Vial : 3 Sample Multiplier: 1

Instrument :
 BNA_G
 ClientSampleId :
 SBLK173

Integration Parameters: LSCINT.P

Integrator: RTE
 Smoothing : OFF Filtering: 5
 Sampling : 1 Min Area: 0.1 % of largest Peak
 Start Thrs: 0.2 Max Peaks: 100
 Stop Thrs : 0 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\SFAM-EPA-BG052124.MA.M
 Title : SVOA CALIBRATION

37	20.041	2901	2902	2904	rBV2	1379	936	0.10%	0.010%
38	20.118	2913	2915	2916	rBV2	1995	1318	0.14%	0.014%
39	20.329	2950	2951	2953	rBV2	1245	989	0.11%	0.010%
40	20.588	2993	2995	2996	rBV2	1404	962	0.10%	0.010%
41	20.646	3004	3005	3007	rBV2	3010	2396	0.26%	0.025%
42	20.776	3025	3027	3030	rBV3	1611	1841	0.20%	0.019%
43	21.105	3081	3083	3085	rBV3	2732	2262	0.24%	0.024%
44	21.516	3147	3153	3162	rVB	420027	663716	71.51%	6.953%
45	21.604	3167	3168	3170	rBV2	3211	3083	0.33%	0.032%
46	21.798	3199	3201	3204	rVB4	4372	2945	0.32%	0.031%
47	21.998	3233	3235	3237	rBV2	3636	3072	0.33%	0.032%
48	22.198	3267	3269	3271	rVB2	4303	3490	0.38%	0.037%
49	22.280	3281	3283	3290	rVB8	4073	7606	0.82%	0.080%
50	22.803	3369	3372	3373	rBV3	3440	3321	0.36%	0.035%
51	22.950	3391	3397	3403	rVB7	7676	16482	1.78%	0.173%
52	23.114	3424	3425	3431	rVB6	3500	4502	0.49%	0.047%
53	23.602	3506	3508	3509	rBV2	3348	2957	0.32%	0.031%
54	23.666	3517	3519	3520	rBV2	2685	1755	0.19%	0.018%
55	23.708	3522	3526	3533	rVB7	11880	24014	2.59%	0.252%
56	24.078	3587	3589	3593	rBV5	3315	3705	0.40%	0.039%
57	24.401	3633	3644	3654	rBV	357204	928083	100.00%	9.723%
58	24.606	3670	3679	3692	rVB2	272016	733981	79.09%	7.689%
59	25.082	3758	3760	3762	rBV3	2566	2610	0.28%	0.027%
60	25.253	3787	3789	3792	rBV3	3919	4280	0.46%	0.045%
61	25.523	3833	3835	3836	rBV2	3035	1169	0.13%	0.012%
62	25.670	3857	3860	3861	rBV3	7307	7160	0.77%	0.075%
63	25.887	3895	3897	3899	rVB2	3964	2509	0.27%	0.026%
64	26.304	3966	3968	3969	rBV2	4659	2152	0.23%	0.023%
65	26.904	4069	4070	4071	rBV	3386	1864	0.20%	0.020%
66	27.591	4185	4187	4188	rBV2	3624	1883	0.20%	0.020%
67	28.038	4261	4263	4265	rVB3	3567	2066	0.22%	0.022%
68	28.478	4336	4338	4339	rBV2	5968	5271	0.57%	0.055%
69	29.260	4469	4471	4472	rBV2	3668	3578	0.39%	0.037%
70	29.524	4514	4516	4517	rBV	2925	1661	0.18%	0.017%
71	29.859	4571	4573	4574	rBV2	3776	1776	0.19%	0.019%
72	29.906	4579	4581	4586	rBV4	2927	5112	0.55%	0.054%
73	30.241	4637	4638	4641	rBV2	3260	3113	0.34%	0.033%
74	30.617	4701	4702	4703	rBV	3779	1939	0.21%	0.020%
75	31.128	4787	4789	4790	rBV2	3080	2313	0.25%	0.024%
76	31.845	4909	4911	4914	rBV4	3309	4504	0.49%	0.047%

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG060624\
Data File : BG061515.D
Acq On : 6 Jun 2024 18:23
Operator : MA/JU
Sample : PB161173BL
Misc :
ALS Vial : 3 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
SBLK173

Integration Parameters: LSCINT.P
Integrator: RTE
Smoothing : OFF Filtering: 5
Sampling : 1 Min Area: 0.1 % of largest Peak
Start Thrs: 0.2 Max Peaks: 100
Stop Thrs : 0 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\SFAM-EPA-BG052124.MA.M
Title : SVOA CALIBRATION

77	31.939	4925	4927	4928	rVB2	3534	2316	0.25%	0.024%
78	32.409	5004	5007	5009	rBV4	3620	4743	0.51%	0.050%




Sum of corrected areas: 9545261

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG060624\
Data File : BG061515.D
Acq On : 6 Jun 2024 18:23
Operator : MA/JU
Sample : PB161173BL
Misc :
ALS Vial : 3 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
SBLK173

Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\SFAM-EPA-BG052124.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

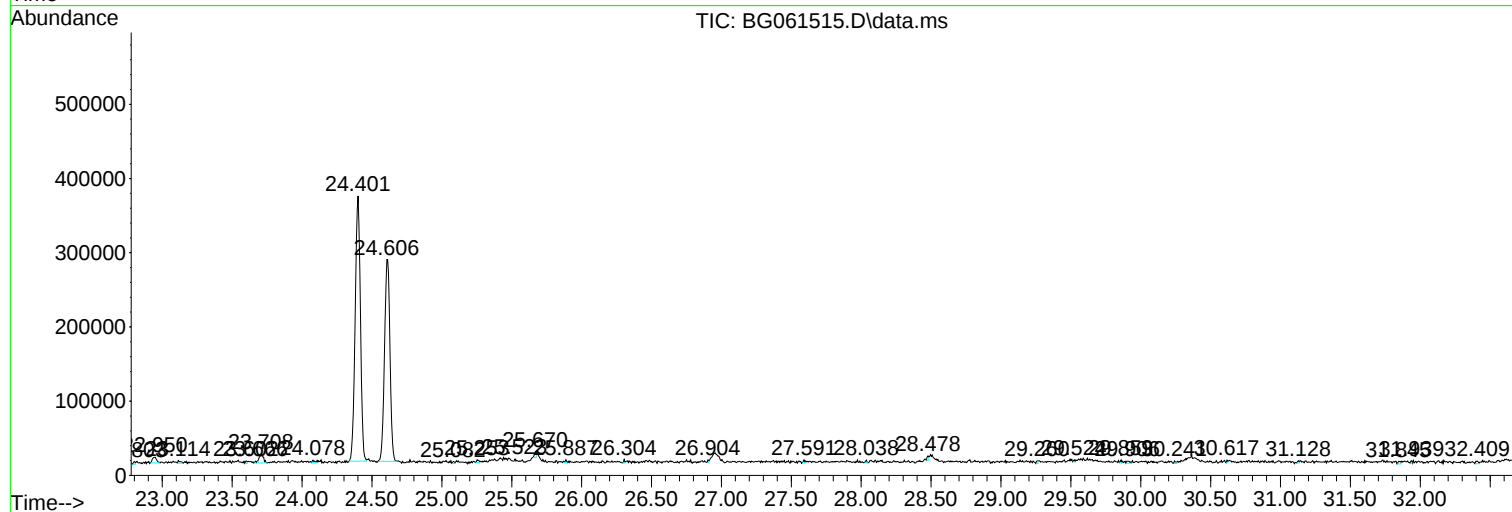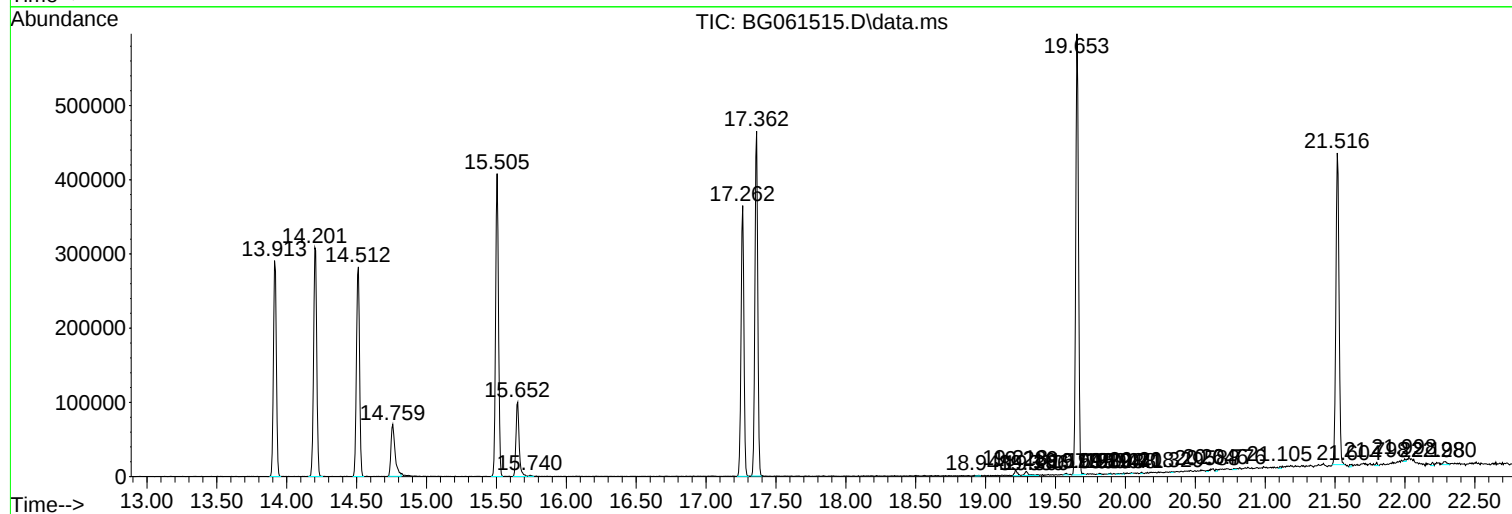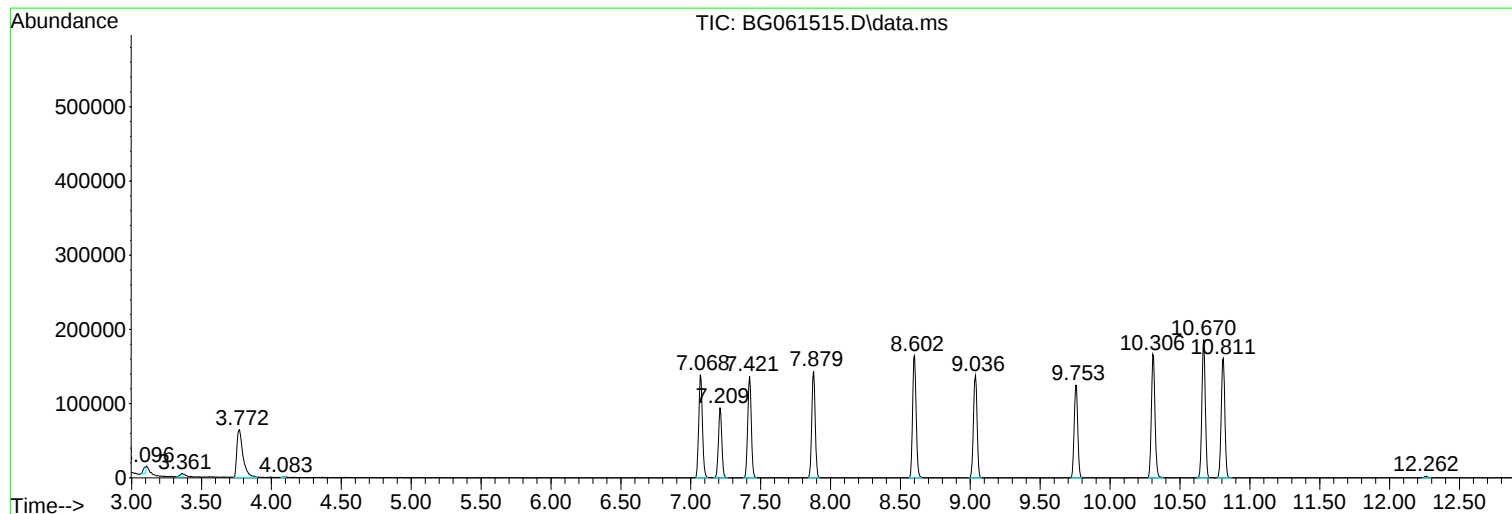

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG060624\
Data File : BG061515.D
Acq On : 6 Jun 2024 18:23
Operator : MA/JU
Sample : PB161173BL
Misc :
ALS Vial : 3 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
SBLK173

Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\SFAM-EPA-BG052124.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG060624\
Data File : BG061515.D
Acq On : 6 Jun 2024 18:23
Operator : MA/JU
Sample : PB161173BL
Misc :
ALS Vial : 3 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
SBLK173

Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\SFAM-EPA-BG052124.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--
				#	RT Resp Conc