

Data Path : Z:\HPCHEM1\BNA G\DATA\BG060716\
Data File : BG022212.D
Acq On : 7 Jun 2016 20:07
Operator : UM/SJ
Sample : H3387-02
Misc :
ALS Vial : 6 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
SP16-LF2RES

Integration Parameters: rteint.p
Integrator: RTE
Smoothing : ON Filtering: 5
Sampling : 1 Min Area: 3 % of largest Peak
Start Thrs: 0.2 Max Peaks: 100
Stop Thrs : 0 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
Peak separation: 5

Method : Z:\HPCHEM1\BNA_G\METHODS\8270-BG060616.M
Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

Signal : TIC

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	5.667	474	481	498	rBV	123660	244387	9.74%	2.717%
2	7.277	747	755	769	rBV	79628	165554	6.60%	1.841%
3	7.647	810	818	832	rBV	289413	582887	23.24%	6.481%
4	8.117	891	898	909	rBV	56844	112279	4.48%	1.248%
5	8.440	946	953	964	rBV	281813	563024	22.45%	6.260%
6	9.286	1090	1097	1116	rBV	186855	422644	16.85%	4.699%
7	10.937	1370	1378	1390	rBV	87891	191223	7.62%	2.126%
8	13.370	1784	1792	1807	rBV	793843	1398757	55.77%	15.551%
9	14.744	2019	2026	2039	rBV2	185717	343525	13.70%	3.819%
10	16.231	2273	2279	2299	rBV2	591634	1043069	41.59%	11.597%
11	17.494	2486	2494	2508	rBV	247171	451150	17.99%	5.016%
12	20.085	2928	2935	2945	rBV	1729681	2507941	100.00%	27.883%
13	21.766	3213	3221	3232	rBV	259313	493892	19.69%	5.491%
14	25.062	3770	3782	3794	rBV2	149246	474128	18.91%	5.271%


Sum of corrected areas: 8994460

Data Path : Z:\HPCHEM1\BNA G\DATA\BG060716\
Data File : BG022212.D
Acq On : 7 Jun 2016 20:07
Operator : UM/SJ
Sample : H3387-02
Misc :
ALS Vial : 6 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
SP16-LF2RES

Quant Method : Z:\HPCHEM1\BNA G\METHODS\8270-BG060616.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\DATABASE\NIST02.L
TIC Integration Parameters: LSCINT.P

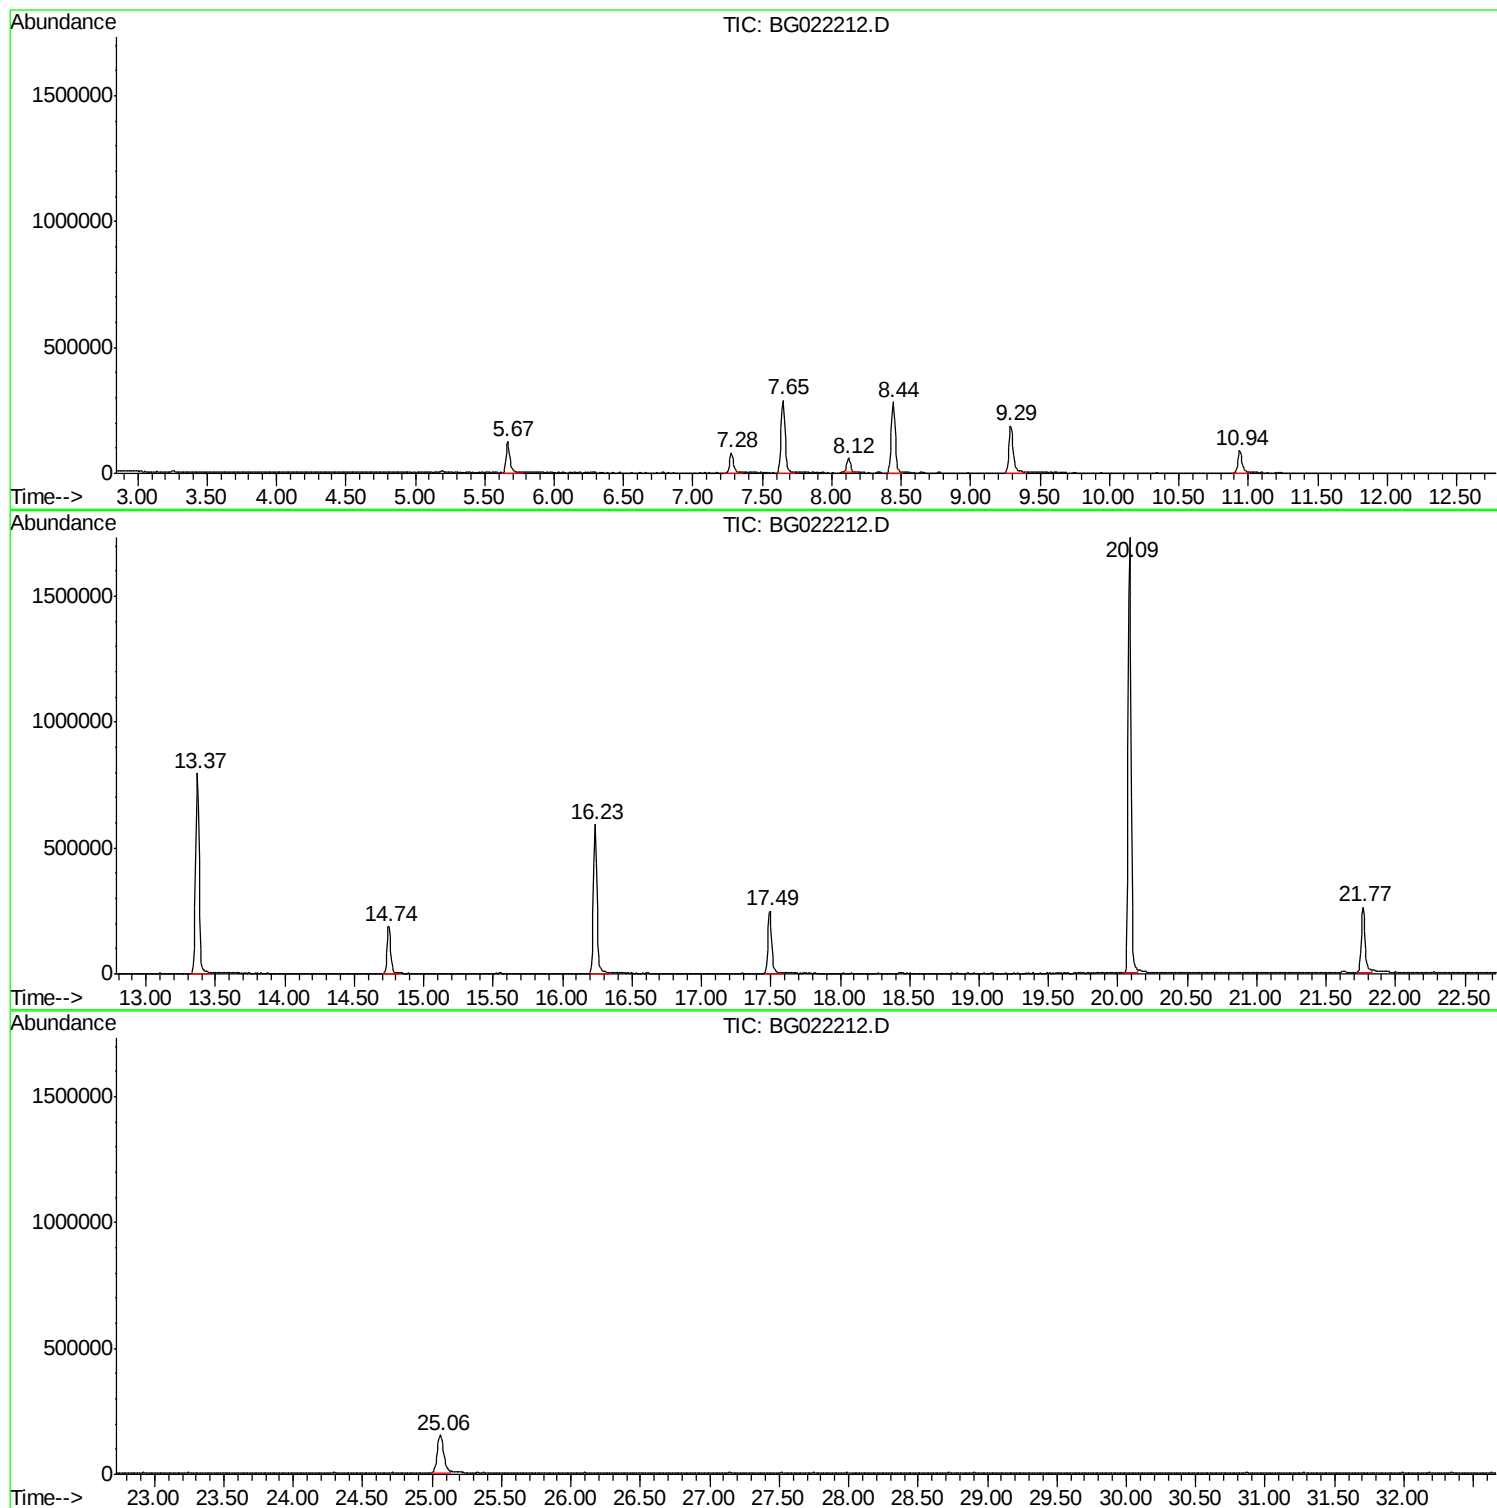

Data Path : Z:\HPCHEM1\BNA G\DATA\BG060716\
Data File : BG022212.D
Acq On : 7 Jun 2016 20:07
Operator : UM/SJ
Sample : H3387-02
Misc :
ALS Vial : 6 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
SP16-LF2RES










Quant Method : Z:\HPCHEM1\BNA G\METHODS\8270-BG060616.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\DATABASE\NIST02.L
TIC Integration Parameters: LSCINT.P

Peak Number 1 unknown7.65 Concentration Rank 1

R.T.	EstConc	Area	Relative to ISTD	R.T.
7.65	103.83 ng	582887	1,4-Dichlorobenzene-d4	8.12

Hit#	of	Tentative ID	MW	MolForm	CAS#	Qual
1	5	3-Chloro-6-fluoro-pyrazine	132	C4H2ClFN2	1000146-10-7	38
2		(E)-3-Chloro-2-methyl-2-pentenal	132	C6H9ClO	031357-76-3	25
3		Amphetaminil	250	C17H18N2	017590-01-1	12
4		Xenon	132	Xe	007440-63-3	9
5		4-Chloro-6-fluoro-pyrimidine	132	C4H2ClFN2	051422-01-6	9

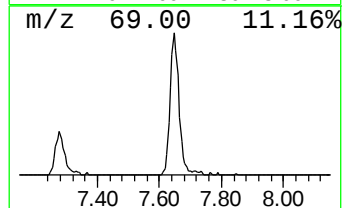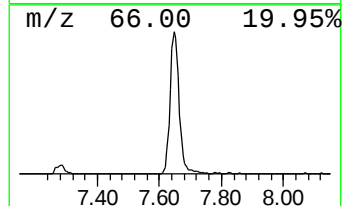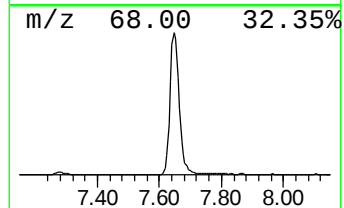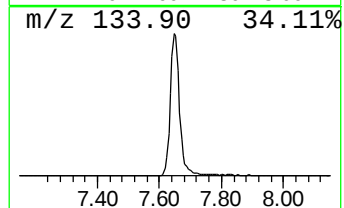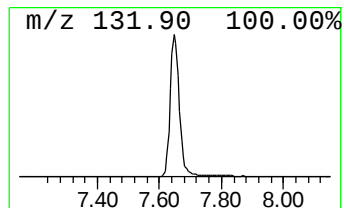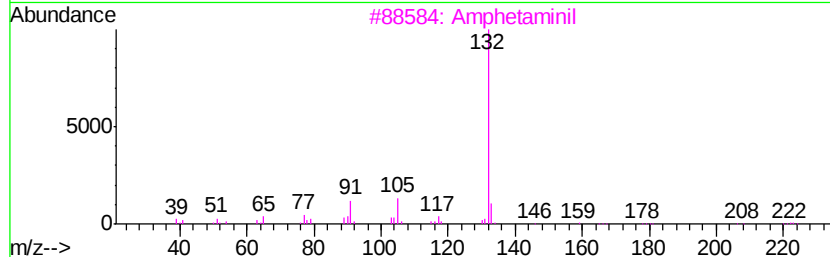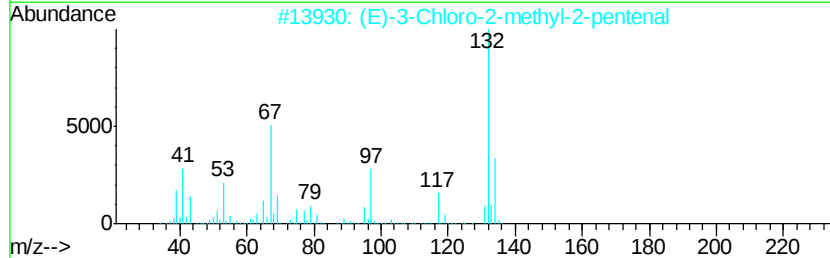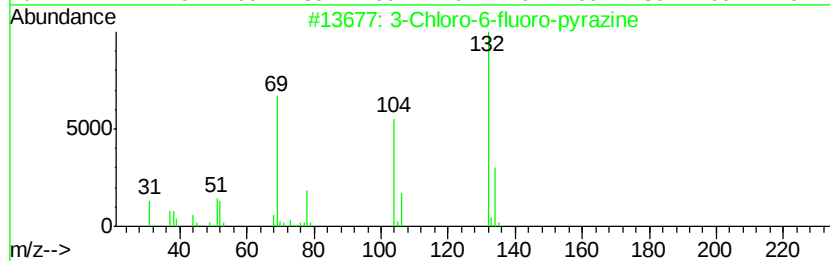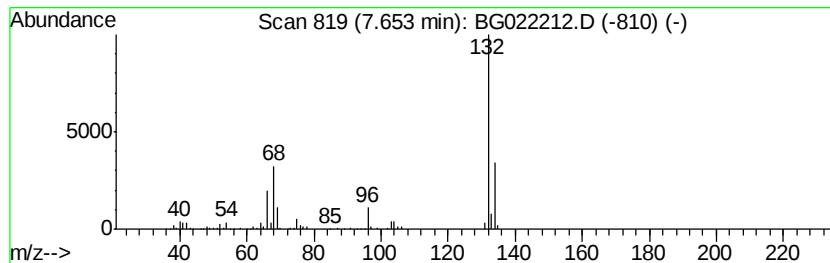

Data Path : Z:\HPCHEM1\BNA_G\DATA\BG060716\
Data File : BG022212.D
Acq On : 7 Jun 2016 20:07
Operator : UM/SJ
Sample : H3387-02
Misc :
ALS Vial : 6 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
SP16-LF2RES

Quant Method : Z:\HPCHEM1\BNA_G\METHODS\8270-BG060616.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\DATABASE\NIST02.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc
unknown7.65	7.65	103.8	ng	582887	1	8.12	112279	20.0