

Data Path : Z:\HPCHEM1\BNA G\DATA\BG060716\
 Data File : BG022213.D
 Acq On : 7 Jun 2016 20:47
 Operator : UM/SJ
 Sample : H3387-03
 Misc :
 ALS Vial : 7 Sample Multiplier: 1

Instrument :
 BNA_G
 ClientSampleId :
 SP16-LF2MW4

Integration Parameters: rteint.p
 Integrator: RTE
 Smoothing : ON Filtering: 5
 Sampling : 1 Min Area: 3 % of largest Peak
 Start Thrs: 0.2 Max Peaks: 100
 Stop Thrs : 0 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\HPCHEM1\BNA_G\METHODS\8270-BG060616.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

Signal : TIC

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	5.664	474	481	495	rBV	112260	224556	9.66%	2.679%
2	7.274	745	755	772	rBV	71059	148667	6.39%	1.774%
3	7.650	811	819	833	rBV	261711	532244	22.89%	6.350%
4	8.120	892	899	908	rBV	52976	105468	4.54%	1.258%
5	8.443	946	954	971	rBV	264138	544175	23.41%	6.493%
6	9.290	1090	1098	1114	rBV	176770	392004	16.86%	4.677%
7	10.941	1368	1379	1392	rBV	79285	175826	7.56%	2.098%
8	13.367	1785	1792	1810	rBV	727836	1320411	56.80%	15.754%
9	14.748	2019	2027	2038	rBV3	178960	319746	13.75%	3.815%
10	16.234	2273	2280	2296	rBV2	553221	965419	41.53%	11.519%
11	17.492	2487	2494	2506	rBV2	235407	410808	17.67%	4.902%
12	20.083	2928	2935	2950	rBV	1567290	2324787	100.00%	27.738%
13	21.763	3214	3221	3235	rBV	226013	468599	20.16%	5.591%
14	25.065	3770	3783	3796	rBV2	134900	448547	19.29%	5.352%


Sum of corrected areas: 8381257

Data Path : Z:\HPCHEM1\BNA G\DATA\BG060716\
Data File : BG022213.D
Acq On : 7 Jun 2016 20:47
Operator : UM/SJ
Sample : H3387-03
Misc :
ALS Vial : 7 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
SP16-LF2MW4

Quant Method : Z:\HPCHEM1\BNA G\METHODS\8270-BG060616.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\DATABASE\NIST02.L
TIC Integration Parameters: LSCINT.P

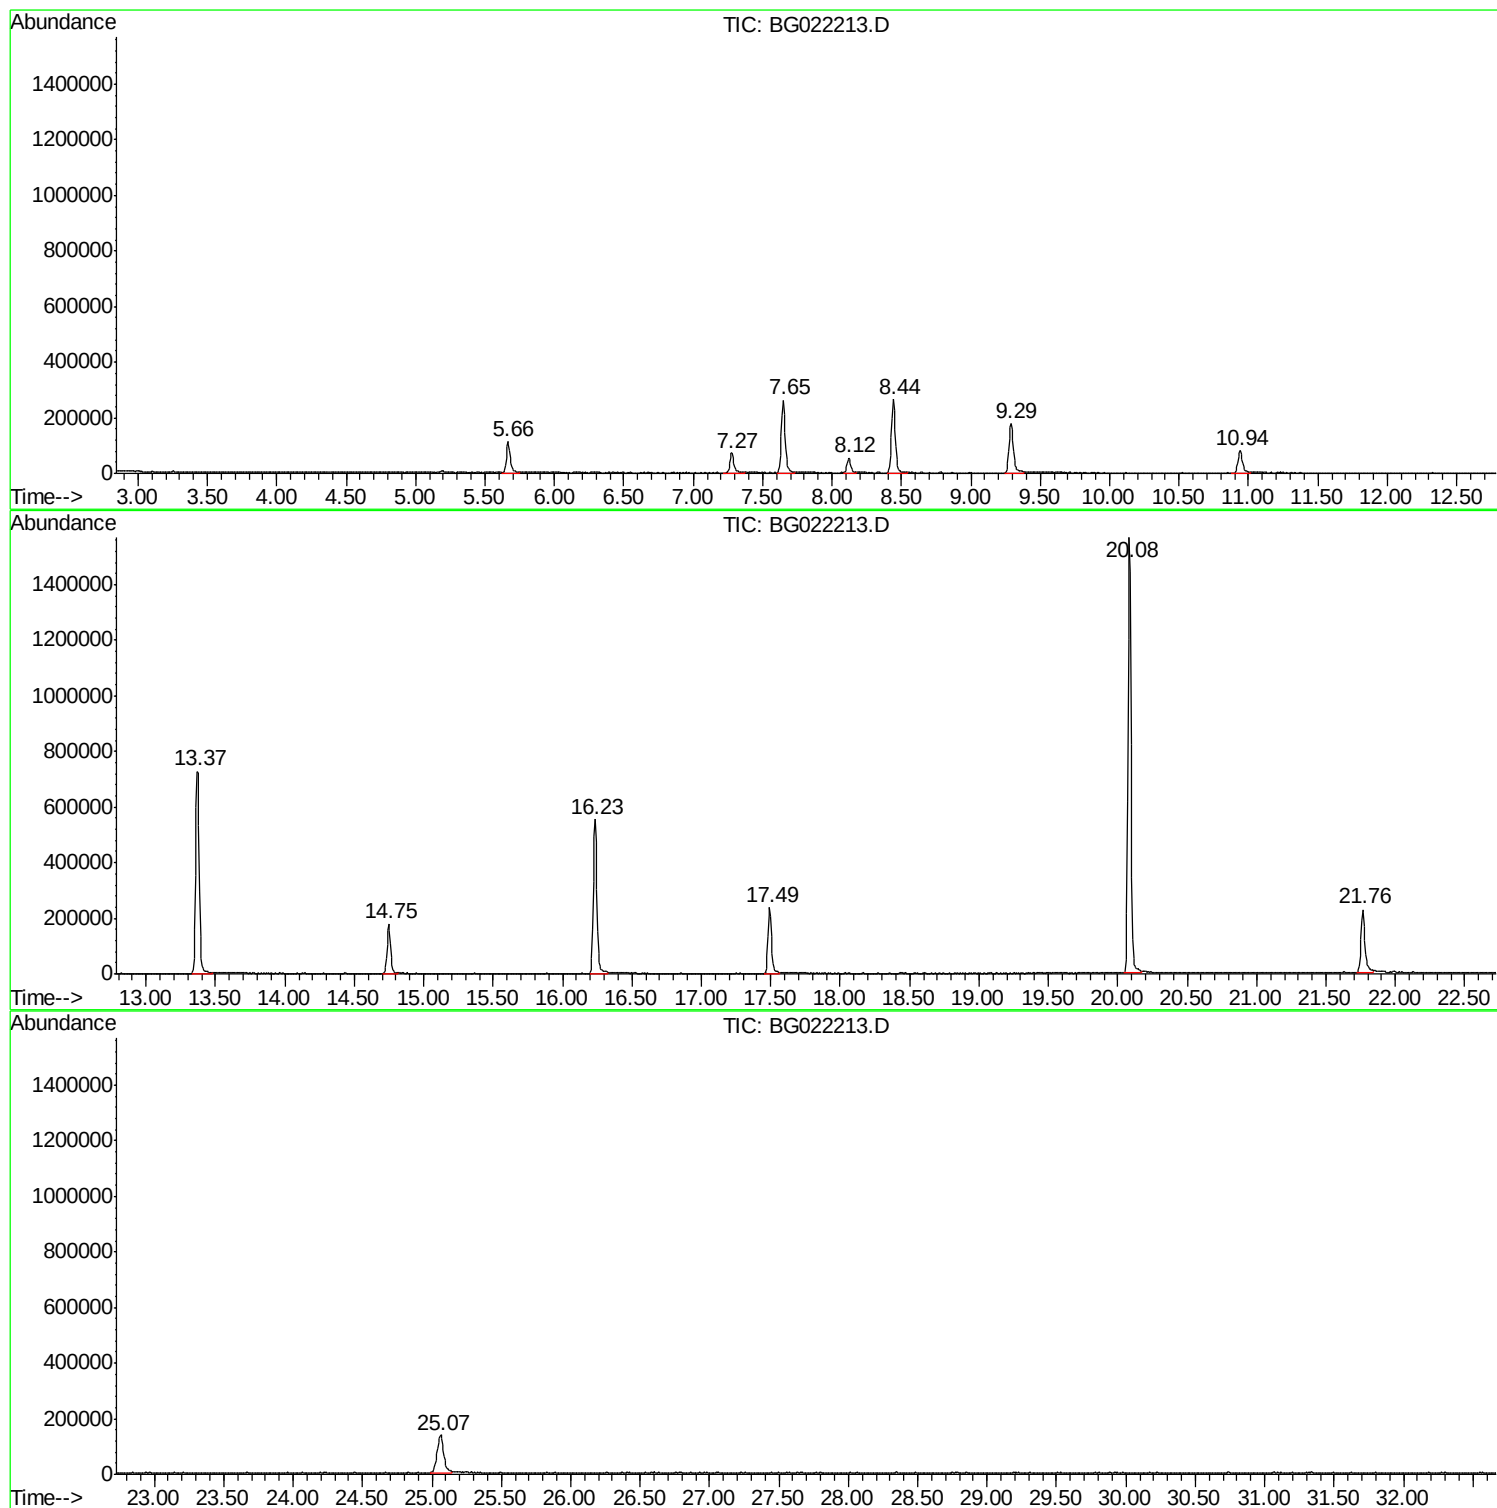

Data Path : Z:\HPCHEM1\BNA G\DATA\BG060716\
Data File : BG022213.D
Acq On : 7 Jun 2016 20:47
Operator : UM/SJ
Sample : H3387-03
Misc :
ALS Vial : 7 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
SP16-LF2MW4










Quant Method : Z:\HPCHEM1\BNA G\METHODS\8270-BG060616.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\DATABASE\NIST02.L
TIC Integration Parameters: LSCINT.P

Peak Number 1 3-Chloro-6-fluoro-pyrazine Concentration Rank 2

R.T.	EstConc	Area	Relative to ISTD	R.T.
7.65	100.93 ng	532244	1,4-Dichlorobenzene-d4	8.12

Hit#	of	Tentative ID	MW	MolForm	CAS#	Qual
1	5	3-Chloro-6-fluoro-pyrazine	132	C4H2ClFN2	1000146-10-7	50
2		(E)-3-Chloro-2-methyl-2-pentenal	132	C6H9ClO	031357-76-3	33
3		Amphetaminil	250	C17H18N2	017590-01-1	25
4		5-Fluoro-2-chloropyrimidine	132	C4H2ClFN2	062802-42-0	9
5		5-Aminoindole	132	C8H8N2	005192-03-0	9

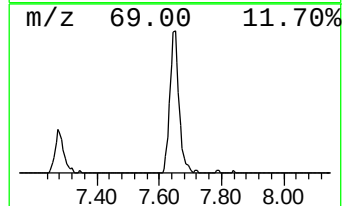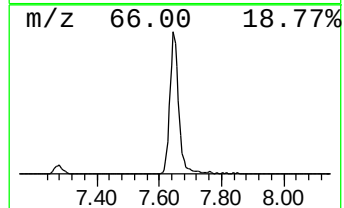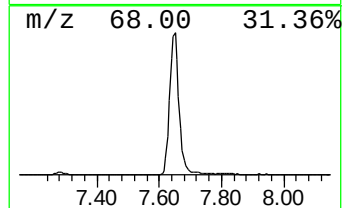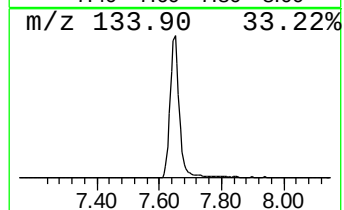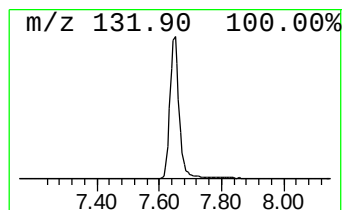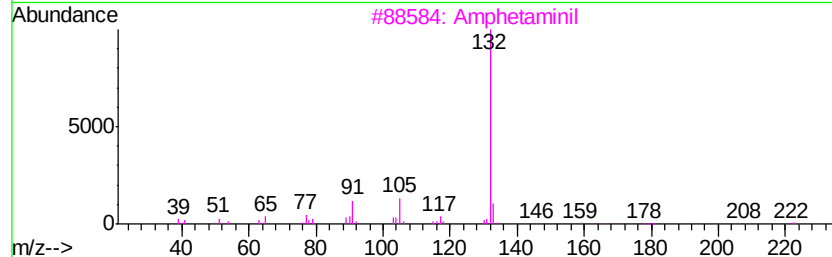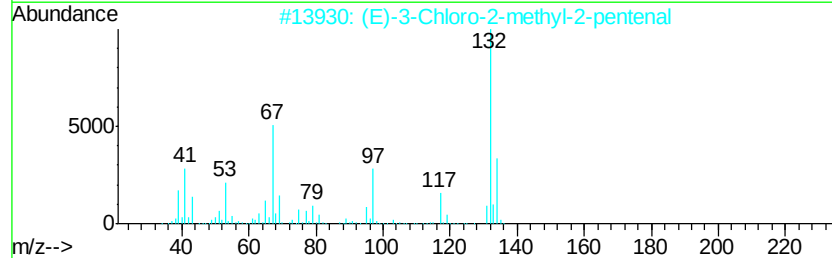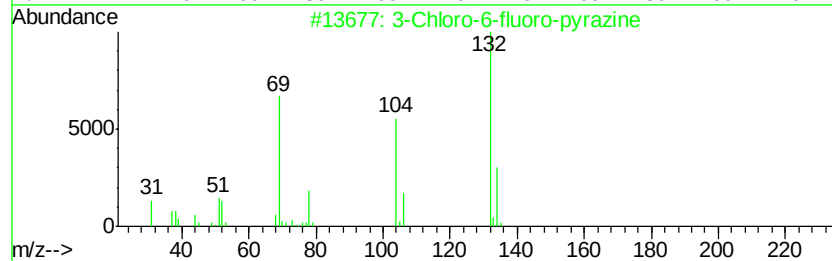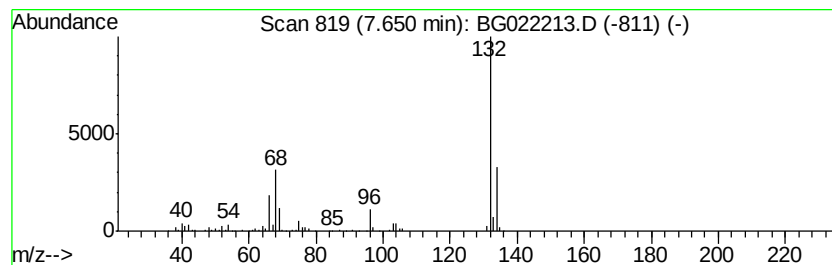

Data Path : Z:\HPCHEM1\BNA_G\DATA\BG060716\
Data File : BG022213.D
Acq On : 7 Jun 2016 20:47
Operator : UM/SJ
Sample : H3387-03
Misc :
ALS Vial : 7 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
SP16-LF2MW4

Quant Method : Z:\HPCHEM1\BNA_G\METHODS\8270-BG060616.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\DATABASE\NIST02.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc
3-Chloro-6-fluoro...	7.65	100.9	ng	532244	1	8.12	105468	20.0