

Data Path : Z:\HPCHEM1\BNA G\DATA\BG060716\
 Data File : BG022214.D
 Acq On : 7 Jun 2016 21:28
 Operator : UM/SJ
 Sample : H3387-04
 Misc :
 ALS Vial : 8 Sample Multiplier: 1

Instrument :
 BNA_G
 ClientSampleId :
 SP16-LF2MW4-9007

Integration Parameters: rteint.p
 Integrator: RTE
 Smoothing : ON Filtering: 5
 Sampling : 1 Min Area: 3 % of largest Peak
 Start Thrs: 0.2 Max Peaks: 100
 Stop Thrs : 0 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\HPCHEM1\BNA_G\METHODS\8270-BG060616.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

Signal : TIC

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	5.665	474	481	494	rBV	101564	202567	9.36%	2.479%
2	7.275	748	755	771	rBV	61817	128883	5.96%	1.577%
3	7.645	811	818	833	rBV	258166	523294	24.18%	6.404%
4	8.121	887	899	913	rBV	54210	112519	5.20%	1.377%
5	8.444	945	954	975	rBV	266082	549699	25.40%	6.727%
6	9.290	1089	1098	1117	rBV	176852	396824	18.34%	4.856%
7	10.941	1371	1379	1391	rBV	79317	178911	8.27%	2.189%
8	13.368	1785	1792	1809	rBV	766718	1343905	62.10%	16.445%
9	14.748	2020	2027	2038	rBV2	175574	316655	14.63%	3.875%
10	16.235	2273	2280	2292	rBV	566745	957408	44.24%	11.716%
11	17.492	2487	2494	2507	rBV	226098	405276	18.73%	4.959%
12	20.083	2929	2935	2956	rBV	1490594	2164094	100.00%	26.482%
13	21.764	3215	3221	3233	rBV2	226947	461935	21.35%	5.653%
14	25.054	3771	3781	3794	rBV	131913	429938	19.87%	5.261%


Sum of corrected areas: 8171908

Data Path : Z:\HPCHEM1\BNA G\DATA\BG060716\
Data File : BG022214.D
Acq On : 7 Jun 2016 21:28
Operator : UM/SJ
Sample : H3387-04
Misc :
ALS Vial : 8 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
SP16-LF2MW4-9007

Quant Method : Z:\HPCHEM1\BNA G\METHODS\8270-BG060616.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\DATABASE\NIST02.L
TIC Integration Parameters: LSCINT.P

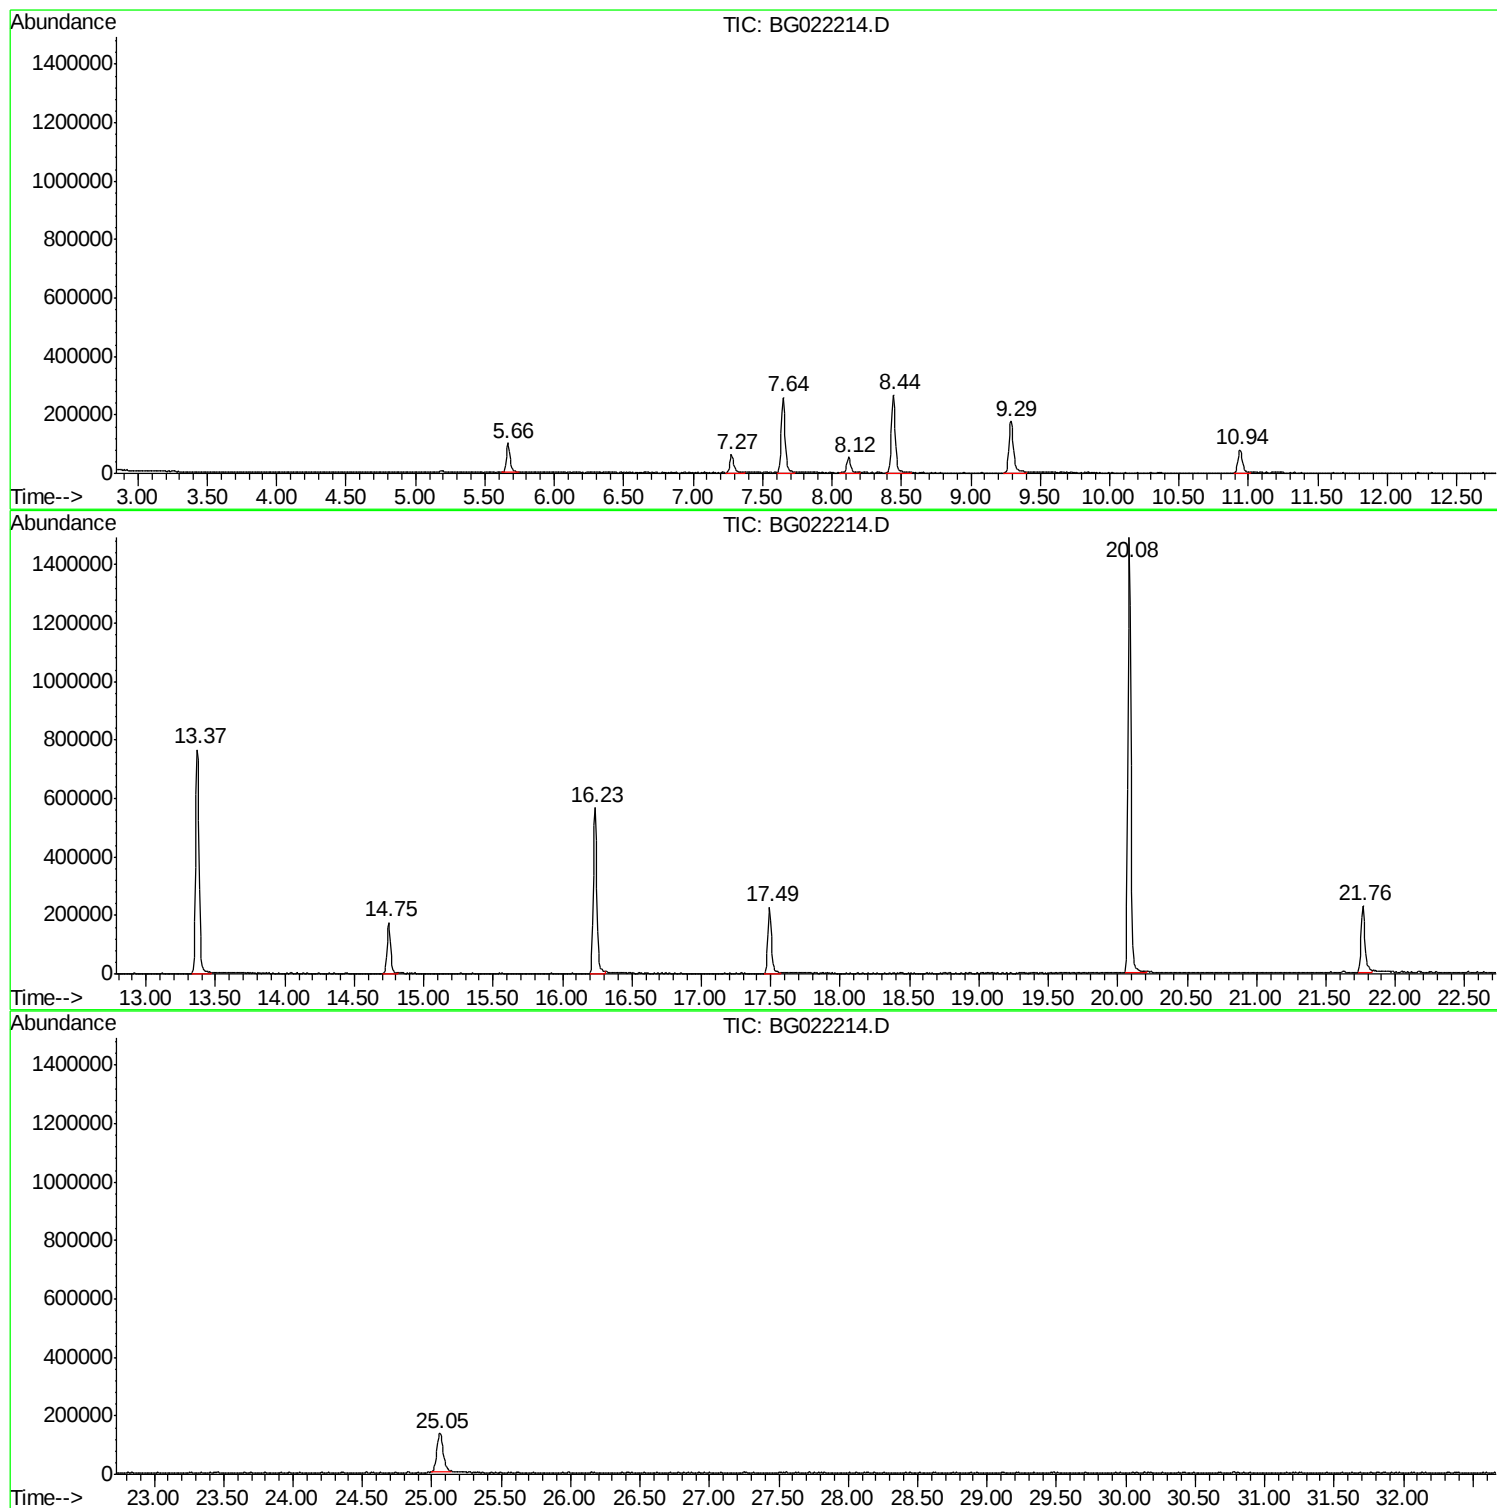

Data Path : Z:\HPCHEM1\BNA G\DATA\BG060716\
Data File : BG022214.D
Acq On : 7 Jun 2016 21:28
Operator : UM/SJ
Sample : H3387-04
Misc :
ALS Vial : 8 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
SP16-LF2MW4-9007










Quant Method : Z:\HPCHEM1\BNA G\METHODS\8270-BG060616.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\DATABASE\NIST02.L
TIC Integration Parameters: LSCINT.P

Peak Number 1 unknown7.64 Concentration Rank 2

R.T.	EstConc	Area	Relative to ISTD	R.T.
7.64	93.01 ng	523294	1,4-Dichlorobenzene-d4	8.12

Hit#	of	Tentative ID	MW	MolForm	CAS#	Qual
1	5	3-Chloro-6-fluoro-pyrazine	132	C4H2ClFN2	1000146-10-7	25
2		(E)-3-Chloro-2-methyl-2-pentenal	132	C6H9ClO	031357-76-3	17
3		Tranvlcyproline-propionyl	189	C12H15NO	1000123-86-3	12
4		5-Fluoro-2-chloropyrimidine	132	C4H2ClFN2	062802-42-0	9
5		4-Chloro-6-fluoro-pyrimidine	132	C4H2ClFN2	051422-01-6	9

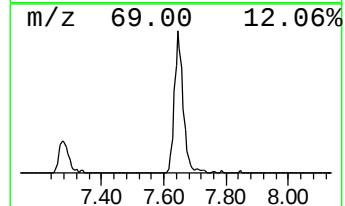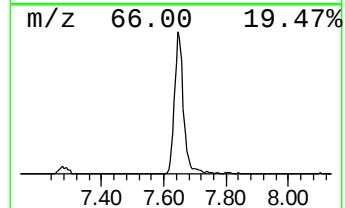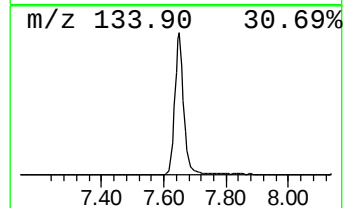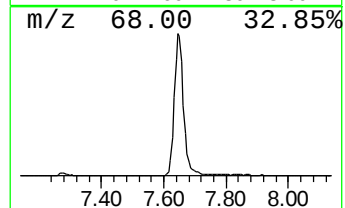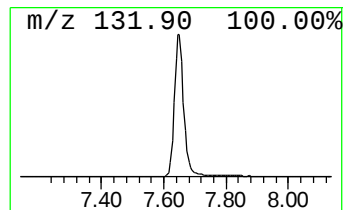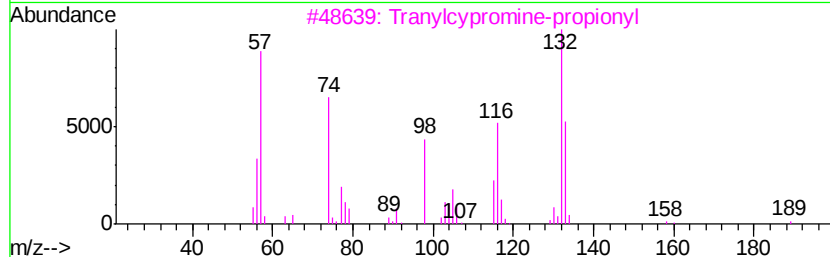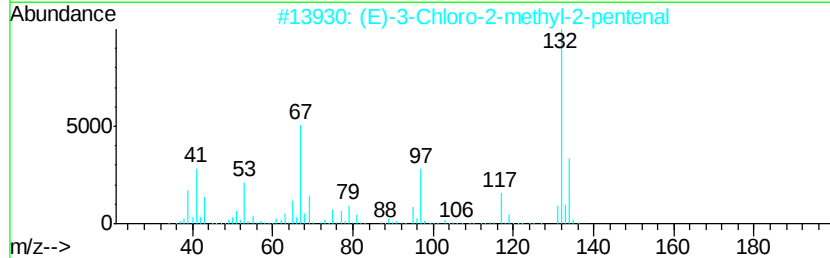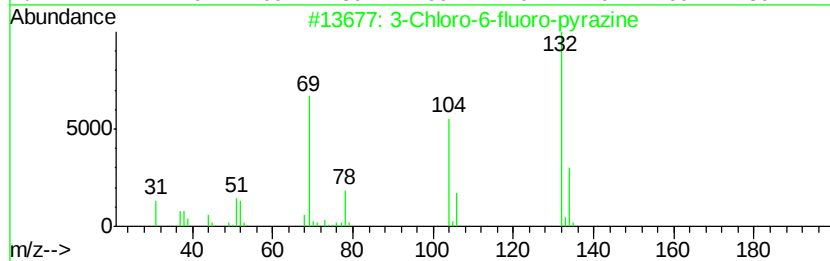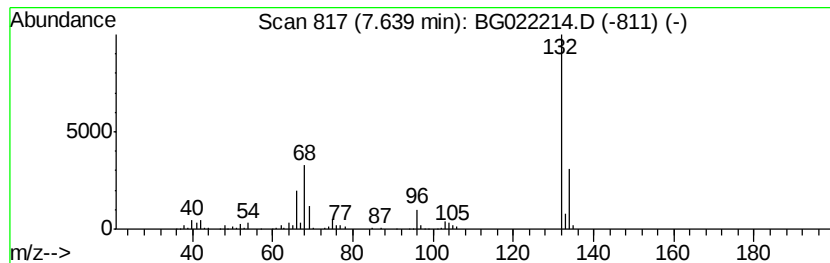

Data Path : Z:\HPCHEM1\BNA_G\DATA\BG060716\
Data File : BG022214.D
Acq On : 7 Jun 2016 21:28
Operator : UM/SJ
Sample : H3387-04
Misc :
ALS Vial : 8 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
SP16-LF2MW4-9007

Quant Method : Z:\HPCHEM1\BNA_G\METHODS\8270-BG060616.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\DATABASE\NIST02.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc
unknown7.64	7.64	93.0	ng	523294	1	8.12	112519	20.0