

Data Path : Z:\HPCHEM1\BNA G\DATA\BG060716\
 Data File : BG022220.D
 Acq On : 8 Jun 2016 1:27
 Operator : UM/SJ
 Sample : H3426-04
 Misc :
 ALS Vial : 14 Sample Multiplier: 1

Instrument :
 BNA_G
 ClientSampleId :
 GW-6

Integration Parameters: rteint.p
 Integrator: RTE
 Smoothing : ON Filtering: 5
 Sampling : 1 Min Area: 3 % of largest Peak
 Start Thrs: 0.2 Max Peaks: 100
 Stop Thrs : 0 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\HPCHEM1\BNA_G\METHODS\8270-BG060616.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

Signal : TIC

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	5.664	475	481	494	rBV	115223	229362	10.57%	2.867%
2	7.274	747	755	773	rBV	81504	166063	7.65%	2.076%
3	7.644	808	818	832	rBV	271457	536316	24.71%	6.703%
4	8.120	892	899	911	rBV2	55381	110928	5.11%	1.386%
5	8.444	945	954	964	rBV	238505	474976	21.88%	5.937%
6	9.290	1090	1098	1113	rBV	175370	380060	17.51%	4.750%
7	10.935	1370	1378	1392	rBV	81895	186544	8.59%	2.332%
8	13.367	1785	1792	1808	rBV	719097	1223456	56.37%	15.292%
9	14.748	2020	2027	2039	rBV3	180177	327062	15.07%	4.088%
10	16.234	2273	2280	2292	rBV	536834	901117	41.52%	11.263%
11	17.492	2487	2494	2506	rBV2	228412	402104	18.53%	5.026%
12	20.083	2928	2935	2950	rBV	1480026	2170386	100.00%	27.128%
13	21.763	3213	3221	3234	rBV2	227435	458523	21.13%	5.731%
14	25.059	3771	3782	3799	rBV3	133416	433784	19.99%	5.422%


Sum of corrected areas: 8000681

Data Path : Z:\HPCHEM1\BNA G\DATA\BG060716\
Data File : BG022220.D
Acq On : 8 Jun 2016 1:27
Operator : UM/SJ
Sample : H3426-04
Misc :
ALS Vial : 14 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
GW-6

Quant Method : Z:\HPCHEM1\BNA G\METHODS\8270-BG060616.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\DATABASE\NIST02.L
TIC Integration Parameters: LSCINT.P

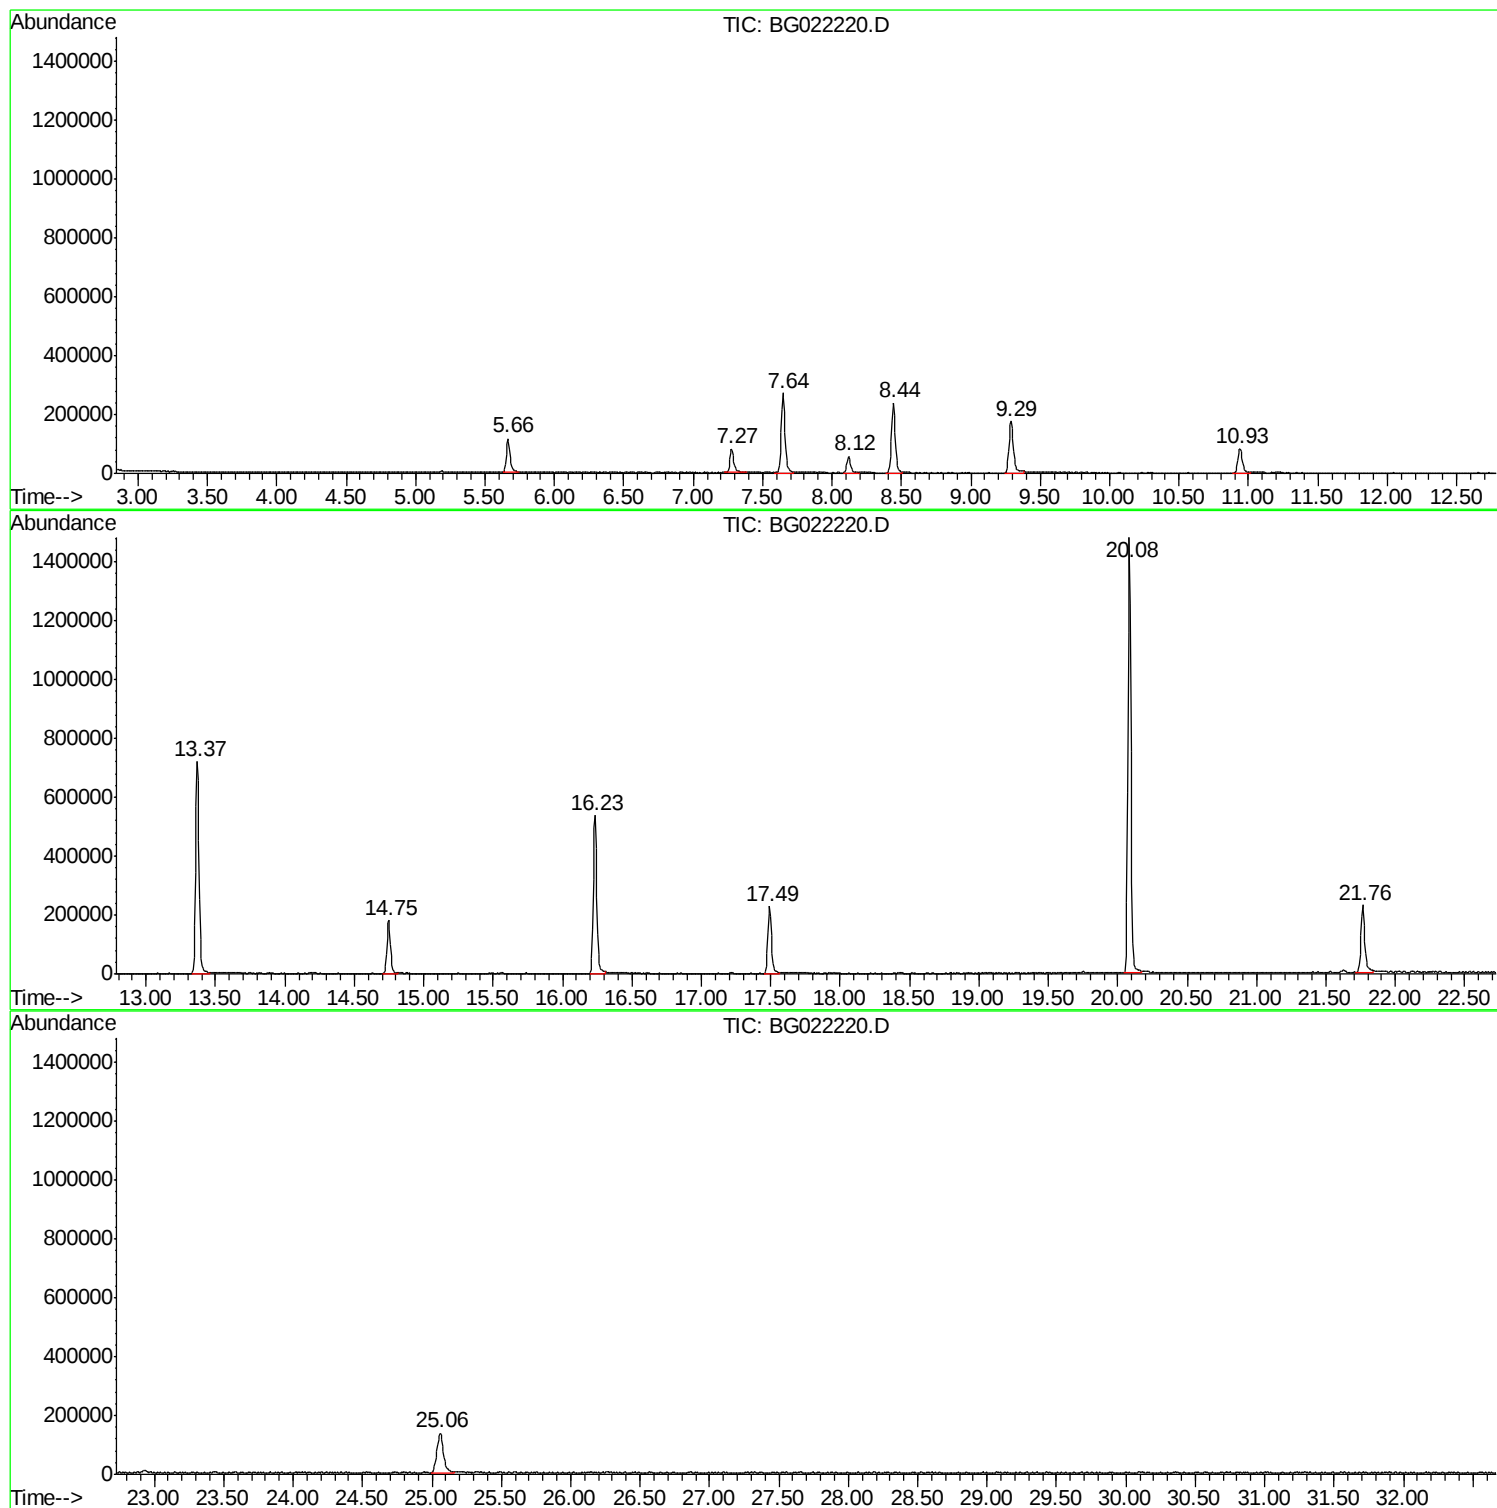

Data Path : Z:\HPCHEM1\BNA G\DATA\BG060716\
Data File : BG022220.D
Acq On : 8 Jun 2016 1:27
Operator : UM/SJ
Sample : H3426-04
Misc :
ALS Vial : 14 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
GW-6










Quant Method : Z:\HPCHEM1\BNA G\METHODS\8270-BG060616.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\DATABASE\NIST02.L
TIC Integration Parameters: LSCINT.P

Peak Number 1 unknown7.64 Concentration Rank 1

R.T.	EstConc	Area	Relative to ISTD	R.T.
7.64	96.70 ng	536316	1,4-Dichlorobenzene-d4	8.12

Hit#	of	Tentative ID	MW	MolForm	CAS#	Qual
1	5	3-Chloro-6-fluoro-pyrazine	132	C4H2ClFN2	1000146-10-7	25
2		(E)-3-Chloro-2-methyl-2-pentenal	132	C6H9ClO	031357-76-3	25
3		4-Chloro-2-fluoro-pyrimidine	132	C4H2ClFN2	051422-00-5	9
4		4-Chloro-6-fluoro-pyrimidine	132	C4H2ClFN2	051422-01-6	9
5		Xenon	132	Xe	007440-63-3	9

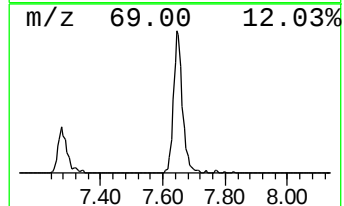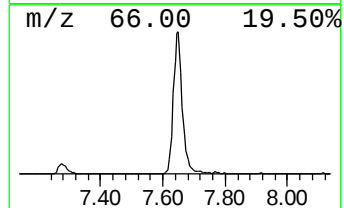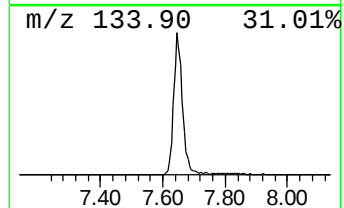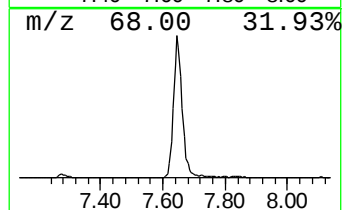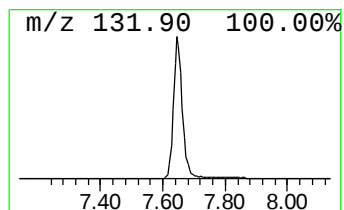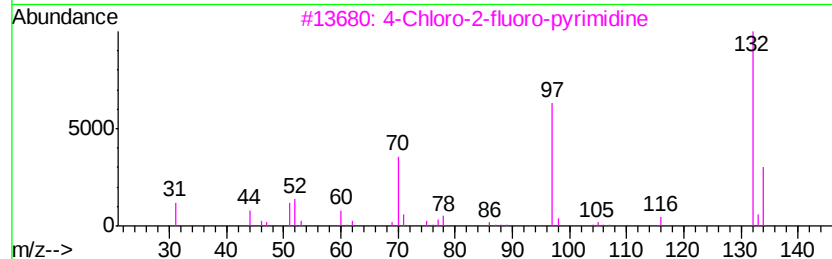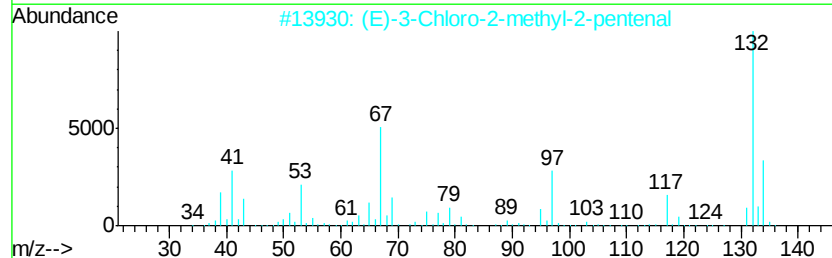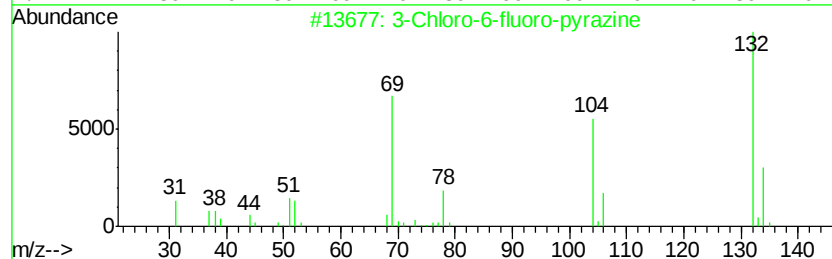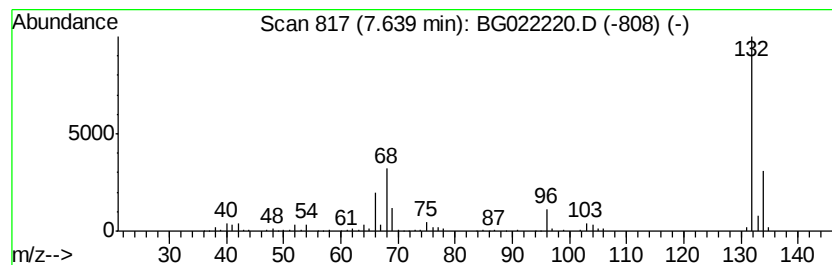

Data Path : Z:\HPCHEM1\BNA_G\DATA\BG060716\
Data File : BG022220.D
Acq On : 8 Jun 2016 1:27
Operator : UM/SJ
Sample : H3426-04
Misc :
ALS Vial : 14 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
GW-6

Quant Method : Z:\HPCHEM1\BNA_G\METHODS\8270-BG060616.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\DATABASE\NIST02.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc
unknown7.64	7.64	96.7	ng	536316	1	8.12	110928	20.0