


Data Path : Z:\HPCHEM1\BNA G\DATA\BG060716\
 Data File : BG022207.D
 Acq On : 7 Jun 2016 16:44
 Operator : UM/SJ
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_G
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\HPCHEM1\BNA_G\METHODS\8270-BG060616.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Mon Jun 06 16:12:45 2016

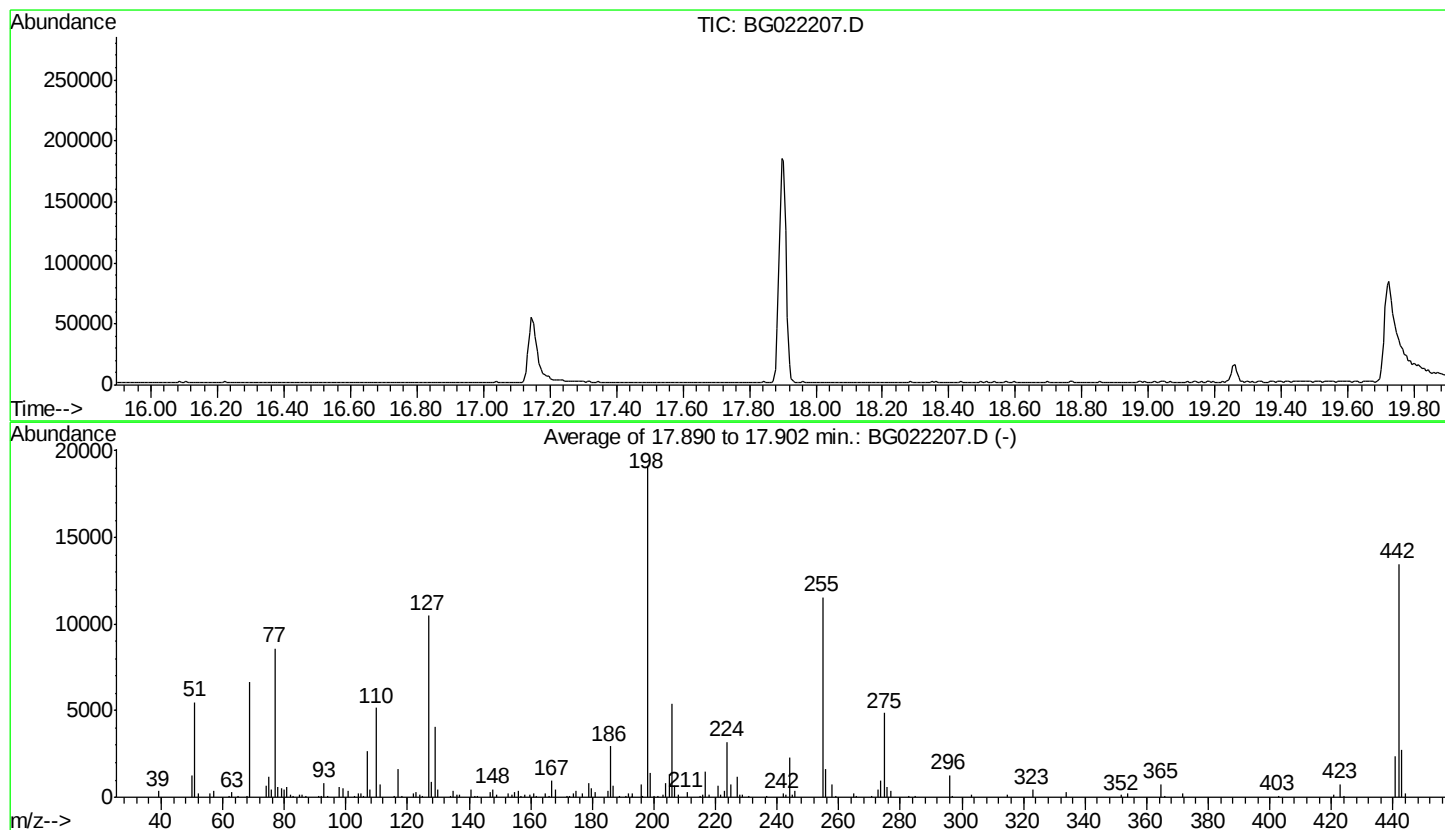

AutoFind: Scans 2562, 2563, 2564; Background Corrected with Scan 2556

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	28.6	5471	PASS
68	69	0.00	2	1.1	71	PASS
69	198	0.00	100	34.6	6628	PASS
70	69	0.00	2	0.0	0	PASS
127	198	10	80	54.8	10492	PASS
197	198	0.00	2	0.0	0	PASS
198	198	100	100	100.0	19149	PASS
199	198	5	9	7.4	1416	PASS
275	198	10	60	25.4	4863	PASS
365	198	1	100	4.0	767	PASS
441	442	0.01	24	17.6	2363	PASS
442	198	50	100	70.3	13456	PASS
443	442	15	24	20.3	2728	PASS