

Data Path : Z:\HPCHEM1\BNA G\DATA\BG060717\
 Data File : BG027303.D
 Acq On : 8 Jun 2017 3:48
 Operator : SJ/MA
 Sample : I3488-03
 Misc :
 ALS Vial : 18 Sample Multiplier: 1

Instrument :
 BNA_G
 ClientSampleId :

Quant Time: Jun 08 06:14:31 2017
 Quant Method : Z:\HPCHEM1\BNA G\METHODS\8270-BG060517.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Mon Jun 05 16:00:35 2017
 Response via : Initial Calibration


Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Dichlorobenzene-d4	8.56	152	43040	20.00	ng	-0.02
21) Naphthalene-d8	11.38	136	200351	20.00	ng	-0.02
38) Acenaphthene-d10	15.14	164	135610	20.00	ng	-0.02
63) Phenanthrene-d10	17.89	188	347833	20.00	ng	-0.03
75) Chrysene-d12	22.27	240	395571	20.00	ng	-0.04
86) Perylene-d12	25.95	264	365099	20.00	ng	-0.07
System Monitoring Compounds						
5) 2-Fluorophenol	6.14	112	450216	159.62	ng	-0.02
7) Phenol-d6	7.69	99	585575	141.44	ng	-0.01
23) Nitrobenzene-d5	9.72	82	390739	122.65	ng	-0.02
41) 2,4,6-Tribromophenol	16.62	330	331962	185.90	ng	-0.02
44) 2-Fluorobiphenyl	13.77	172	952678	98.28	ng	-0.02
78) Terphenyl-d14	20.46	244	1662450	107.21	ng	-0.03
Target Compounds						
15) Benzyl Alcohol	8.88	79	5982	2.05	ng	Qvalue # 45


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\HPCHEM1\BNA G\DATA\BG060717\
Data File : BG027303.D
Acq On : 8 Jun 2017 3:48
Operator : SJ/MA
Sample : I3488-03
Misc :
ALS Vial : 18 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :

Quant Time: Jun 08 06:14:31 2017
Quant Method : Z:\HPCHEM1\BNA G\METHODS\8270-BG060517.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Mon Jun 05 16:00:35 2017
Response via : Initial Calibration

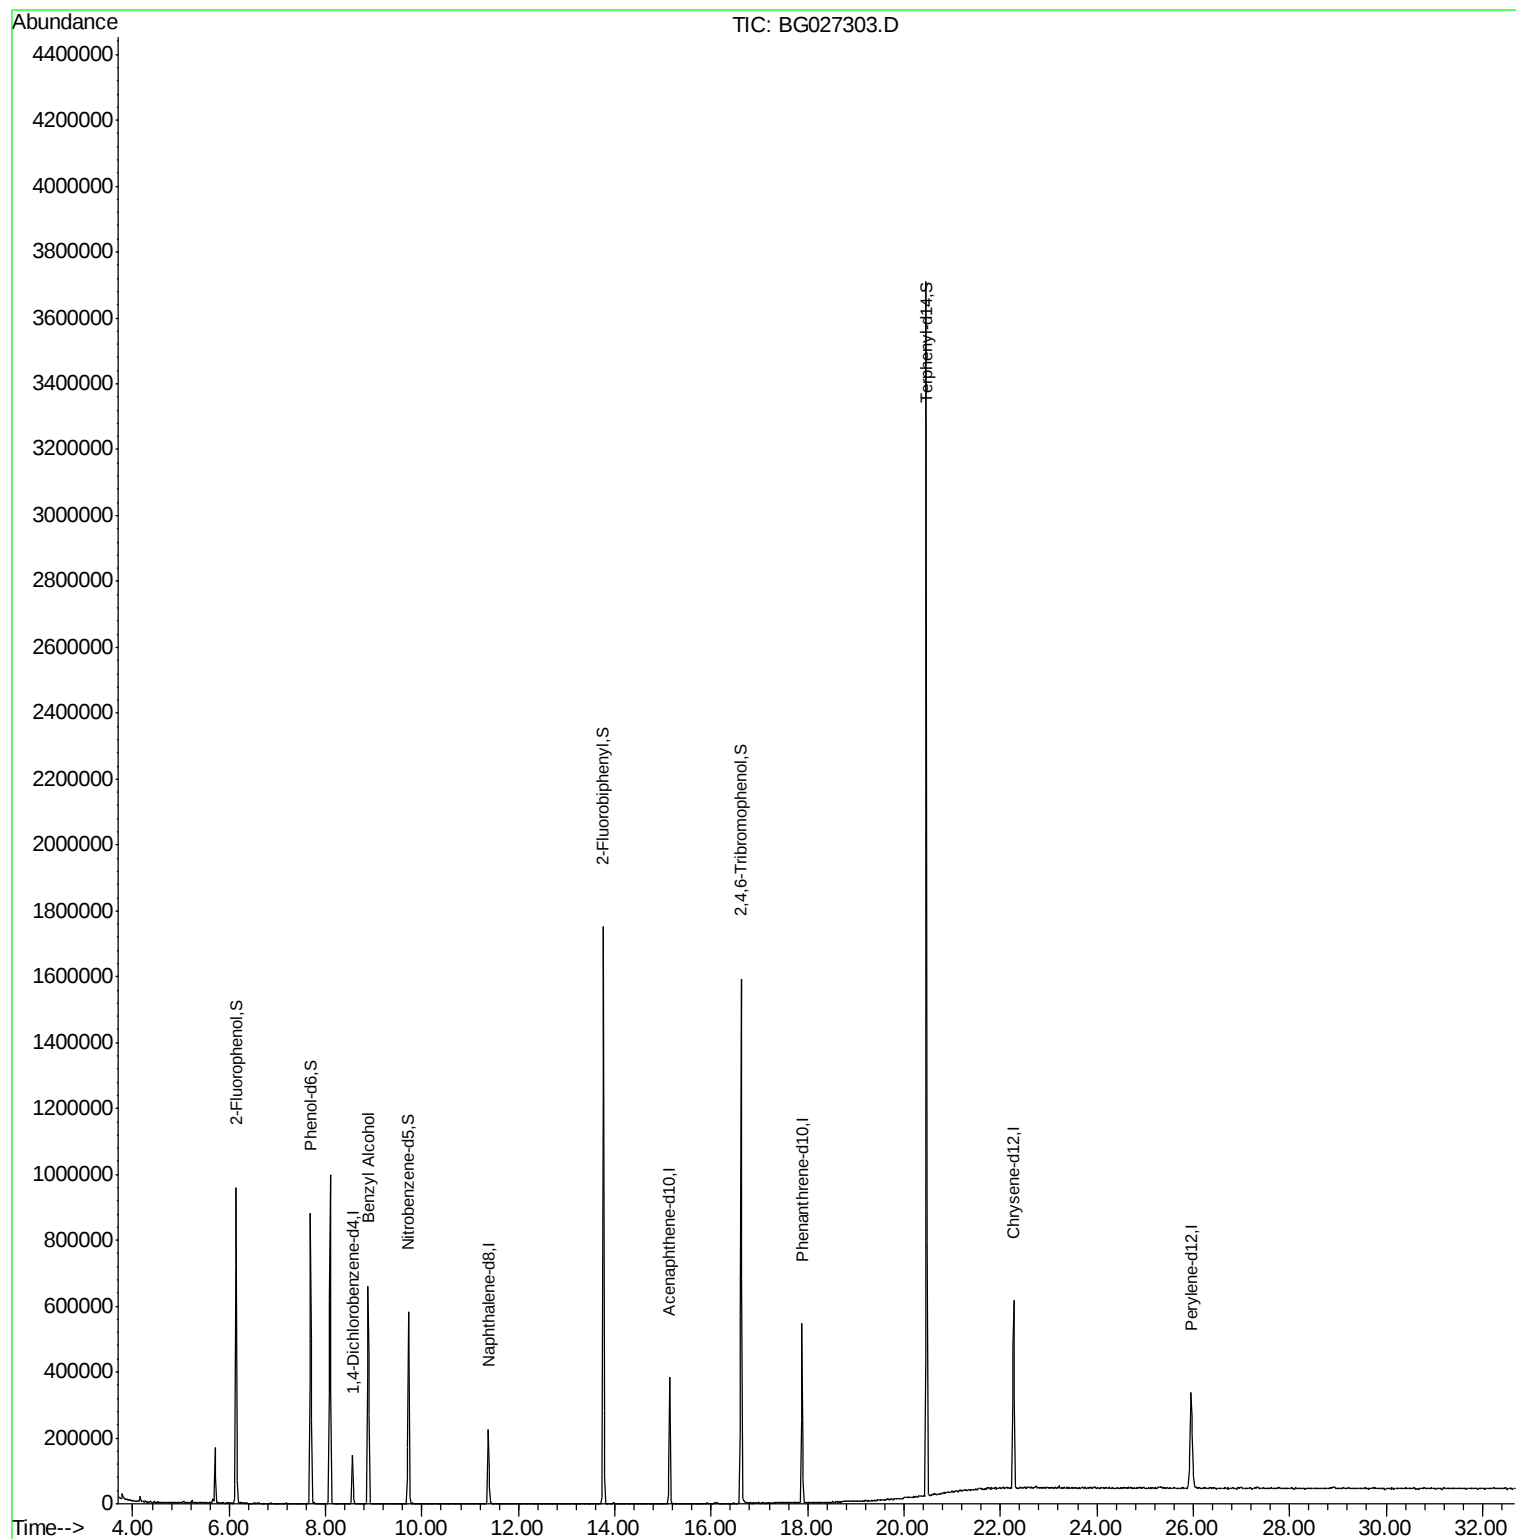

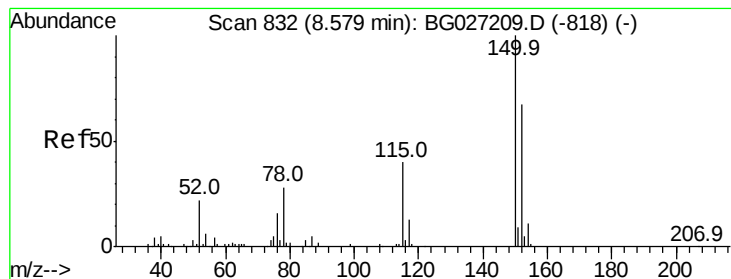

#1

1,4-Dichlorobenzene-d4

Concen: 20.00 ng

RT: 8.56 min Scan# 829

Delta R.T. -0.02 min

Lab File: BG027303.D

Acq: 8 Jun 2017 3:48

Instrument :

BNA_G

ClientSampled :


Tot Ion:152 Resp: 43040

Ion Ratio Lower Upper

152 100

150 163.0 114.0 171.0




115 69.7 48.1 72.1

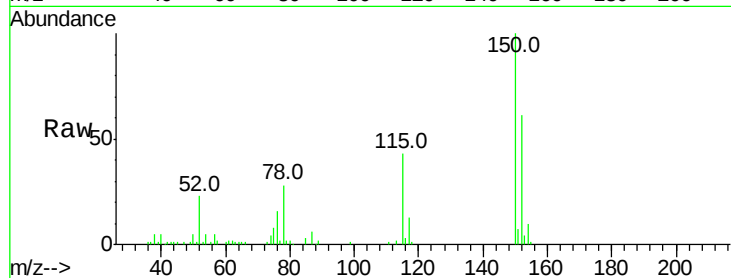

Abundance Ion 152.00 (151.70 to 152.70): E

Ion 150.00 (149.70 to 150.70): E

Ion 115.00 (114.70 to 115.70): E

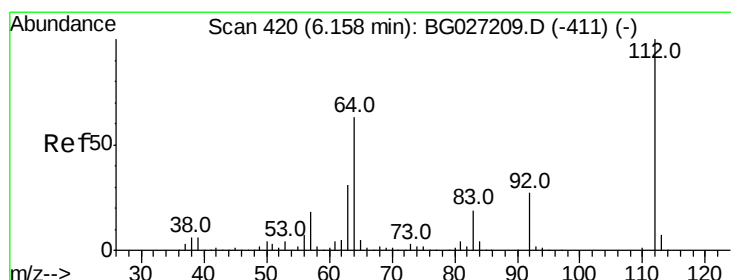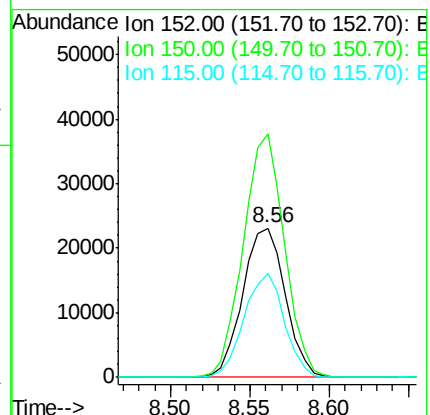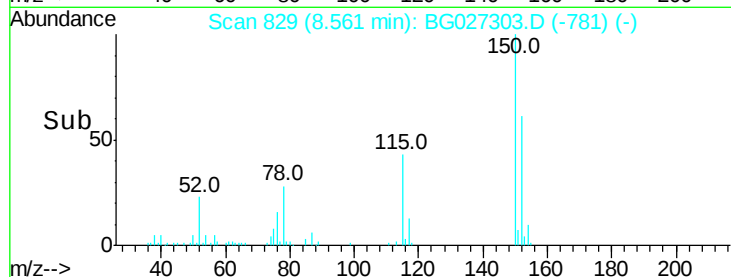

#5

2-Fluorophenol

Concen: 159.62 ng

RT: 6.14 min Scan# 417

Delta R.T. -0.02 min

Lab File: BG027303.D

Acq: 8 Jun 2017 3:48


Tgt Ion:112 Resp: 450216

Ion Ratio Lower Upper

112 100

64 67.8 61.8 92.6



63 33.2 37.2 55.8#

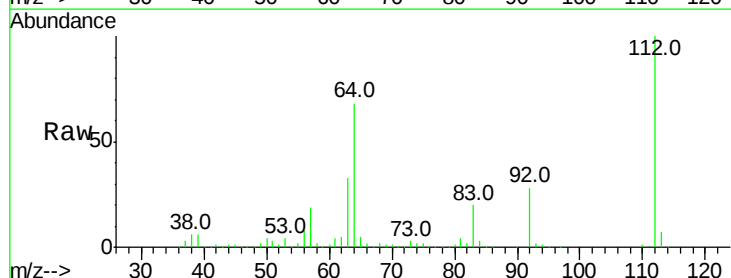

Abundance Ion 112.00 (111.70 to 112.70): E

Ion 64.00 (63.70 to 64.70): BGC

Ion 63.00 (62.70 to 63.70): BGC

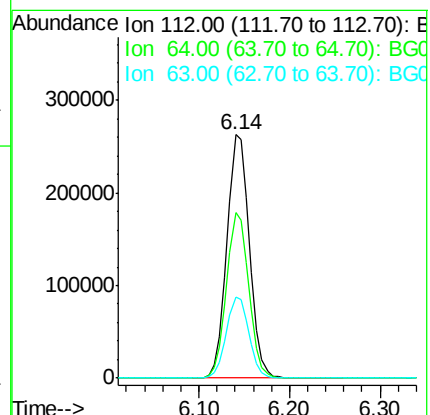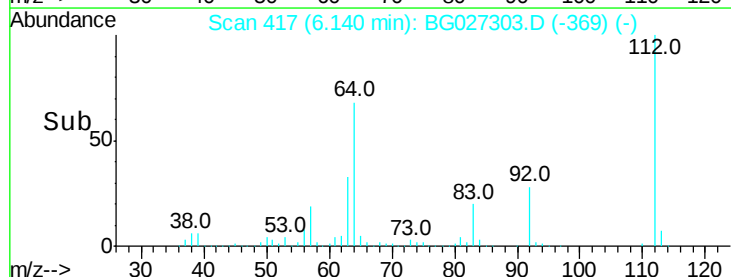



#7

Phenol-d6

Concen: 141.44 ng

RT: 7.69 min Scan# 681

Delta R.T. -0.01 min

Lab File: BG027303.D

Acq: 8 Jun 2017 3:48

Instrument :

BNA_G

ClientSampleId :


Tot Ion: 99 Resp: 585575

Ion Ratio Lower Upper




99 100

42 16.9 20.5 30.7#

71 31.8 37.6 56.4#

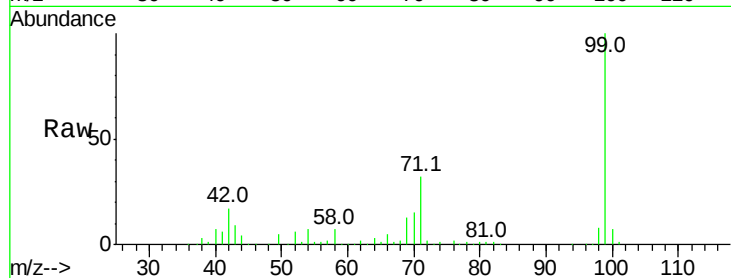

Abundance Ion 99.00 (98.70 to 99.70): BGC
Ion 42.00 (41.70 to 42.70): BGC
Ion 71.00 (70.70 to 71.70): BGC

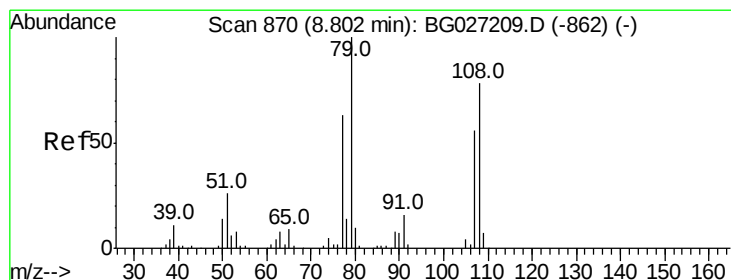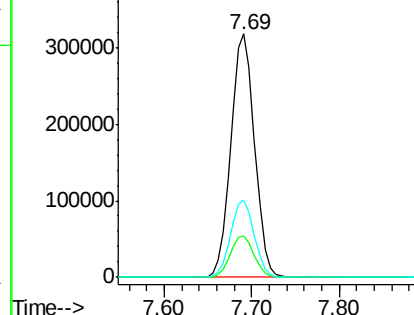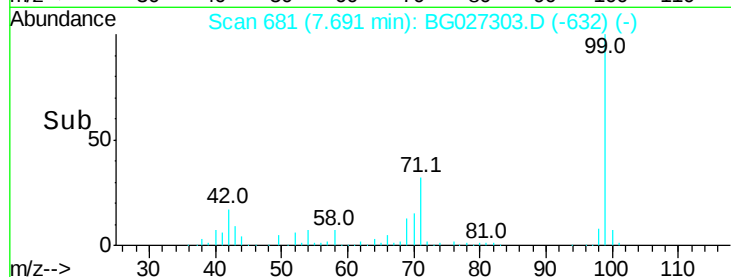

#15

Benzyl Alcohol

Concen: 2.05 ng

RT: 8.88 min Scan# 884

Delta R.T. 0.08 min

Lab File: BG027303.D

Acq: 8 Jun 2017 3:48


Tgt Ion: 79 Resp: 5982

Ion Ratio Lower Upper



79 100


108 29.7 45.5 68.3#

77 123.8 54.3 81.5#

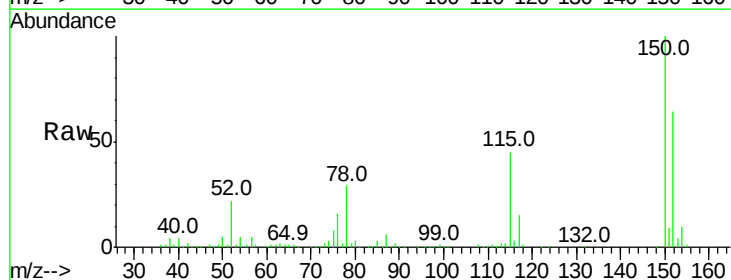

Abundance Ion 79.00 (78.70 to 79.70): BGC
Ion 108.00 (107.70 to 108.70): BGC
Ion 77.00 (76.70 to 77.70): BGC

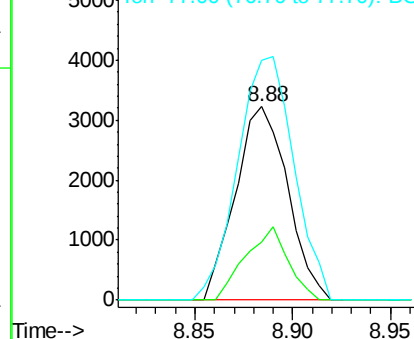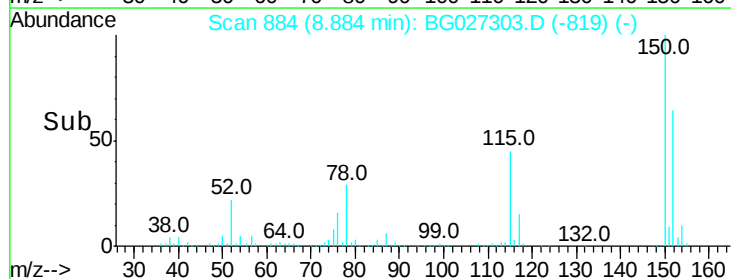


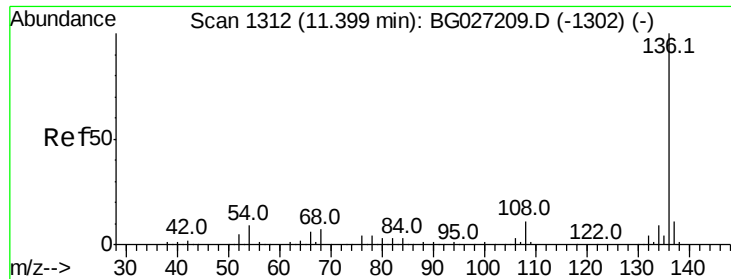




#21
Naphthalene-d8
Concen: 20.00 ng
RT: 11.38 min Scan# 1308
Delta R.T. -0.02 min
Lab File: BG027303.D
Acq: 8 Jun 2017 3:48

Instrument :
BNA_G
ClientSampleId :

Tot Ion:136	Resp:	200351
Ion Ratio	Lower	Upper
136	100	
137	11.1	8.9 13.3
54	10.4	9.3 13.9
68	8.0	5.1 7.7#

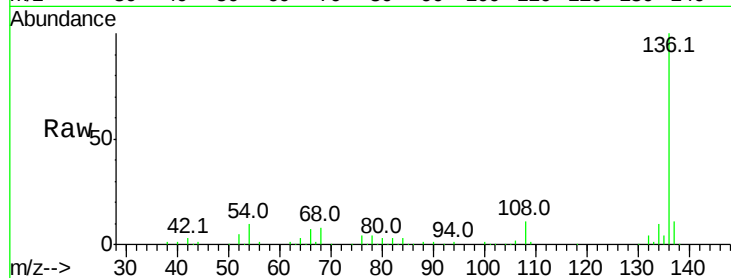


Abundance Ion 136.00 (135.70 to 136.70): BGC
Ion 137.00 (136.70 to 137.70): BGC
Ion 54.00 (53.70 to 54.70): BGC
Ion 68.00 (67.70 to 68.70): BGC

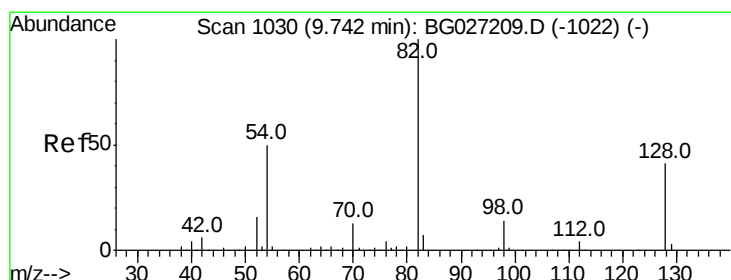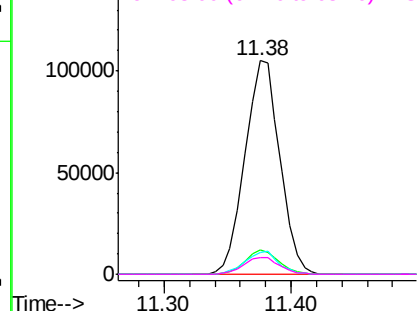
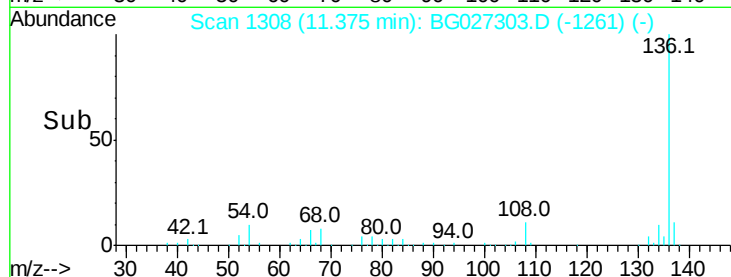



#23
Nitrobenzene-d5
Concen: 122.65 ng
RT: 9.72 min Scan# 1026
Delta R.T. -0.02 min
Lab File: BG027303.D
Acq: 8 Jun 2017 3:48

Tgt Ion: 82	Resp:	390739
Ion Ratio	Lower	Upper
82	100	
128	40.3	26.4 39.6#
54	51.9	49.4 74.2

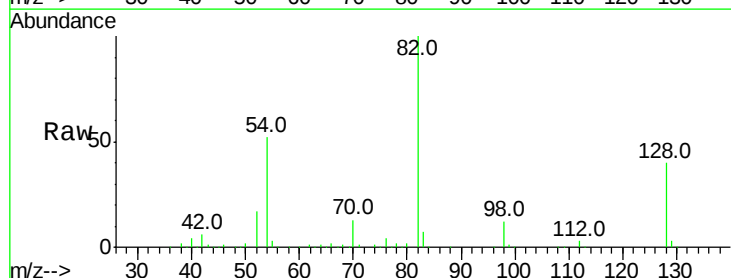

Abundance Ion 82.00 (81.70 to 82.70): BGC
Ion 128.00 (127.70 to 128.70): BGC
Ion 54.00 (53.70 to 54.70): BGC



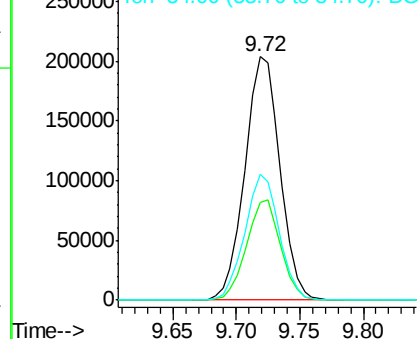
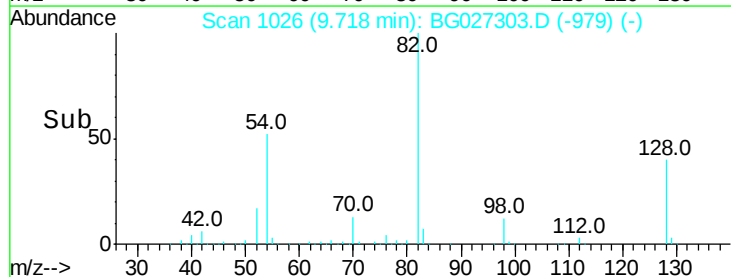


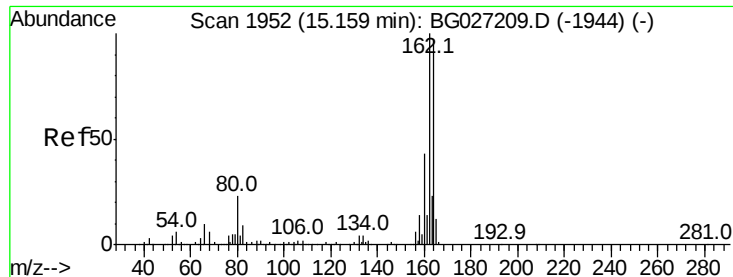

#38
 Acenaphthene-d10
 Concen: 20.00 ng
 RT: 15.14 min Scan# 1948
 Delta R.T. -0.02 min
 Lab File: BG027303.D
 Acq: 8 Jun 2017 3:48




Instrument :
 BNA_G
 ClientSampleId :

Tot Ion:164 Resp: 135610
 Ion Ratio Lower Upper
 164 100
 162 101.7 85.1 127.7
 160 43.9 34.7 52.1

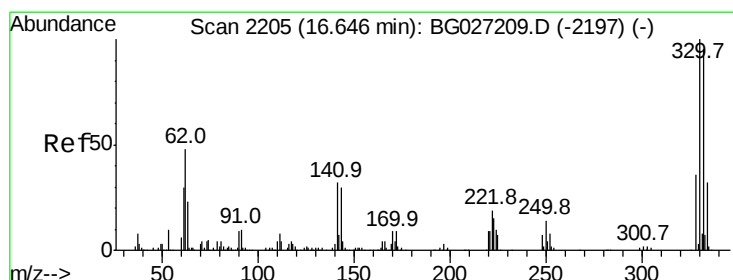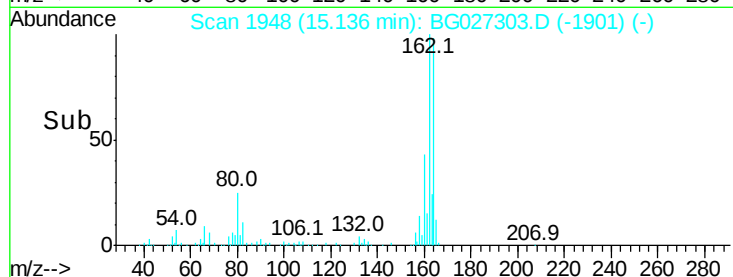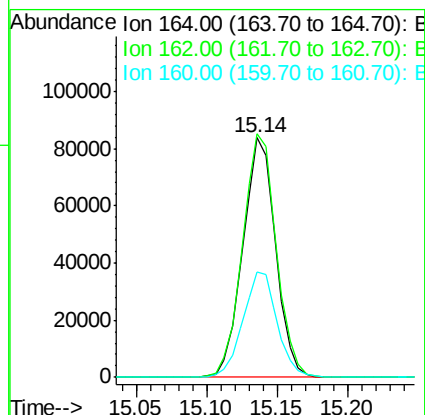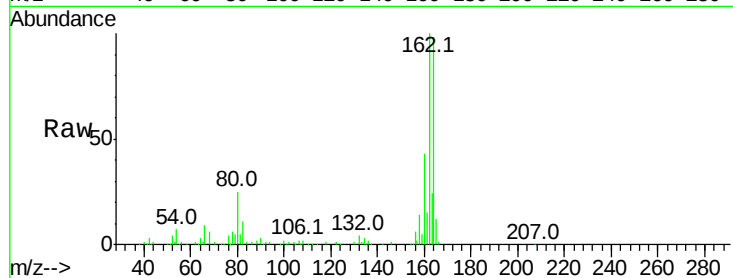

#41
 2,4,6-Tribromophenol
 Concen: 185.90 ng
 RT: 16.62 min Scan# 2201
 Delta R.T. -0.02 min
 Lab File: BG027303.D
 Acq: 8 Jun 2017 3:48

Tgt Ion:330 Resp: 331962
 Ion Ratio Lower Upper
 330 100
 332 96.3 77.3 115.9
 141 32.8 32.1 48.1


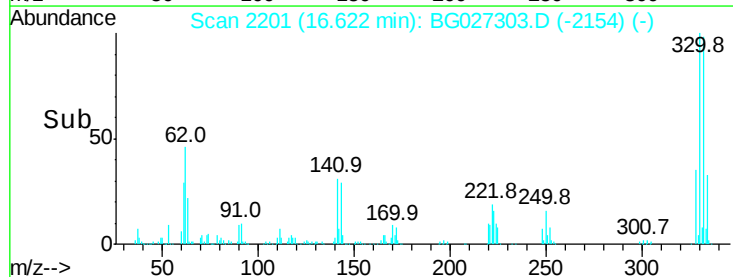
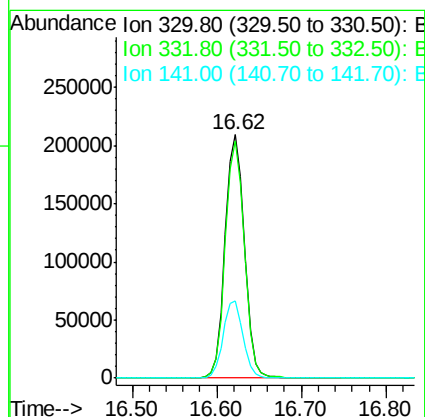
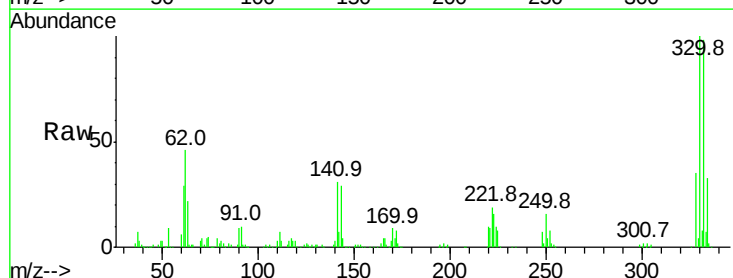




#44
2-Fluorobiphenyl
Concen: 98.28 ng
RT: 13.77 min Scan# 1715
Delta R.T. -0.02 min
Lab File: BG027303.D
Acq: 8 Jun 2017 3:48




Instrument :
BNA_G
ClientSampleId :


Tot Ion:172 Resp: 952678
Ion Ratio Lower Upper
172 100
171 37.2 32.2 48.2
170 24.9 21.8 32.6

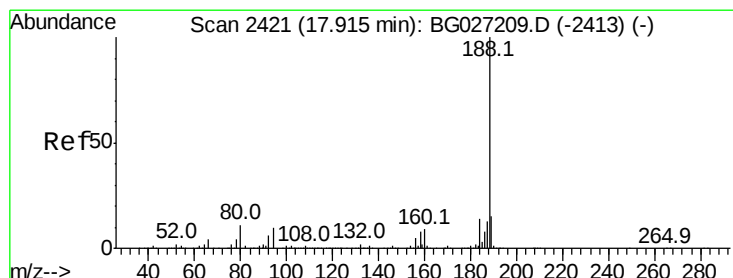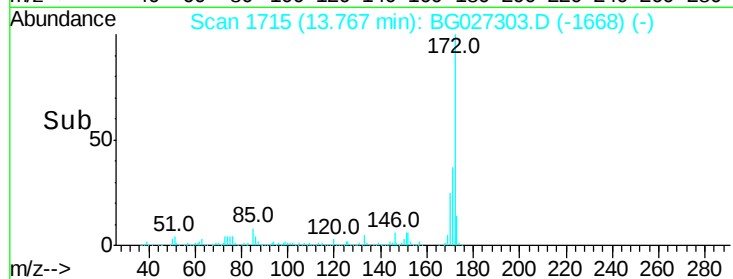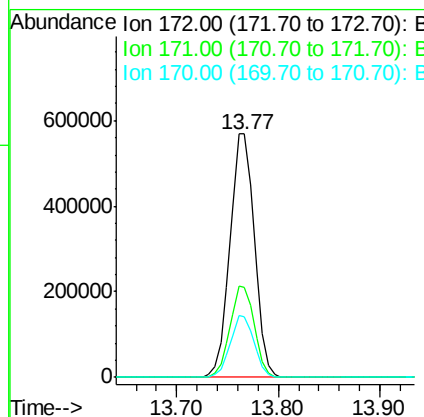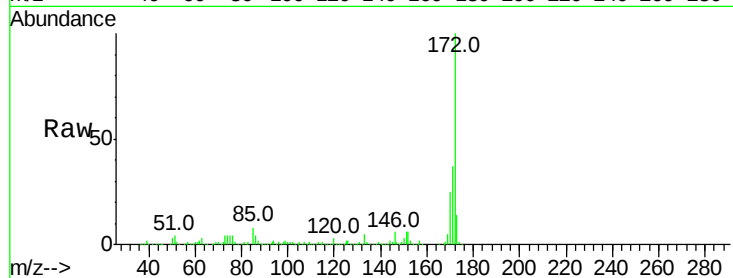

#63
Phenanthrene-d10
Concen: 20.00 ng
RT: 17.89 min Scan# 2416
Delta R.T. -0.03 min
Lab File: BG027303.D
Acq: 8 Jun 2017 3:48

Tgt Ion:188 Resp: 347833
Ion Ratio Lower Upper
188 100
94 10.6 5.8 8.8#
80 12.8 7.5 11.3#

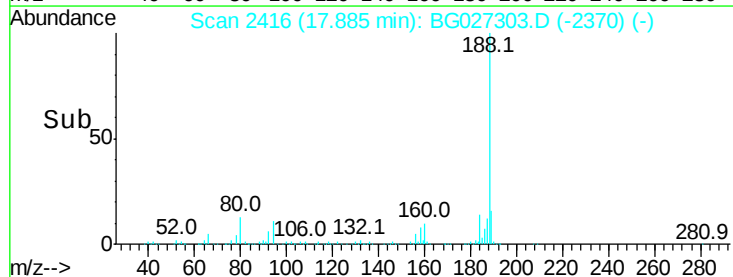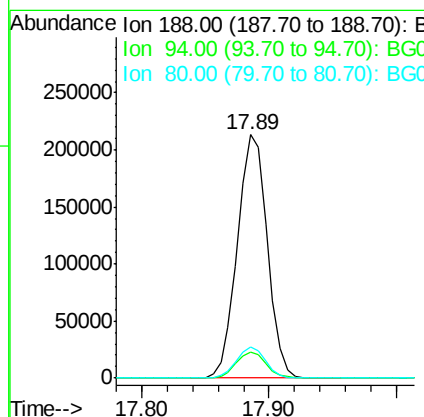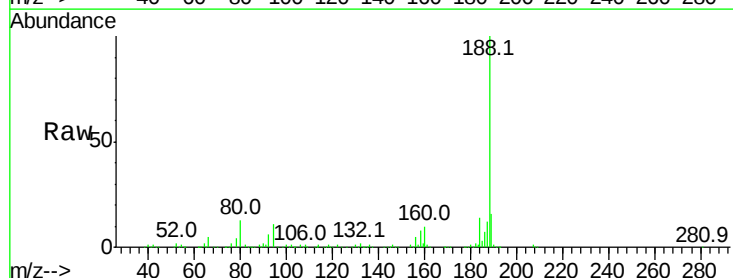

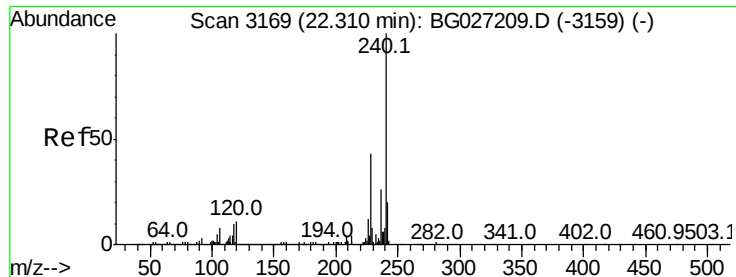

#75

Chrysene-d12

Concen: 20.00 ng

RT: 22.27 min Scan# 3163

Delta R.T. -0.04 min

Lab File: BG027303.D

Acq: 8 Jun 2017 3:48

Instrument :

BNA_G

ClientSampleId :


Tot Ion:240 Resp: 395571

Ion Ratio Lower Upper

240 100

120 11.2 5.7 8.5#




236 25.4 22.2 33.4

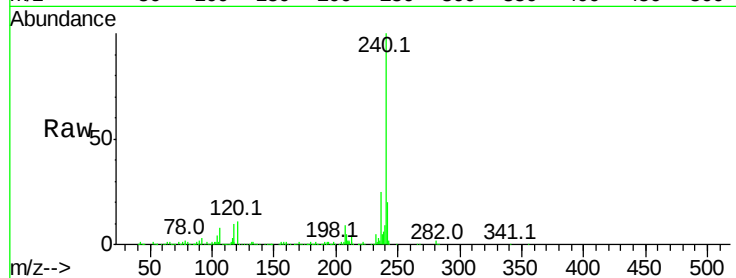

Abundance Ion 240.00 (239.70 to 240.70): E

Ion 120.00 (119.70 to 120.70): E

Ion 236.00 (235.70 to 236.70): E

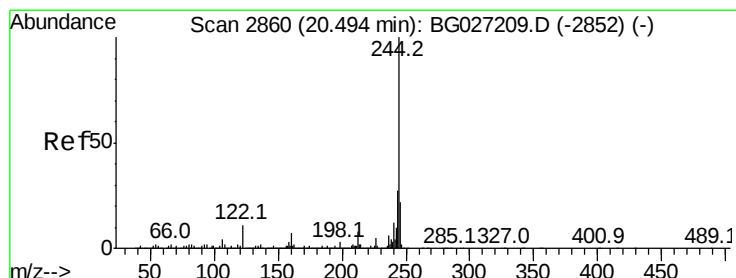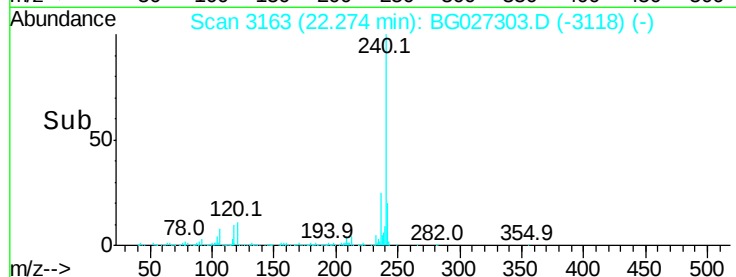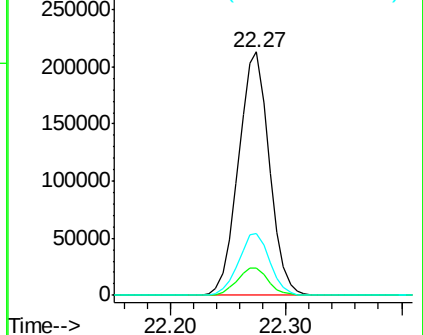

#78

Terphenyl-d14

Concen: 107.21 ng

RT: 20.46 min Scan# 2855

Delta R.T. -0.03 min

Lab File: BG027303.D

Acq: 8 Jun 2017 3:48


Tgt Ion:244 Resp: 1662450

Ion Ratio Lower Upper

244 100

212 8.3 10.0 15.0#



122 12.4 8.6 12.8

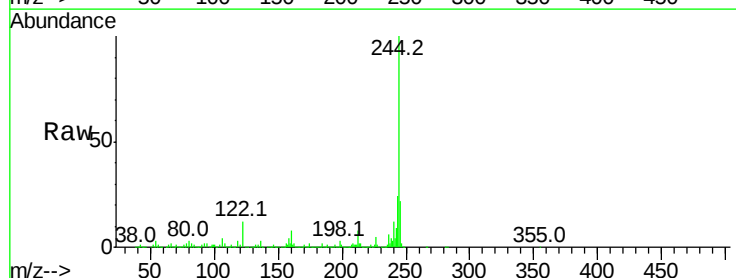


Abundance Ion 244.00 (243.70 to 244.70): E

Ion 212.00 (211.70 to 212.70): E

Ion 122.00 (121.70 to 122.70): E

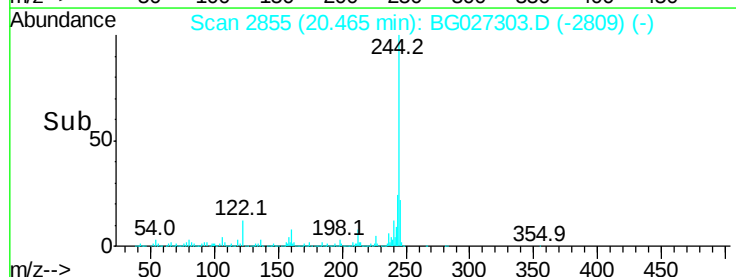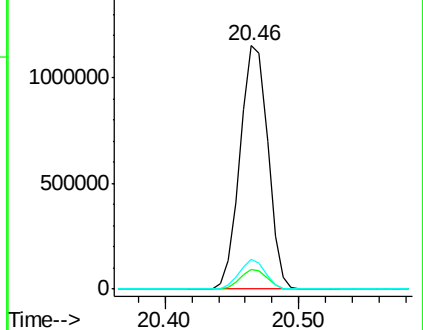


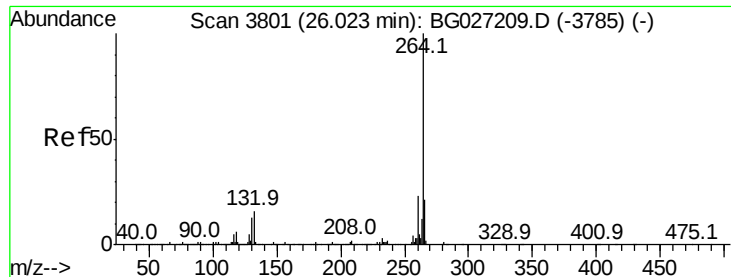

#86
 Pervlene-d12
 Concen: 20.00 ng
 RT: 25.95 min Scan# 3789
 Delta R.T. -0.07 min
 Lab File: BG027303.D
 Acq: 8 Jun 2017 3:48

Instrument :
 BNA_G
 ClientSampleId :

Tot Ion	Ratio	Lower	Upper
264	100		
260	23.9	21.8	32.8
265	22.3	18.2	27.4

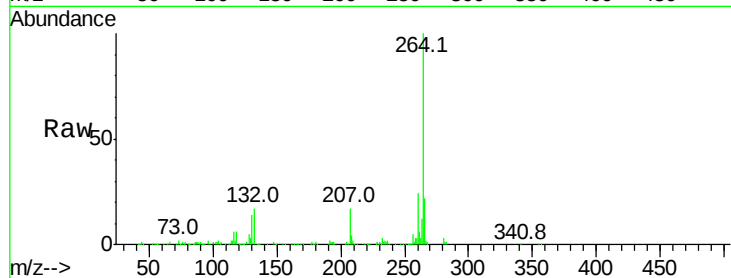

Abundance Ion 264.00 (263.70 to 264.70): E
 Ion 260.00 (259.70 to 260.70): E
 Ion 265.00 (264.70 to 265.70): E

