
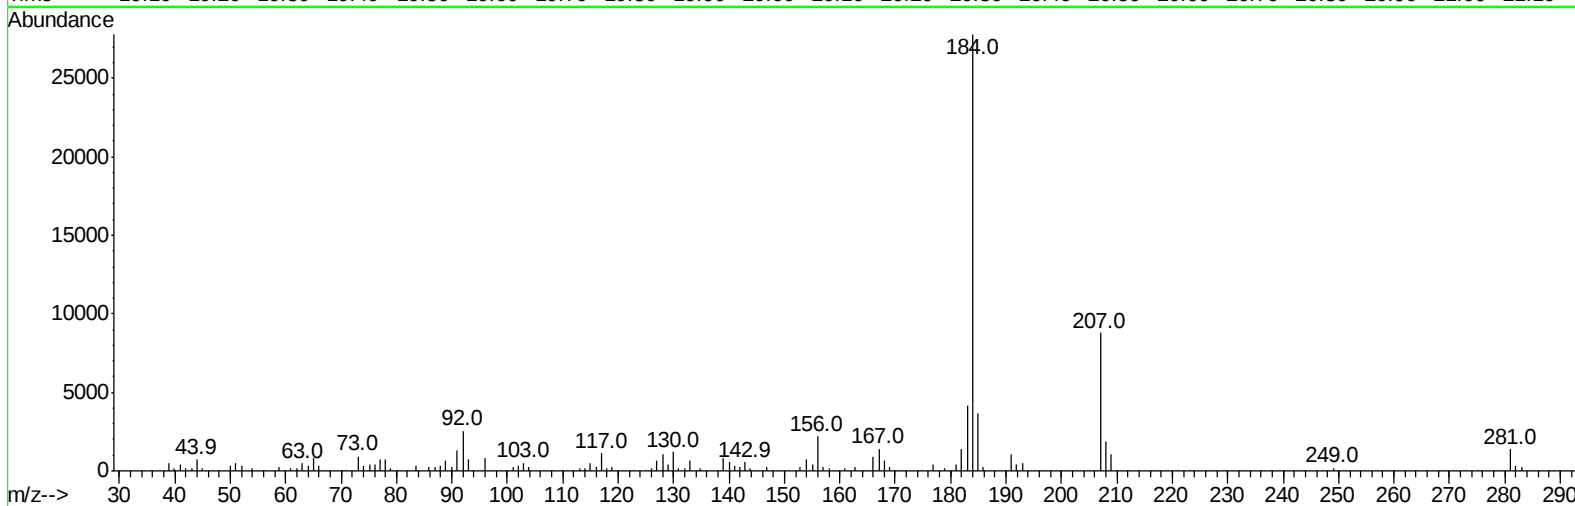


Data Path : Z:\HPCHEM1\BNA G\Data\BG060717\
Data File : BG027286.D
Acq On : 7 Jun 2017 16:41
Operator : SJ/MA
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Jun 08 09:26:55 2017
Quant Method : Z:\HPCHEM1\BNA G\METHODS\8270-BG060517.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Mon Jun 05 16:00:35 2017
Response via : Initial Calibration

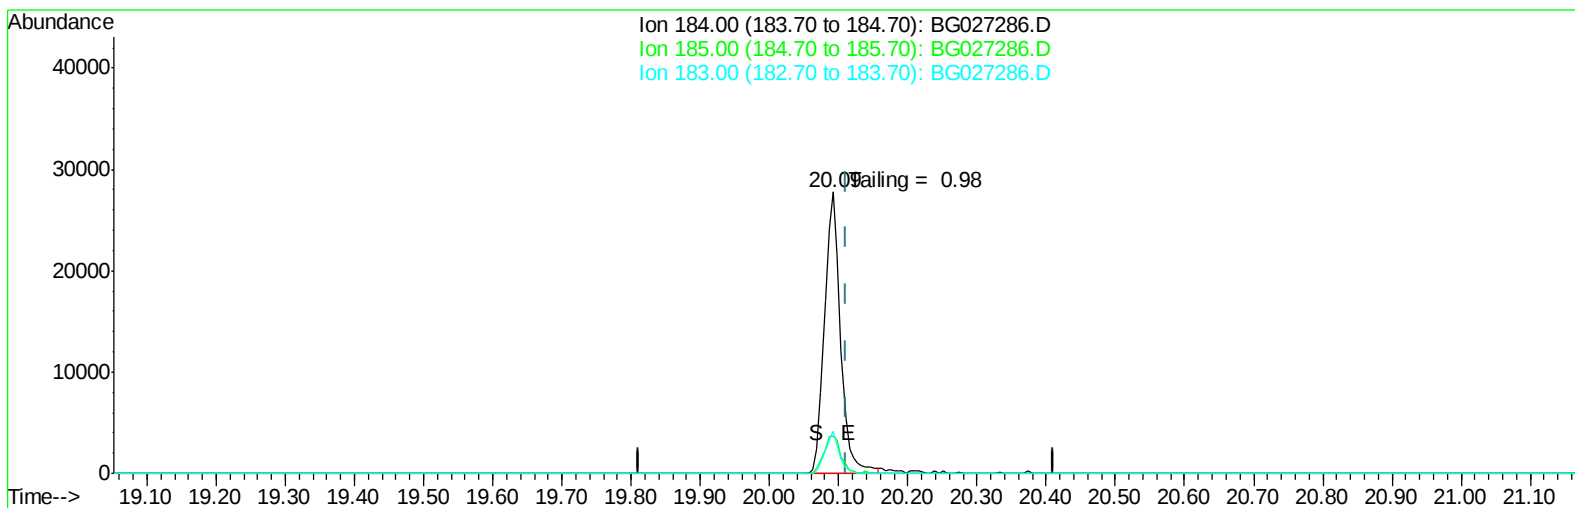

TIC: BG027286.D

(76) Benzidine



20.092min (-0.020) 0.00ng

response 44834

Ion	Exp%	Act%
184.00	100	100
185.00	16.30	13.26
183.00	13.80	14.93
0.00	0.00	0.00

Data Path : Z:\HPCHEM1\BNA G\Data\BG060717\
Data File : BG027286.D
Acq On : 7 Jun 2017 16:41
Operator : SJ/MA
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Jun 08 09:26:55 2017
Quant Method : Z:\HPCHEM1\BNA G\METHODS\8270-BG060517.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Mon Jun 05 16:00:35 2017
Response via : Initial Calibration

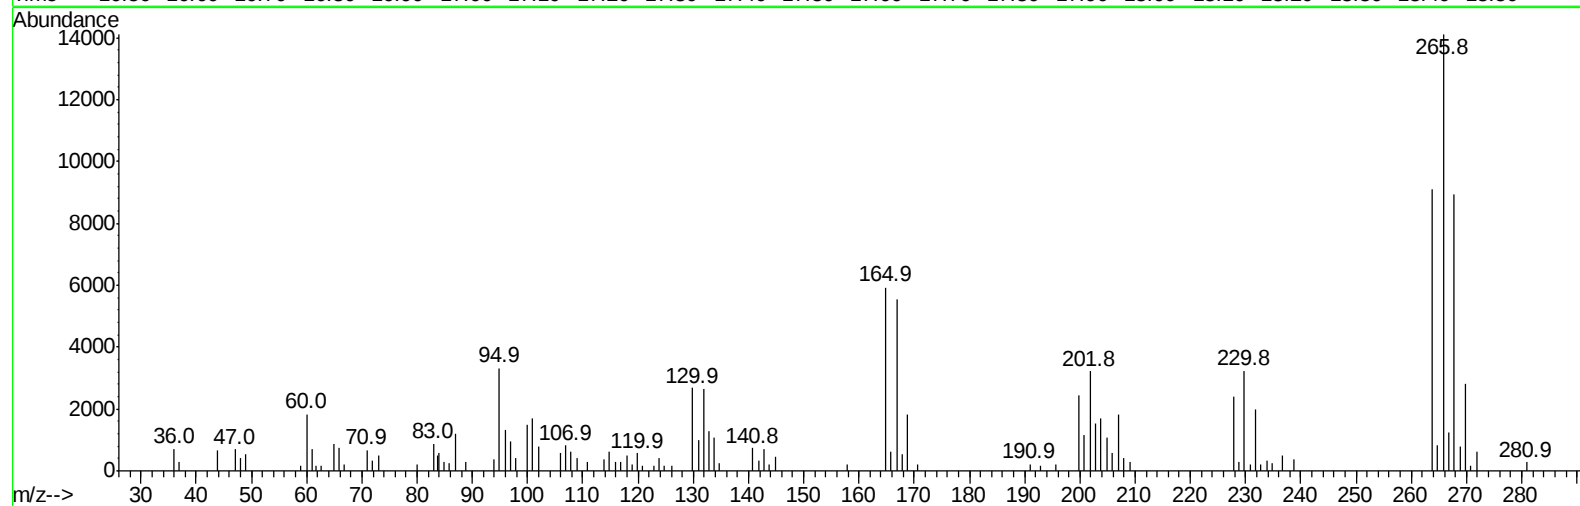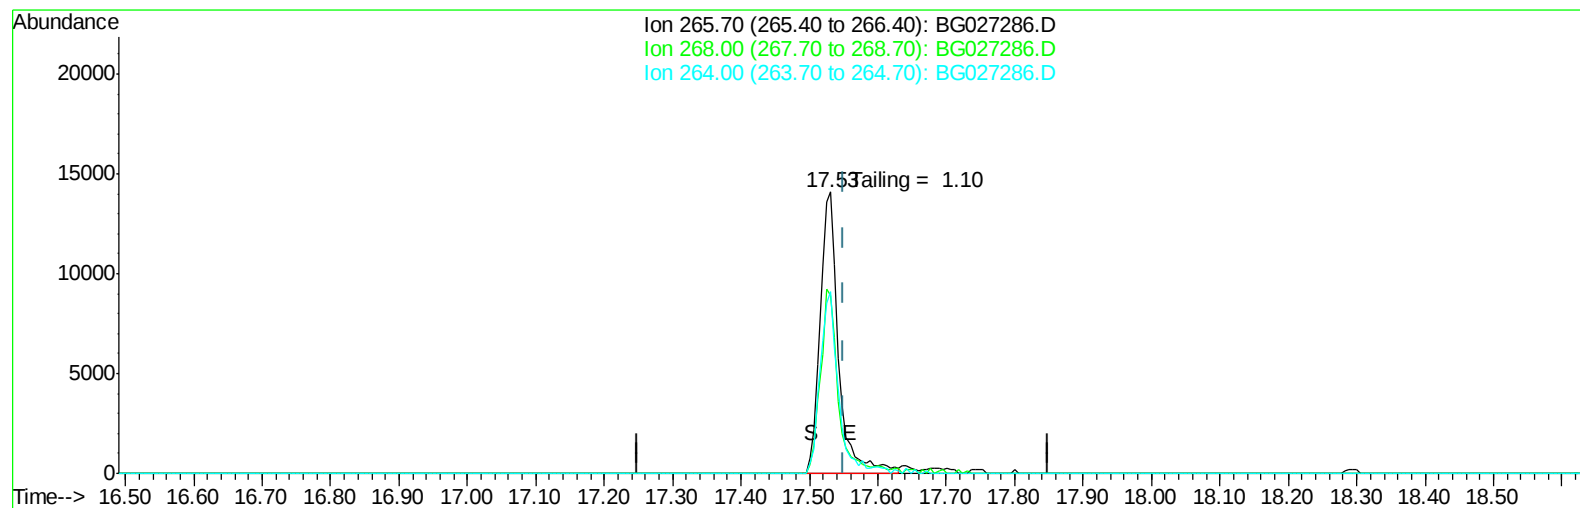

TIC: BG027286.D

(69) Pentachlorophenol (C)

17.530min (-0.020) 0.00ng

response 26436

Ion	Exp%	Act%
265.70	100	100
268.00	60.70	63.38
264.00	62.60	64.62
0.00	0.00	0.00