
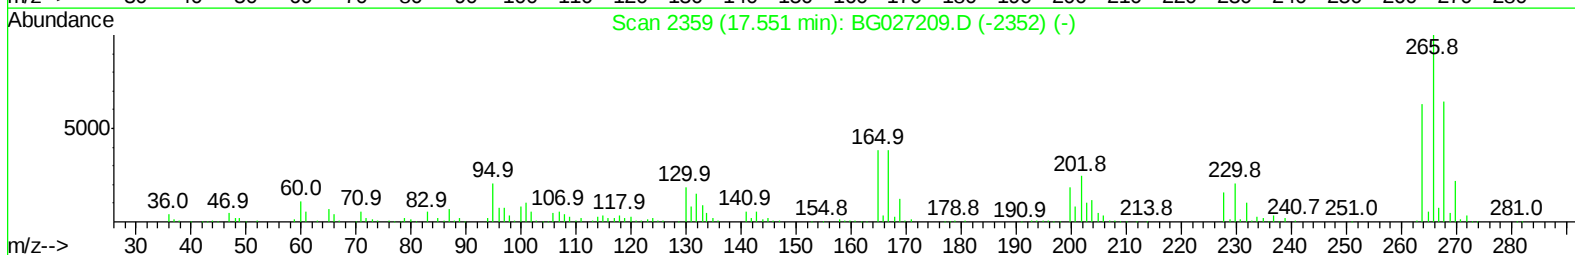
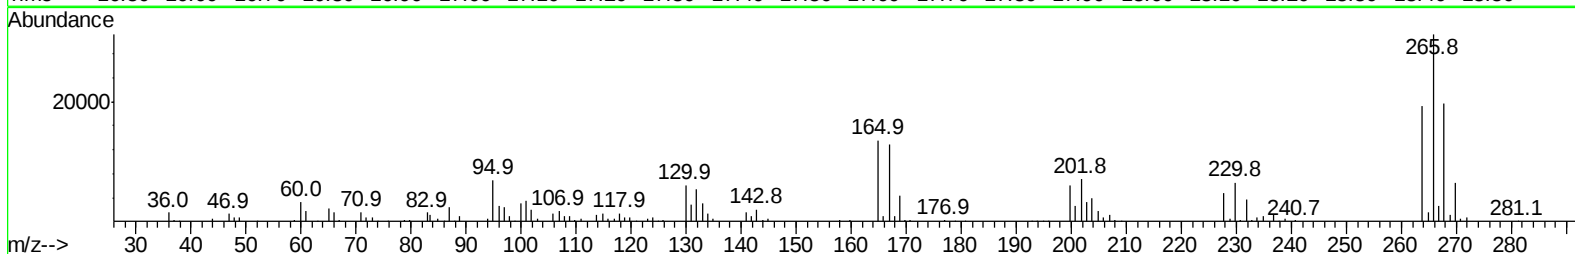


Data Path : Z:\HPCHEM1\BNA G\Data\BG060717\
Data File : BG027305.D
Acq On : 8 Jun 2017 5:57
Operator : SJ/MA
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Jun 08 09:28:08 2017
Quant Method : Z:\HPCHEM1\BNA G\METHODS\8270-BG060517.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Mon Jun 05 16:00:35 2017
Response via : Initial Calibration

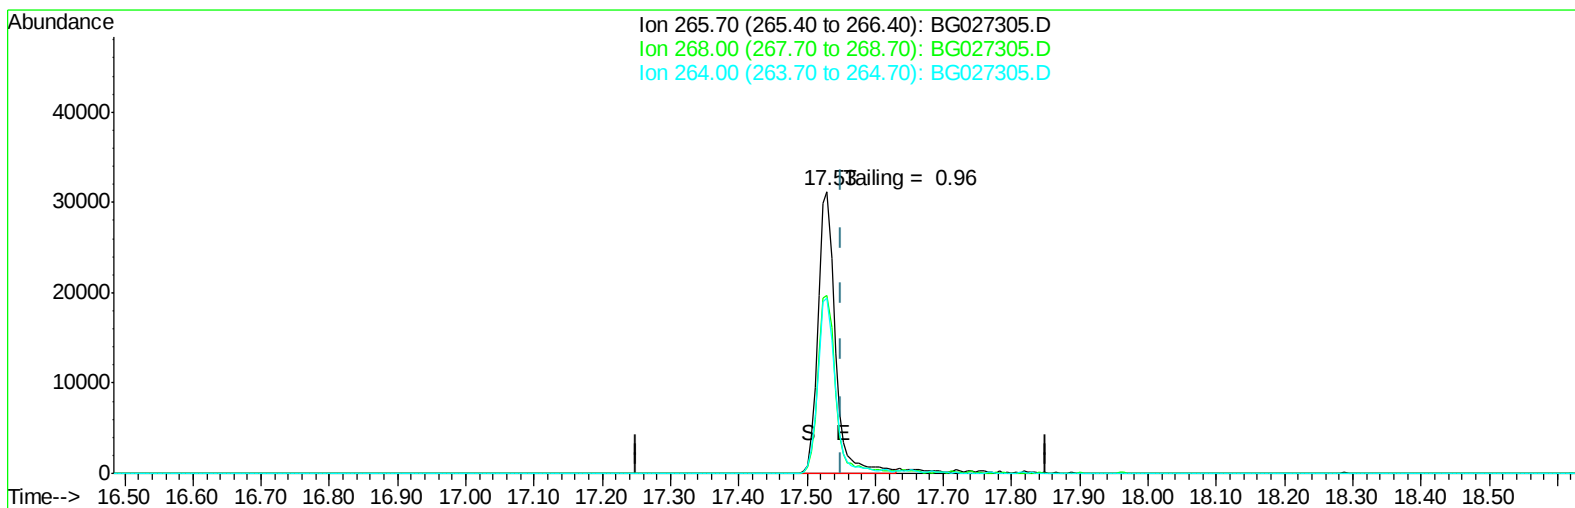

TIC: BG027305.D

(69) Pentachlorophenol (C)




17.530min (-0.020) 0.00ng

response 54423

Ion	Exp%	Act%
265.70	100	100
268.00	60.70	63.29
264.00	62.60	62.11
0.00	0.00	0.00

Data Path : Z:\HPCHEM1\BNA G\Data\BG060717\
Data File : BG027305.D
Acq On : 8 Jun 2017 5:57
Operator : SJ/MA
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Jun 08 09:28:08 2017
Quant Method : Z:\HPCHEM1\BNA G\METHODS\8270-BG060517.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Mon Jun 05 16:00:35 2017
Response via : Initial Calibration

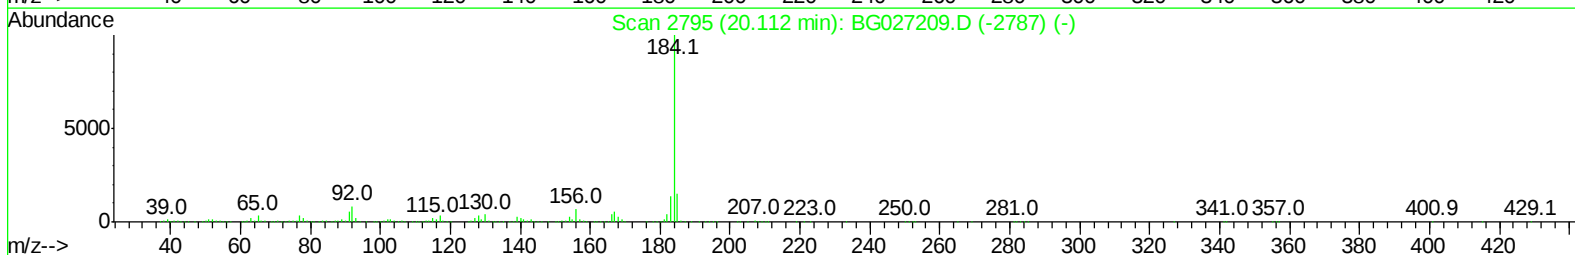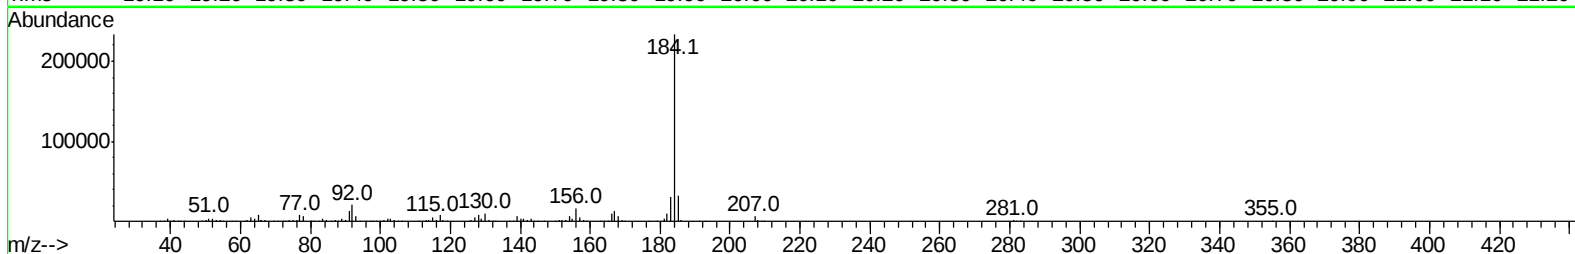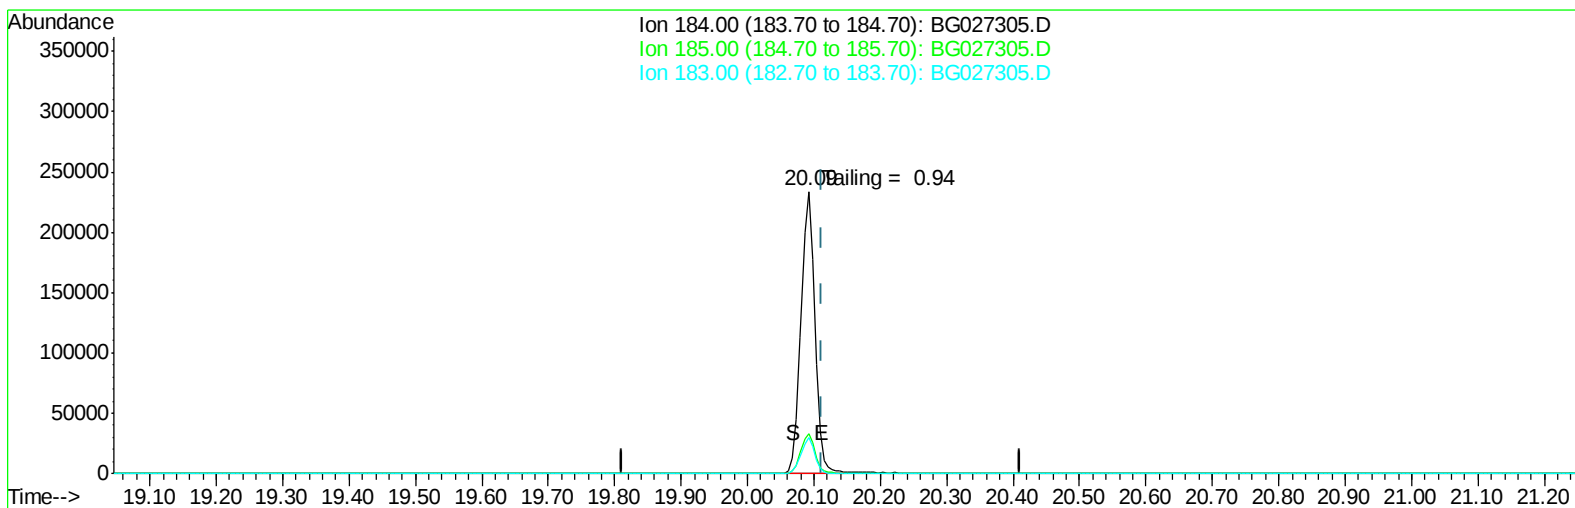

TIC: BG027305.D

(76) Benzidine

20.092min (-0.020) 0.00ng

response 333082

Ion	Exp%	Act%
184.00	100	100
185.00	16.30	13.95
183.00	13.80	12.83
0.00	0.00	0.00