


Data Path : Z:\HPCHEM1\BNA G\Data\BG060717\  
 Data File : BG027305.D  
 Acq On : 8 Jun 2017 5:57  
 Operator : SJ/MA  
 Sample : DFTPP  
 Misc :  
 ALS Vial : 1 Sample Multiplier: 1

Instrument :  
 BNA\_G  
 ClientSampleId :  
 DFTPP

Integration File: rteint.p

Method : Z:\HPCHEM1\BNA\_G\METHODS\8270-BG060517.M  
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION  
 Last Update : Mon Jun 05 16:00:35 2017

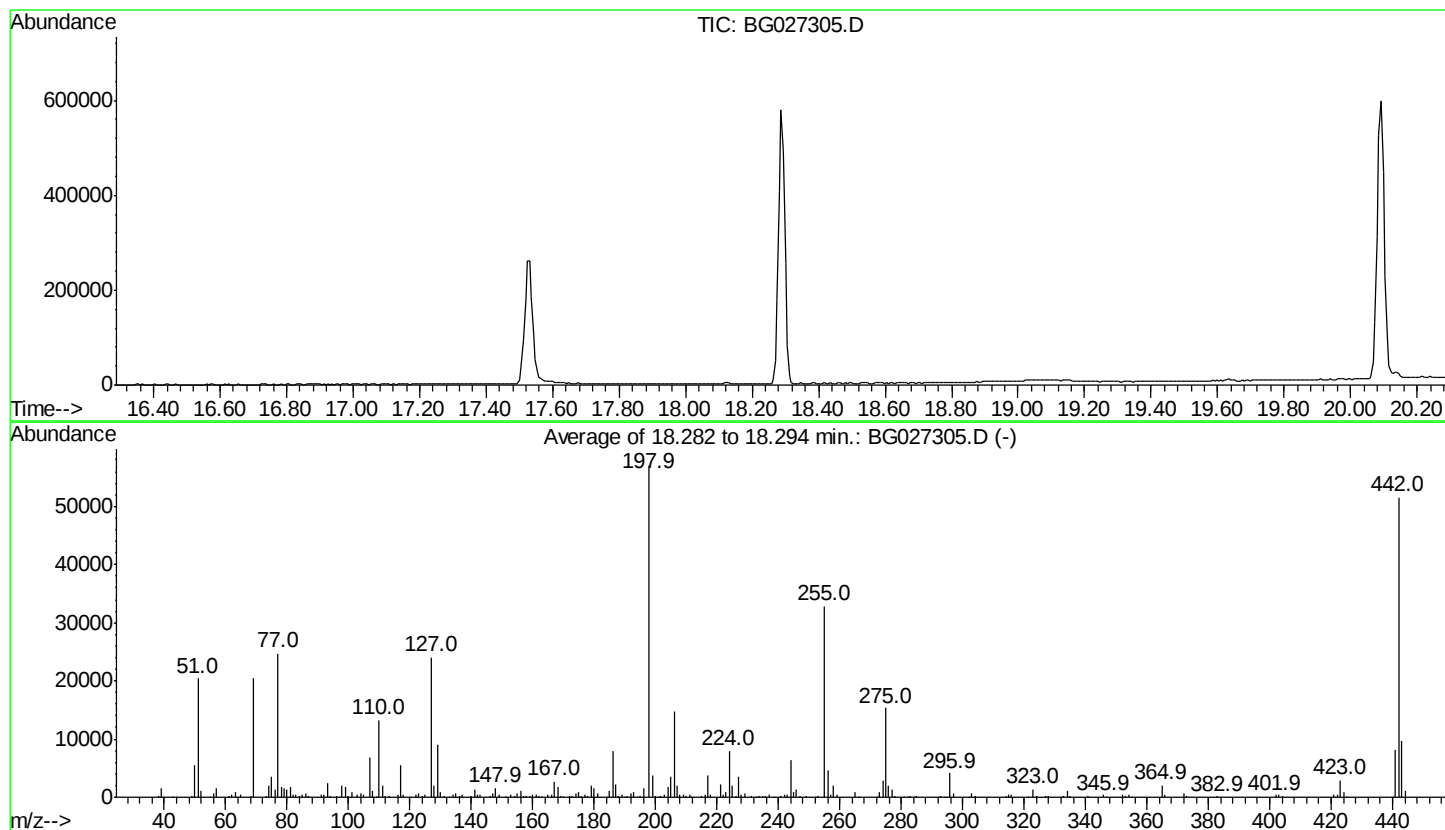

AutoFind: Scans 2484, 2485, 2486; Background Corrected with Scan 2478

| Target Mass | Rel. to Mass | Lower Limit% | Upper Limit% | Rel. Abn% | Raw Abn | Result Pass/Fail |
|-------------|--------------|--------------|--------------|-----------|---------|------------------|
| 51          | 198          | 10           | 80           | 35.7      | 20373   | PASS             |
| 68          | 69           | 0.00         | 2            | 1.0       | 199     | PASS             |
| 69          | 198          | 0.00         | 100          | 35.7      | 20362   | PASS             |
| 70          | 69           | 0.00         | 2            | 0.0       | 0       | PASS             |
| 127         | 198          | 10           | 80           | 42.1      | 23997   | PASS             |
| 197         | 198          | 0.00         | 2            | 0.0       | 0       | PASS             |
| 198         | 198          | 100          | 100          | 100.0     | 56997   | PASS             |
| 199         | 198          | 5            | 9            | 6.5       | 3692    | PASS             |
| 275         | 198          | 10           | 60           | 27.0      | 15401   | PASS             |
| 365         | 198          | 1            | 100          | 3.5       | 2018    | PASS             |
| 441         | 442          | 0.01         | 24           | 15.7      | 8098    | PASS             |
| 442         | 198          | 50           | 100          | 90.5      | 51560   | PASS             |
| 443         | 442          | 15           | 24           | 18.8      | 9718    | PASS             |