

Data Path : Z:\HPCHEM1\BNA_G\DATA\BG060815\
 Data File : BG017543.D
 Acq On : 8 Jun 2015 15:09
 Operator : TP/IZ
 Sample : G2464-17 5X
 Misc :
 ALS Vial : 6 Sample Multiplier: 1

Instrument :
 BNA_G
 ClientSampleId :
 SB-14AS

Integration Parameters: rteint.p
 Integrator: RTE
 Smoothing : ON
 Sampling : 1
 Start Thrs: 0.2
 Stop Thrs : 0
 Filtering: 5
 Min Area: 3 % of largest Peak
 Max Peaks: 100
 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\HPCHEM1\BNA_G\METHODS\8270-BG060315.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

Signal : TIC

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	2.745	7	10	14	rVB5	6750	9580	2.46%	0.311%
2	4.197	254	257	262	rVB5	2743	4919	1.26%	0.160%
3	4.714	341	345	348	rBV6	5113	6305	1.62%	0.204%
4	5.201	421	428	438	rVB2	55769	83745	21.50%	2.716%
5	6.823	698	704	715	rBV	55922	95197	24.44%	3.088%
6	7.152	754	760	766	rBV	62066	95020	24.39%	3.082%
7	7.610	832	838	843	rBV	72870	111704	28.67%	3.623%
8	7.928	886	892	898	rVB	48163	72141	18.52%	2.340%
9	8.774	1031	1036	1046	rBV2	32377	59522	15.28%	1.931%
10	10.407	1308	1314	1325	rVB	95546	161842	41.55%	5.249%
11	12.898	1732	1738	1747	rBV	78632	127317	32.68%	4.129%
12	13.750	1876	1883	1887	rBV6	7167	13819	3.55%	0.448%
13	14.279	1964	1973	1981	rBV3	145393	225584	57.91%	7.316%
14	14.344	1981	1984	1989	rVB3	4427	6299	1.62%	0.204%
15	15.336	2150	2153	2157	rVB3	3586	4412	1.13%	0.143%
16	15.548	2185	2189	2194	rBV4	2303	4000	1.03%	0.130%
17	15.783	2224	2229	2238	rBV2	66836	100045	25.68%	3.245%
18	17.034	2434	2442	2446	rBV2	184745	262109	67.28%	8.501%
19	17.076	2446	2449	2455	rVB	47806	67869	17.42%	2.201%
20	17.170	2460	2465	2469	rVB3	10871	15858	4.07%	0.514%
21	17.240	2471	2477	2478	rBV4	2558	4496	1.15%	0.146%
22	17.910	2587	2591	2594	rBV4	7680	11073	2.84%	0.359%
23	17.963	2594	2600	2605	rVB6	10586	20396	5.24%	0.662%
24	18.033	2608	2612	2613	rBV3	2963	3973	1.02%	0.129%
25	18.110	2620	2625	2629	rBV4	12374	22169	5.69%	0.719%
26	18.157	2631	2633	2636	rVB4	5207	4502	1.16%	0.146%
27	18.221	2640	2644	2645	rBV3	4303	4629	1.19%	0.150%
28	18.421	2674	2678	2681	rVB4	5024	5842	1.50%	0.189%
29	18.462	2681	2685	2693	rVB9	5053	9396	2.41%	0.305%
30	18.985	2772	2774	2779	rVB6	5657	7970	2.05%	0.258%
31	19.103	2789	2794	2799	rBV	105697	133309	34.22%	4.324%
32	19.208	2810	2812	2815	rBV4	3972	4807	1.23%	0.156%
33	19.467	2848	2856	2861	rBV	95936	141524	36.33%	4.590%
34	19.543	2866	2869	2872	rVB6	8047	10813	2.78%	0.351%

Data Path : Z:\HPCHEM1\BNA_G\DATA\BG060815\
Data File : BG017543.D
Acq On : 8 Jun 2015 15:09
Operator : TP/IZ
Sample : G2464-17 5X
Misc :
ALS Vial : 6 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
SB-14AS

Integration Parameters: rteint.p
Integrator: RTE
Smoothing : ON Filtering: 5
Sampling : 1 Min Area: 3 % of largest Peak
Start Thrs: 0.2 Max Peaks: 100
Stop Thrs : 0 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
Peak separation: 5

Method : Z:\HPCHEM1\BNA_G\METHODS\8270-BG060315.M
Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

35	19.673	2884	2891	2896	rBV2	173562	228353	58.62%	7.406%
36	19.796	2905	2912	2914	rBV7	13906	29427	7.55%	0.954%
37	19.884	2923	2927	2929	rBV5	5631	8351	2.14%	0.271%
38	19.931	2929	2935	2937	rVV7	9755	18503	4.75%	0.600%
39	19.966	2937	2941	2945	rVB4	15705	25393	6.52%	0.824%
40	20.066	2956	2958	2961	rVB4	10602	9191	2.36%	0.298%
41	20.266	2987	2992	2996	rBV7	10504	20030	5.14%	0.650%
42	20.483	3027	3029	3033	rBV5	6252	5601	1.44%	0.182%
43	20.530	3035	3037	3038	rBV3	7338	5234	1.34%	0.170%
44	20.554	3039	3041	3043	rBV3	8658	7360	1.89%	0.239%
45	20.959	3106	3110	3114	rBV6	13642	22330	5.73%	0.724%
46	21.230	3150	3156	3160	rBV2	266180	389557	100.00%	12.635%
47	21.265	3160	3162	3167	rVB	46378	55120	14.15%	1.788%
48	22.798	3418	3423	3426	rBV2	45727	82633	21.21%	2.680%
49	23.468	3532	3537	3543	rVB	158643	263958	67.76%	8.561%


Sum of corrected areas: 3083227

Data Path : Z:\HPCHEM1\BNA_G\DATA\BG060815\
Data File : BG017543.D
Acq On : 8 Jun 2015 15:09
Operator : TP/IZ
Sample : G2464-17 5X
Misc :
ALS Vial : 6 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
SB-14AS

Quant Method : Z:\HPCHEM1\BNA_G\METHODS\8270-BG060315.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\DATABASE\NIST02.L
TIC Integration Parameters: LSCINT.P

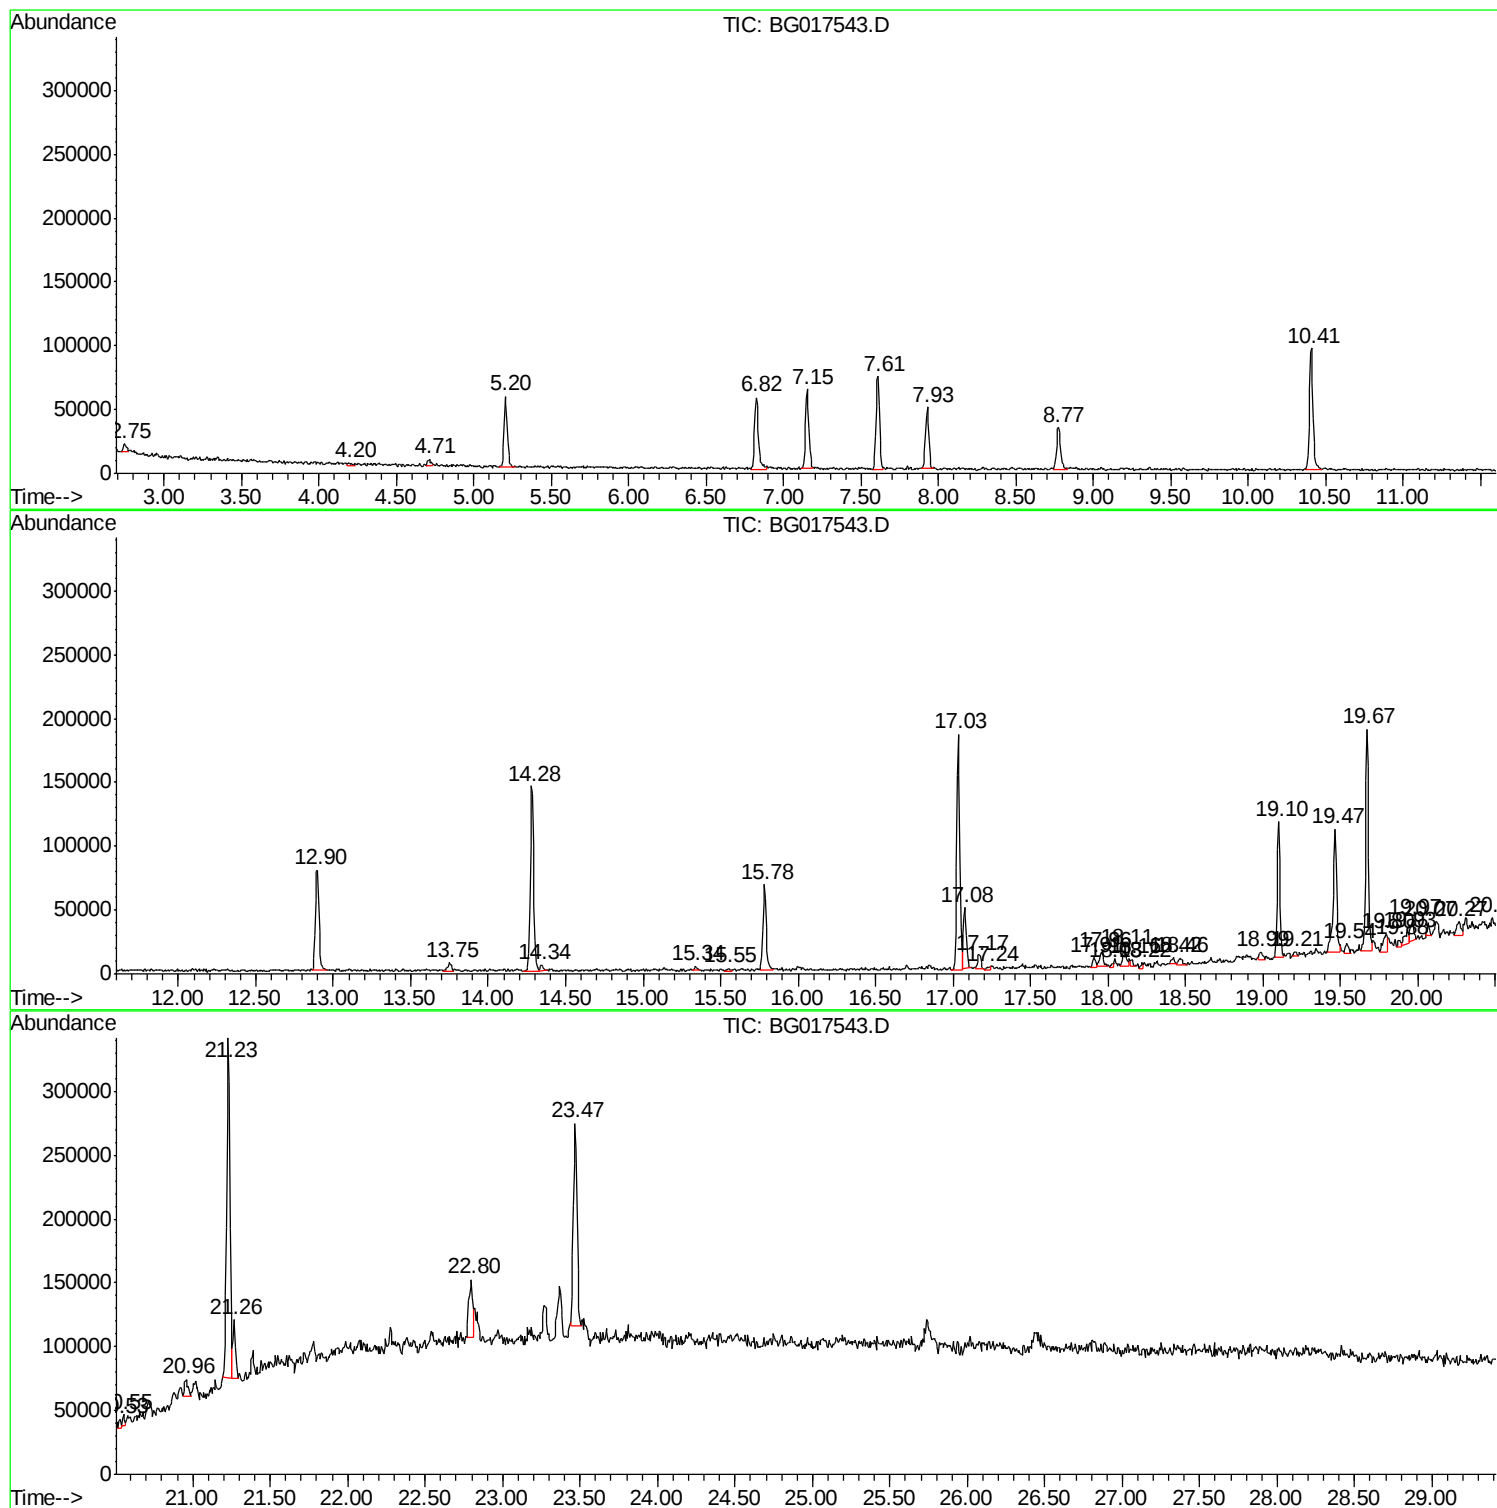

Data Path : Z:\HPCHEM1\BNA_G\DATA\BG060815\
Data File : BG017543.D
Acq On : 8 Jun 2015 15:09
Operator : TP/IZ
Sample : G2464-17 5X
Misc :
ALS Vial : 6 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
SB-14AS










Quant Method : Z:\HPCHEM1\BNA_G\METHODS\8270-BG060315.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\DATABASE\NIST02.L
TIC Integration Parameters: LSCINT.P

Peak Number 1 unknown7.15 Concentration Rank 1

R.T.	EstConc	Area	Relative to ISTD	R.T.
7.15	17.01 ng	95020	1,4-Dichlorobenzene-d4	7.61

Hit#	of	5	Tentative ID	MW	MolForm	CAS#	Qual
1			1,3-Cyclopentanedione, 2-chloro-	132	C5H5ClO2	014203-19-1	25
2			3-Chloro-6-fluoro-pyrazine	132	C4H2ClFN2	1000146-10-7	14
3			5-Fluoro-2-chloropyrimidine	132	C4H2ClFN2	062802-42-0	10
4			Benzimidazole, 2-heptyl-	216	C14H20N2	005851-49-0	10
5			L-Proline, 1-(chlorocarbonyl)-, ...	191	C7H10ClN03	085665-59-4	10

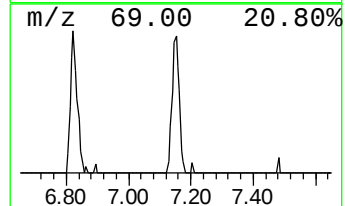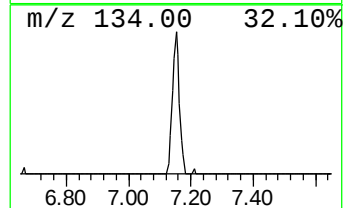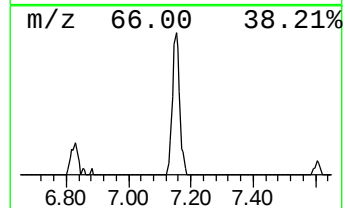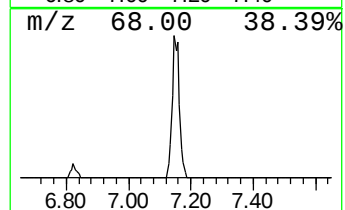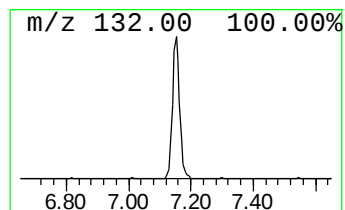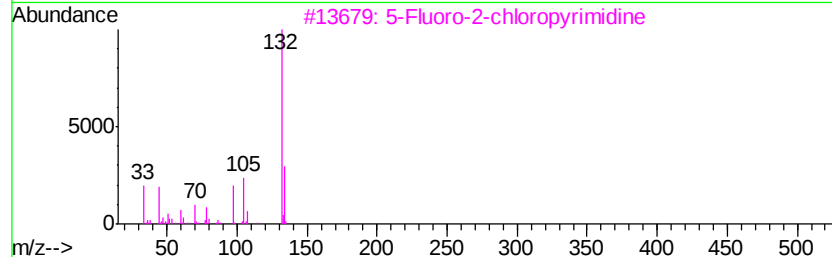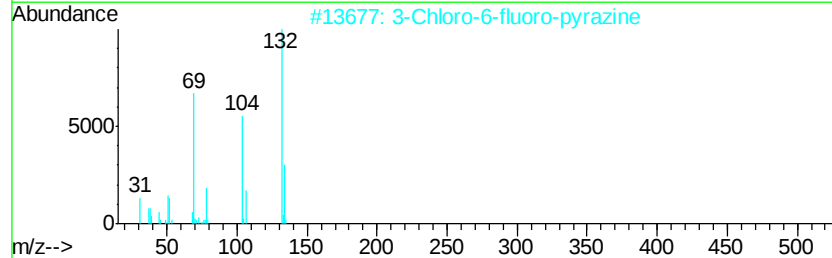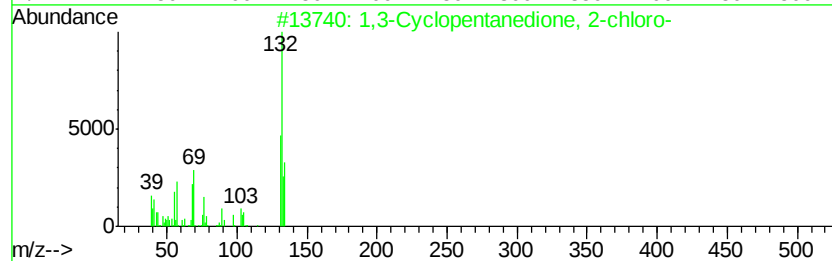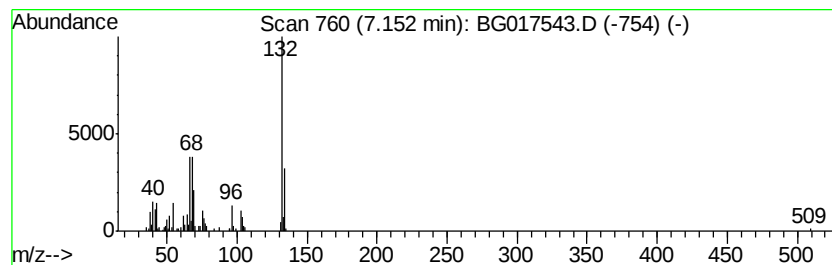

Data Path : Z:\HPCHEM1\BNA_G\DATA\BG060815\
Data File : BG017543.D
Acq On : 8 Jun 2015 15:09
Operator : TP/IZ
Sample : G2464-17 5X
Misc :
ALS Vial : 6 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
SB-14AS

Quant Method : Z:\HPCHEM1\BNA_G\METHODS\8270-BG060315.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\DATABASE\NIST02.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc
unknown7.15	7.15	17.0	ng	95020	1	7.61	111704	20.0