


Data Path : Z:\HPCHEM1\BNA_G\Data\BG060815\
 Data File : BG017538.D
 Acq On : 8 Jun 2015 11:41
 Operator : TP/IZ
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_G
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\HPCHEM1\BNA_G\METHODS\8270-BG060315.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Mon Jun 08 18:39:50 2015

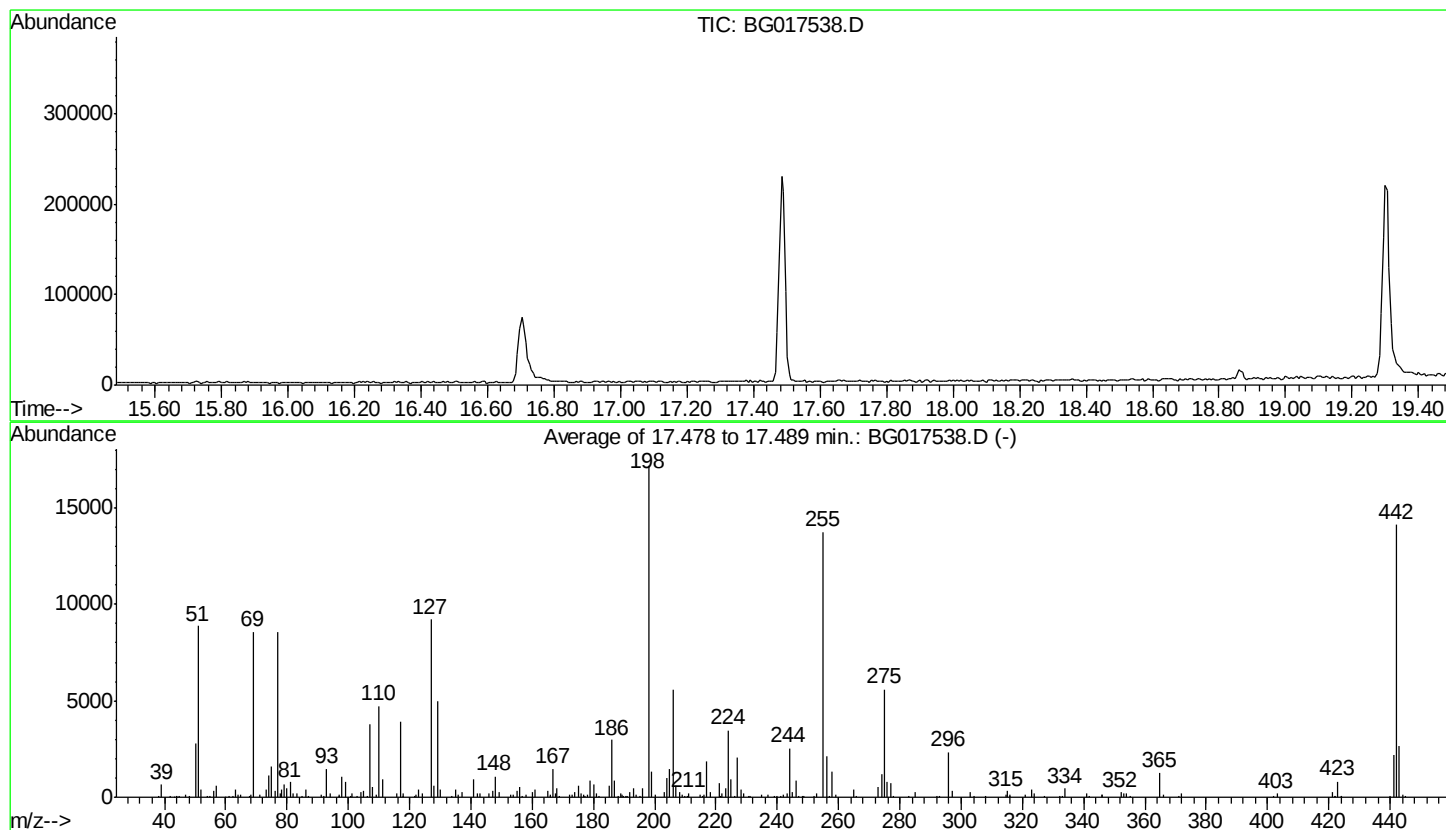

AutoFind: Scans 2517, 2518, 2519; Background Corrected with Scan 2511

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	51.7	8879	PASS
68	69	0.00	2	1.9	161	PASS
69	198	0.00	100	50.0	8592	PASS
70	69	0.00	2	0.0	0	PASS
127	198	10	80	53.5	9201	PASS
197	198	0.00	2	0.0	0	PASS
198	198	100	100	100.0	17184	PASS
199	198	5	9	7.6	1308	PASS
275	198	10	60	32.5	5592	PASS
365	198	1	100	7.4	1277	PASS
441	442	0.01	24	15.4	2172	PASS
442	198	50	100	82.0	14099	PASS
443	442	15	24	18.8	2649	PASS