


Data Path : Z:\HPCHEM1\BNA_G\Data\BG060815\
Data File : BG017552.D
Acq On : 9 Jun 2015 00:13
Operator : TP/IZ
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
DFTPP

Integration File: rteint.p

Method : Z:\HPCHEM1\BNA_G\METHODS\8270-BG060315.M
Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
Last Update : Mon Jun 08 18:39:50 2015

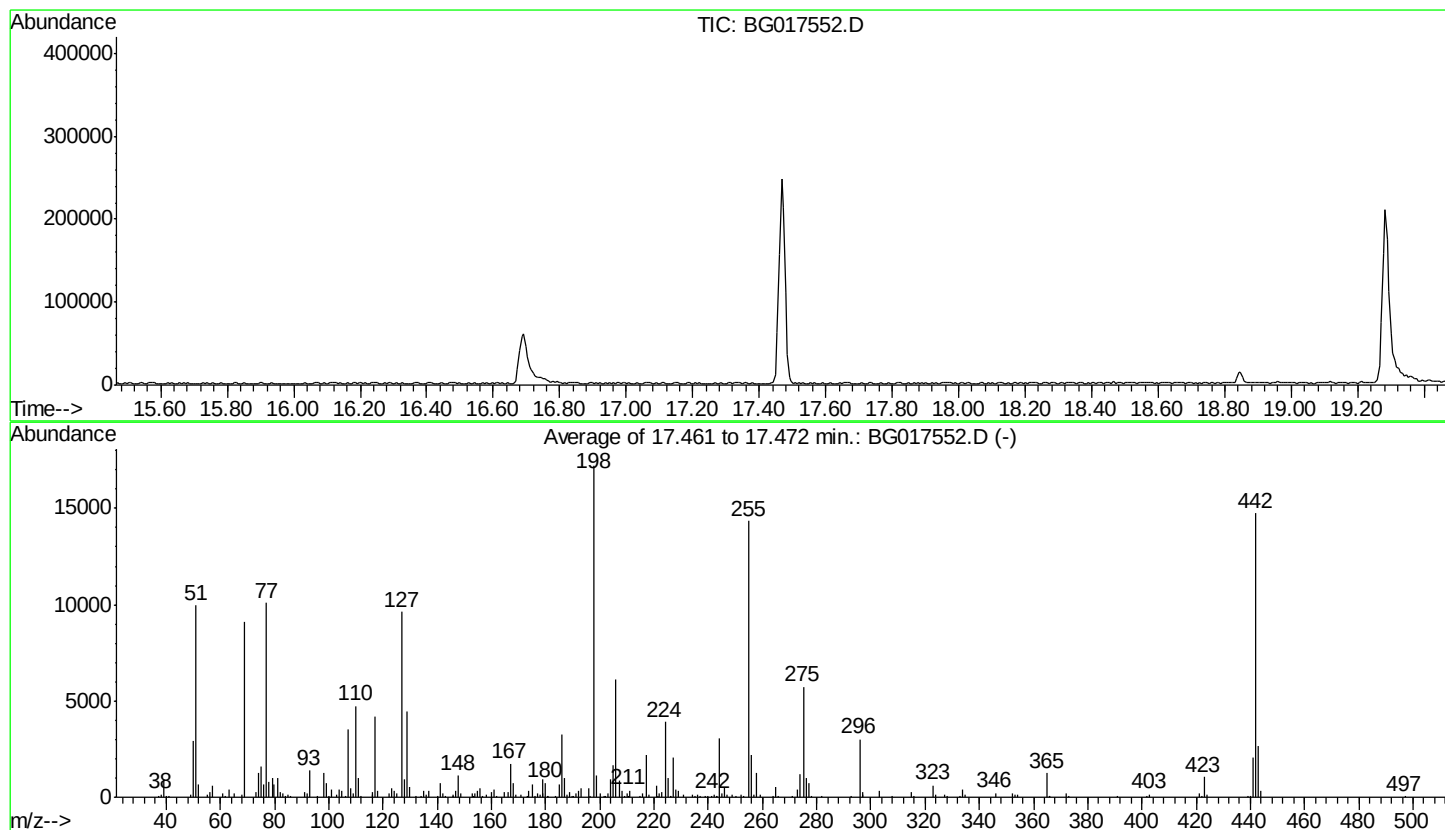

AutoFind: Scans 2514, 2515, 2516; Background Corrected with Scan 2508

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	57.8	9961	PASS
68	69	0.00	2	1.2	107	PASS
69	198	0.00	100	53.0	9123	PASS
70	69	0.00	2	0.0	0	PASS
127	198	10	80	55.9	9623	PASS
197	198	0.00	2	0.0	0	PASS
198	198	100	100	100.0	17219	PASS
199	198	5	9	6.5	1120	PASS
275	198	10	60	33.3	5741	PASS
365	198	1	100	7.3	1249	PASS
441	442	0.01	24	14.1	2082	PASS
442	198	50	100	85.6	14732	PASS
443	442	15	24	18.3	2693	PASS