
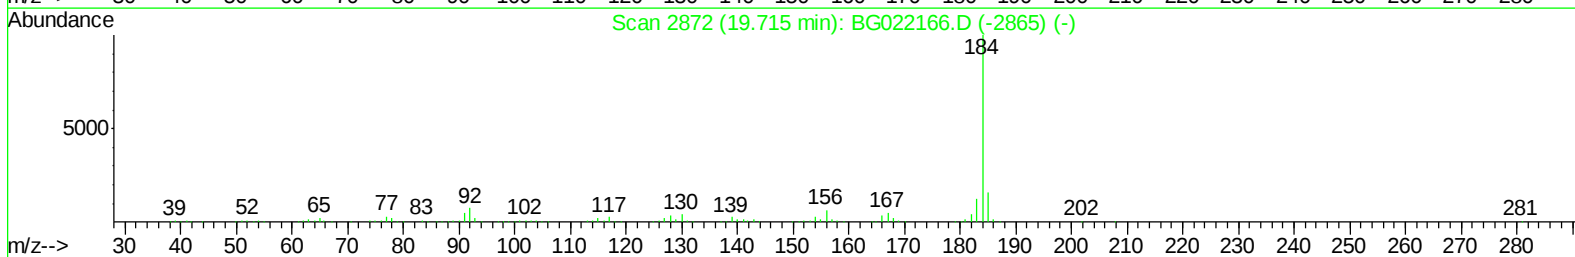
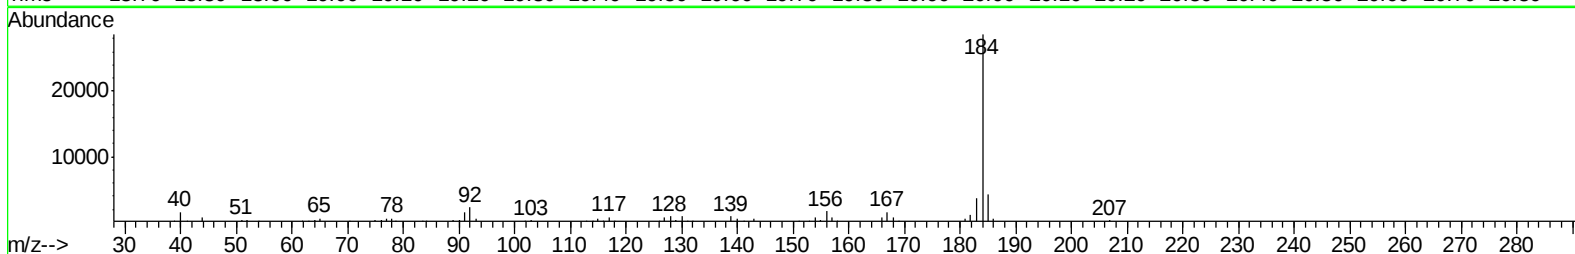


Data Path : Z:\HPCHEM1\BNA_G\DATA\BG060816\
Data File : BG022225.D
Acq On : 8 Jun 2016 6:43
Operator : UM/SJ
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Jun 09 07:31:24 2016
Quant Method : Z:\HPCHEM1\BNA_G\METHODS\8270-BG060616.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Mon Jun 06 16:12:45 2016
Response via : Initial Calibration

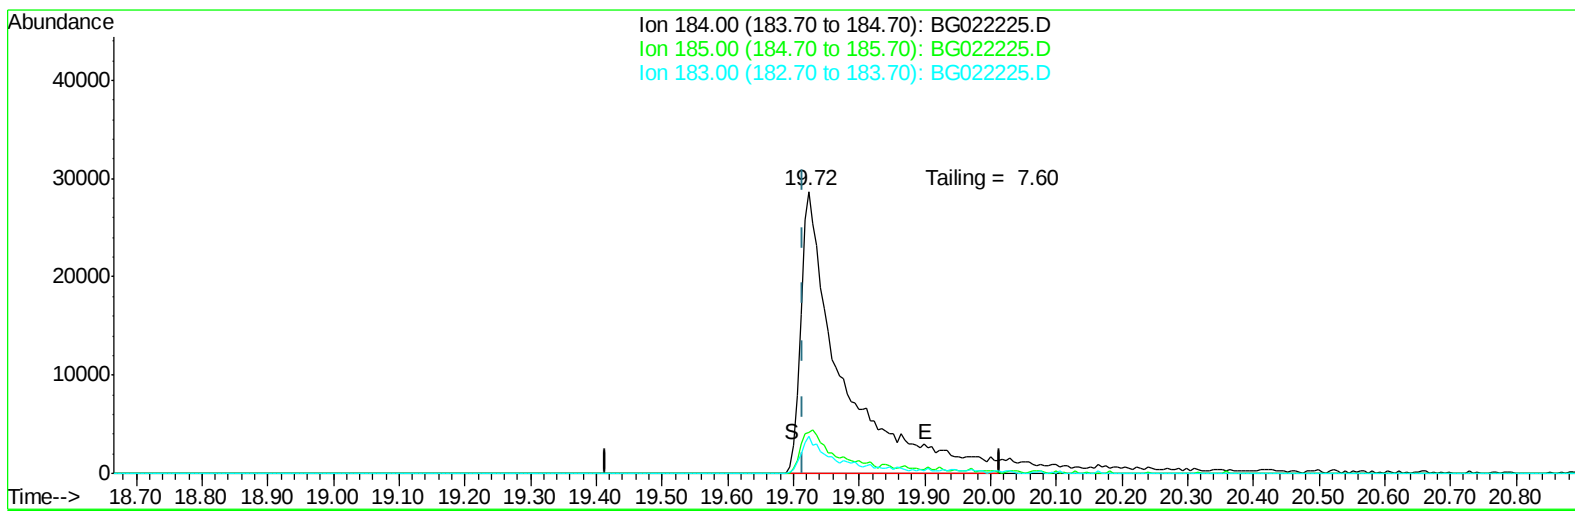

TIC: BG022225.D

(76) Benzidine




19.723min (+0.009) 0.00ng m

response 125861

Ion	Exp%	Act%
184.00	100	100
185.00	14.40	14.60
183.00	12.80	13.09
0.00	0.00	0.00

Data Path : Z:\HPCHEM1\BNA_G\DATA\BG060816\
Data File : BG022225.D
Acq On : 8 Jun 2016 6:43
Operator : UM/SJ
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Jun 09 07:31:24 2016
Quant Method : Z:\HPCHEM1\BNA_G\METHODS\8270-BG060616.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Mon Jun 06 16:12:45 2016
Response via : Initial Calibration

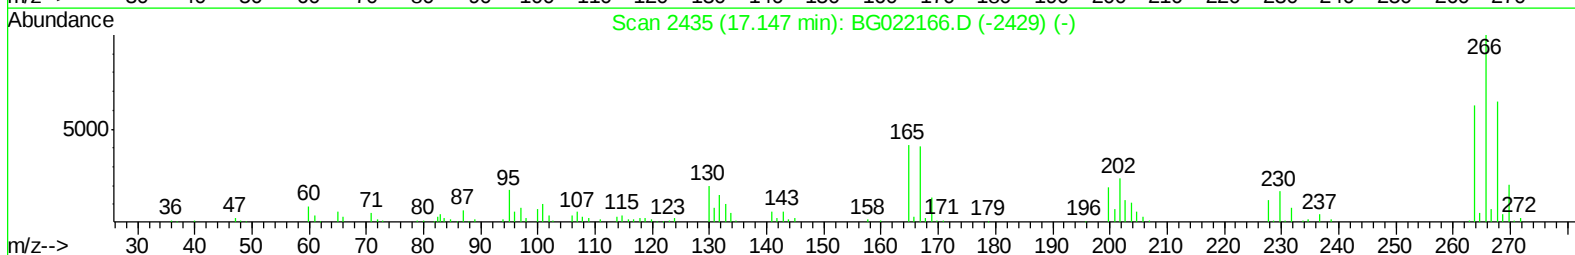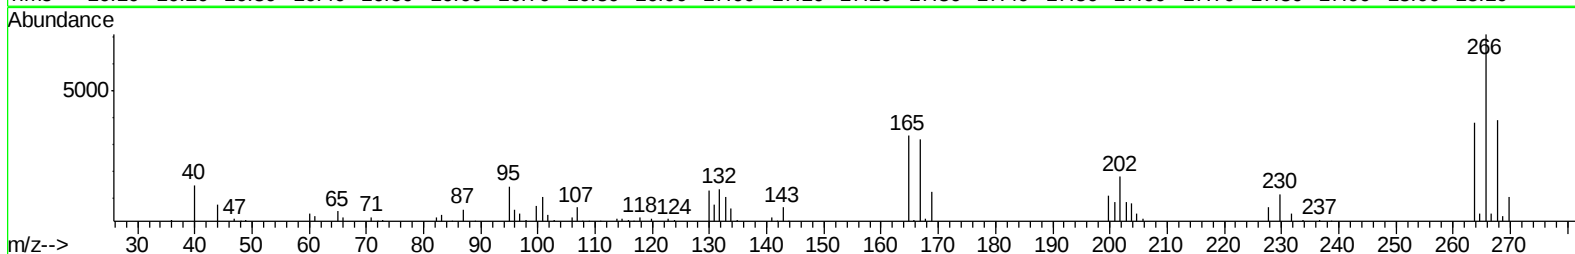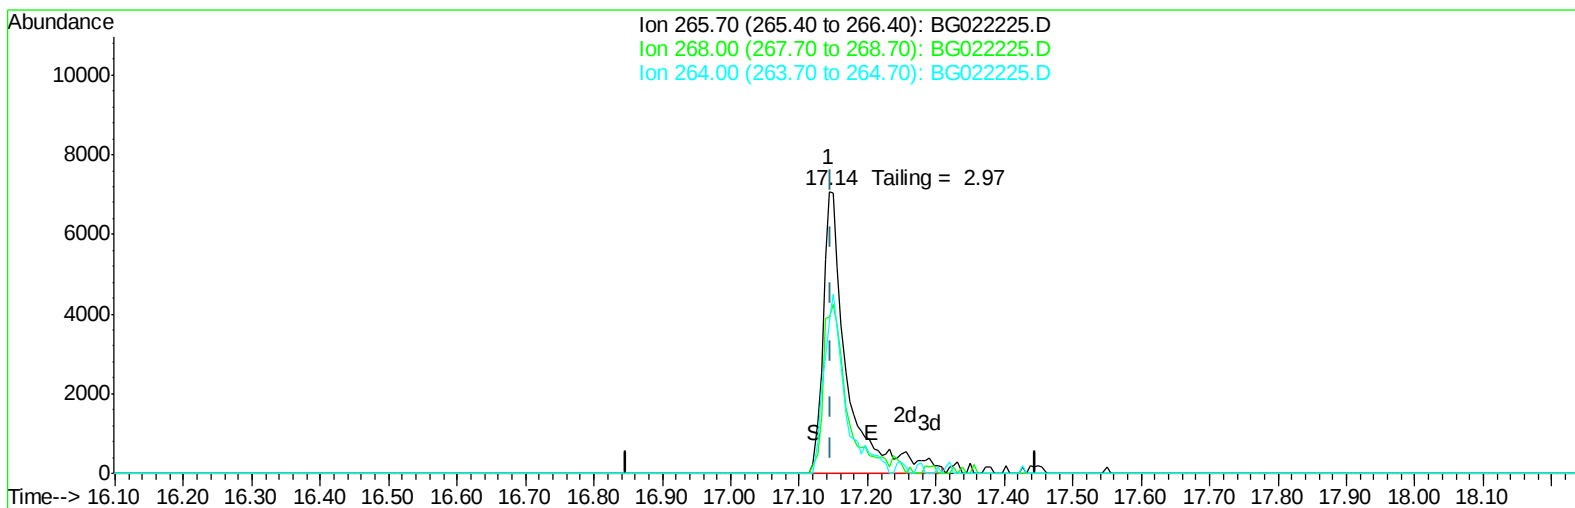

TIC: BG022225.D

(69) Pentachlorophenol (C)

17.144min (-0.003) 0.00ng

response 16004

Ion	Exp%	Act%
265.70	100	100
268.00	68.10	60.08
264.00	67.20	59.77
0.00	0.00	0.00