
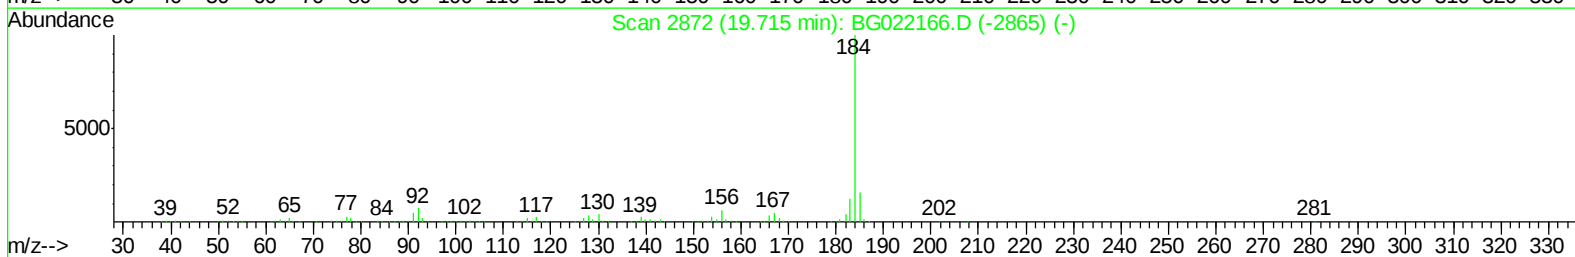
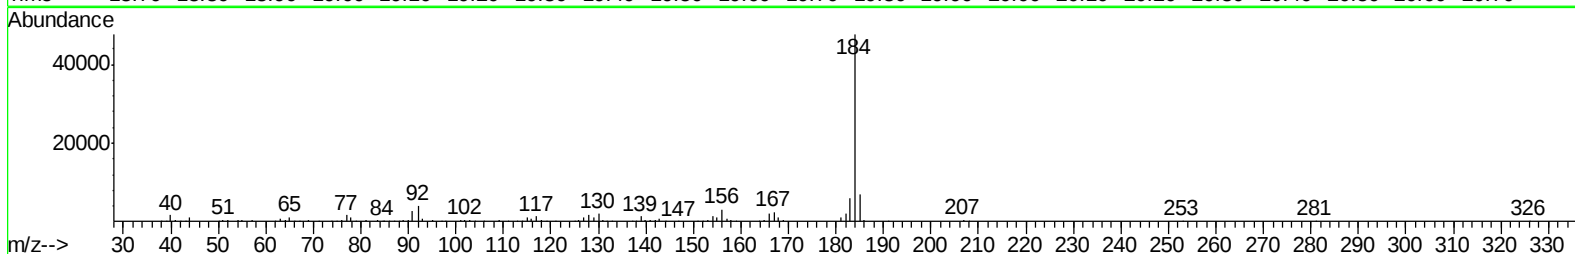


Data Path : Z:\HPCHEM1\BNA_G\DATA\BG060816\
Data File : BG022241.D
Acq On : 8 Jun 2016 19:33
Operator : UM/SJ
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Jun 09 07:34:49 2016
Quant Method : Z:\HPCHEM1\BNA_G\METHODS\8270-BG060616.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Mon Jun 06 16:12:45 2016
Response via : Initial Calibration

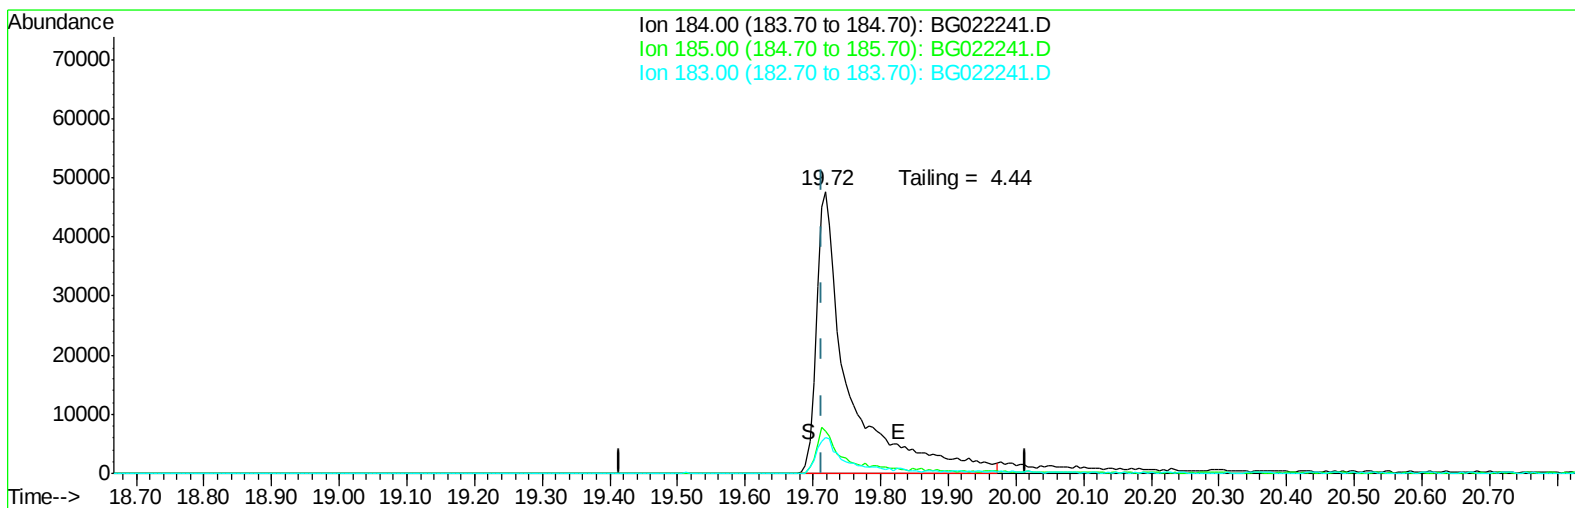

TIC: BG022241.D

(76) Benzidine




19.719min (+0.004) 92822.14ng

response 135930

Ion	Exp%	Act%
184.00	100	100
185.00	14.40	14.88
183.00	12.80	12.95
0.00	0.00	0.00

Data Path : Z:\HPCHEM1\BNA_G\DATA\BG060816\
Data File : BG022241.D
Acq On : 8 Jun 2016 19:33
Operator : UM/SJ
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Jun 09 07:34:49 2016
Quant Method : Z:\HPCHEM1\BNA_G\METHODS\8270-BG060616.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Mon Jun 06 16:12:45 2016
Response via : Initial Calibration

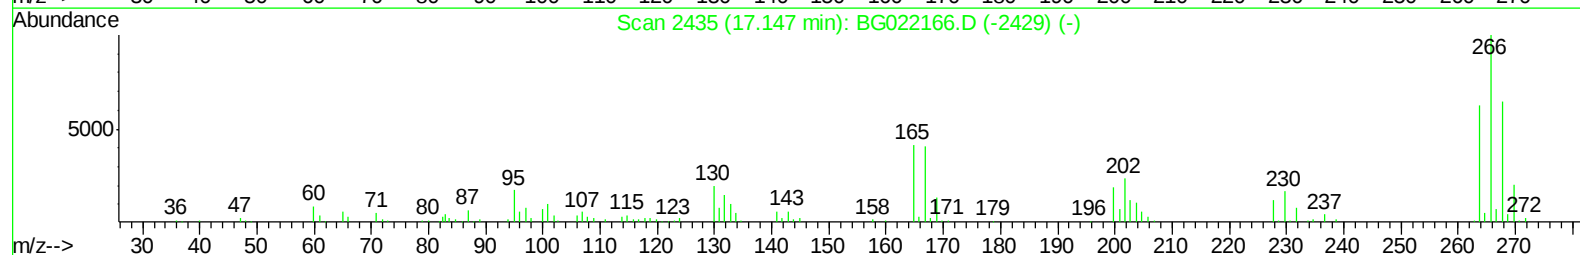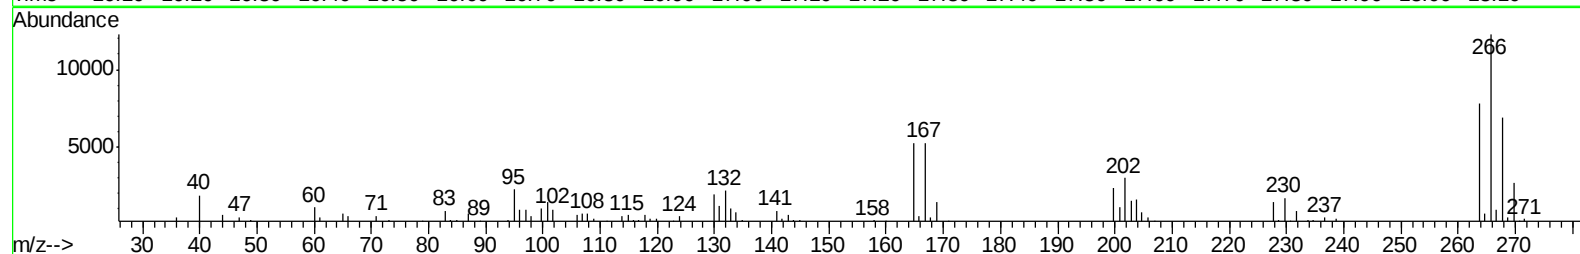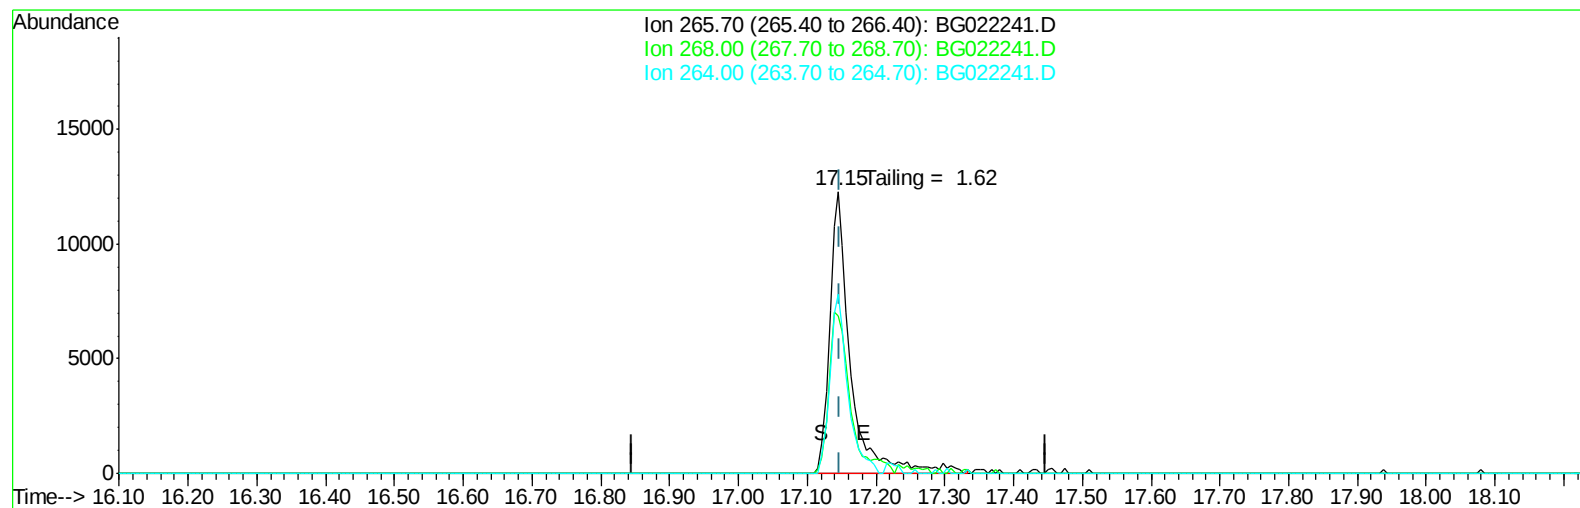

TIC: BG022241.D

(69) Pentachlorophenol (C)

17.145min (-0.002) 0.00ng

response 24194

Ion	Exp%	Act%
265.70	100	100
268.00	68.10	59.56
264.00	67.20	68.70
0.00	0.00	0.00