


Data Path : Z:\HPCHEM1\BNA G\DATA\BG060816\
 Data File : BG022241.D
 Acq On : 8 Jun 2016 19:33
 Operator : UM/SJ
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_G
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\HPCHEM1\BNA_G\METHODS\8270-BG060616.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Mon Jun 06 16:12:45 2016

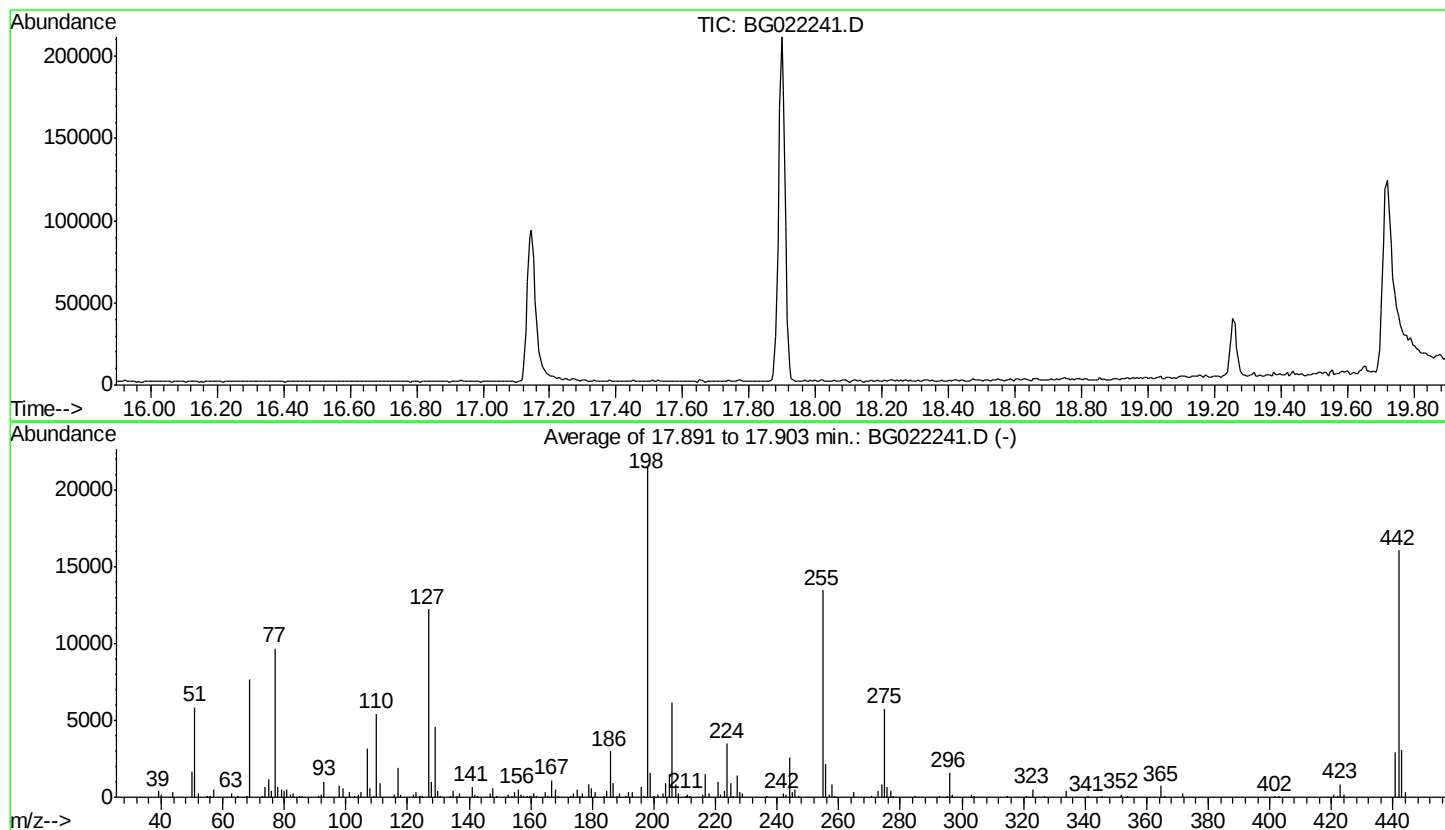

AutoFind: Scans 2562, 2563, 2564; Background Corrected with Scan 2556

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	27.0	5834	PASS
68	69	0.00	2	0.7	55	PASS
69	198	0.00	100	35.7	7697	PASS
70	69	0.00	2	0.0	0	PASS
127	198	10	80	56.7	12227	PASS
197	198	0.00	2	0.4	90	PASS
198	198	100	100	100.0	21578	PASS
199	198	5	9	7.3	1568	PASS
275	198	10	60	26.7	5770	PASS
365	198	1	100	3.4	744	PASS
441	442	0.01	24	18.1	2905	PASS
442	198	50	100	74.4	16047	PASS
443	442	15	24	19.3	3096	PASS