
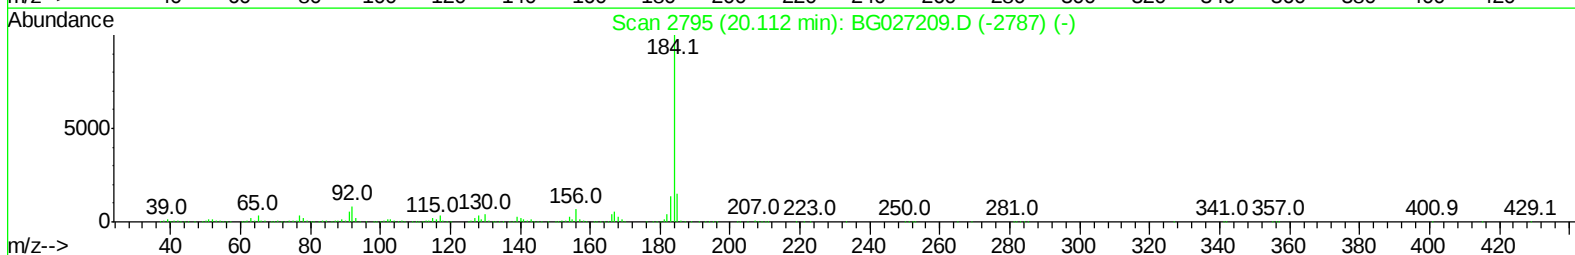
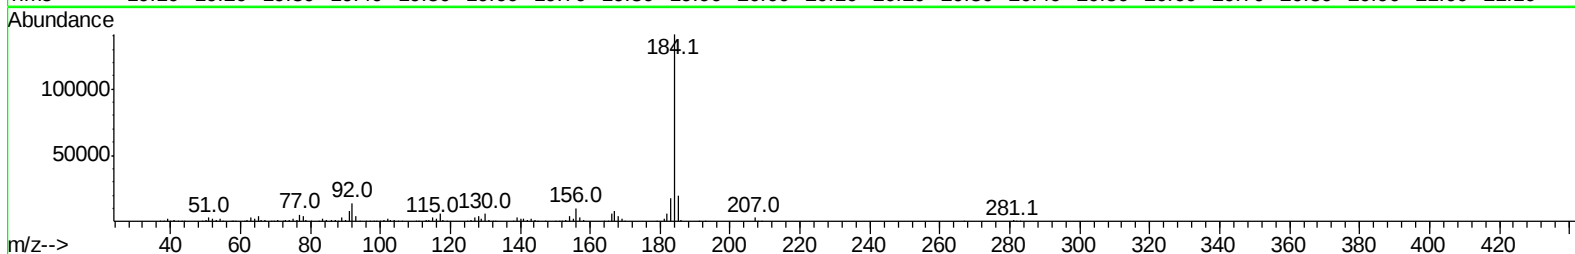


Data Path : Z:\HPCHEM1\BNA G\Data\BG060817\
Data File : BG027334.D
Acq On : 9 Jun 2017 2:11
Operator : SJ/MA
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Jun 09 09:02:07 2017
Quant Method : Z:\HPCHEM1\BNA G\METHODS\8270-BG060517.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Mon Jun 05 16:00:35 2017
Response via : Initial Calibration

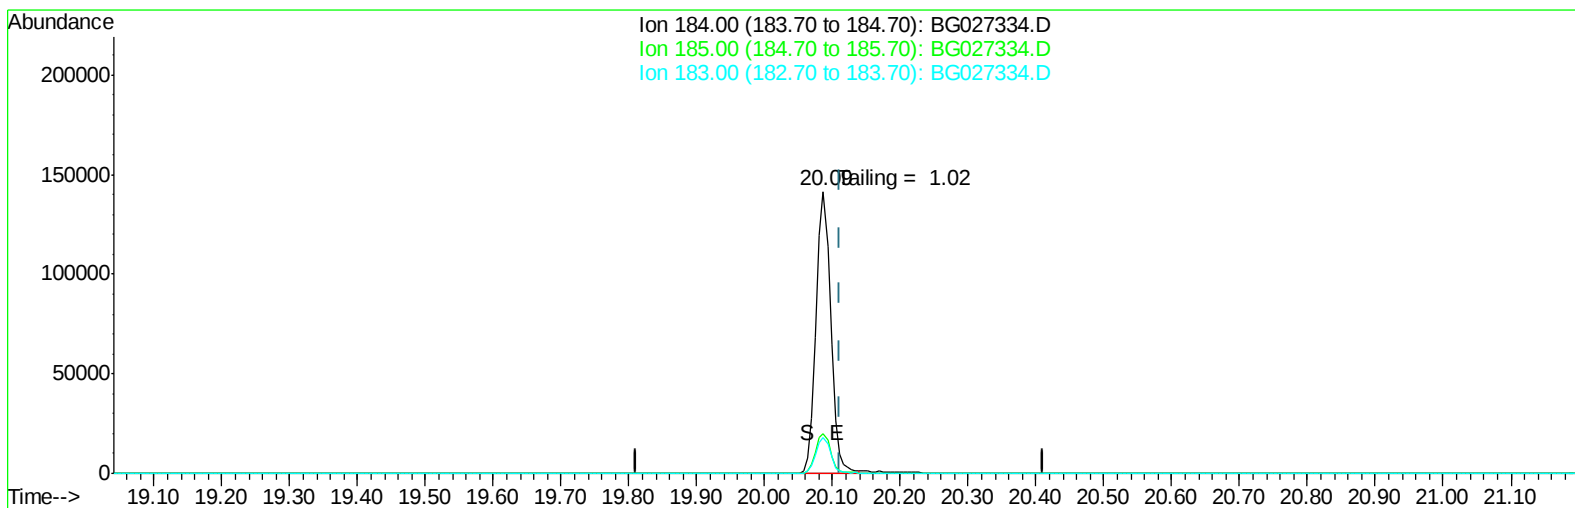

TIC: BG027334.D

(76) Benzidine




20.087min (-0.025) 116925.12ng

response 211332

Ion	Exp%	Act%
184.00	100	100
185.00	16.30	14.08
183.00	13.80	12.53
0.00	0.00	0.00

Data Path : Z:\HPCHEM1\BNA G\Data\BG060817\
Data File : BG027334.D
Acq On : 9 Jun 2017 2:11
Operator : SJ/MA
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Jun 09 09:02:07 2017
Quant Method : Z:\HPCHEM1\BNA G\METHODS\8270-BG060517.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Mon Jun 05 16:00:35 2017
Response via : Initial Calibration

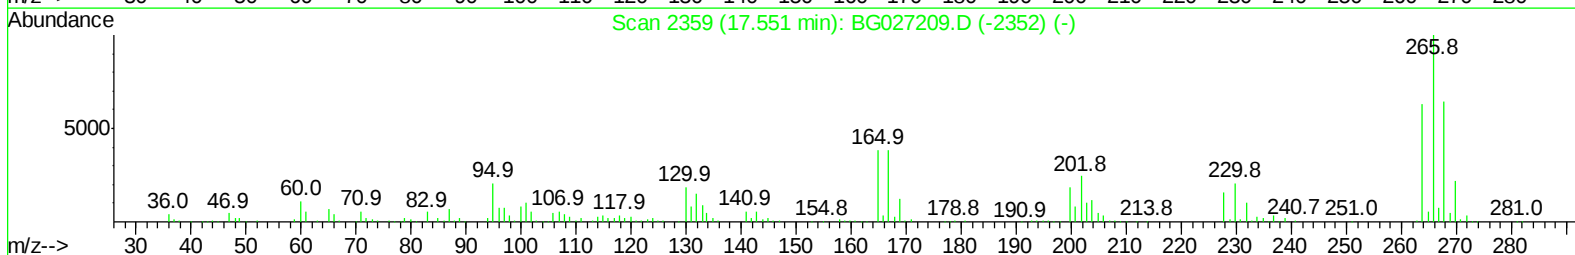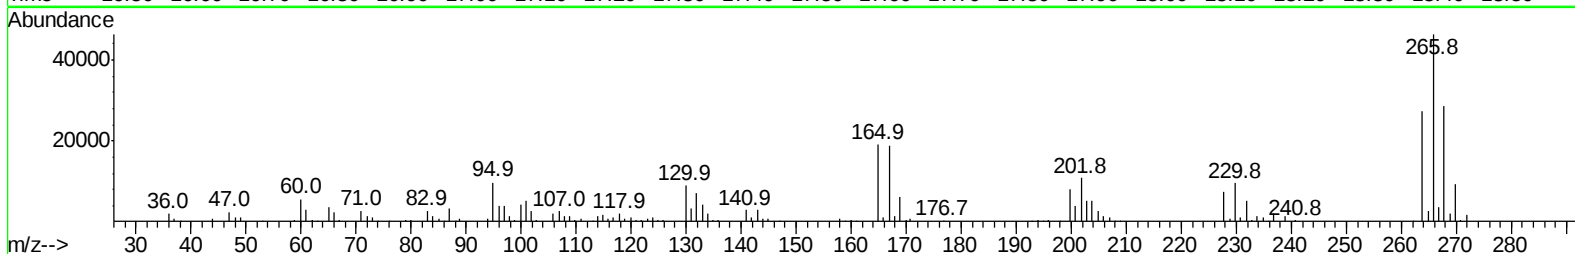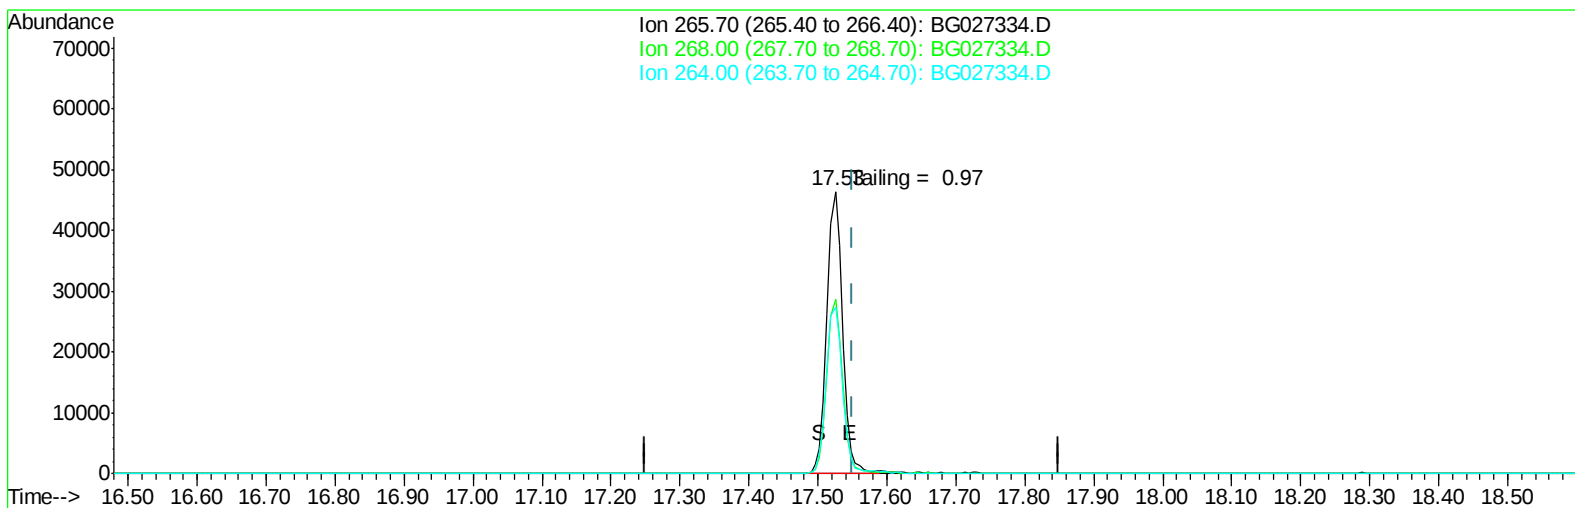

TIC: BG027334.D

(69) Pentachlorophenol (C)

17.525min (-0.025) 89175.91ng

response 72533

Ion	Exp%	Act%
265.70	100	100
268.00	60.70	61.62
264.00	62.60	59.08
0.00	0.00	0.00