


Data Path : Z:\HPCHEM1\BNA_G\DATA\BG060817\
 Data File : BG027317.D
 Acq On : 8 Jun 2017 14:06
 Operator : SJ/MA
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_G
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\HPCHEM1\BNA_G\METHODS\8270-BG060517.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Mon Jun 05 16:00:35 2017

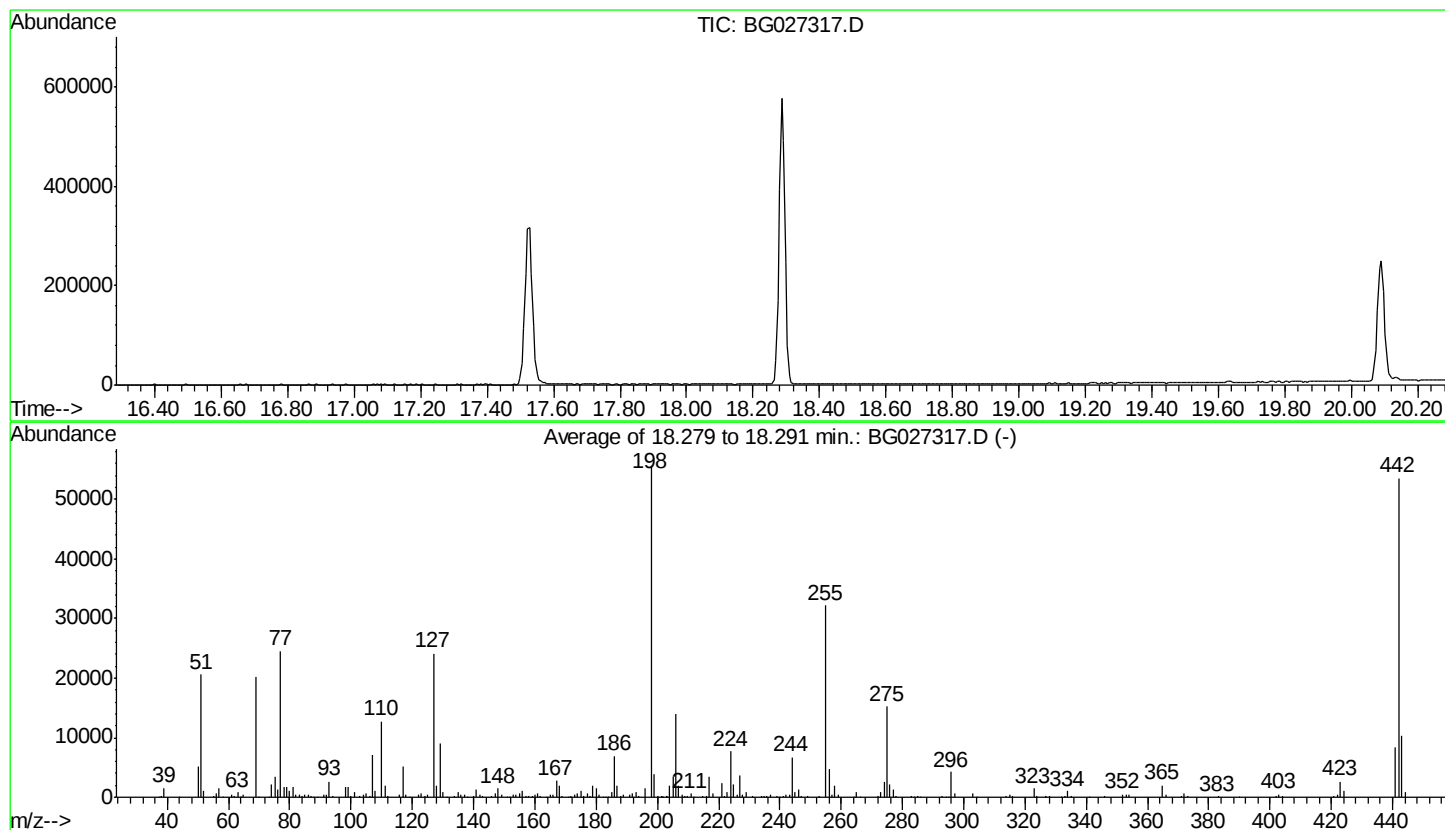

AutoFind: Scans 2483, 2484, 2485; Background Corrected with Scan 2476

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	37.0	20584	PASS
68	69	0.00	2	0.0	0	PASS
69	198	0.00	100	36.3	20205	PASS
70	69	0.00	2	0.3	54	PASS
127	198	10	80	43.3	24085	PASS
197	198	0.00	2	0.0	0	PASS
198	198	100	100	100.0	55680	PASS
199	198	5	9	7.0	3882	PASS
275	198	10	60	27.3	15193	PASS
365	198	1	100	3.5	1963	PASS
441	442	0.01	24	15.7	8394	PASS
442	198	50	100	96.3	53629	PASS
443	442	15	24	19.1	10228	PASS