


Data Path : Z:\HPCHEM1\BNA_G\DATA\BG060817\
 Data File : BG027334.D
 Acq On : 9 Jun 2017 2:11
 Operator : SJ/MA
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_G
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\HPCHEM1\BNA_G\METHODS\8270-BG060517.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Mon Jun 05 16:00:35 2017

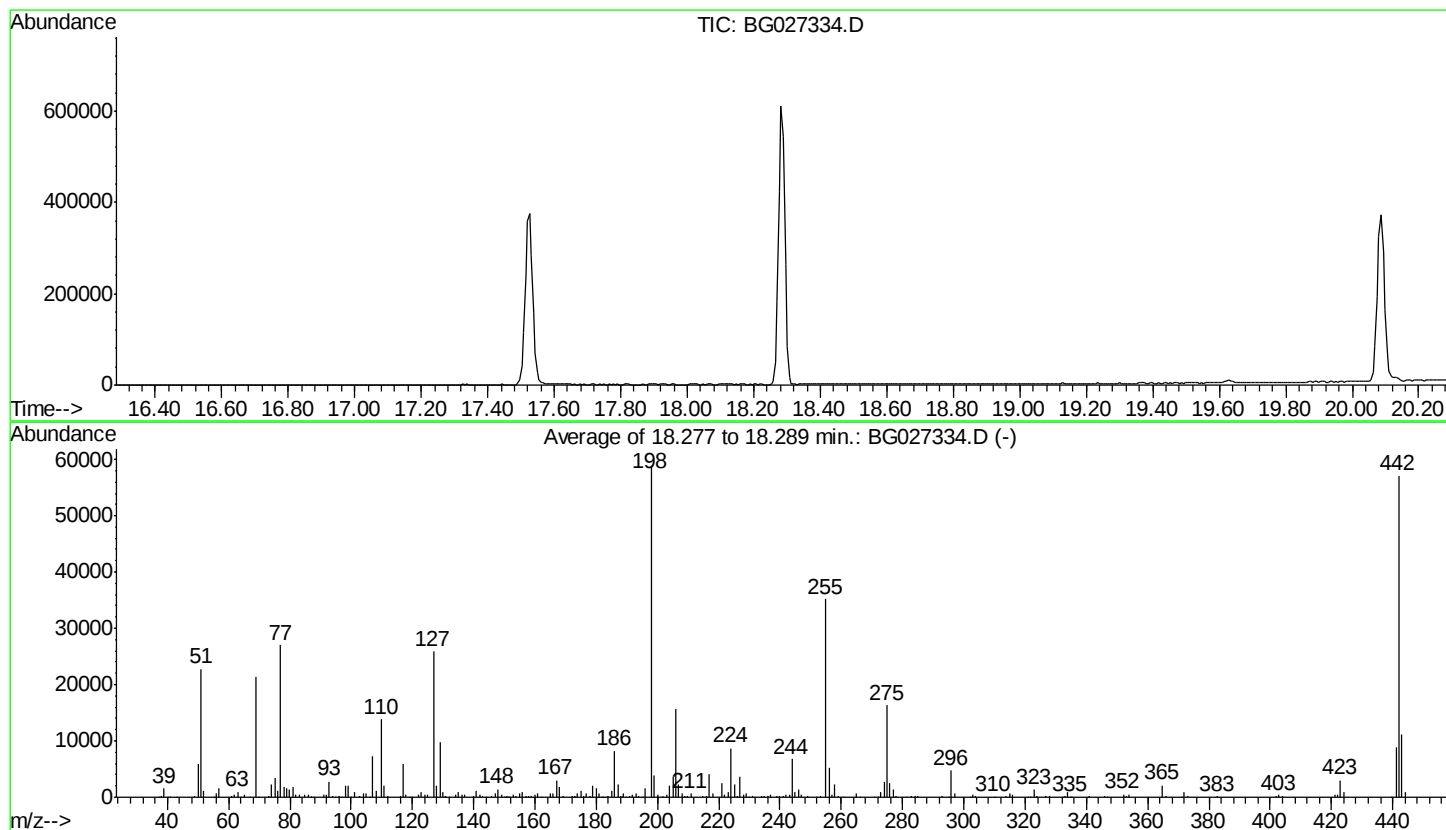

AutoFind: Scans 2483, 2484, 2485; Background Corrected with Scan 2477

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	38.7	22776	PASS
68	69	0.00	2	0.0	0	PASS
69	198	0.00	100	36.4	21458	PASS
70	69	0.00	2	0.3	56	PASS
127	198	10	80	44.0	25917	PASS
197	198	0.00	2	0.0	0	PASS
198	198	100	100	100.0	58896	PASS
199	198	5	9	6.7	3959	PASS
275	198	10	60	27.7	16307	PASS
365	198	1	100	3.5	2070	PASS
441	442	0.01	24	15.5	8890	PASS
442	198	50	100	97.1	57181	PASS
443	442	15	24	19.4	11073	PASS