


Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG060820\
 Data File : BG045637.D
 Acq On : 8 Jun 2020 10:07
 Operator : CG/JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_G
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\SVOASRV\HPCHEM1\BNA_G\METHODS\8270-BG051520.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Mon Jun 01 15:07:00 2020

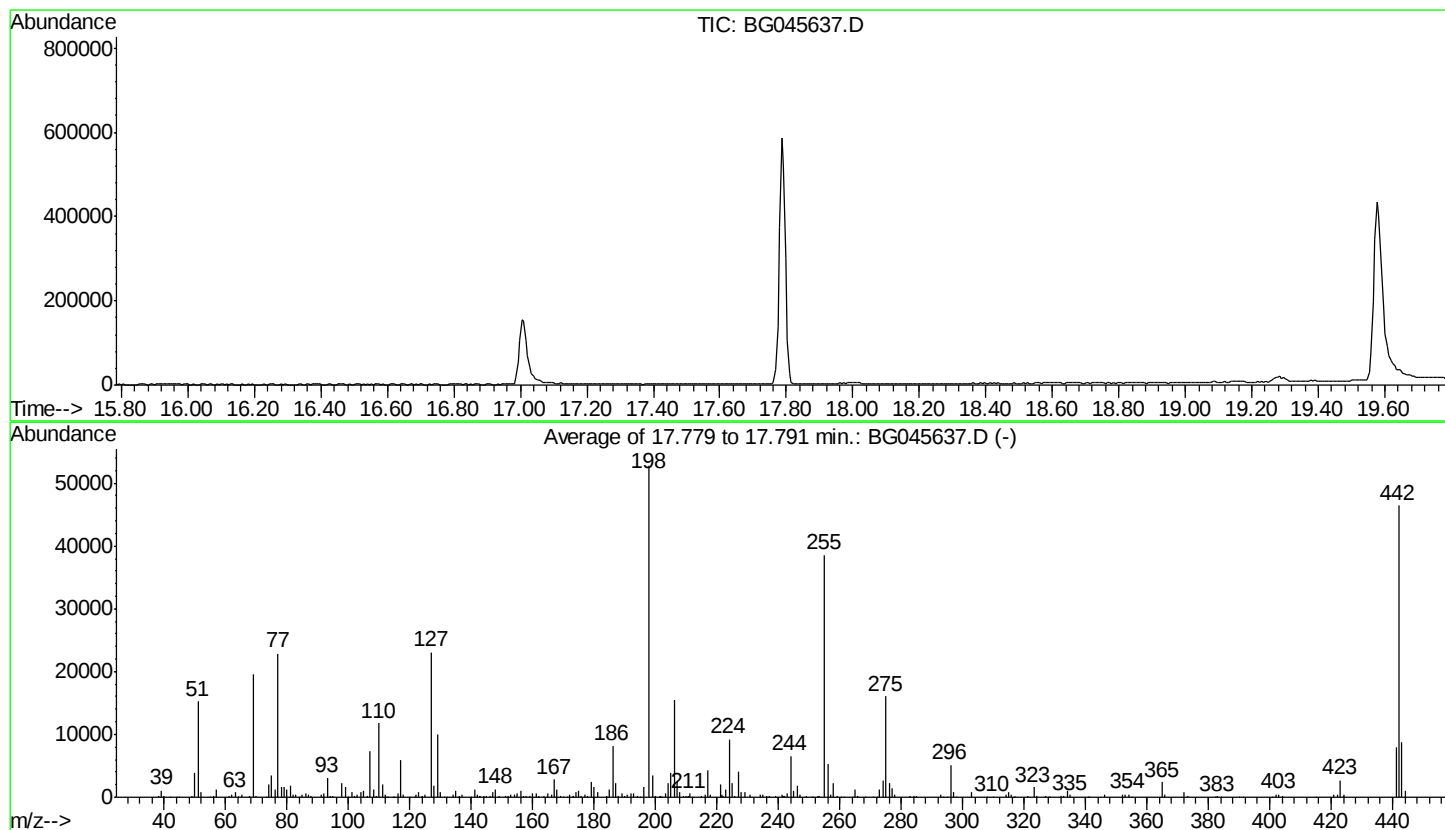

AutoFind: Scans 2501, 2502, 2503; Background Corrected with Scan 2495

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	28.8	15220	PASS
68	69	0.00	2	1.2	228	PASS
69	198	0.00	100	36.9	19488	PASS
70	69	0.00	2	0.8	160	PASS
127	198	10	80	43.6	23032	PASS
197	198	0.00	2	0.0	0	PASS
198	198	100	100	100.0	52773	PASS
199	198	5	9	6.7	3533	PASS
275	198	10	60	30.3	16012	PASS
365	198	1	100	4.5	2358	PASS
441	198	0.01	100	15.1	7990	PASS
442	198	50	100	88.0	46426	PASS
443	442	15	24	19.1	8858	PASS