
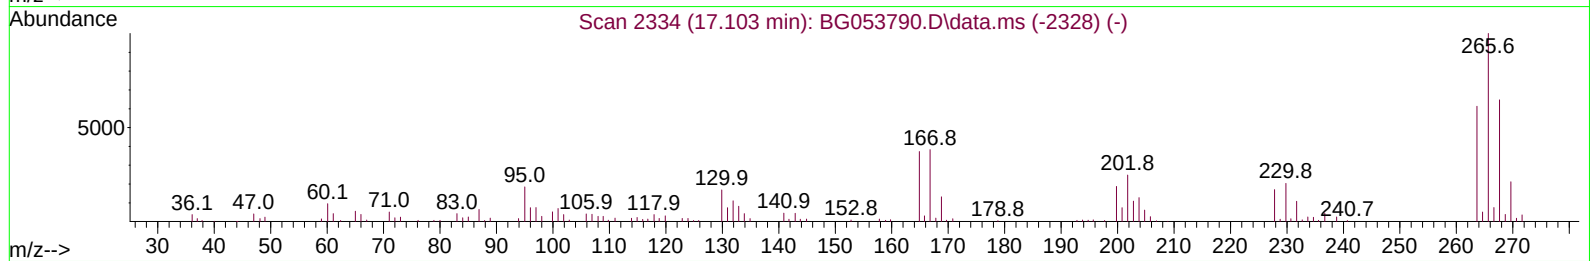
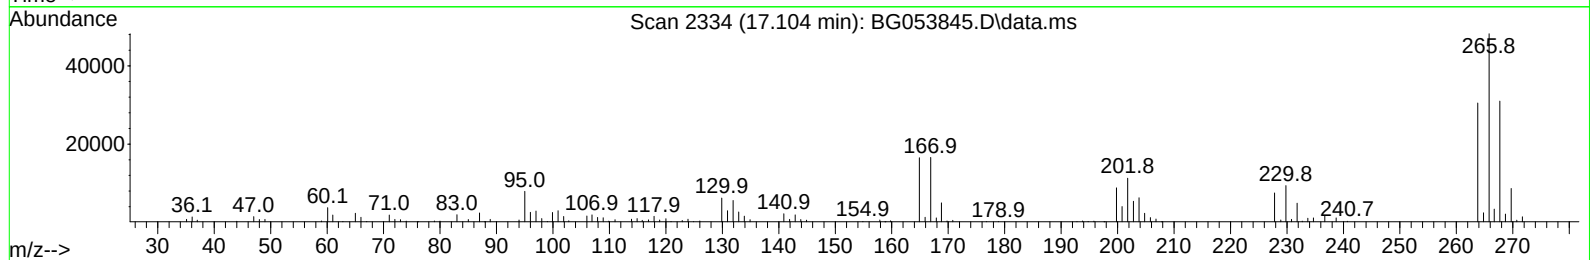


Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG060822\
Data File : BG053845.D
Acq On : 8 Jun 2022 9:30
Operator : CG/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Jun 08 18:47:42 2022
Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\8270-BG060222.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Thu Jun 02 23:22:27 2022
Response via : Initial Calibration

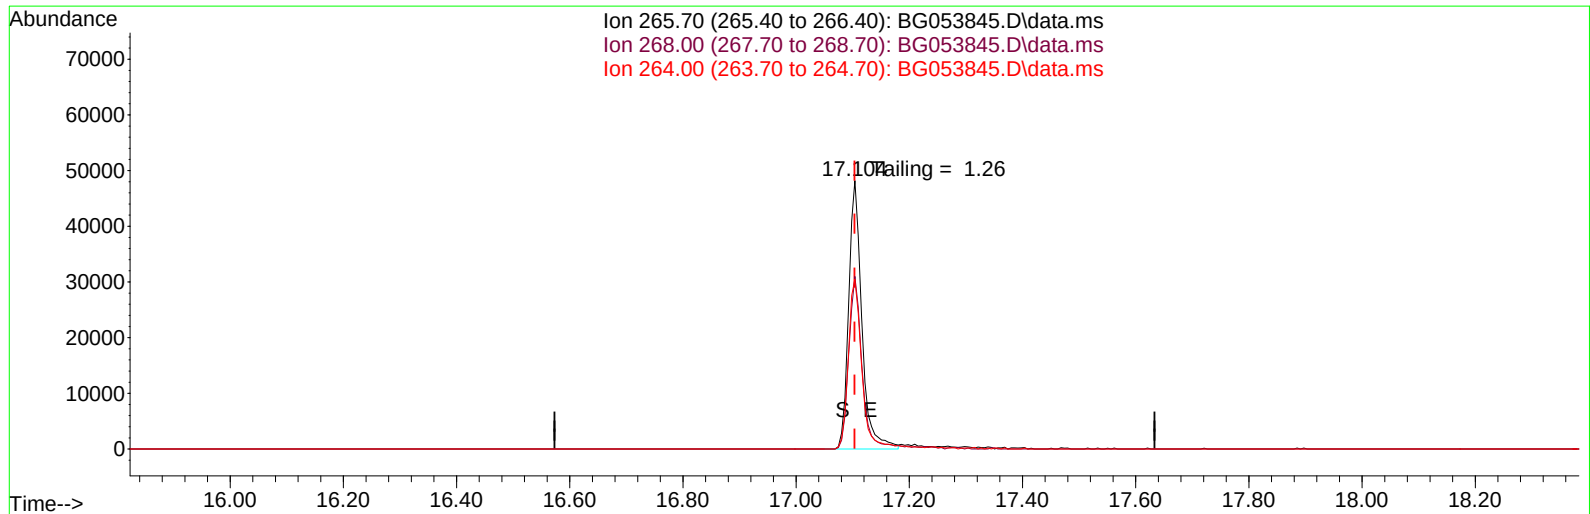

TIC: BG053845.D\data.ms

(70) Pentachlorophenol (C)




17.104min (+ 0.001) 28920.95 ng

response 80582

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	70.20	68.62
264.00	66.20	63.24
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG060822\
Data File : BG053845.D
Acq On : 8 Jun 2022 9:30
Operator : CG/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Jun 08 18:47:42 2022
Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\8270-BG060222.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Thu Jun 02 23:22:27 2022
Response via : Initial Calibration

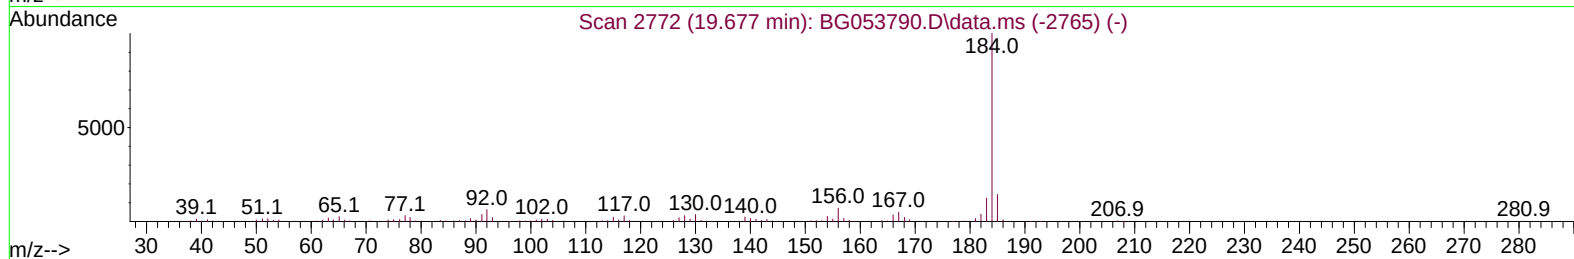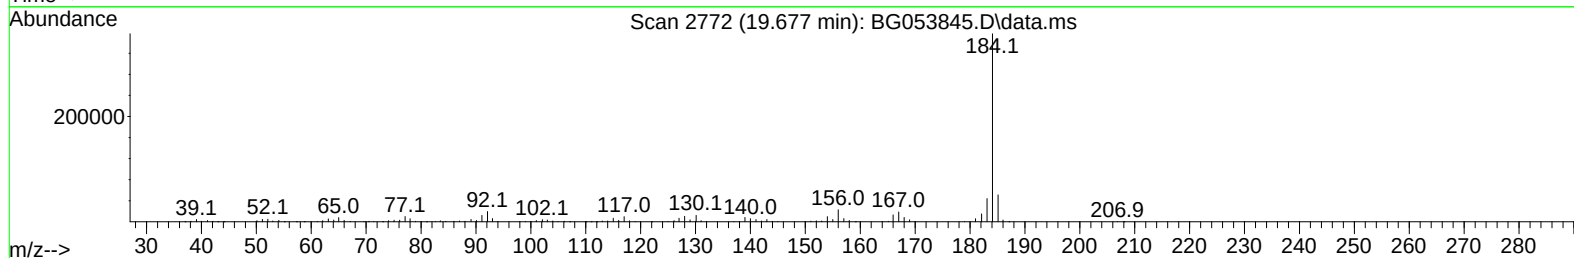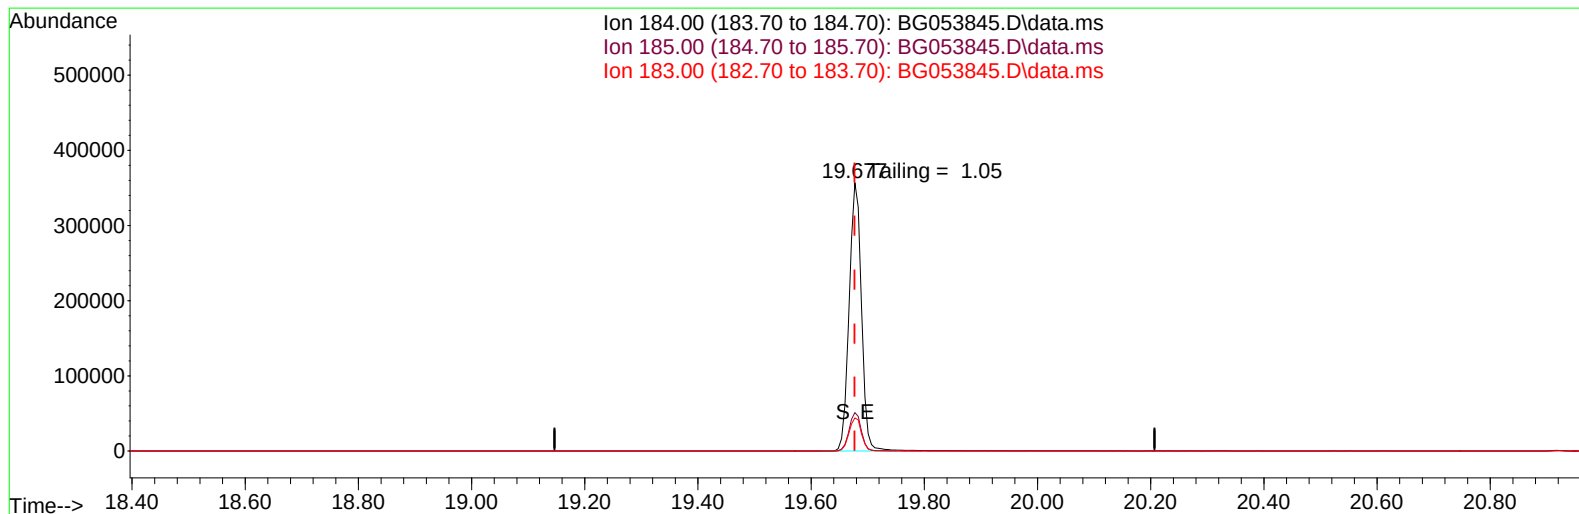

TIC: BG053845.D\data.ms

(77) Benzidine

19.677min (+ 0.001) 0.00 ng

response 537362

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	14.70	14.30
183.00	11.10	12.38
0.00	0.00	0.00