
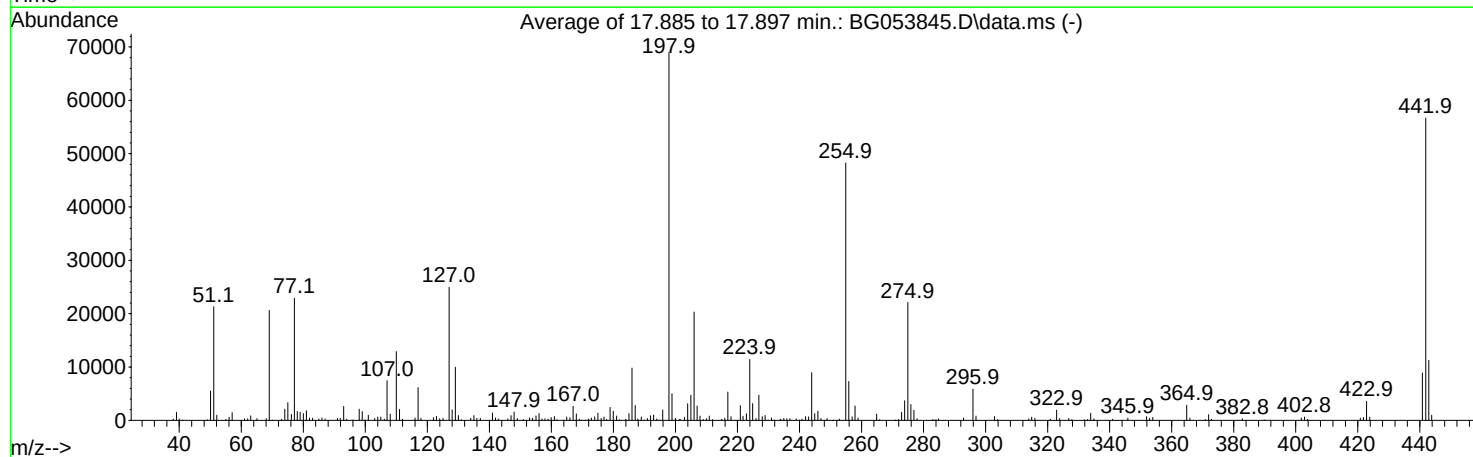


Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG060822\
 Data File : BG053845.D
 Acq On : 8 Jun 2022 9:30
 Operator : CG/JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_G
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\8270-BG060222.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Thu Jun 02 23:22:27 2022

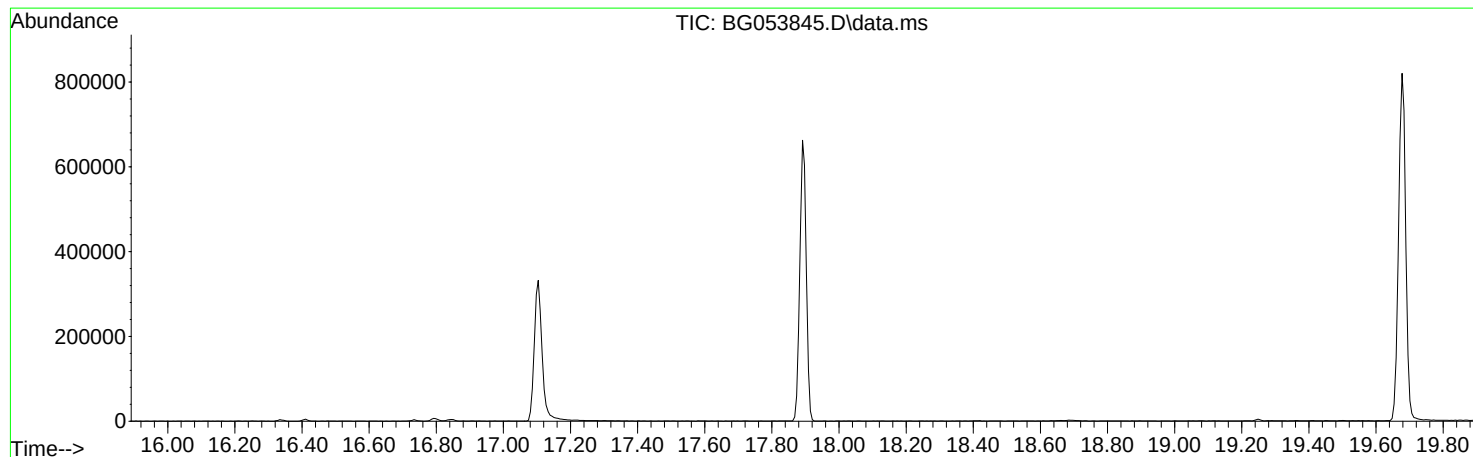




AutoFind: Scans 2467, 2468, 2469; Background Corrected with Scan 2460

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	30.9	21293	PASS
68	69	0.00	2	1.6	322	PASS
69	198	0.00	100	29.9	20621	PASS
70	69	0.00	2	0.3	67	PASS
127	198	10	80	36.2	24952	PASS
197	198	0.00	2	0.0	0	PASS
198	198	100	100	100.0	68957	PASS
199	198	5	9	7.3	5003	PASS
275	198	10	60	32.0	22096	PASS
365	198	1	100	4.1	2840	PASS
441	198	0.01	100	12.9	8872	PASS
442	442	50	100	100.0	56661	PASS
443	442	15	24	19.9	11261	PASS

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG060822\
Data File : BG053845.D
Acq On : 8 Jun 2022 9:30
Operator : CG/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
DFTPP

Quant Time: Jun 08 18:47:42 2022
Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\8270-BG060222.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Thu Jun 02 23:22:27 2022
Response via : Initial Calibration

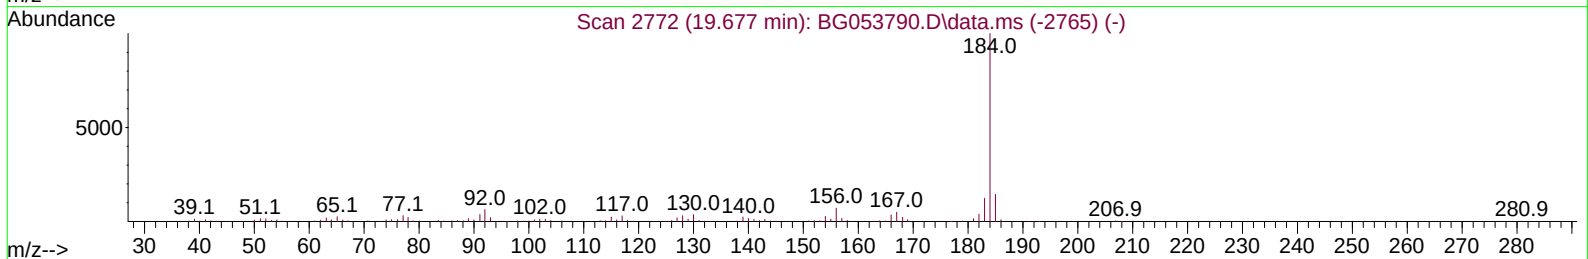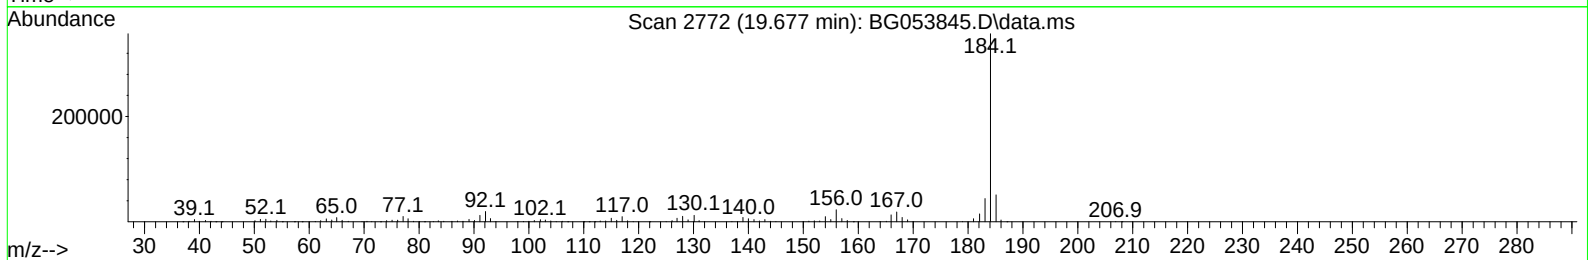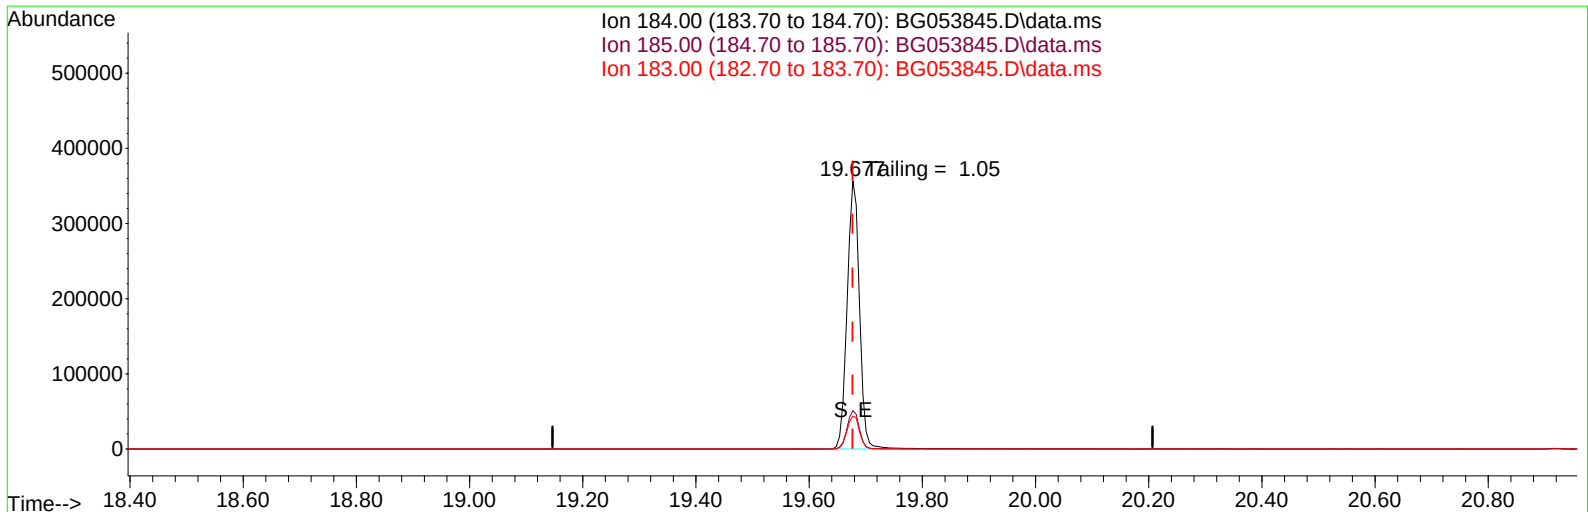

TIC: BG053845.D\data.ms

(77) Benzidine

19.677min (+ 0.001) 0.00 ng

response 537362

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	14.70	14.30
183.00	11.10	12.38
0.00	0.00	0.00

DDT Breakdown

Date	Instrument Name	DFTPP Data File
6/8/2022	BNA_G	<u>BG053845.D</u>
Compound Name	Response	Retention Time
DDT	268387	20.92
DDD	1251	20.47
DDE	111	19.97
SUM(DDD+DDE)	SUM(DDT+DDD+DDE)	% Breakdown Of DDT
1362	269749	0.50

Instrument :
BNA_G
ClientSampleId :
DFTPP