

Data Path : Z:\HPCHEM1\BNA_G\DATA\BG060915\
 Data File : BG017579.D
 Acq On : 9 Jun 2015 18:30
 Operator : TP/IZ
 Sample : PB83868TB
 Misc :
 ALS Vial : 9 Sample Multiplier: 1

Instrument :
 BNA_G
 ClientSampleId :
 PB83868TB

Quant Time: Jun 10 05:36:58 2015
 Quant Method : Z:\HPCHEM1\BNA_G\METHODS\8270-BG060315.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Wed Jun 10 05:08:16 2015
 Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Dichlorobenzene-d4	7.57	152	12629	20.00	ng	0.00
21) Naphthalene-d8	10.37	136	47830	20.00	ng	0.00
38) Acenaphthene-d10	14.25	164	31625	20.00	ng	0.00
63) Phenanthrene-d10	17.00	188	78253	20.00	ng	0.00
75) Chrysene-d12	21.20	240	108835	20.00	ng	0.00
86) Perylene-d12	23.41	264	106016	20.00	ng	-0.01
System Monitoring Compounds						
5) 2-Fluorophenol	5.16	112	100561	140.29	ng	0.00
7) Phenol-d6	6.78	99	123533	126.50	ng	0.00
23) Nitrobenzene-d5	8.73	82	88627	92.50	ng	0.00
41) 2,4,6-Tribromophenol	15.75	330	65930	150.10	ng	0.00
44) 2-Fluorobiphenyl	12.86	172	195258	93.14	ng	0.00
78) Terphenyl-d14	19.64	244	461988	87.73	ng	0.00


Target Compounds	Qvalue
------------------	--------


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\HPCHEM1\BNA_G\DATA\BG060915\
Data File : BG017579.D
Acq On : 9 Jun 2015 18:30
Operator : TP/IZ
Sample : PB83868TB
Misc :
ALS Vial : 9 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
PB83868TB

Quant Time: Jun 10 05:36:58 2015
Quant Method : Z:\HPCHEM1\BNA_G\METHODS\8270-BG060315.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Wed Jun 10 05:08:16 2015
Response via : Initial Calibration

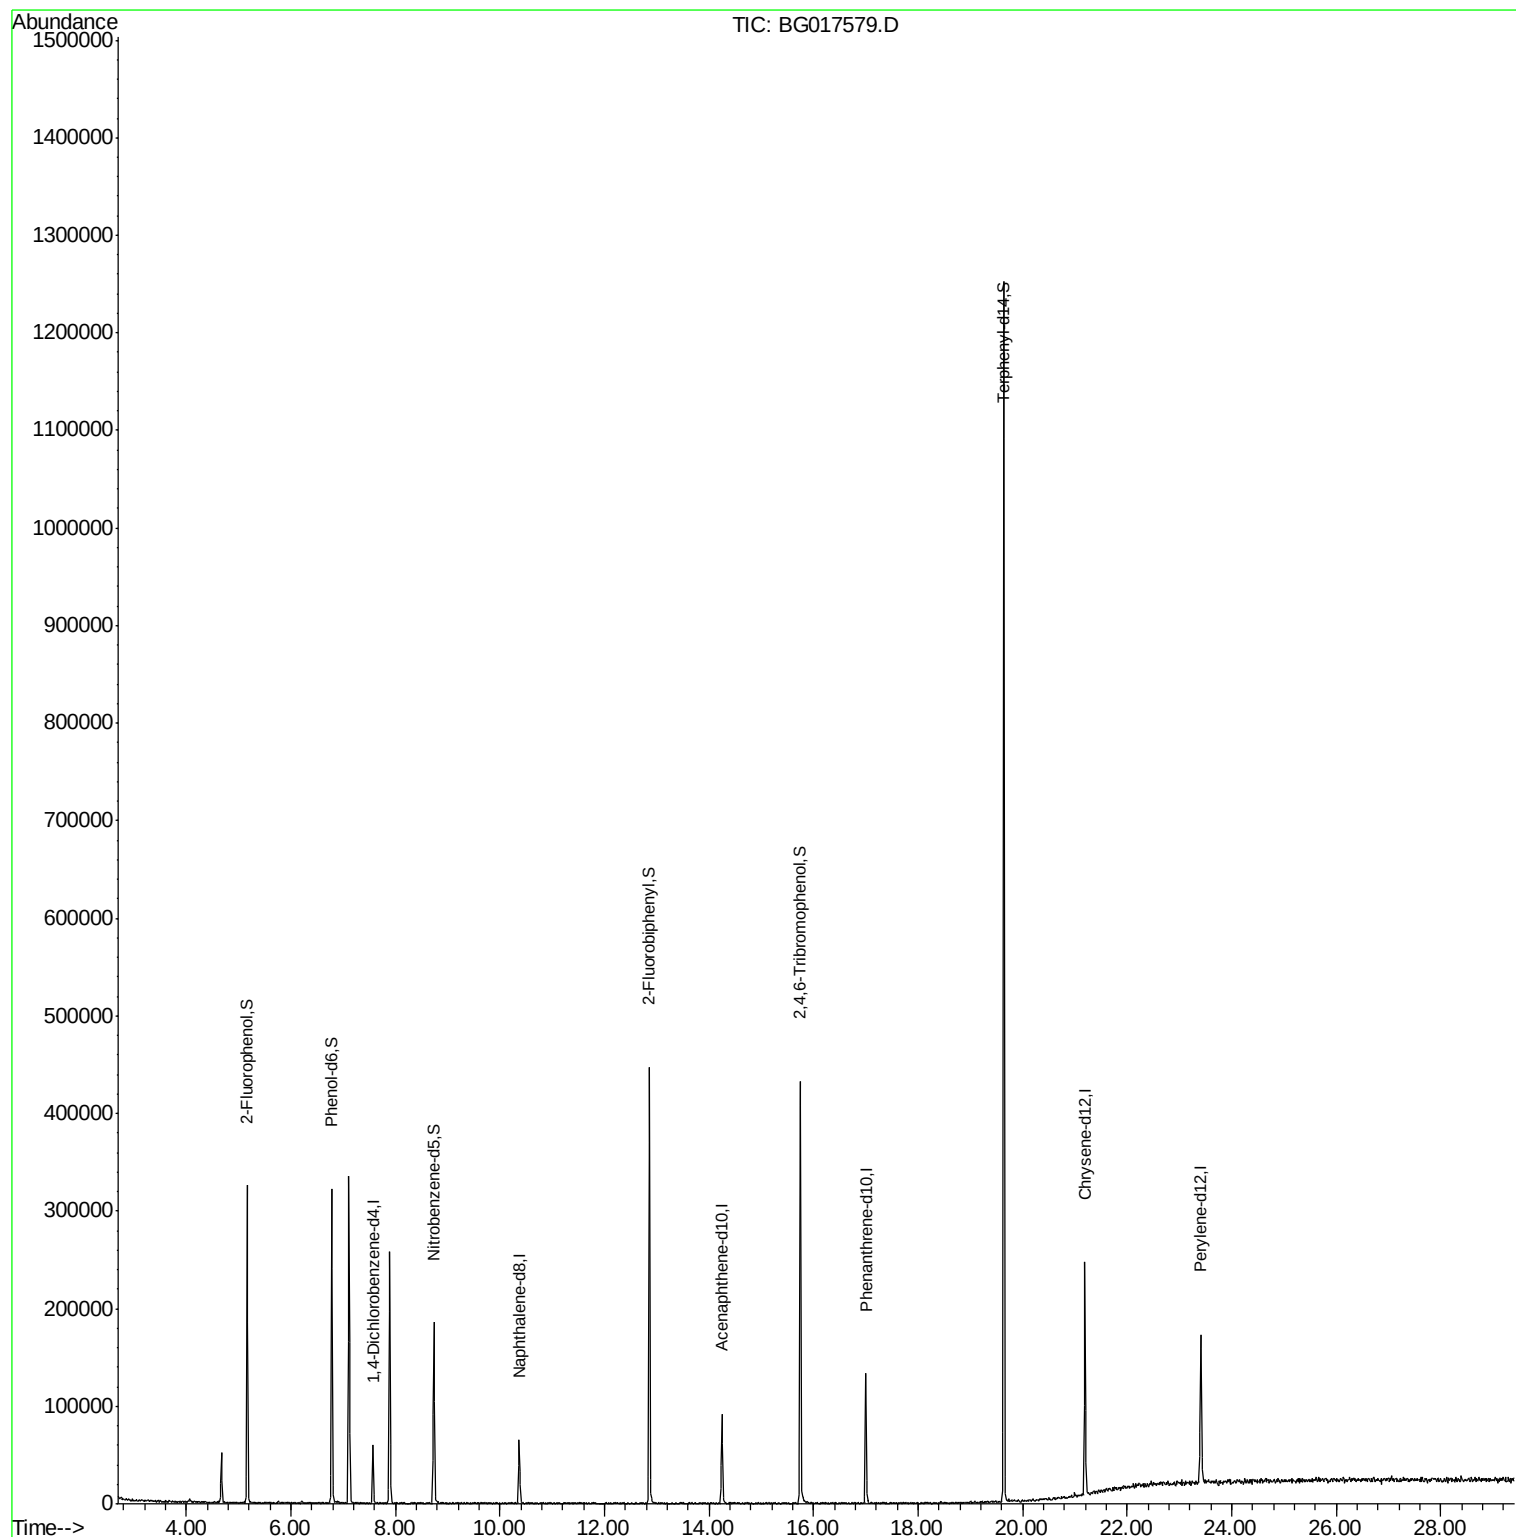

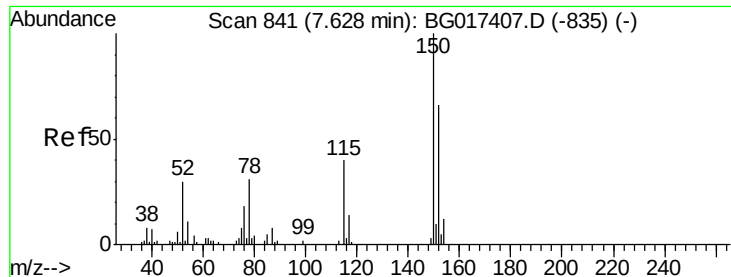


#1




1,4-Dichlorobenzene-d4
Concen: 20.00 ng
RT: 7.57 min Scan# 831
Delta R.T. 0.00 min
Lab File: BG017579.D
Acq: 9 Jun 2015 18:30

Instrument :
BNA_G
ClientSampleId :
PB83868TB

Tgt Ion:152 Resp: 12629
Ion Ratio Lower Upper
152 100
150 150.2 121.7 182.5
115 68.0 48.6 73.0

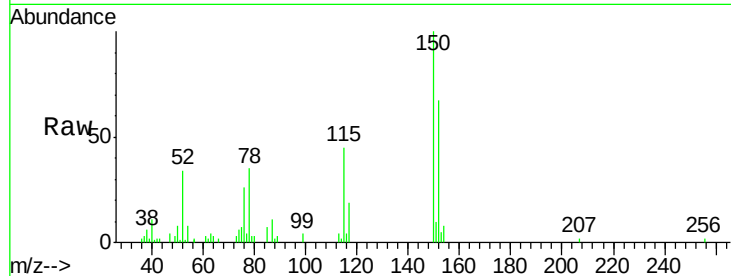


Abundance Ion 152.00 (151.70 to 152.70): E
Ion 150.00 (149.70 to 150.70): E
Ion 115.00 (114.70 to 115.70): E

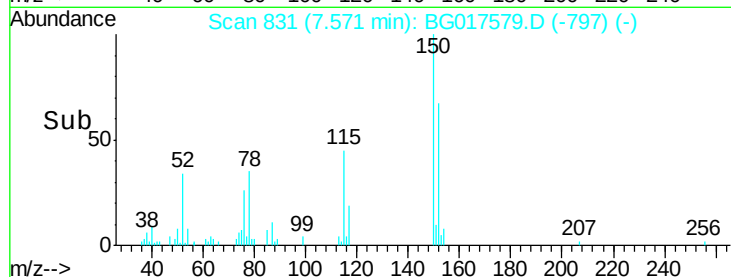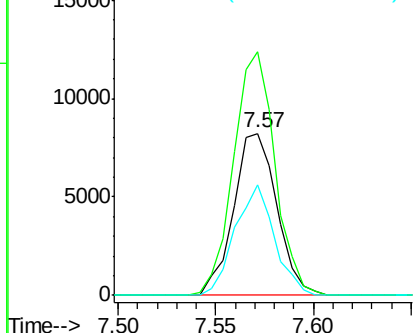



#5


2-Fluorophenol
Concen: 140.29 ng
RT: 5.16 min Scan# 421
Delta R.T. 0.00 min
Lab File: BG017579.D
Acq: 9 Jun 2015 18:30

Tgt Ion:112 Resp: 100561
Ion Ratio Lower Upper
112 100
64 65.0 51.6 77.4
63 44.7 33.3 49.9



Abundance Ion 112.00 (111.70 to 112.70): E
Ion 64.00 (63.70 to 64.70): BGC
Ion 63.00 (62.70 to 63.70): BGC

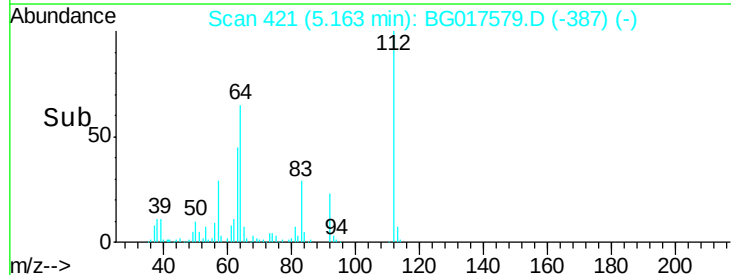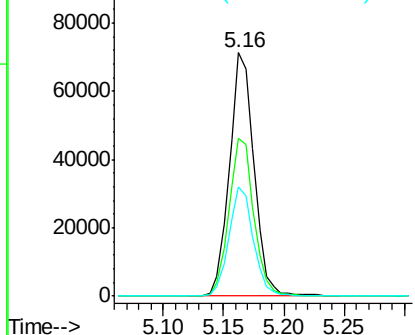

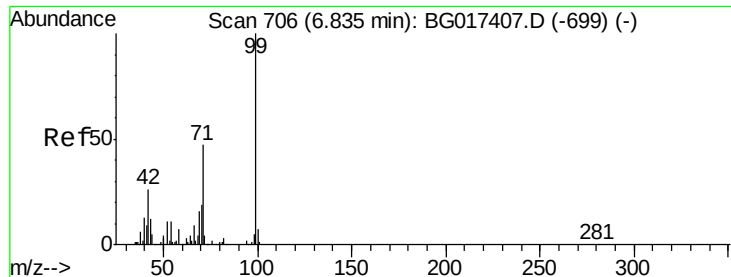

#7

Phenol-d6

Concen: 126.50 ng

RT: 6.78 min Scan# 697

Delta R.T. 0.00 min

Lab File: BG017579.D

Acq: 9 Jun 2015 18:30

Instrument :

BNA_G

ClientSampleId :

PB83868TB


Tgt Ion: 99 Resp: 123533

Ion Ratio Lower Upper




99 100

42 32.0 21.0 31.6#

71 57.9 37.2 55.8#

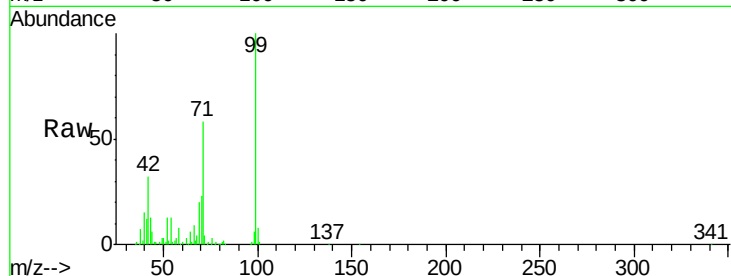

Abundance Ion 99.00 (98.70 to 99.70): BGC
Ion 42.00 (41.70 to 42.70): BGC
Ion 71.00 (70.70 to 71.70): BGC

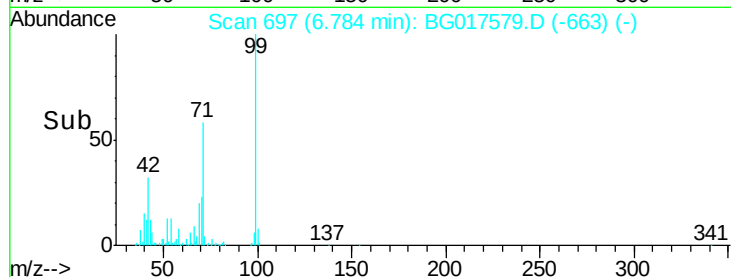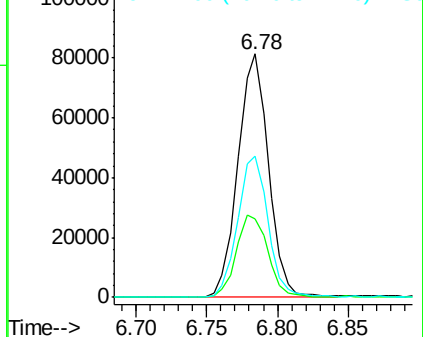

#21

Naphthalene-d8

Concen: 20.00 ng

RT: 10.37 min Scan# 1307

Delta R.T. 0.00 min

Lab File: BG017579.D

Acq: 9 Jun 2015 18:30

Tgt Ion: 136 Resp: 47830


Ion Ratio Lower Upper

136 100



137 9.0 7.9 11.9


54 10.1 7.2 10.8

68 4.4 4.5 6.7#



Abundance Ion 136.00 (135.70 to 136.70): BGC
Ion 137.00 (136.70 to 137.70): BGC
Ion 54.00 (53.70 to 54.70): BGC
Ion 68.00 (67.70 to 68.70): BGC

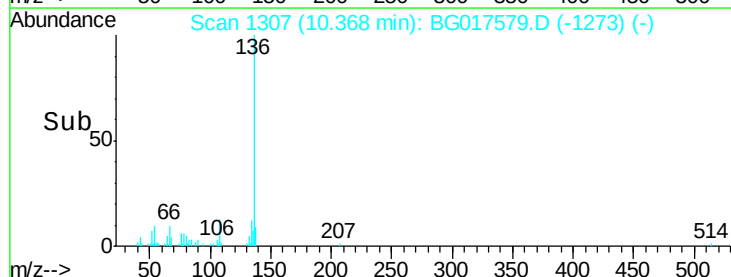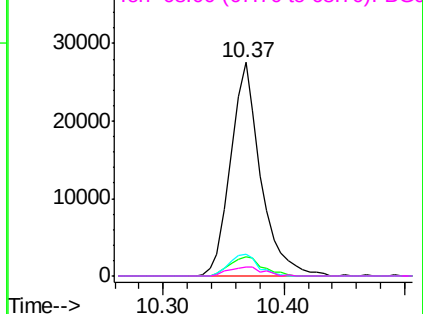


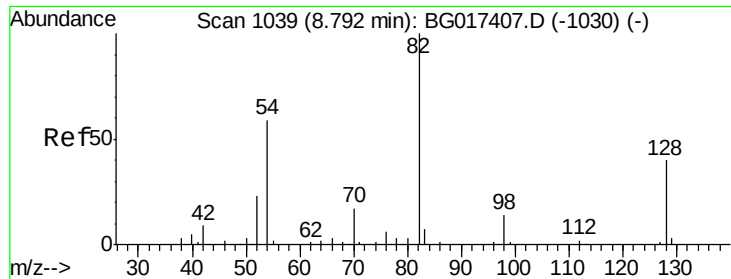




#23
 Nitrobenzene-d5
 Concen: 92.50 ng
 RT: 8.73 min Scan# 1029
 Delta R.T. -0.00 min
 Lab File: BG017579.D
 Acq: 9 Jun 2015 18:30

Instrument :
 BNA_G
 ClientSampleId :
 PB83868TB

Tgt Ion: 82 Resp: 88627
 Ion Ratio Lower Upper
 82 100
 128 42.3 32.2 48.4
 54 64.9 47.4 71.2




Abundance Ion 82.00 (81.70 to 82.70): BGC
 Ion 128.00 (127.70 to 128.70): BGC
 Ion 54.00 (53.70 to 54.70): BGC

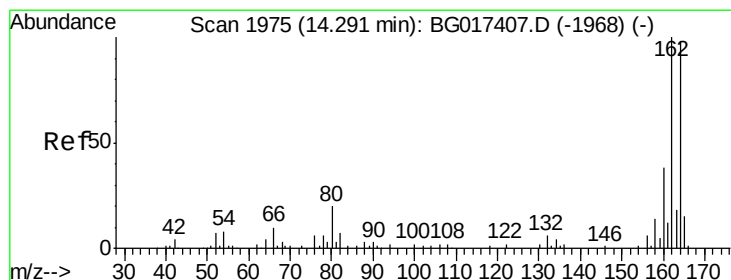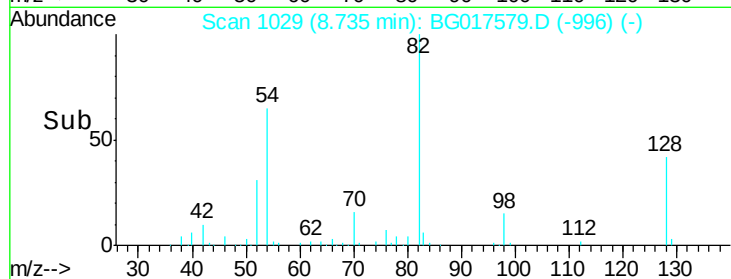
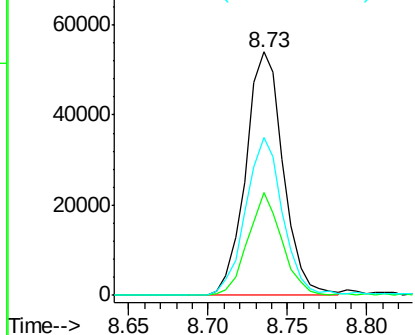



#38
 Acenaphthene-d10
 Concen: 20.00 ng
 RT: 14.25 min Scan# 1968
 Delta R.T. 0.00 min
 Lab File: BG017579.D
 Acq: 9 Jun 2015 18:30

Tgt Ion: 164 Resp: 31625
 Ion Ratio Lower Upper
 164 100
 162 91.6 81.8 122.6
 160 44.2 31.0 46.4

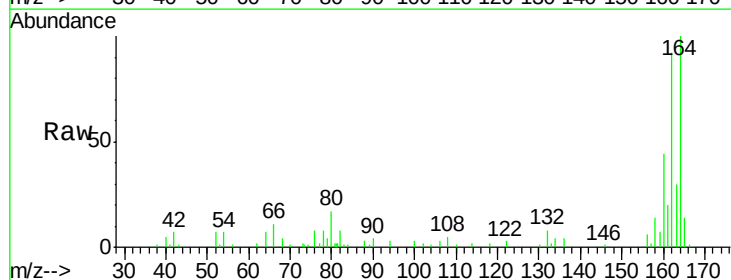

Abundance Ion 164.00 (163.70 to 164.70): BGC
 Ion 162.00 (161.70 to 162.70): BGC
 Ion 160.00 (159.70 to 160.70): BGC

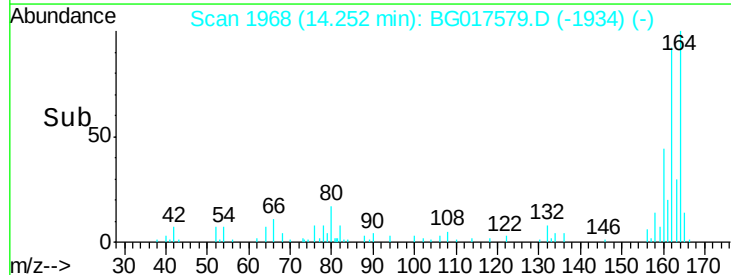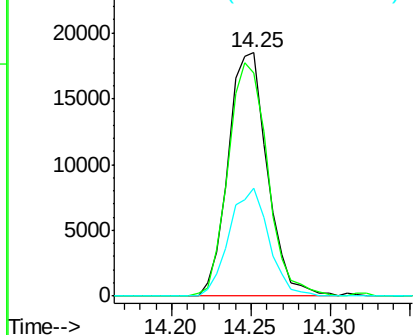


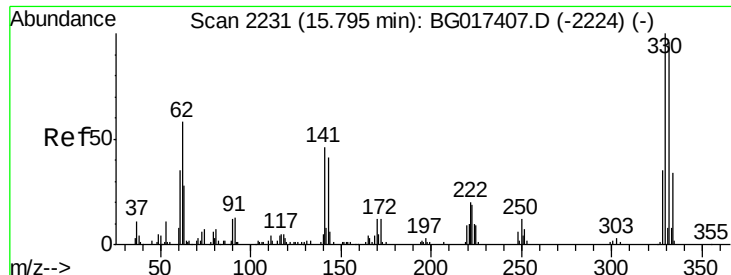




#41
 2,4,6-Tribromophenol
 Concen: 150.10 ng
 RT: 15.75 min Scan# 2223
 Delta R.T. -0.00 min
 Lab File: BG017579.D
 Acq: 9 Jun 2015 18:30

Instrument :
 BNA_G
 ClientSampleId :
 PB83868TB

Tgt Ion:330 Resp: 65930
 Ion Ratio Lower Upper
 330 100
 332 94.5 75.9 113.9
 141 51.2 40.2 60.4

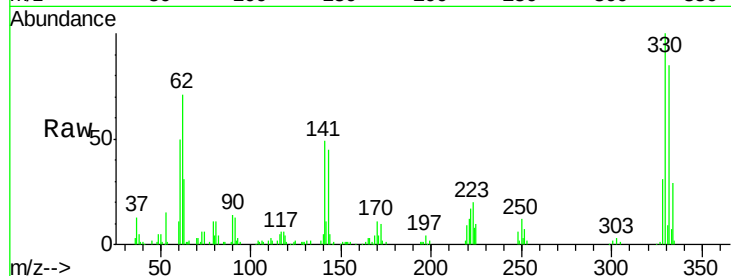


Abundance Ion 329.80 (329.50 to 330.50): E
 Ion 331.80 (331.50 to 332.50): E
 Ion 141.00 (140.70 to 141.70): E

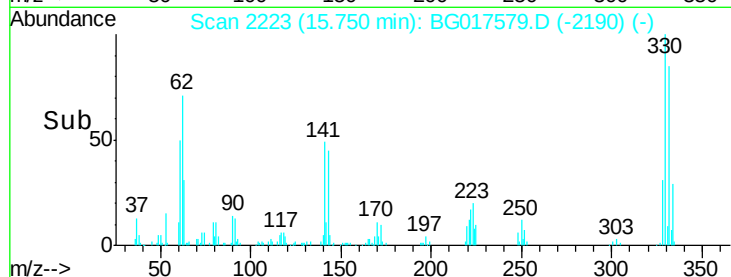
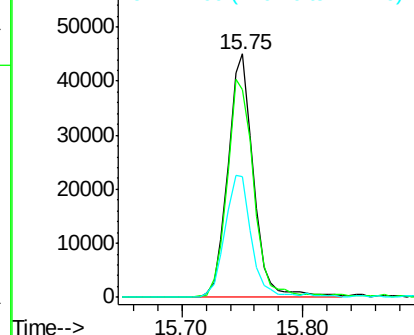



#44
 2-Fluorobiphenyl
 Concen: 93.14 ng
 RT: 12.86 min Scan# 1731
 Delta R.T. -0.00 min
 Lab File: BG017579.D
 Acq: 9 Jun 2015 18:30

Tgt Ion:172 Resp: 195258
 Ion Ratio Lower Upper
 172 100
 171 36.0 29.0 43.6
 170 23.4 18.9 28.3



Abundance Ion 172.00 (171.70 to 172.70): E
 Ion 171.00 (170.70 to 171.70): E
 Ion 170.00 (169.70 to 170.70): E

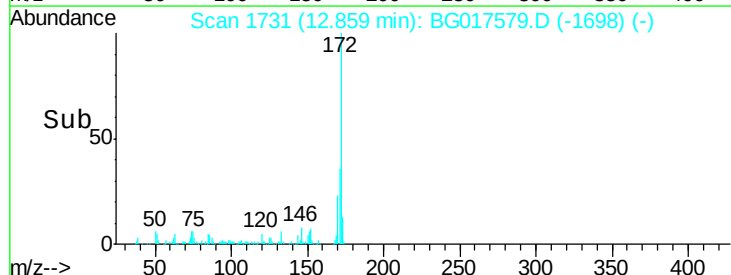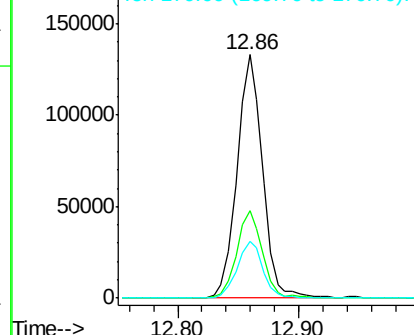

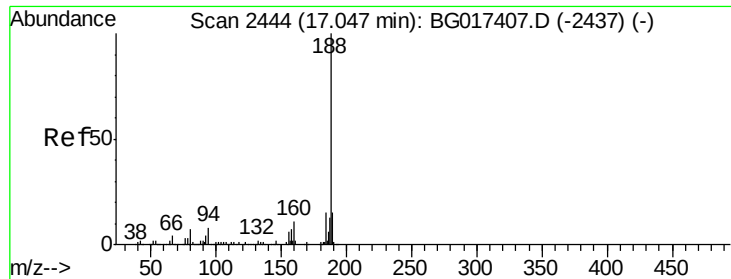

#63

Phenanthrene-d10

Concen: 20.00 ng

RT: 17.00 min Scan# 2436

Delta R.T. -0.00 min

Lab File: BG017579.D

Acq: 9 Jun 2015 18:30

Instrument :

BNA_G

ClientSampleId :

PB83868TB


Tgt Ion:188 Resp: 78253

Ion Ratio Lower Upper

188 100

94 6.1 6.3 9.5#




80 8.3 5.2 7.8#

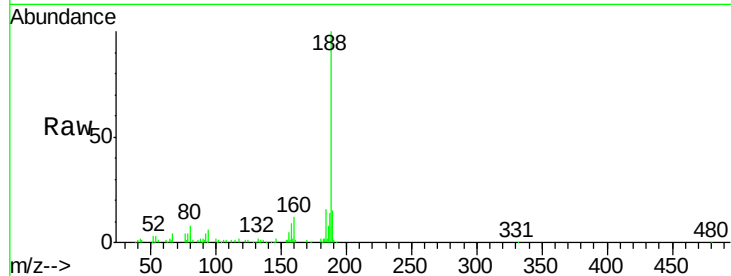

Abundance Ion 188.00 (187.70 to 188.70): E

Ion 94.00 (93.70 to 94.70): BGC

Ion 80.00 (79.70 to 80.70): BGC

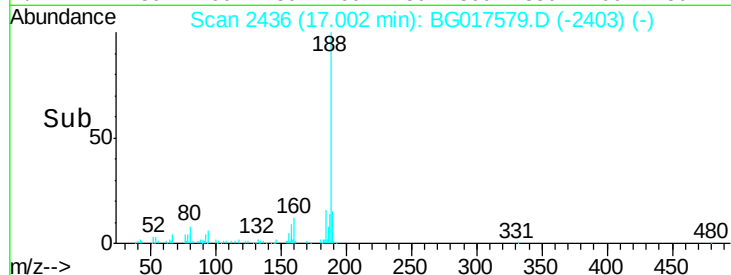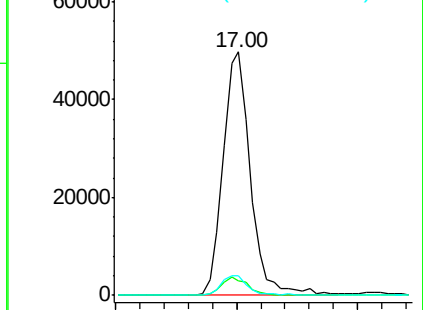

#75

Chrysene-d12

Concen: 20.00 ng

RT: 21.20 min Scan# 3150

Delta R.T. -0.00 min

Lab File: BG017579.D

Acq: 9 Jun 2015 18:30


Tgt Ion:240 Resp: 108835

Ion Ratio Lower Upper

240 100

120 7.6 6.5 9.7



236 26.4 20.8 31.2




Abundance Ion 240.00 (239.70 to 240.70): E

Ion 120.00 (119.70 to 120.70): E

Ion 236.00 (235.70 to 236.70): E

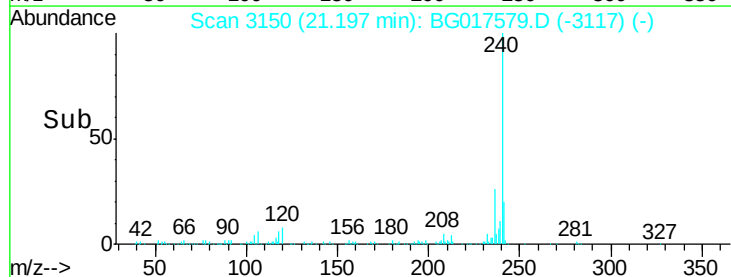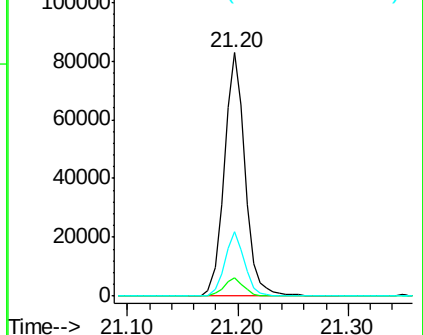

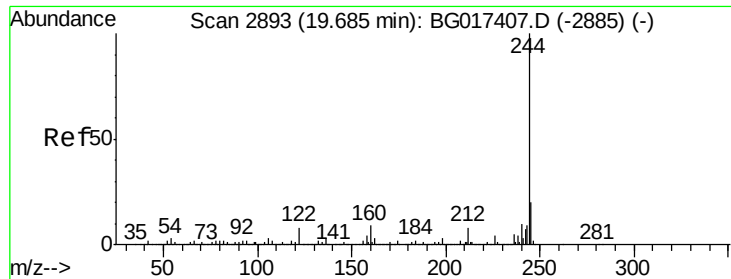

#78

Terphenyl-d14

Concen: 87.73 ng

RT: 19.64 min Scan# 2885

Delta R.T. -0.00 min

Lab File: BG017579.D

Acq: 9 Jun 2015 18:30

Instrument :

BNA_G

ClientSampleId :

PB83868TB


Tgt Ion:244 Resp: 461988

Ion Ratio Lower Upper

244 100

212 8.4 6.4 9.6




122 8.4 6.6 10.0

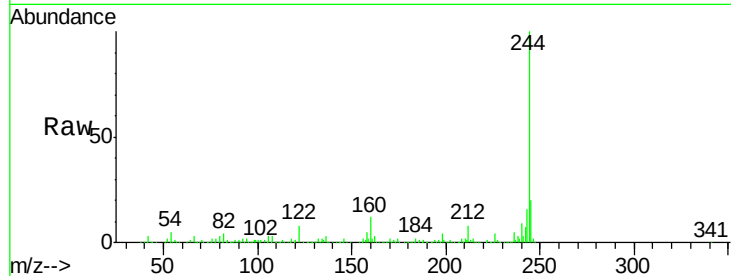

Abundance Ion 244.00 (243.70 to 244.70): E

Ion 212.00 (211.70 to 212.70): E

Ion 122.00 (121.70 to 122.70): E

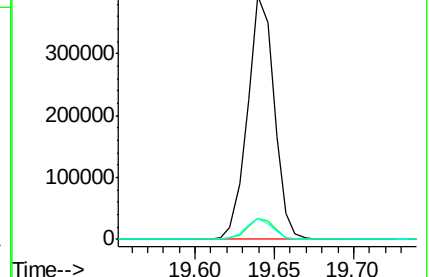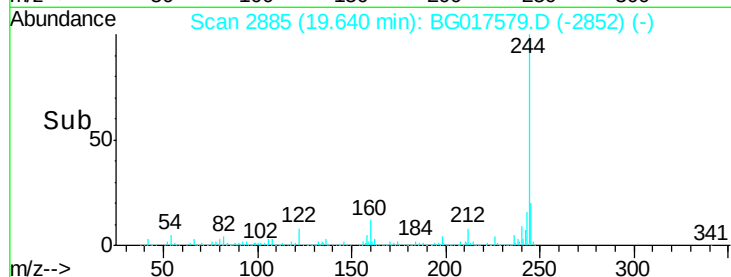

#86

Perylene-d12

Concen: 20.00 ng

RT: 23.41 min Scan# 3527

Delta R.T. -0.01 min

Lab File: BG017579.D

Acq: 9 Jun 2015 18:30


Tgt Ion:264 Resp: 106016

Ion Ratio Lower Upper

264 100

260 24.4 18.2 27.4

265 22.5 15.8 23.6



Abundance Ion 264.00 (263.70 to 264.70): E

Ion 260.00 (259.70 to 260.70): E

Ion 265.00 (264.70 to 265.70): E

