

Data Path : Z:\HPCHEM1\BNA_G\DATA\BG060915\
 Data File : BG017598.D
 Acq On : 10 Jun 2015 7:19
 Operator : TP/IZ
 Sample : G2552-01 5X
 Misc :
 ALS Vial : 25 Sample Multiplier: 1

Instrument :
 BNA_G
 ClientSampleId :
 SW-028

Integration Parameters: rteint.p
 Integrator: RTE
 Smoothing : ON
 Sampling : 1
 Start Thrs: 0.2
 Stop Thrs : 0
 Filtering: 5
 Min Area: 3 % of largest Peak
 Max Peaks: 100
 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\HPCHEM1\BNA_G\METHODS\8270-BG060315.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

Signal : TIC

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	2.718	3	5	9	rVB3	8729	9719	2.54%	0.308%
2	4.680	335	339	345	rBV2	11219	16370	4.27%	0.518%
3	5.168	417	422	433	rVB	93858	148568	38.77%	4.704%
4	6.789	691	698	710	rBV	98050	166226	43.38%	5.263%
5	7.118	748	754	763	rVB	102741	170081	44.39%	5.385%
6	7.571	826	831	838	rBV	93813	148292	38.70%	4.695%
7	7.894	877	886	893	rBV	80973	123621	32.26%	3.914%
8	8.740	1022	1030	1039	rBV	62924	106241	27.73%	3.364%
9	10.368	1300	1307	1317	rBV	128432	208653	54.46%	6.606%
10	12.859	1725	1731	1740	rBV	124239	191786	50.05%	6.072%
11	13.711	1871	1876	1882	rBV	17642	25054	6.54%	0.793%
12	14.245	1960	1967	1975	rBV2	172956	261479	68.24%	8.278%
13	15.750	2216	2223	2230	rBV	113208	168582	44.00%	5.337%
14	17.001	2430	2436	2440	rBV	218573	299177	78.08%	9.472%
15	17.042	2440	2443	2447	rVB	12051	15810	4.13%	0.501%
16	17.912	2587	2591	2593	rBV4	3631	4403	1.15%	0.139%
17	18.012	2603	2608	2613	rVB5	2544	5039	1.32%	0.160%
18	19.069	2782	2788	2793	rBV	24597	37229	9.72%	1.179%
19	19.433	2842	2850	2854	rBV2	24125	37506	9.79%	1.187%
20	19.639	2880	2885	2894	rVB	220273	281667	73.51%	8.917%
21	19.757	2900	2905	2907	rBV5	5336	9595	2.50%	0.304%
22	20.033	2950	2952	2954	rVV3	4510	4035	1.05%	0.128%
23	20.914	3099	3102	3106	rBV6	14733	22954	5.99%	0.727%
24	20.990	3112	3115	3118	rBV5	9654	14583	3.81%	0.462%
25	21.108	3133	3135	3136	rBV2	10610	7497	1.96%	0.237%
26	21.196	3144	3150	3155	rBV	289976	383163	100.00%	12.131%
27	23.417	3523	3528	3536	rVB2	155475	291312	76.03%	9.223%


Sum of corrected areas: 3158642

Data Path : Z:\HPCHEM1\BNA_G\DATA\BG060915\
Data File : BG017598.D
Acq On : 10 Jun 2015 7:19
Operator : TP/IZ
Sample : G2552-01 5X
Misc :
ALS Vial : 25 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
SW-028

Quant Method : Z:\HPCHEM1\BNA_G\METHODS\8270-BG060315.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\DATABASE\NIST02.L
TIC Integration Parameters: LSCINT.P

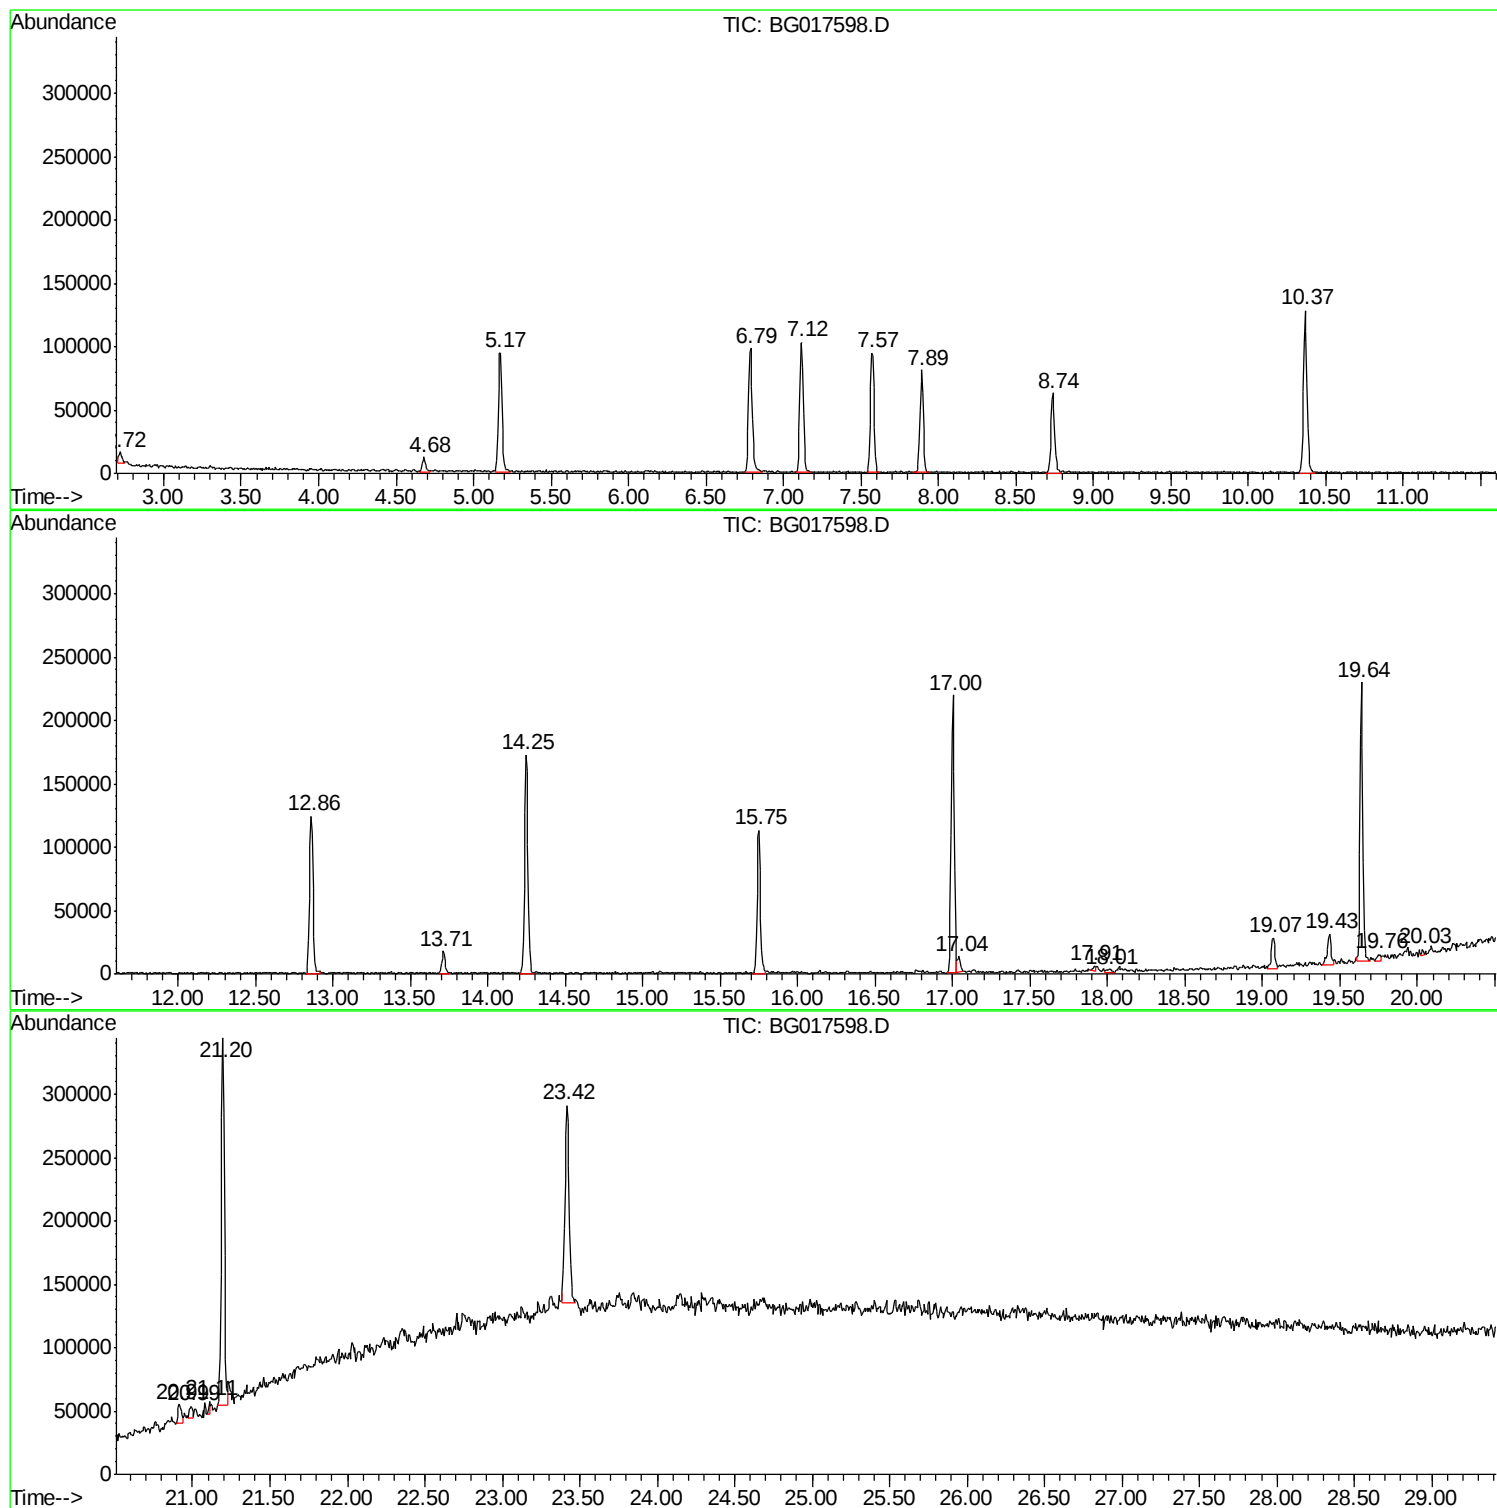

Data Path : Z:\HPCHEM1\BNA_G\DATA\BG060915\
Data File : BG017598.D
Acq On : 10 Jun 2015 7:19
Operator : TP/IZ
Sample : G2552-01 5X
Misc :
ALS Vial : 25 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
SW-028










Quant Method : Z:\HPCHEM1\BNA_G\METHODS\8270-BG060315.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\DATABASE\NIST02.L
TIC Integration Parameters: LSCINT.P

Peak Number 1 2-Pentanone, 4-hydroxy-4-me... Concentration Rank 4

R.T.	EstConc	Area	Relative to ISTD	R.T.
4.68	2.21 ng	16370	1,4-Dichlorobenzene-d4	7.58

Hit# of	5	Tentative ID	MW	MolForm	CAS#	Qual
1	2-Pentanone, 4-hydroxy-4-methyl-	116	C6H12O2	000123-42-2	53	
2	Formamide, N-butyl-	101	C5H11NO	000871-71-6	25	
3	3-Nonanol	144	C9H20O	000624-51-1	9	
4	3-Octanol	130	C8H18O	000589-98-0	9	
5	Butanal, 3-methyl-, oxime	101	C5H11NO	000626-90-4	9	

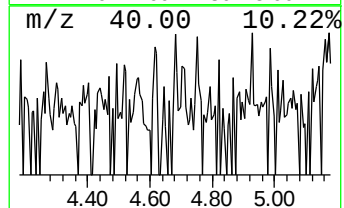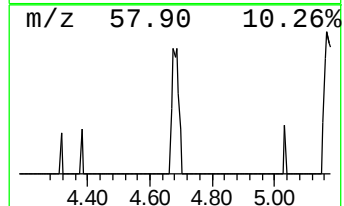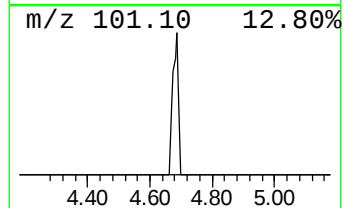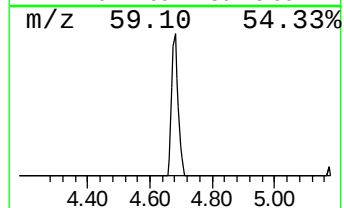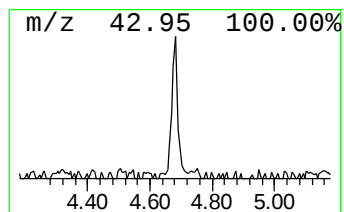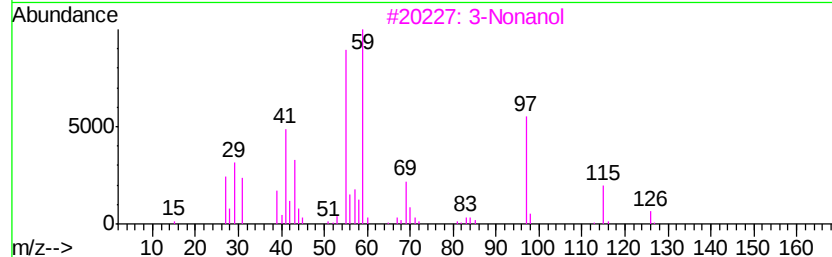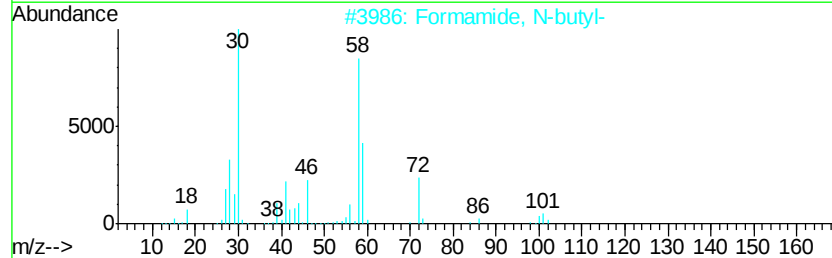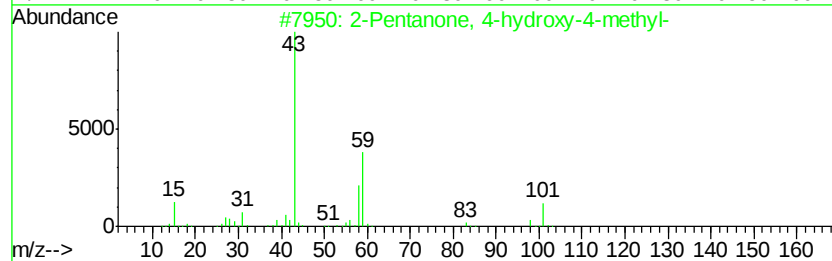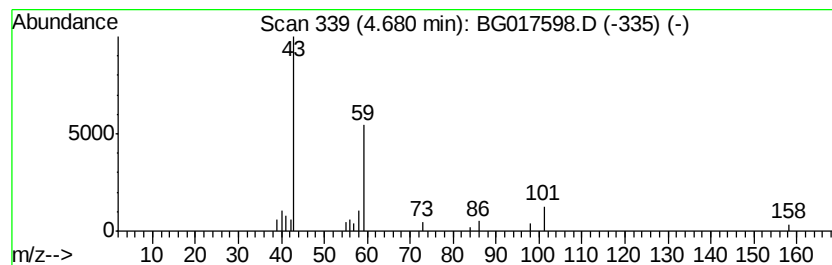

Data Path : Z:\HPCHEM1\BNA_G\DATA\BG060915\
Data File : BG017598.D
Acq On : 10 Jun 2015 7:19
Operator : TP/IZ
Sample : G2552-01 5X
Misc :
ALS Vial : 25 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
SW-028










Quant Method : Z:\HPCHEM1\BNA_G\METHODS\8270-BG060315.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\DATABASE\NIST02.L
TIC Integration Parameters: LSCINT.P

Peak Number 2 unknown7.12 Concentration Rank 1

R.T.	EstConc	Area	Relative to ISTD	R.T.
7.12	22.94 ng	170081	1,4-Dichlorobenzene-d4	7.58

Hit#	of	Tentative ID	MW	MolForm	CAS#	Qual
1	5	1,3-Cyclopentanedione, 2-chloro-	132	C5H5ClO2	014203-19-1	22
2		1H-Benzimidazole, 2-methyl-	132	C8H8N2	000615-15-6	18
3		3-Chloro-6-fluoro-pyrazine	132	C4H2ClFN2	1000146-10-7	14
4		1,3,4-Thiadiazole-2(3H)-thione, ...	132	C3H4N2S2	029490-19-5	14
5		(E)-3-Chloro-2-methyl-2-pentenal	132	C6H9ClO	031357-76-3	10

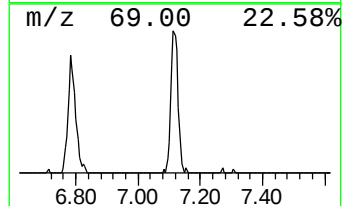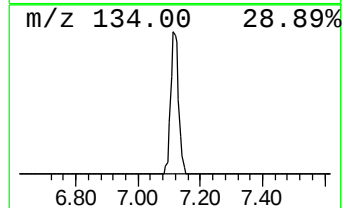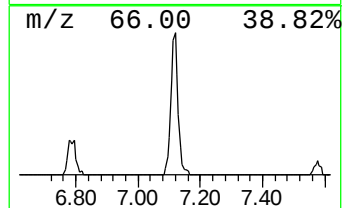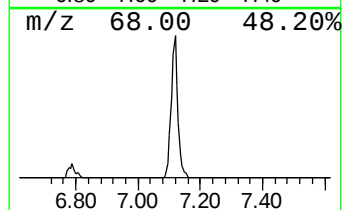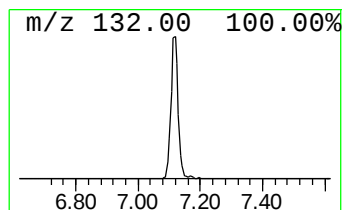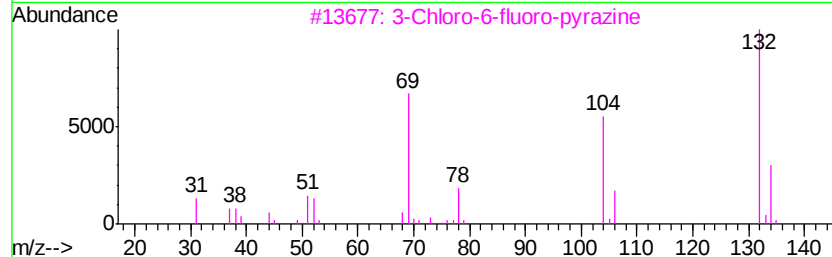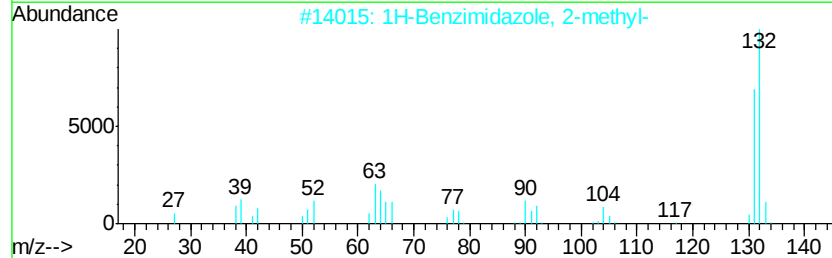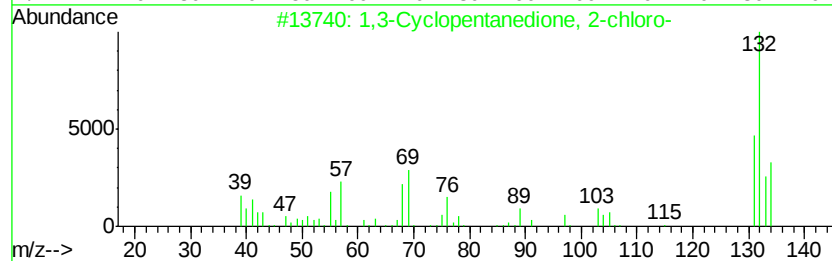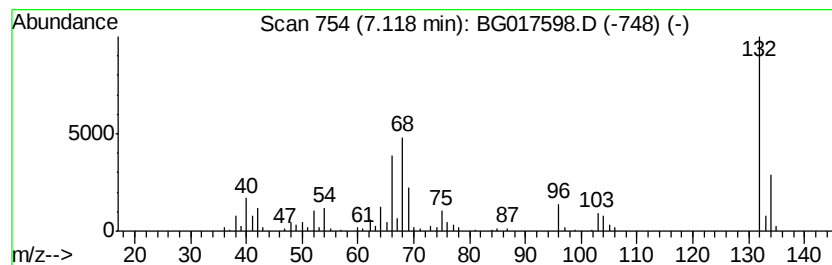

Data Path : Z:\HPCHEM1\BNA_G\DATA\BG060915\
Data File : BG017598.D
Acq On : 10 Jun 2015 7:19
Operator : TP/IZ
Sample : G2552-01 5X
Misc :
ALS Vial : 25 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
SW-028

Quant Method : Z:\HPCHEM1\BNA_G\METHODS\8270-BG060315.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\DATABASE\NIST02.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc
2-Pentanone, 4-hy...	4.68	2.2	ng	16370	1	7.58	148292	20.0
unknown7.12	7.12	22.9	ng	170081	1	7.58	148292	20.0