


Data Path : Z:\HPCHEM1\BNA_G\DATA\BG060915\
 Data File : BG017571.D
 Acq On : 9 Jun 2015 13:23
 Operator : TP/IZ
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_G
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\HPCHEM1\BNA_G\METHODS\8270-BG060315.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Mon Jun 08 18:39:50 2015

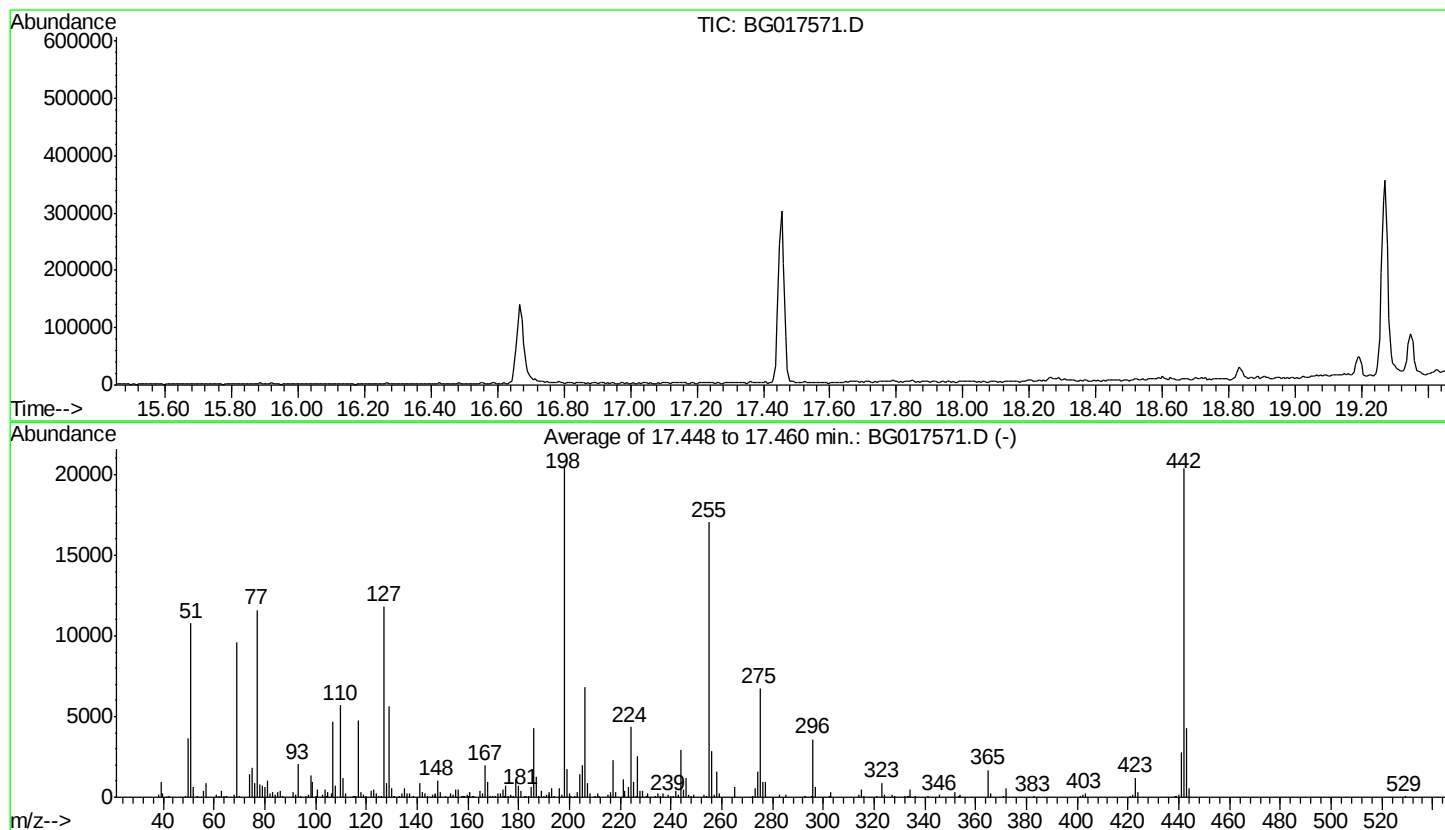

AutoFind: Scans 2512, 2513, 2514; Background Corrected with Scan 2505

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	52.5	10777	PASS
68	69	0.00	2	1.8	168	PASS
69	198	0.00	100	46.6	9570	PASS
70	69	0.00	2	1.0	97	PASS
127	198	10	80	57.4	11799	PASS
197	198	0.00	2	0.8	168	PASS
198	198	100	100	100.0	20546	PASS
199	198	5	9	8.7	1786	PASS
275	198	10	60	32.8	6739	PASS
365	198	1	100	8.3	1701	PASS
441	442	0.01	24	13.5	2745	PASS
442	198	50	100	99.3	20395	PASS
443	442	15	24	20.9	4270	PASS