


Data Path : Z:\HPCHEM1\BNA_G\DATA\BG060915\
 Data File : BG017584.D
 Acq On : 9 Jun 2015 22:36
 Operator : TP/IZ
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_G
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\HPCHEM1\BNA_G\METHODS\8270-BG060315.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Mon Jun 08 18:39:50 2015

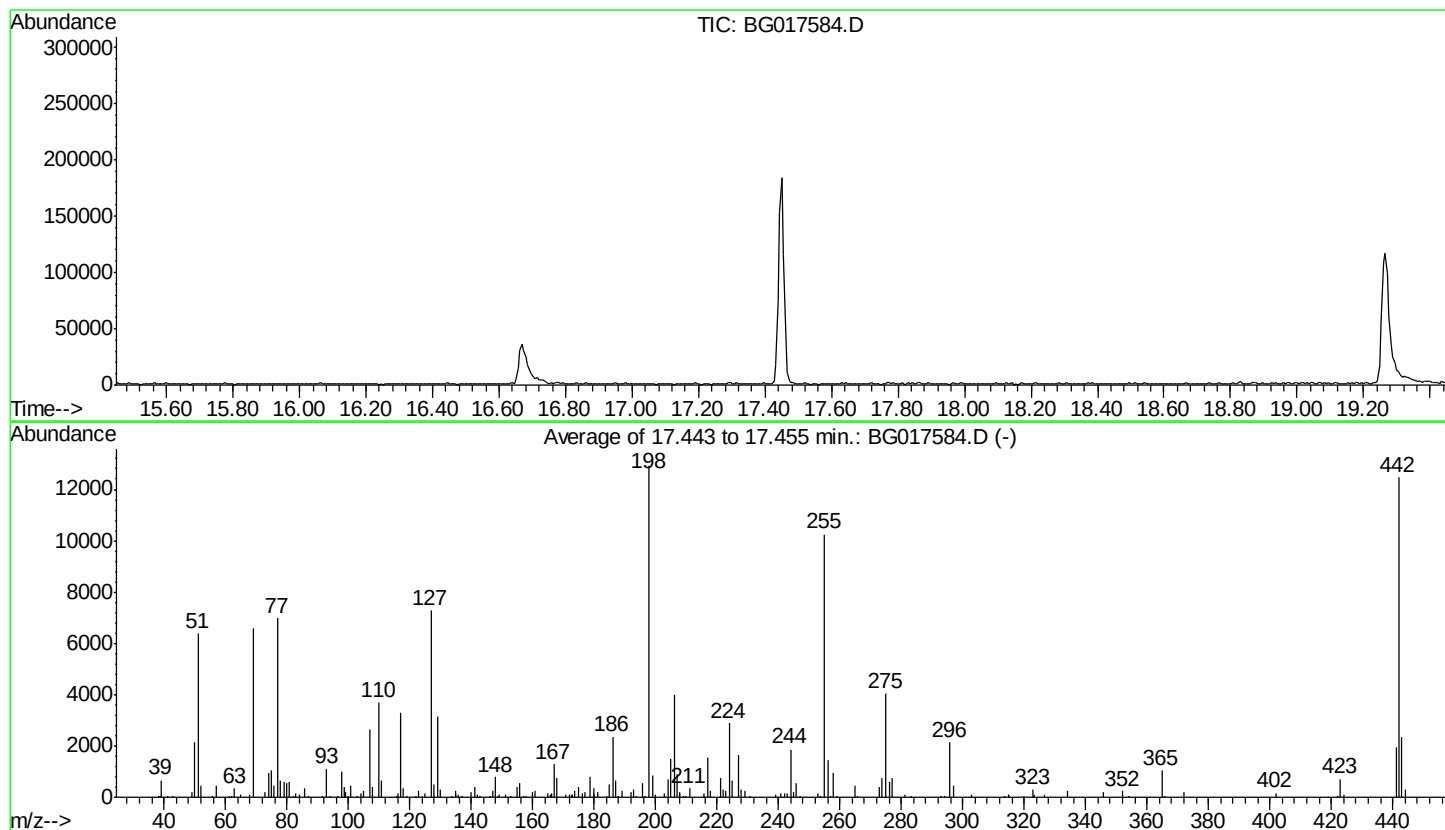

AutoFind: Scans 2511, 2512, 2513; Background Corrected with Scan 2505

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	49.3	6374	PASS
68	69	0.00	2	1.8	122	PASS
69	198	0.00	100	51.1	6605	PASS
70	69	0.00	2	0.0	0	PASS
127	198	10	80	56.3	7277	PASS
197	198	0.00	2	0.0	0	PASS
198	198	100	100	100.0	12924	PASS
199	198	5	9	6.8	873	PASS
275	198	10	60	31.1	4023	PASS
365	198	1	100	8.0	1030	PASS
441	442	0.01	24	15.8	1970	PASS
442	198	50	100	96.5	12467	PASS
443	442	15	24	18.9	2357	PASS