
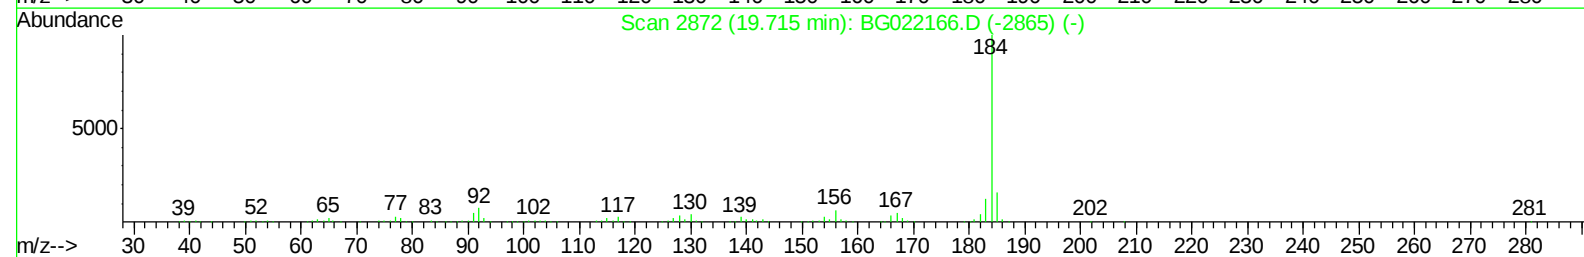
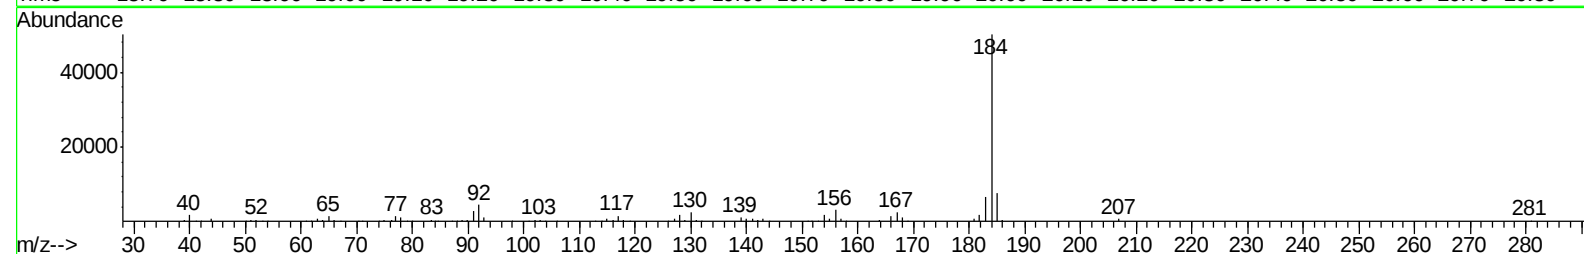


Data Path : Z:\HPCHEM1\BNA_G\DATA\BG060916\
Data File : BG022258.D
Acq On : 9 Jun 2016 7:45
Operator : UM/SJ
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Jun 10 08:06:18 2016
Quant Method : Z:\HPCHEM1\BNA_G\METHODS\8270-BG060616.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Mon Jun 06 16:12:45 2016
Response via : Initial Calibration

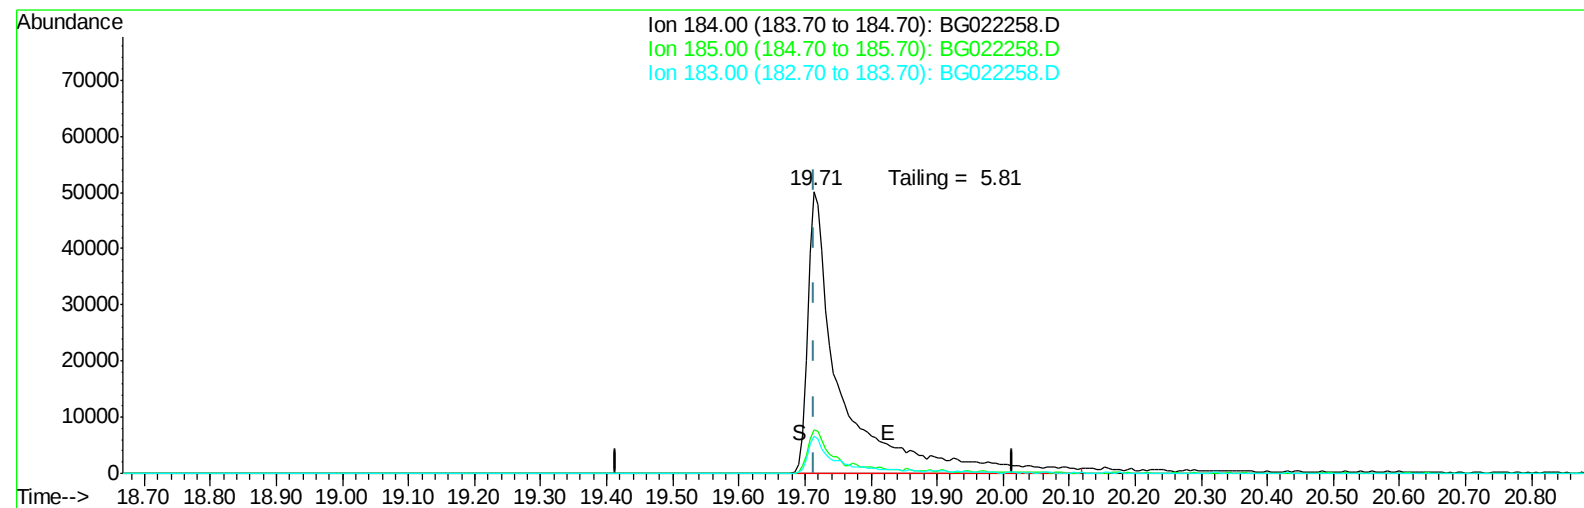

TIC: BG022258.D

(76) Benzidine




19.713min (-0.002) 0.00ng

response 154229

Ion	Exp%	Act%
184.00	100	100
185.00	14.40	15.51
183.00	12.80	13.01
0.00	0.00	0.00

Data Path : Z:\HPCHEM1\BNA_G\DATA\BG060916\
Data File : BG022258.D
Acq On : 9 Jun 2016 7:45
Operator : UM/SJ
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Jun 10 08:06:18 2016
Quant Method : Z:\HPCHEM1\BNA_G\METHODS\8270-BG060616.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Mon Jun 06 16:12:45 2016
Response via : Initial Calibration

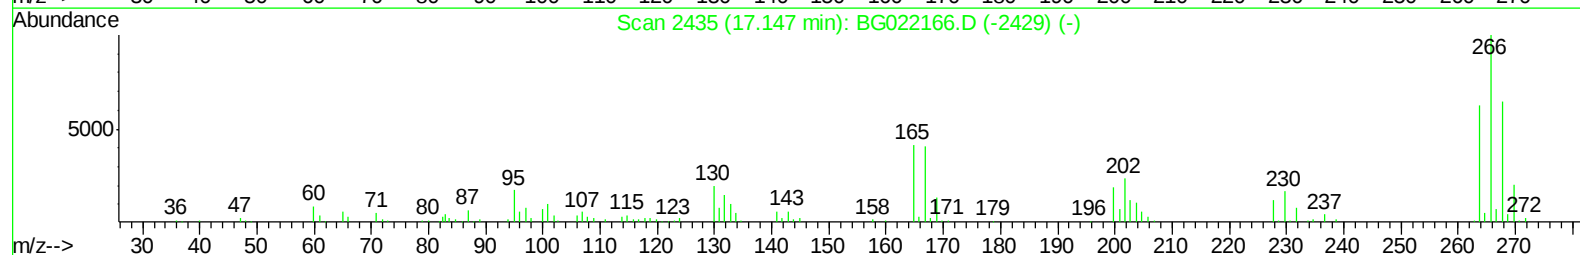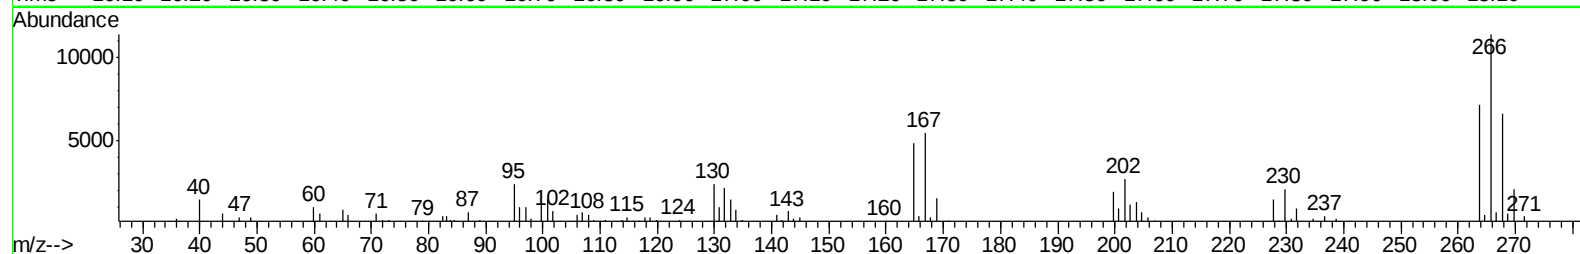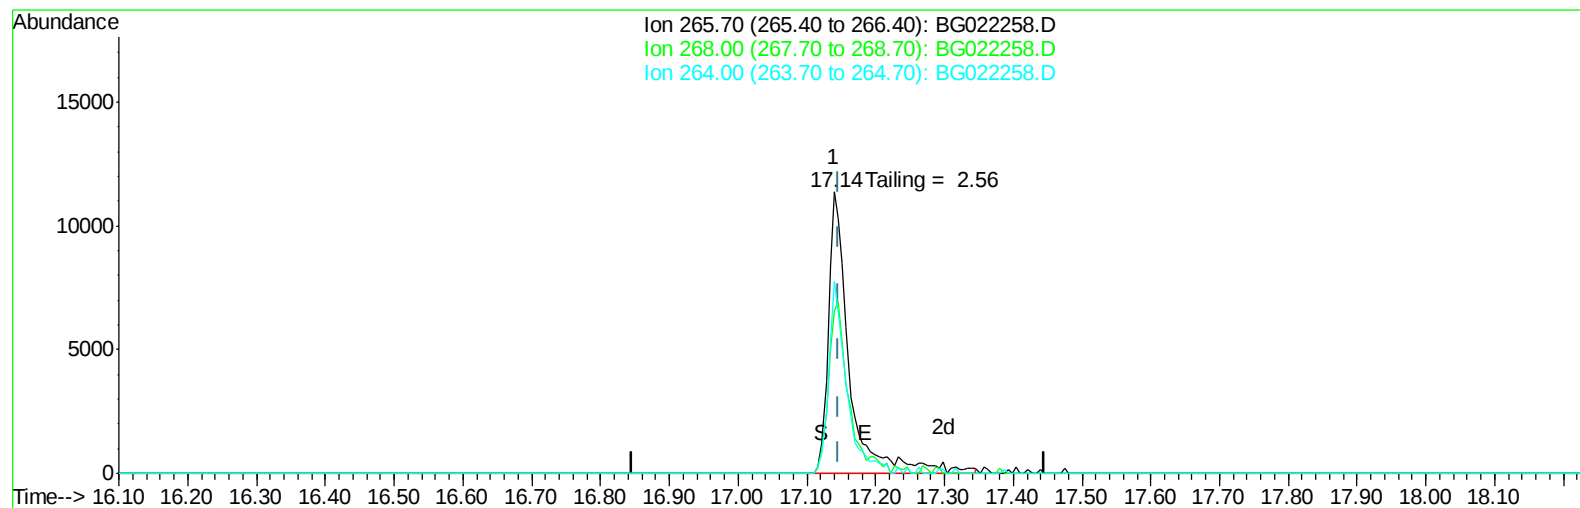

TIC: BG022258.D

(69) Pentachlorophenol (C)

17.140min (-0.007) 0.00ng

response 22299

Ion	Exp%	Act%
265.70	100	100
268.00	68.10	63.48
264.00	67.20	68.18
0.00	0.00	0.00