


Data Path : Z:\HPCHEM1\BNA G\DATA\BG060916\
 Data File : BG022258.D
 Acq On : 9 Jun 2016 7:45
 Operator : UM/SJ
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_G
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\HPCHEM1\BNA_G\METHODS\8270-BG060616.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Mon Jun 06 16:12:45 2016

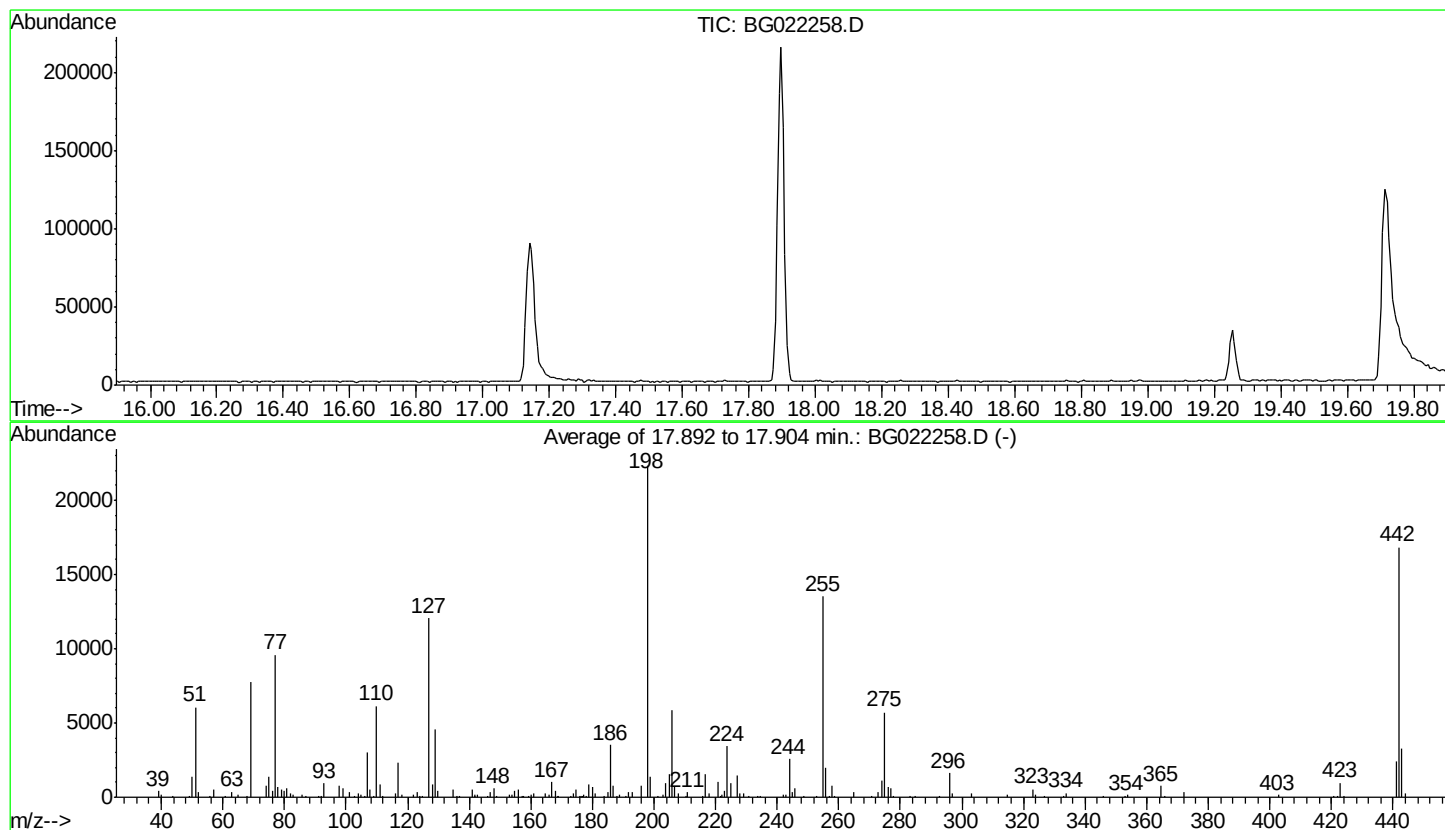

AutoFind: Scans 2562, 2563, 2564; Background Corrected with Scan 2555

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	27.1	6060	PASS
68	69	0.00	2	0.7	53	PASS
69	198	0.00	100	34.7	7757	PASS
70	69	0.00	2	0.0	0	PASS
127	198	10	80	54.0	12049	PASS
197	198	0.00	2	0.0	0	PASS
198	198	100	100	100.0	22333	PASS
199	198	5	9	6.4	1422	PASS
275	198	10	60	25.5	5705	PASS
365	198	1	100	3.4	756	PASS
441	442	0.01	24	14.4	2430	PASS
442	198	50	100	75.4	16845	PASS
443	442	15	24	19.6	3302	PASS