


Data Path : Z:\HPCHEM1\BNA G\DATA\BG060916\
Data File : BG022274.D
Acq On : 10 Jun 2016 00:19
Operator : UM/SJ
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
DFTPP

Integration File: rteint.p

Method : Z:\HPCHEM1\BNA_G\METHODS\8270-BG060616.M
Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
Last Update : Mon Jun 06 16:12:45 2016

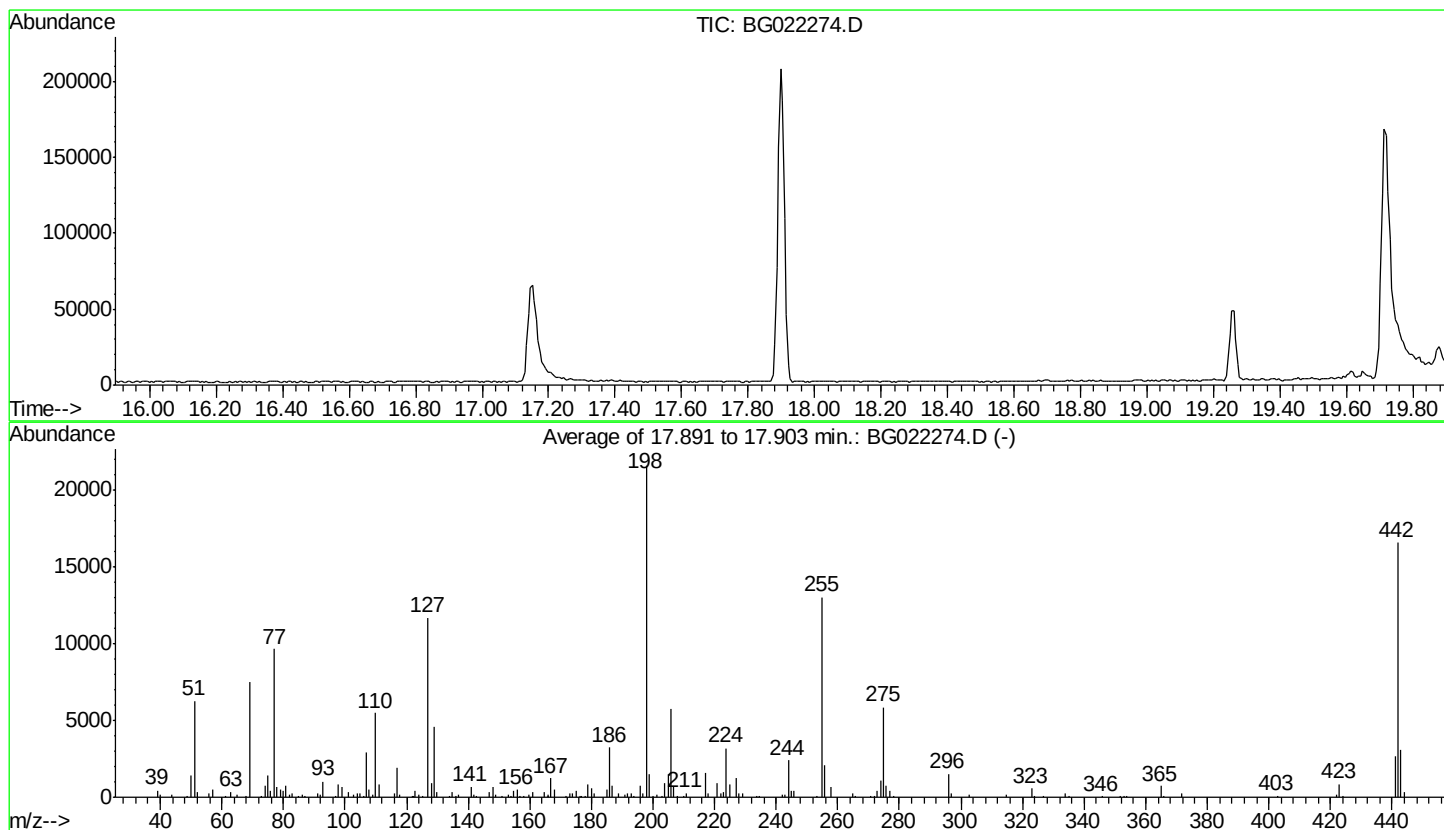

AutoFind: Scans 2562, 2563, 2564; Background Corrected with Scan 2555

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	29.1	6292	PASS
68	69	0.00	2	0.7	55	PASS
69	198	0.00	100	34.8	7530	PASS
70	69	0.00	2	0.0	0	PASS
127	198	10	80	54.1	11691	PASS
197	198	0.00	2	1.0	221	PASS
198	198	100	100	100.0	21613	PASS
199	198	5	9	6.8	1471	PASS
275	198	10	60	27.2	5884	PASS
365	198	1	100	3.3	720	PASS
441	442	0.01	24	16.0	2655	PASS
442	198	50	100	76.8	16603	PASS
443	442	15	24	18.7	3104	PASS