

Data Path : Z:\HPCHEM1\BNA G\DATA\BG060917\
 Data File : BG027361.D
 Acq On : 10 Jun 2017 00:03
 Operator : SJ/MA
 Sample : I3561-03
 Misc :
 ALS Vial : 14 Sample Multiplier: 1

Instrument :
 BNA_G
 ClientSampleId :

Quant Time: Jun 10 03:59:34 2017
 Quant Method : Z:\HPCHEM1\BNA G\METHODS\8270-BG060517.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Mon Jun 05 16:00:35 2017
 Response via : Initial Calibration


Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Dichlorobenzene-d4	8.55	152	47813	20.00	ng	-0.03
21) Naphthalene-d8	11.37	136	220618	20.00	ng	-0.03
38) Acenaphthene-d10	15.13	164	137468	20.00	ng	-0.03
63) Phenanthrene-d10	17.88	188	335283	20.00	ng	-0.03
75) Chrysene-d12	22.27	240	389945	20.00	ng	-0.04
86) Perylene-d12	25.95	264	374322	20.00	ng	-0.07
System Monitoring Compounds						
5) 2-Fluorophenol	6.14	112	8638	2.76	ng	-0.02
7) Phenol-d6	7.69	99	31957	6.95	ng	-0.01
23) Nitrobenzene-d5	9.72	82	92144	26.27	ng	-0.03
41) 2,4,6-Tribromophenol	16.61	330	4594	2.54	ng	-0.03
44) 2-Fluorobiphenyl	13.76	172	191347	19.47	ng	-0.03
78) Terphenyl-d14	20.46	244	209899	13.73	ng	-0.04
Target Compounds						
10) Phenol	7.71	94	27536	5.85	ng	Qvalue 82
15) Benzyl Alcohol	8.78	79	8197	2.53	ng	91
32) Benzoic acid	10.80	122	139	8.07	ng	# 1
35) Caprolactam	12.26	113	2539	2.29	ng	# 82
47) 2-Nitroaniline	14.00	65	84	6.86	ng	# 16
49) Dimethylphthalate	14.56	163	80705	7.40	ng	# 98
50) 2,6-Dinitrotoluene	14.62	165	487	5.81	ng	# 11
61) 4-Nitroaniline	16.38	138	150	5.95	ng	# 1


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\HPCHEM1\BNA G\DATA\BG060917\
Data File : BG027361.D
Acq On : 10 Jun 2017 00:03
Operator : SJ/MA
Sample : I3561-03
Misc :
ALS Vial : 14 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :

Quant Time: Jun 10 03:59:34 2017
Quant Method : Z:\HPCHEM1\BNA G\METHODS\8270-BG060517.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Mon Jun 05 16:00:35 2017
Response via : Initial Calibration

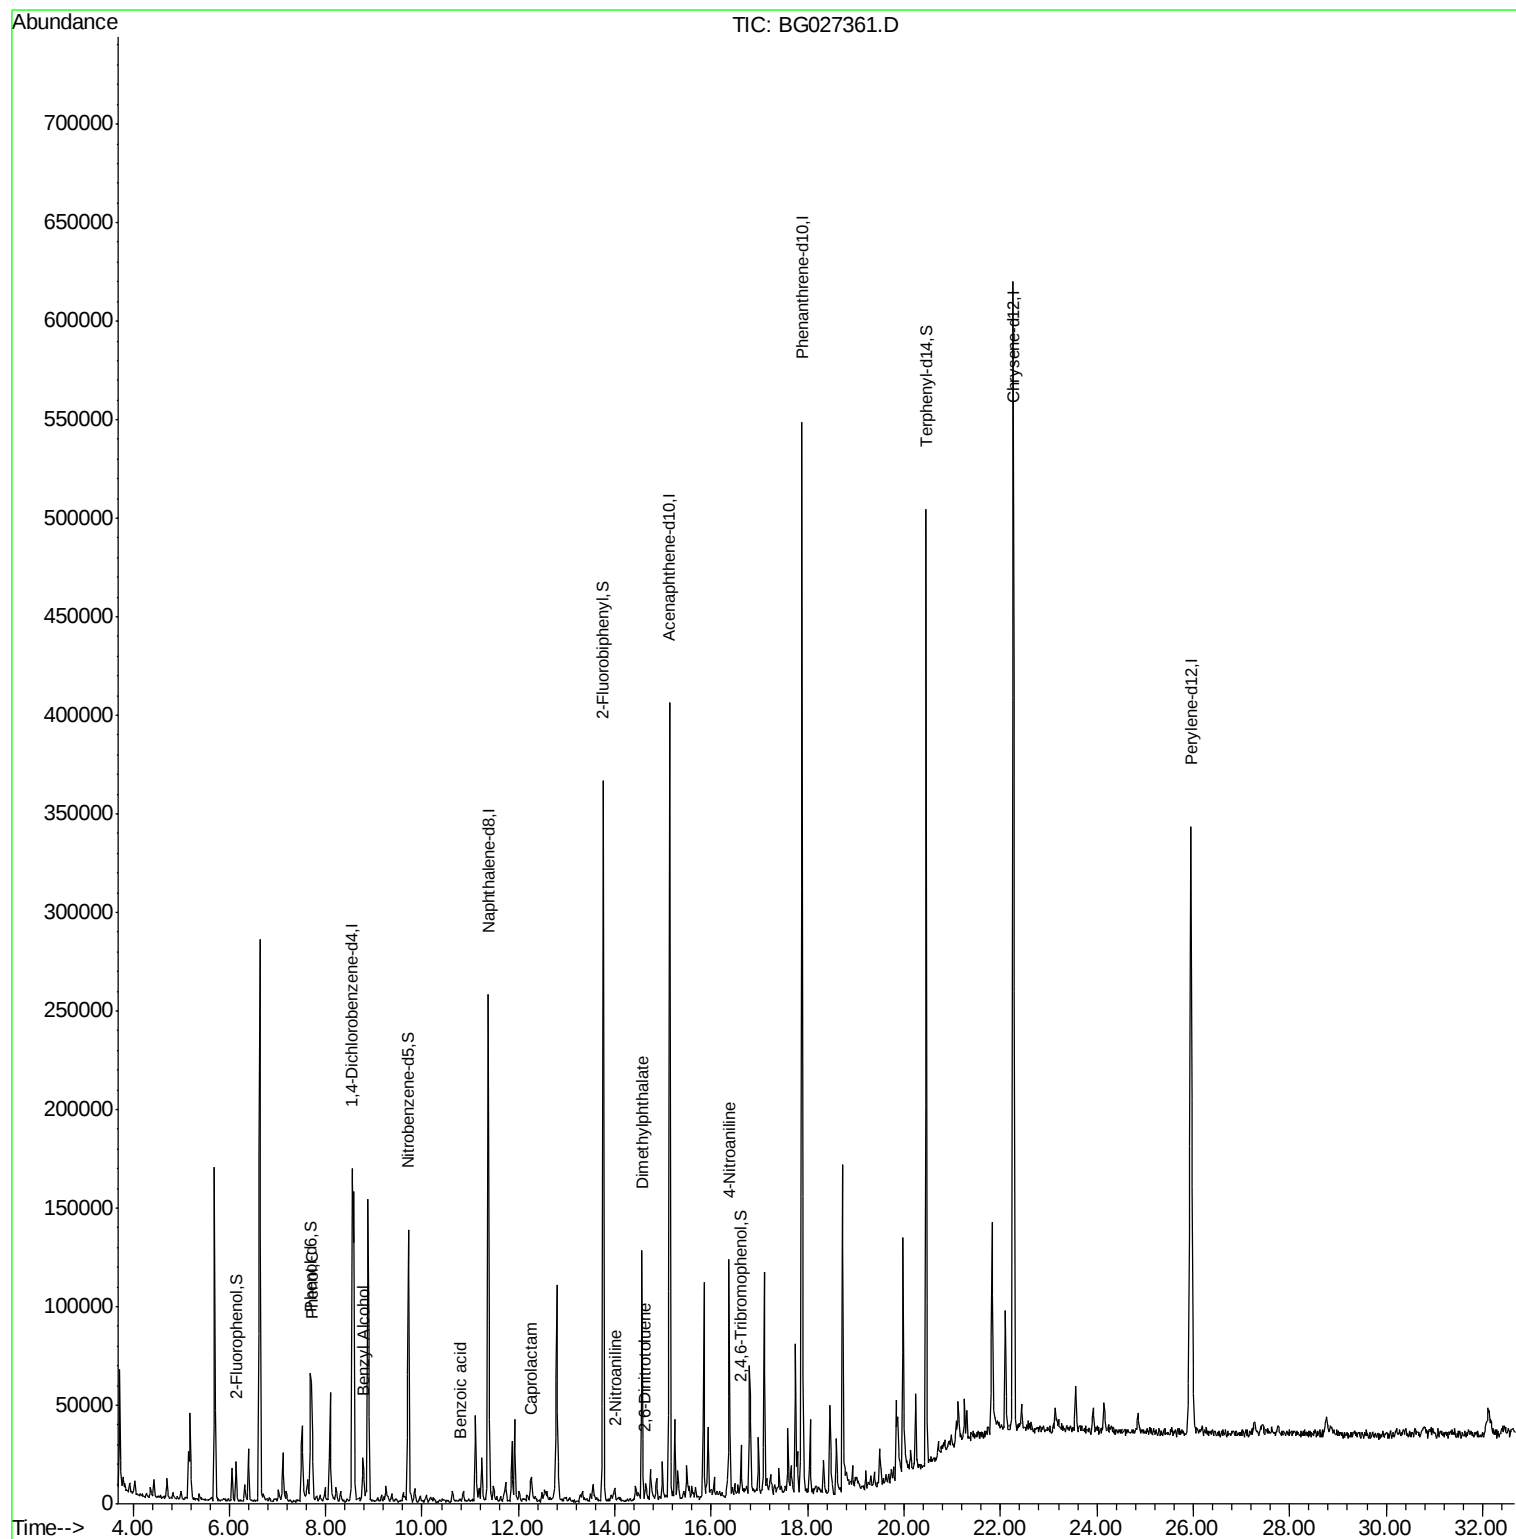

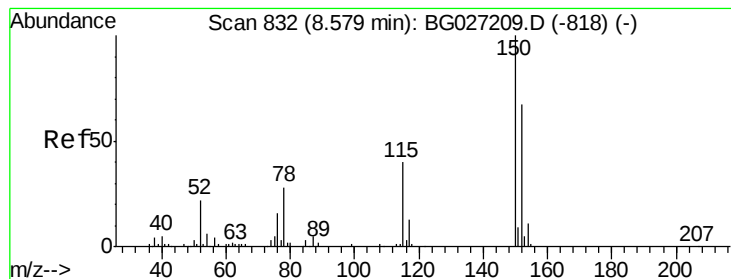

#1

1,4-Dichlorobenzene-d4

Concen: 20.00 ng

RT: 8.55 min Scan# 828

Delta R.T. -0.03 min

Lab File: BG027361.D

Acq: 10 Jun 2017 00:03

Instrument :

BNA_G

ClientSampled :


Tot Ion:152 Resp: 47813

Ion Ratio Lower Upper

152 100

150 154.6 114.0 171.0




115 68.3 48.1 72.1

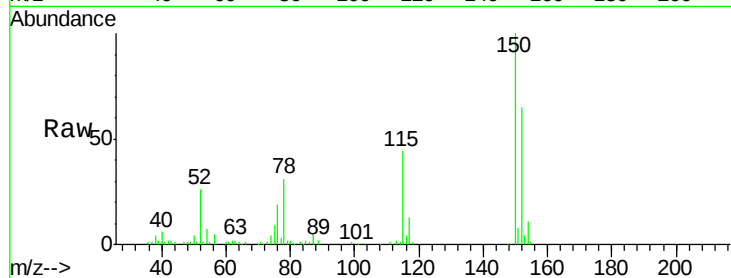

Abundance Ion 152.00 (151.70 to 152.70): E

Ion 150.00 (149.70 to 150.70): E

Ion 115.00 (114.70 to 115.70): E

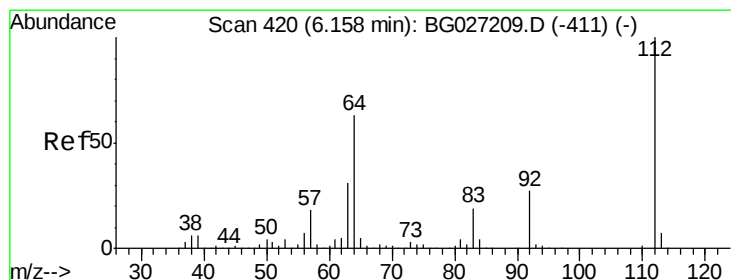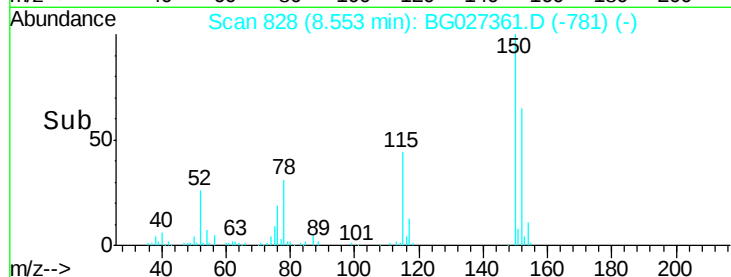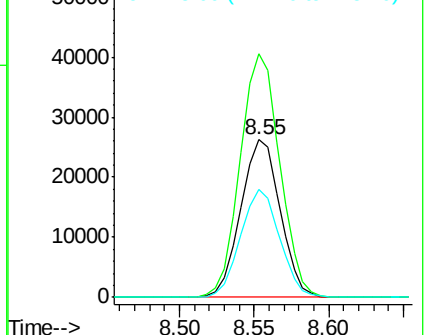

#5

2-Fluorophenol

Concen: 2.76 ng

RT: 6.14 min Scan# 417

Delta R.T. -0.02 min

Lab File: BG027361.D

Acq: 10 Jun 2017 00:03


Tgt Ion:112 Resp: 8638

Ion Ratio Lower Upper

112 100

64 66.2 61.8 92.6



63 29.3 37.2 55.8#

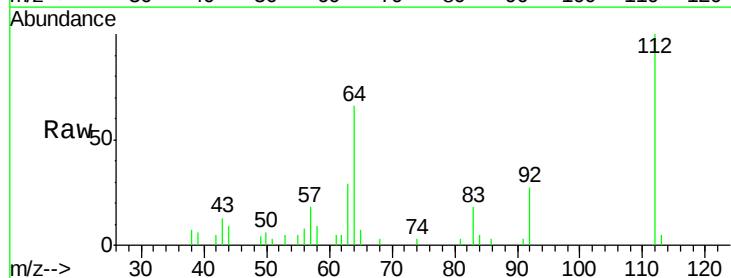


Abundance Ion 112.00 (111.70 to 112.70): E

Ion 64.00 (63.70 to 64.70): BGC

Ion 63.00 (62.70 to 63.70): BGC

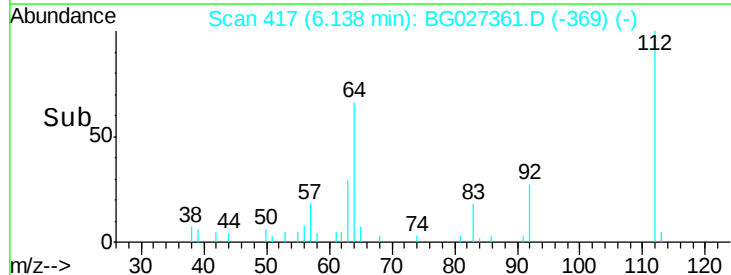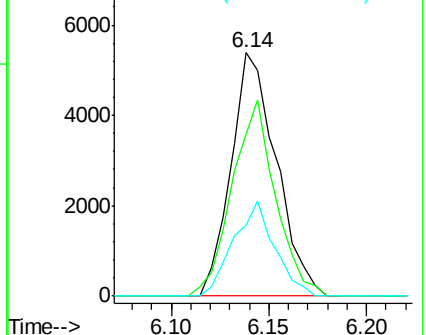

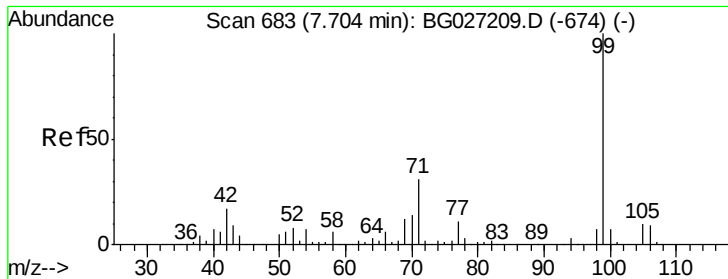

#7

Phenol-d6

Concen: 6.95 ng

RT: 7.69 min Scan# 681

Delta R.T. -0.01 min

Lab File: BG027361.D

Acq: 10 Jun 2017 00:03

Instrument :

BNA_G

ClientSampled :


Tot Ion: 99 Resp: 31957

Ion Ratio Lower Upper




99 100

42 18.3 20.5 30.7#

71 31.8 37.6 56.4#

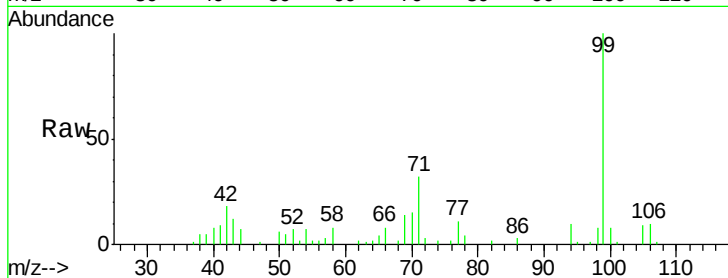

Abundance Ion 99.00 (98.70 to 99.70): BGC
Ion 42.00 (41.70 to 42.70): BGC
Ion 71.00 (70.70 to 71.70): BGC

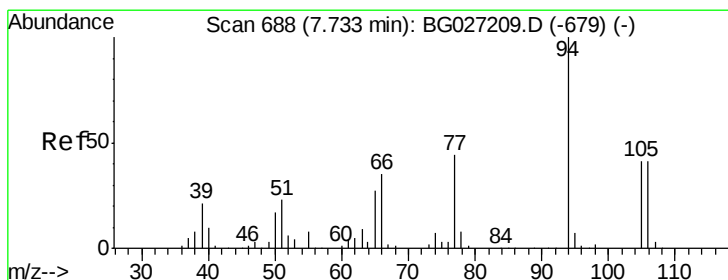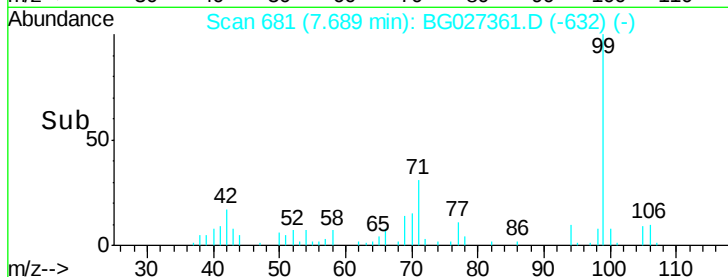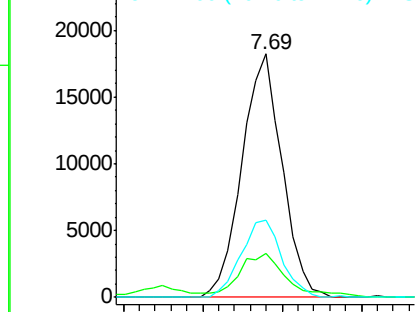

#10

Phenol

Concen: 5.85 ng

RT: 7.71 min Scan# 685

Delta R.T. -0.02 min

Lab File: BG027361.D

Acq: 10 Jun 2017 00:03


Tgt Ion: 94 Resp: 27536

Ion Ratio Lower Upper



94 100


65 35.4 20.6 60.6

66 37.8 35.5 75.5

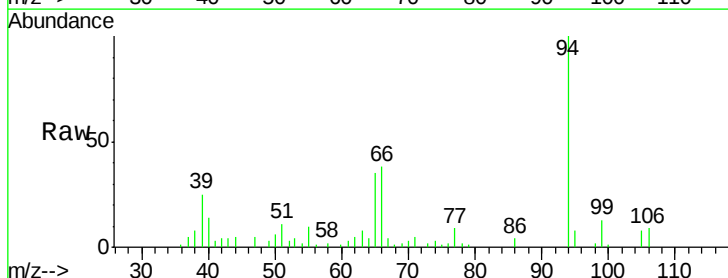

Abundance Ion 94.00 (93.70 to 94.70): BGC
Ion 65.00 (64.70 to 65.70): BGC
Ion 66.00 (65.70 to 66.70): BGC

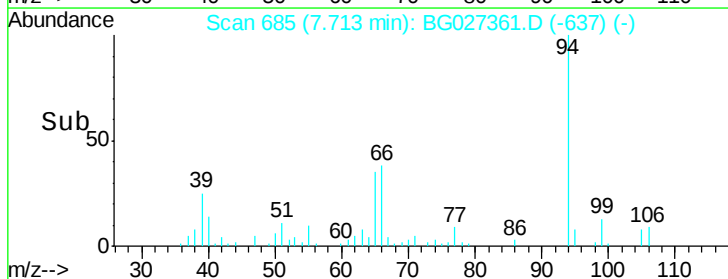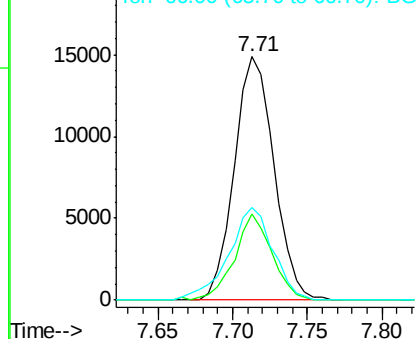

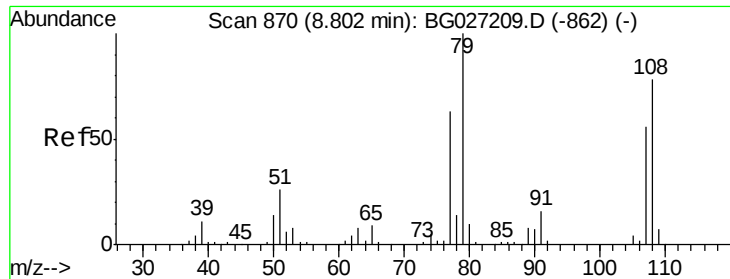

#15

Benzyl Alcohol

Concen: 2.53 ng

RT: 8.78 min Scan# 866

Delta R.T. -0.03 min

Lab File: BG027361.D

Acq: 10 Jun 2017 00:03

Instrument :

BNA_G

ClientSampled :


Tot Ion: 79 Resp: 8197

Ion Ratio Lower Upper




79 100

108 64.0 45.5 68.3

77 61.5 54.3 81.5

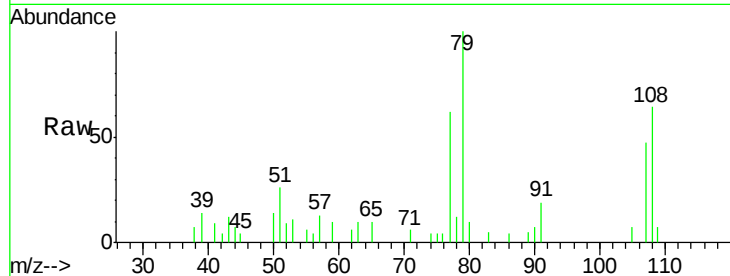

Abundance Ion 79.00 (78.70 to 79.70): BGC
Ion 108.00 (107.70 to 108.70): BGC
Ion 77.00 (76.70 to 77.70): BGC

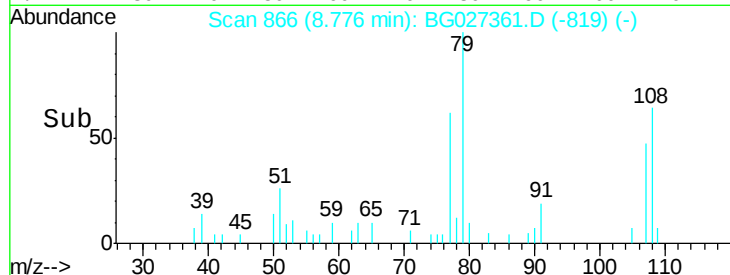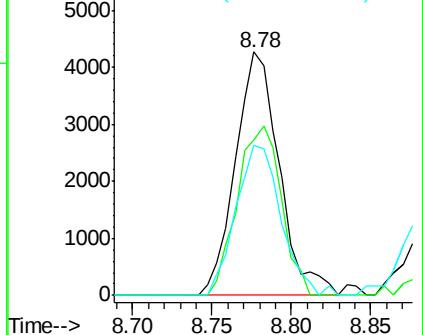

#21

Naphthalene-d8

Concen: 20.00 ng

RT: 11.37 min Scan# 1308

Delta R.T. -0.03 min

Lab File: BG027361.D

Acq: 10 Jun 2017 00:03

Tgt Ion: 136 Resp: 220618


Ion Ratio Lower Upper

136 100



137 10.8 8.9 13.3


54 10.5 9.3 13.9

68 8.7 5.1 7.7#

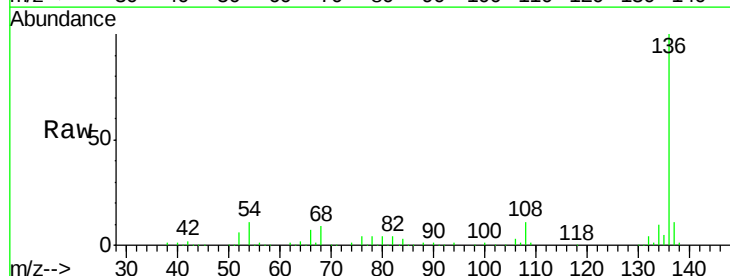

Abundance Ion 136.00 (135.70 to 136.70): BGC
Ion 137.00 (136.70 to 137.70): BGC
Ion 54.00 (53.70 to 54.70): BGC
Ion 68.00 (67.70 to 68.70): BGC



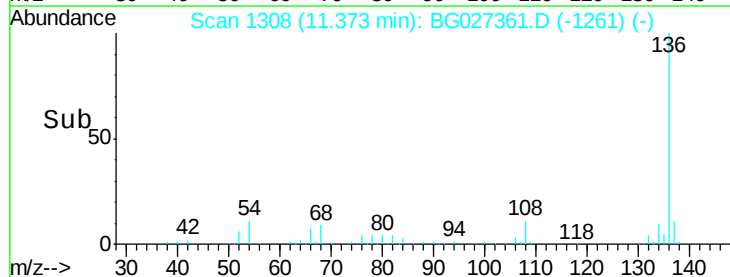
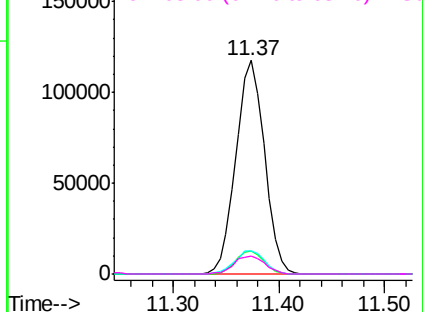


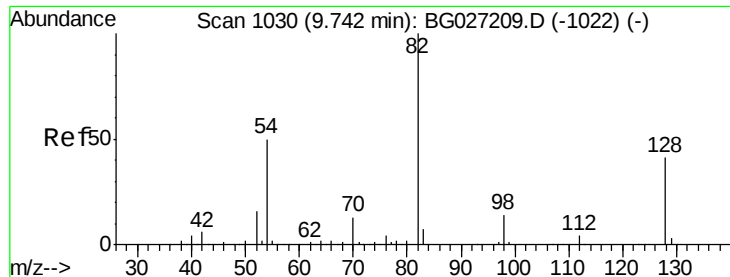

#23
Nitrobenzene-d5
Concen: 26.27 ng
RT: 9.72 min Scan# 1026
Delta R.T. -0.03 min
Lab File: BG027361.D
Acq: 10 Jun 2017 00:03




Instrument :
BNA_G
ClientSampleId :


Tot Ion: 82 Resp: 92144
Ion Ratio Lower Upper
82 100
128 40.1 26.4 39.6#
54 53.0 49.4 74.2

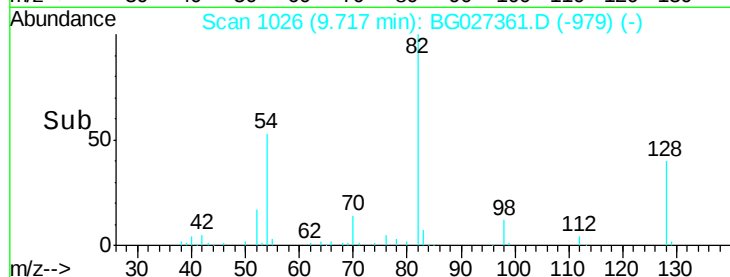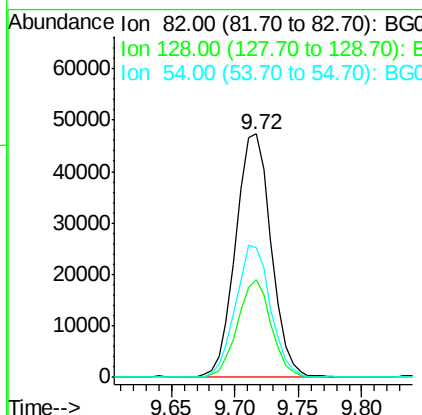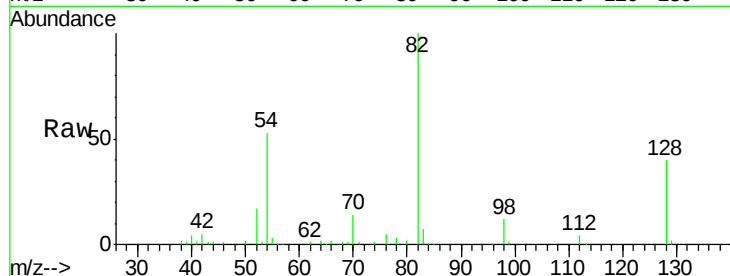

#32
Benzoic acid
Concen: 8.07 ng
RT: 10.80 min Scan# 1211
Delta R.T. 0.15 min
Lab File: BG027361.D
Acq: 10 Jun 2017 00:03

Tgt Ion: 122 Resp: 139
Ion Ratio Lower Upper
122 100
105 0.0 120.1 160.1#
77 0.0 104.6 144.6#

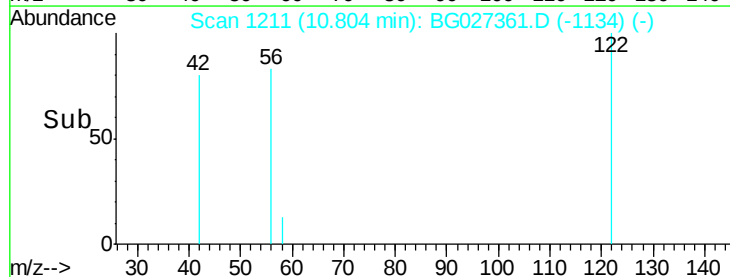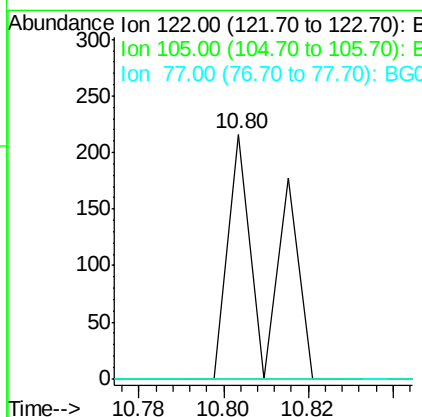

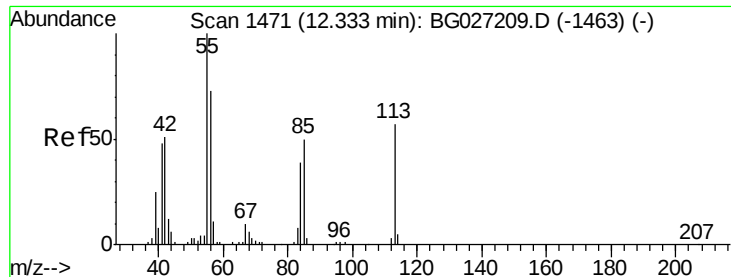

#35

Caprolactam

Concen: 2.29 ng

RT: 12.26 min Scan# 1459

Delta R.T. -0.07 min

Lab File: BG027361.D

Acq: 10 Jun 2017 00:03

Instrument :

BNA_G

ClientSampled :


Tot Ion:113 Resp: 2539

Ion Ratio Lower Upper

113 100

55 191.4 198.6 238.6#




56 133.9 140.4 180.4#

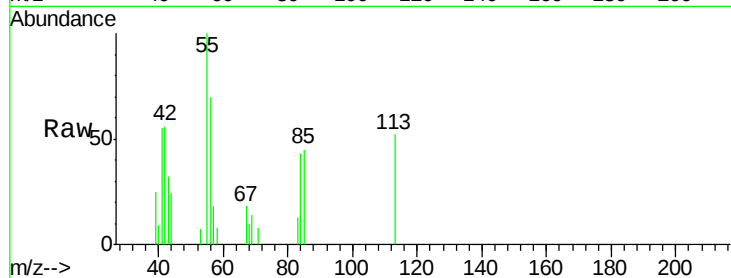

Abundance Ion 113.00 (112.70 to 113.70): E

Ion 55.00 (54.70 to 55.70): BGC

Ion 56.00 (55.70 to 56.70): BGC

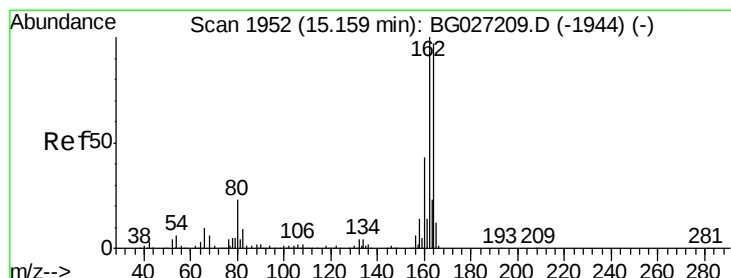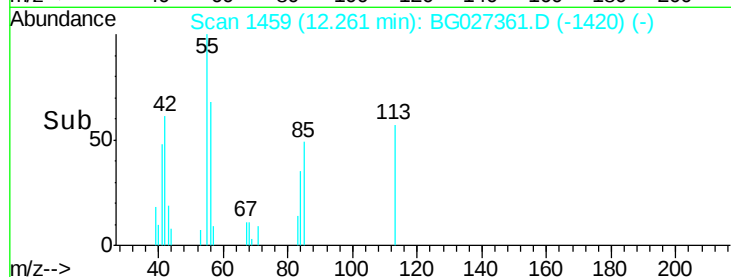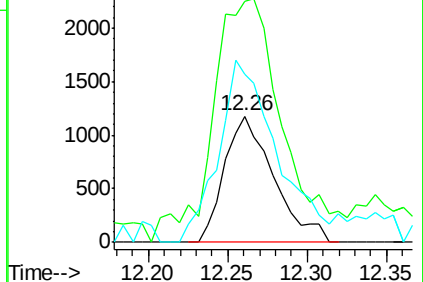

#38

Acenaphthene-d10

Concen: 20.00 ng

RT: 15.13 min Scan# 1948

Delta R.T. -0.03 min

Lab File: BG027361.D

Acq: 10 Jun 2017 00:03


Tgt Ion:164 Resp: 137468

Ion Ratio Lower Upper

164 100

162 105.5 85.1 127.7



160 44.6 34.7 52.1

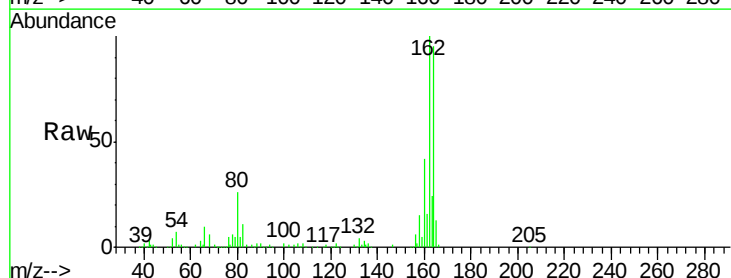


Abundance Ion 164.00 (163.70 to 164.70): E

Ion 162.00 (161.70 to 162.70): E

Ion 160.00 (159.70 to 160.70): E



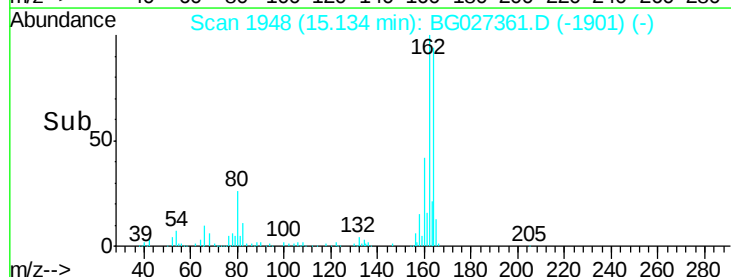
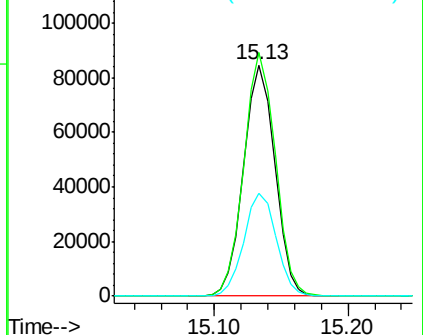


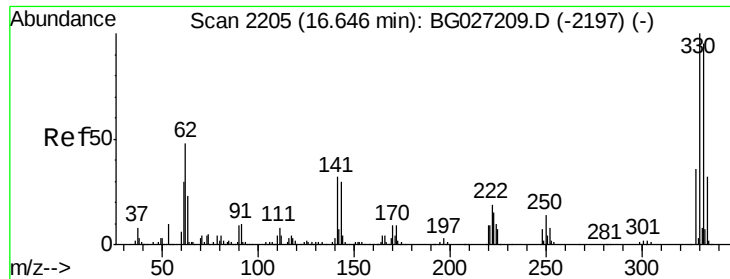

#41
 2,4,6-Tribromophenol
 Concen: 2.54 ng
 RT: 16.61 min Scan# 2200
 Delta R.T. -0.03 min
 Lab File: BG027361.D
 Acq: 10 Jun 2017 00:03




Instrument :
 BNA_G
 ClientSampleId :


Tot Ion:330 Resp: 4594
 Ion Ratio Lower Upper
 330 100
 332 104.9 77.3 115.9
 141 36.4 32.1 48.1

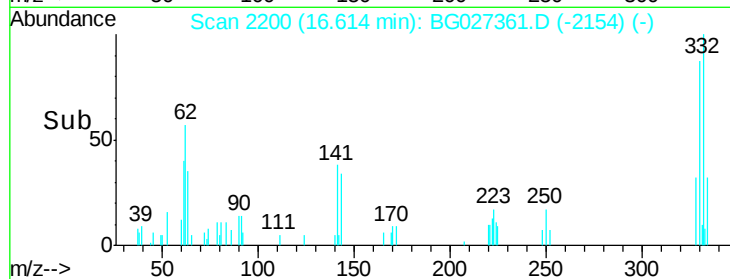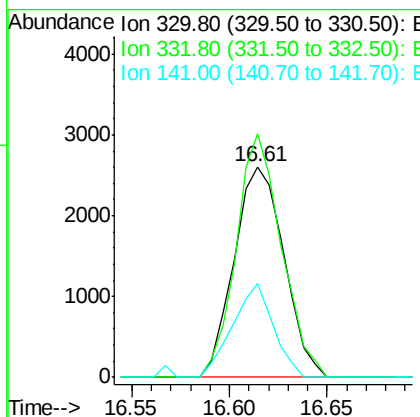

#44
 2-Fluorobiphenyl
 Concen: 19.47 ng
 RT: 13.76 min Scan# 1714
 Delta R.T. -0.03 min
 Lab File: BG027361.D
 Acq: 10 Jun 2017 00:03

Tgt Ion:172 Resp: 191347
 Ion Ratio Lower Upper
 172 100
 171 36.3 32.2 48.2
 170 22.8 21.8 32.6


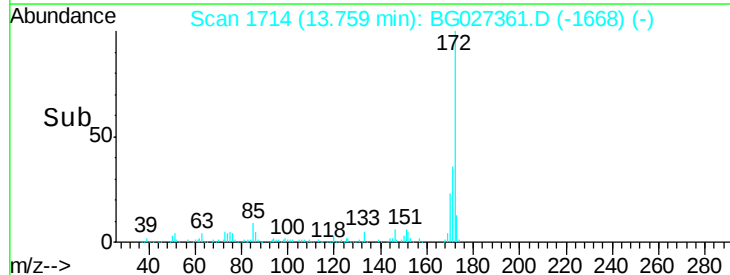
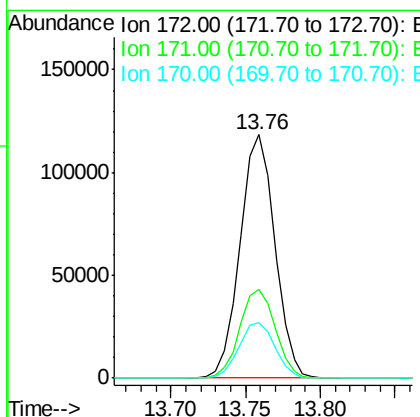



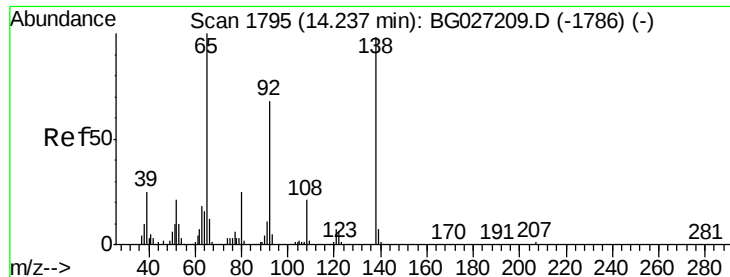

#47
2-Nitroaniline
Concen: 6.86 ng
RT: 14.00 min Scan# 1755
Delta R.T. -0.24 min
Lab File: BG027361.D
Acq: 10 Jun 2017 00:03




Instrument :
BNA_G
ClientSampleId :


Tot Ion: 65 Resp: 84
Ion Ratio Lower Upper
65 100
92 0.0 49.0 73.4#
138 0.0 58.6 87.8#

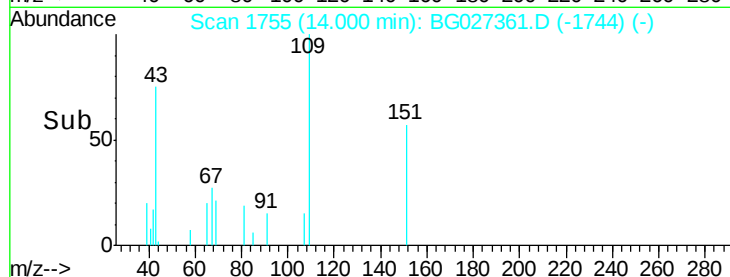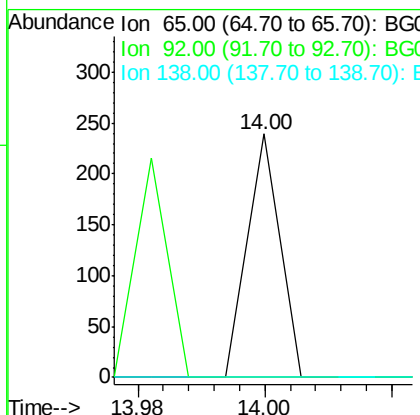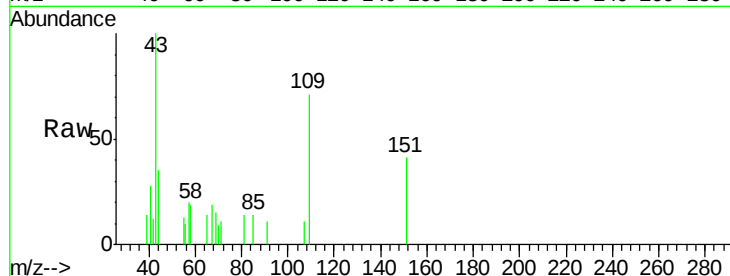

#49
Dimethylphthalate
Concen: 7.40 ng
RT: 14.56 min Scan# 1851
Delta R.T. -0.04 min
Lab File: BG027361.D
Acq: 10 Jun 2017 00:03

Tgt Ion: 163 Resp: 80705
Ion Ratio Lower Upper
163 100
194 3.3 3.8 5.6#
164 10.9 9.3 13.9


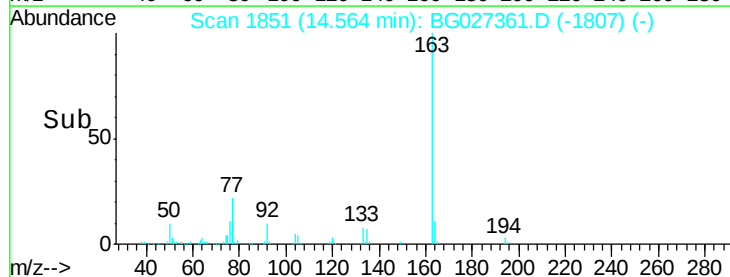
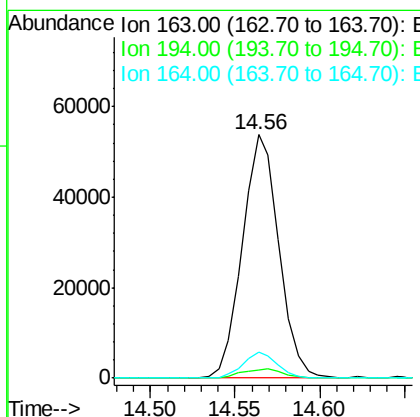



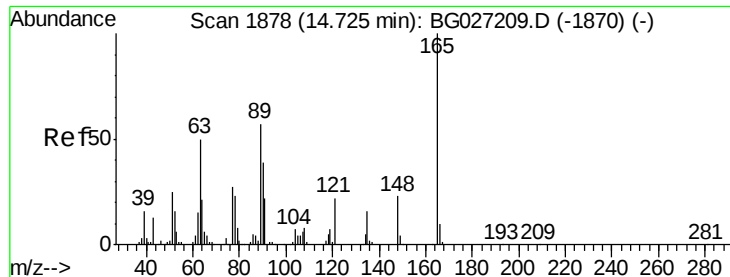

#50
 2,6-Dinitrotoluene
 Concen: 5.81 ng
 RT: 14.62 min Scan# 1861
 Delta R.T. -0.10 min
 Lab File: BG027361.D
 Acq: 10 Jun 2017 00:03




Instrument :
 BNA_G
 ClientSampleId :


Tot Ion:165 Resp: 487
 Ion Ratio Lower Upper
 165 100
 63 0.0 63.9 95.9#
 89 0.0 58.6 88.0#

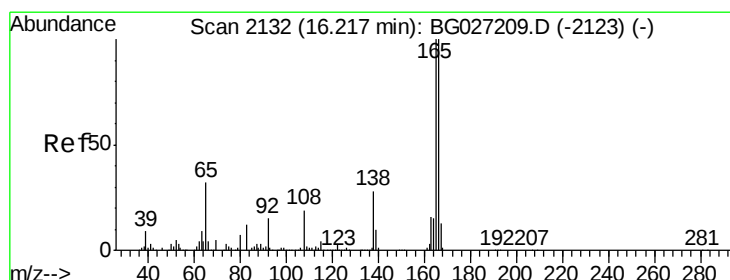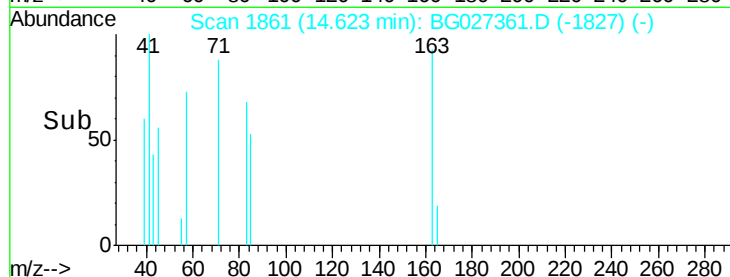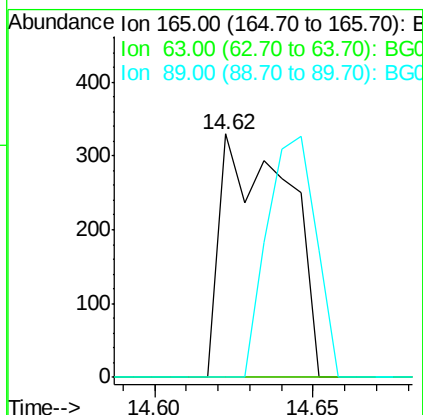

#61
 4-Nitroaniline
 Concen: 5.95 ng
 RT: 16.38 min Scan# 2160
 Delta R.T. 0.16 min
 Lab File: BG027361.D
 Acq: 10 Jun 2017 00:03

Tgt Ion:138 Resp: 150
 Ion Ratio Lower Upper
 138 100
 92 0.0 44.2 84.2#
 108 0.0 104.8 144.8#


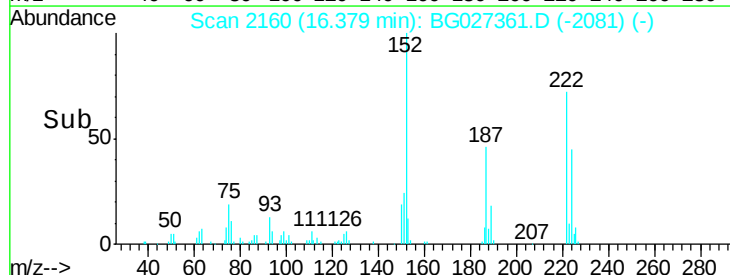
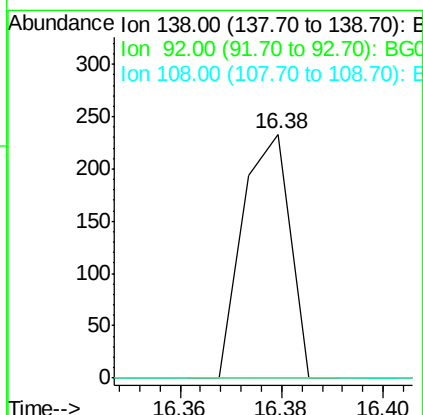



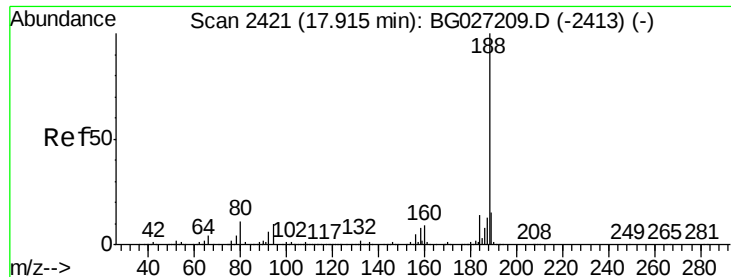

#63
Phenanthrene-d10
Concen: 20.00 ng
RT: 17.88 min Scan# 2416
Delta R.T. -0.03 min
Lab File: BG027361.D
Acq: 10 Jun 2017 00:03




Instrument :
BNA_G
ClientSampleId :


Tot Ion:188 Resp: 335283
Ion Ratio Lower Upper
188 100
94 11.5 5.8 8.8#
80 13.4 7.5 11.3#

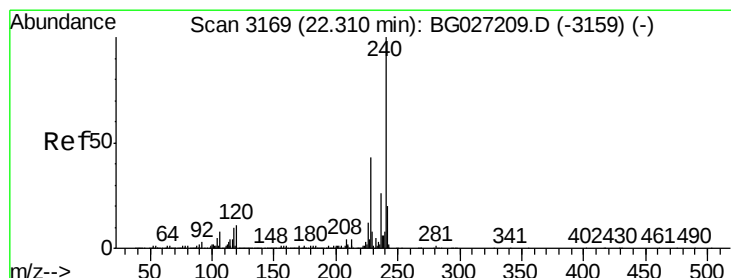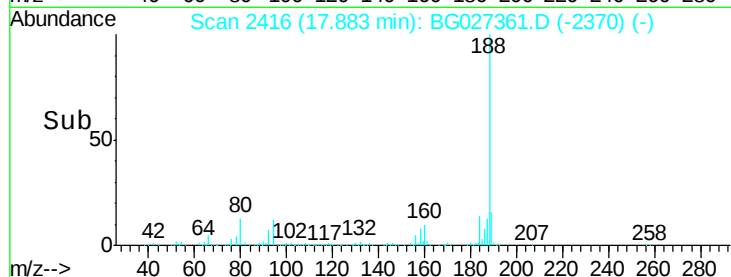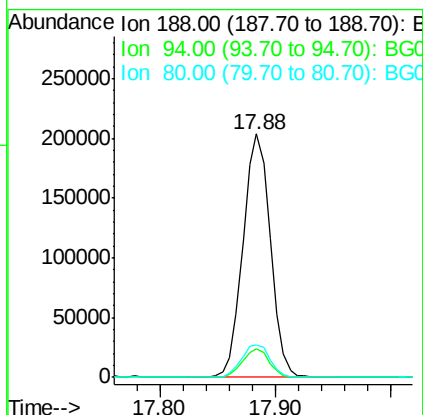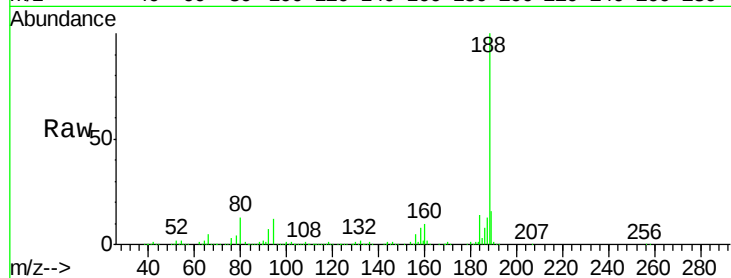

#75
Chrysene-d12
Concen: 20.00 ng
RT: 22.27 min Scan# 3162
Delta R.T. -0.04 min
Lab File: BG027361.D
Acq: 10 Jun 2017 00:03

Tgt Ion:240 Resp: 389945
Ion Ratio Lower Upper
240 100
120 12.0 5.7 8.5#
236 26.0 22.2 33.4

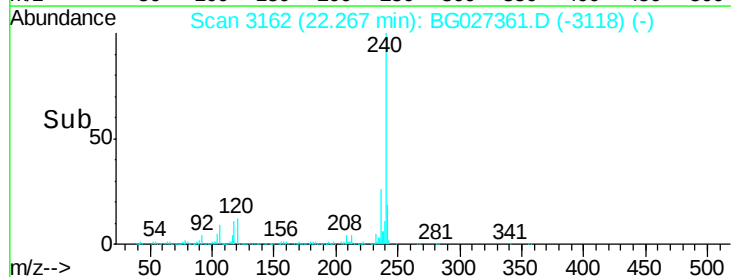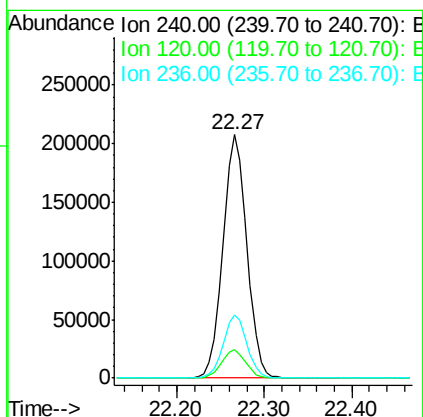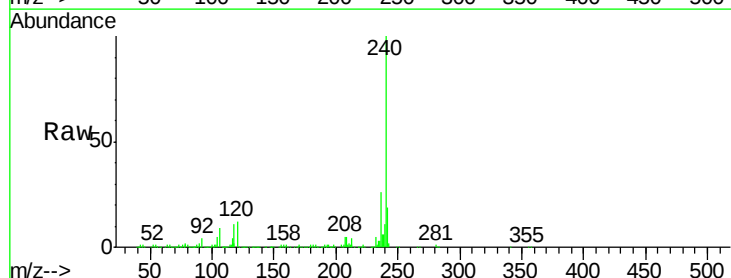

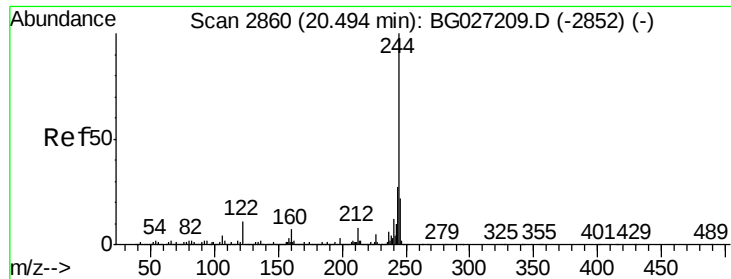

#78

Terphenyl-d14

Concen: 13.73 ng

RT: 20.46 min Scan# 2854

Delta R.T. -0.04 min

Lab File: BG027361.D

Acq: 10 Jun 2017 00:03

Instrument :

BNA_G

ClientSampleId :


Tot Ion:244 Resp: 209899

Ion Ratio Lower Upper




244 100

212 7.1 10.0 15.0#

122 11.7 8.6 12.8

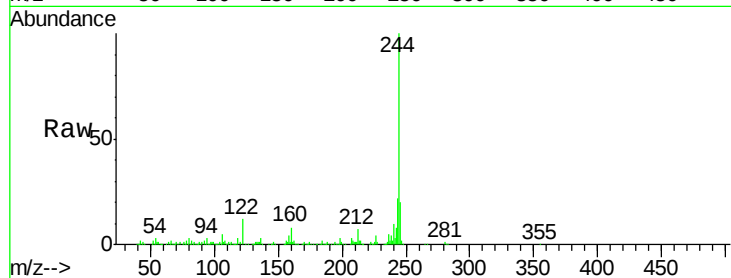

Abundance Ion 244.00 (243.70 to 244.70): E
Ion 212.00 (211.70 to 212.70): E
Ion 122.00 (121.70 to 122.70): E

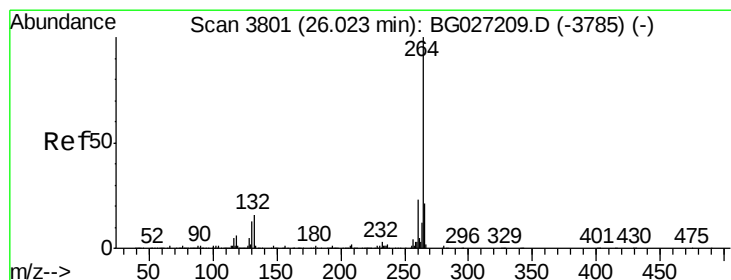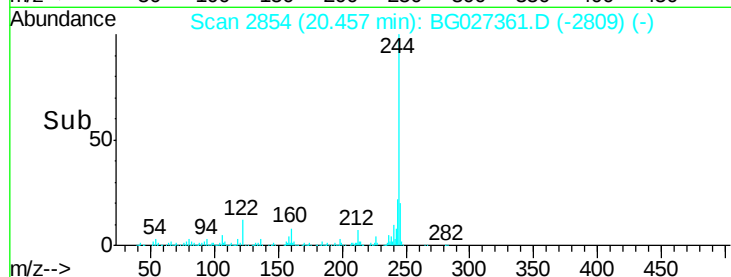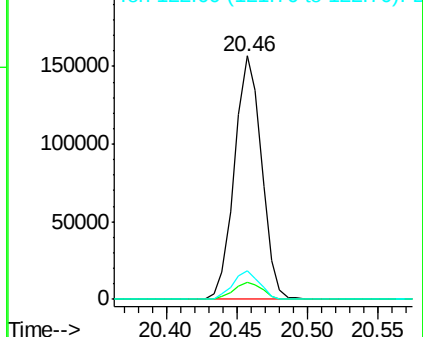

#86

Perylene-d12

Concen: 20.00 ng

RT: 25.95 min Scan# 3789

Delta R.T. -0.07 min

Lab File: BG027361.D

Acq: 10 Jun 2017 00:03


Tgt Ion:264 Resp: 374322

Ion Ratio Lower Upper

264 100

260 24.3 21.8 32.8

265 21.4 18.2 27.4

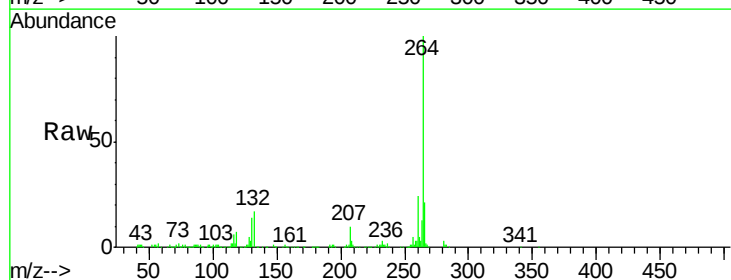

Abundance Ion 264.00 (263.70 to 264.70): E
Ion 260.00 (259.70 to 260.70): E
Ion 265.00 (264.70 to 265.70): E

