


Data Path : Z:\HPCHEM1\BNA_G\Data\BG060917\
 Data File : BG027347.D
 Acq On : 9 Jun 2017 14:45
 Operator : SJ/MA
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_G
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\HPCHEM1\BNA_G\METHODS\8270-BG060517.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Mon Jun 05 16:00:35 2017

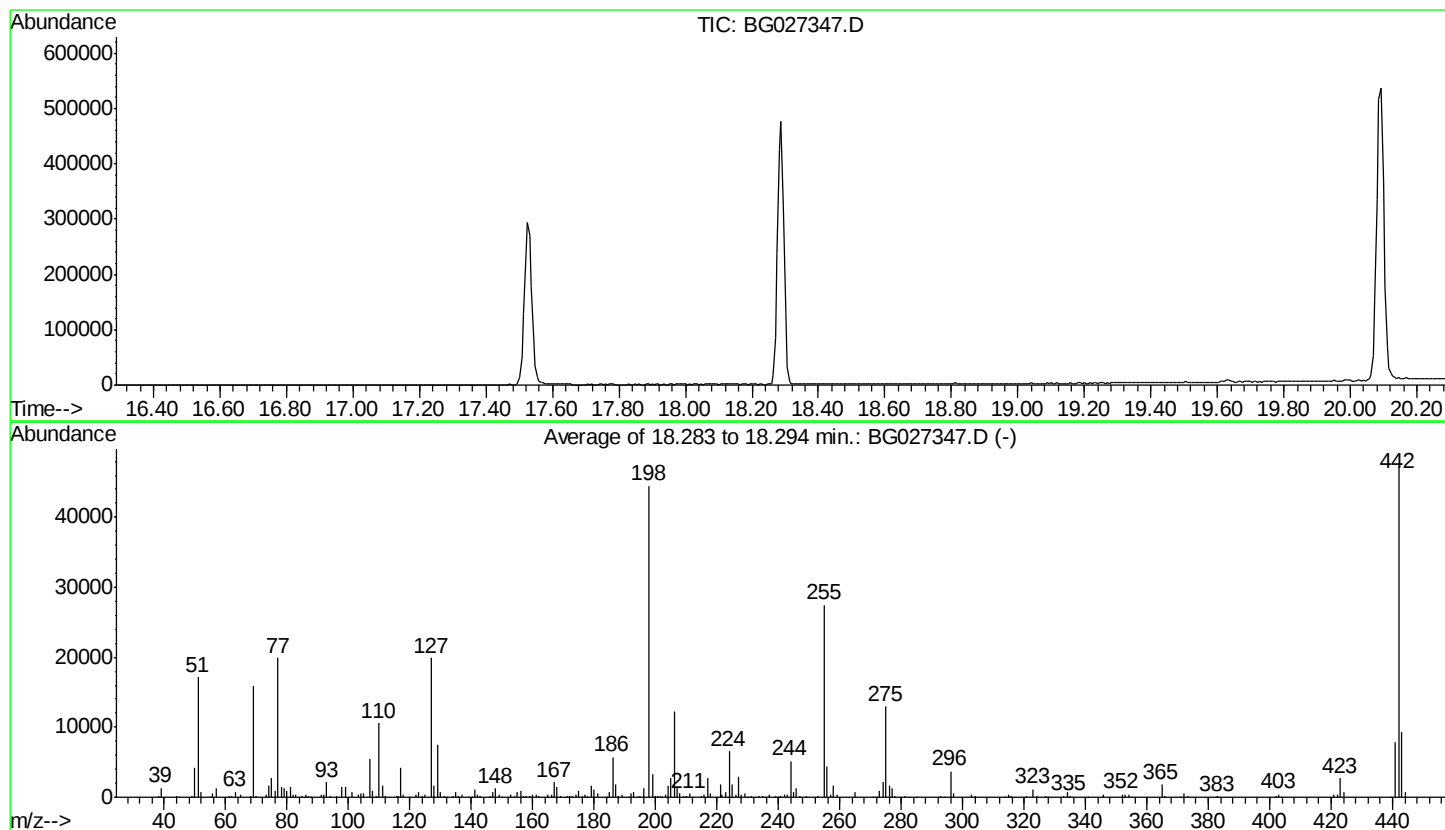

AutoFind: Scans 2484, 2485, 2486; Background Corrected with Scan 2477

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	38.6	17159	PASS
68	69	0.00	2	0.6	103	PASS
69	198	0.00	100	35.6	15853	PASS
70	69	0.00	2	0.8	134	PASS
127	198	10	80	44.6	19866	PASS
197	198	0.00	2	0.0	0	PASS
198	198	100	100	100.0	44501	PASS
199	198	5	9	7.3	3261	PASS
275	198	10	60	29.2	12973	PASS
365	198	1	100	4.0	1787	PASS
441	442	0.01	24	16.5	7799	PASS
442	198	50	100	106.5	47378	FAIL *
443	442	15	24	19.5	9252	PASS