


Data Path : Z:\HPCHEM1\BNA_G\Data\BG060917\
 Data File : BG027348.D
 Acq On : 9 Jun 2017 15:25
 Operator : SJ/MA
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_G
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\HPCHEM1\BNA_G\METHODS\8270-BG060517.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Mon Jun 05 16:00:35 2017

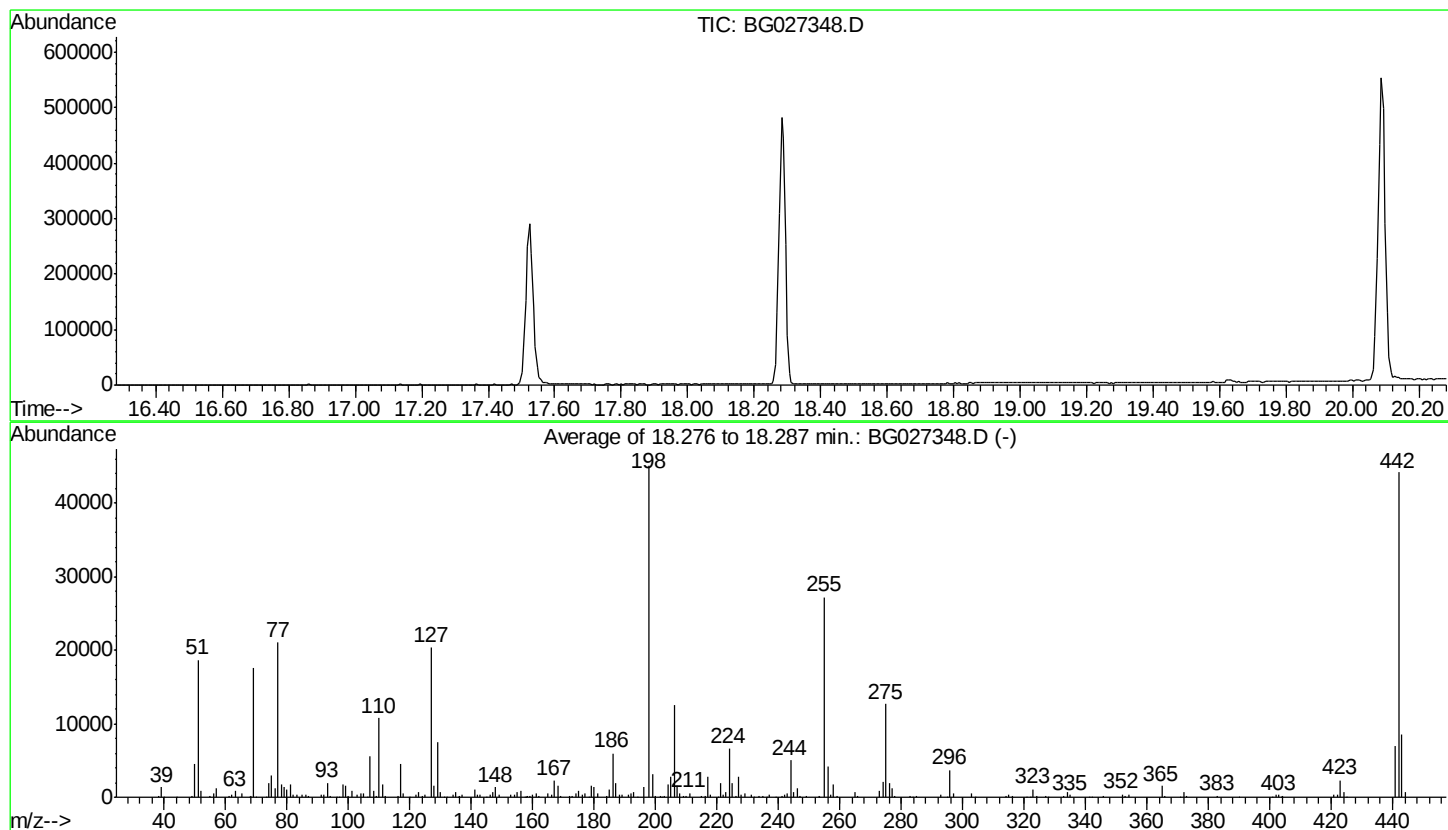

AutoFind: Scans 2483, 2484, 2485; Background Corrected with Scan 2477

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	41.4	18664	PASS
68	69	0.00	2	1.1	195	PASS
69	198	0.00	100	39.0	17584	PASS
70	69	0.00	2	0.3	57	PASS
127	198	10	80	45.1	20366	PASS
197	198	0.00	2	0.0	0	PASS
198	198	100	100	100.0	45109	PASS
199	198	5	9	6.8	3082	PASS
275	198	10	60	28.1	12691	PASS
365	198	1	100	3.4	1528	PASS
441	442	0.01	24	15.9	7030	PASS
442	198	50	100	98.1	44248	PASS
443	442	15	24	19.2	8502	PASS